

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026116.D
 Acq On : 28 Dec 2021 22:42
 Operator : JC/MD
 Sample : M5216-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	130403	138534	16.57%	2.189%
2	1.672	92	96	103	rVB	106115	122161	14.61%	1.930%
3	2.312	195	201	211	rBV	203197	325703	38.96%	5.146%
4	2.501	230	232	233	rBV	783	604	0.07%	0.010%
5	2.709	264	266	268	rBV2	738	982	0.12%	0.016%
6	2.837	285	287	289	rBV	677	570	0.07%	0.009%
7	3.062	323	324	327	rBV	489	566	0.07%	0.009%
8	3.672	423	424	426	rBV	777	566	0.07%	0.009%
9	3.788	442	443	447	rBV	550	735	0.09%	0.012%
10	3.983	473	475	479	rVB	698	708	0.08%	0.011%
11	4.123	496	498	501	rVB	553	548	0.07%	0.009%
12	4.154	501	503	504	rBV	790	606	0.07%	0.010%
13	4.367	536	538	540	rBV	608	712	0.09%	0.011%
14	4.458	545	553	566	rBV2	60729	181937	21.76%	2.875%
15	4.855	616	618	621	rVB2	664	719	0.09%	0.011%
16	4.891	621	624	626	rBV	733	799	0.10%	0.013%
17	5.068	641	653	669	rBV	118221	346866	41.49%	5.481%
18	5.263	682	685	688	rBV2	517	835	0.10%	0.013%
19	5.787	770	771	779	rBV3	895	1633	0.20%	0.026%
20	5.976	790	802	817	rBV2	279393	835937	100.00%	13.208%
21	6.251	843	847	850	rBV	572	582	0.07%	0.009%
22	6.373	863	867	869	rBV2	766	817	0.10%	0.013%
23	6.476	881	884	886	rVB2	468	540	0.06%	0.009%
24	6.586	899	902	905	rBV	804	833	0.10%	0.013%
25	6.769	923	932	944	rBV	196753	460555	55.09%	7.277%
26	7.001	969	970	973	rBV	510	541	0.06%	0.009%
27	7.116	983	989	996	rVB3	3292	7256	0.87%	0.115%
28	7.312	1013	1021	1034	rBV	172449	378542	45.28%	5.981%
29	7.598	1067	1068	1071	rVB	756	558	0.07%	0.009%
30	7.647	1075	1076	1079	rVB	1024	799	0.10%	0.013%
31	7.787	1097	1099	1102	rBV2	737	809	0.10%	0.013%
32	7.811	1102	1103	1108	rVV	712	744	0.09%	0.012%
33	8.068	1143	1145	1148	rVB2	788	985	0.12%	0.016%
34	8.330	1181	1188	1199	rBV	120153	201561	24.11%	3.185%
35	8.476	1209	1212	1217	rBV3	931	1353	0.16%	0.021%
36	8.580	1227	1229	1230	rVV	914	608	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026116.D
 Acq On : 28 Dec 2021 22:42
 Operator : JC/MD
 Sample : M5216-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1248	rVV	427391	664570	79.50%	10.500%
38	8.720	1248	1252	1261	rVB2	5852	10530	1.26%	0.166%
39	8.952	1284	1290	1301	rVV	88904	129677	15.51%	2.049%
40	9.208	1331	1332	1335	rBV	568	582	0.07%	0.009%
41	9.384	1356	1361	1377	rVB	281196	403714	48.29%	6.379%
42	9.726	1414	1417	1420	rBV2	467	671	0.08%	0.011%
43	9.878	1439	1442	1445	rBV	776	1064	0.13%	0.017%
44	9.933	1449	1451	1452	rBV	620	529	0.06%	0.008%
45	10.055	1466	1471	1482	rBV	405365	566646	67.79%	8.953%
46	10.195	1492	1494	1499	rVB3	787	1289	0.15%	0.020%
47	10.244	1499	1502	1505	rBV2	696	806	0.10%	0.013%
48	10.311	1508	1513	1514	rBV2	1264	1601	0.19%	0.025%
49	10.445	1533	1535	1536	rBV2	696	645	0.08%	0.010%
50	10.561	1552	1554	1558	rBV2	656	742	0.09%	0.012%
51	10.750	1583	1585	1587	rBV	696	595	0.07%	0.009%
52	10.927	1612	1614	1617	rVB	767	697	0.08%	0.011%
53	11.030	1629	1631	1635	rVB4	1028	1190	0.14%	0.019%
54	11.122	1643	1646	1650	rVV2	3565	4404	0.53%	0.070%
55	11.195	1652	1658	1666	rVV	299304	374235	44.77%	5.913%
56	11.268	1666	1670	1673	rVV5	1032	1838	0.22%	0.029%
57	11.329	1676	1680	1685	rVB3	3966	6044	0.72%	0.095%
58	11.445	1695	1699	1702	rBV2	634	734	0.09%	0.012%
59	11.482	1702	1705	1708	rVB	1455	1542	0.18%	0.024%
60	11.707	1741	1742	1744	rBV	976	690	0.08%	0.011%
61	11.750	1746	1749	1753	rVB2	2840	3752	0.45%	0.059%
62	11.780	1753	1754	1756	rBV	708	532	0.06%	0.008%
63	11.817	1756	1760	1762	rVB2	647	970	0.12%	0.015%
64	11.841	1762	1764	1766	rBV2	930	954	0.11%	0.015%
65	11.933	1777	1779	1781	rVB2	1586	1009	0.12%	0.016%
66	11.969	1782	1785	1789	rVB2	2492	2648	0.32%	0.042%
67	12.024	1789	1794	1806	rVB	399246	511238	61.16%	8.078%
68	12.128	1806	1811	1813	rBV3	1471	2309	0.28%	0.036%
69	12.219	1822	1826	1832	rBV4	6236	8727	1.04%	0.138%
70	12.323	1837	1843	1850	rVV	434024	565092	67.60%	8.929%
71	12.372	1850	1851	1854	rVB2	669	563	0.07%	0.009%
72	12.494	1866	1871	1873	rBV3	593	979	0.12%	0.015%
73	12.603	1886	1889	1890	rBV2	624	663	0.08%	0.010%
74	12.719	1905	1908	1909	rVB	638	550	0.07%	0.009%
75	12.762	1913	1915	1919	rVV2	1058	1599	0.19%	0.025%
76	12.859	1927	1931	1937	rBV3	1786	3163	0.38%	0.050%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
 Data File : VX026116.D
 Acq On : 28 Dec 2021 22:42
 Operator : JC/MD
 Sample : M5216-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	12.981	1949	1951	1958	rVB2	549	985	0.12%	0.016%
78	13.079	1966	1967	1971	rBV	796	802	0.10%	0.013%
79	13.115	1971	1973	1977	rVB	1016	921	0.11%	0.015%
80	13.146	1977	1978	1980	rBV	856	623	0.07%	0.010%
81	13.426	2023	2024	2028	rVB	665	552	0.07%	0.009%
82	13.542	2041	2043	2046	rVB	750	654	0.08%	0.010%
83	13.591	2046	2051	2058	rBV2	9920	12510	1.50%	0.198%
84	13.658	2060	2062	2066	rBV	508	657	0.08%	0.010%
85	13.695	2066	2068	2071	rVB	791	721	0.09%	0.011%
86	13.774	2077	2081	2083	rBV2	548	667	0.08%	0.011%
87	13.945	2106	2109	2110	rBV	516	544	0.07%	0.009%
88	13.963	2110	2112	2116	rBV3	1630	2160	0.26%	0.034%
89	14.243	2156	2158	2162	rBV2	546	639	0.08%	0.010%
90	14.542	2204	2207	2208	rBV	721	738	0.09%	0.012%
91	14.682	2228	2230	2232	rVB2	742	608	0.07%	0.010%
92	14.877	2260	2262	2266	rBV2	594	614	0.07%	0.010%
93	15.054	2289	2291	2294	rBV2	642	614	0.07%	0.010%
94	15.231	2318	2320	2322	rBV3	614	804	0.10%	0.013%
95	15.438	2351	2354	2355	rBV	569	644	0.08%	0.010%
96	15.481	2358	2361	2365	rBV2	533	984	0.12%	0.016%
97	15.877	2424	2426	2429	rBV	772	636	0.08%	0.010%
98	16.182	2472	2476	2477	rBV2	610	638	0.08%	0.010%
99	16.420	2513	2515	2518	rBV	1062	787	0.09%	0.012%
100	16.737	2565	2567	2570	rBV2	583	860	0.10%	0.014%




Sum of corrected areas: 6328949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026116.D
Acq On : 28 Dec 2021 22:42
Operator : JC/MD
Sample : M5216-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

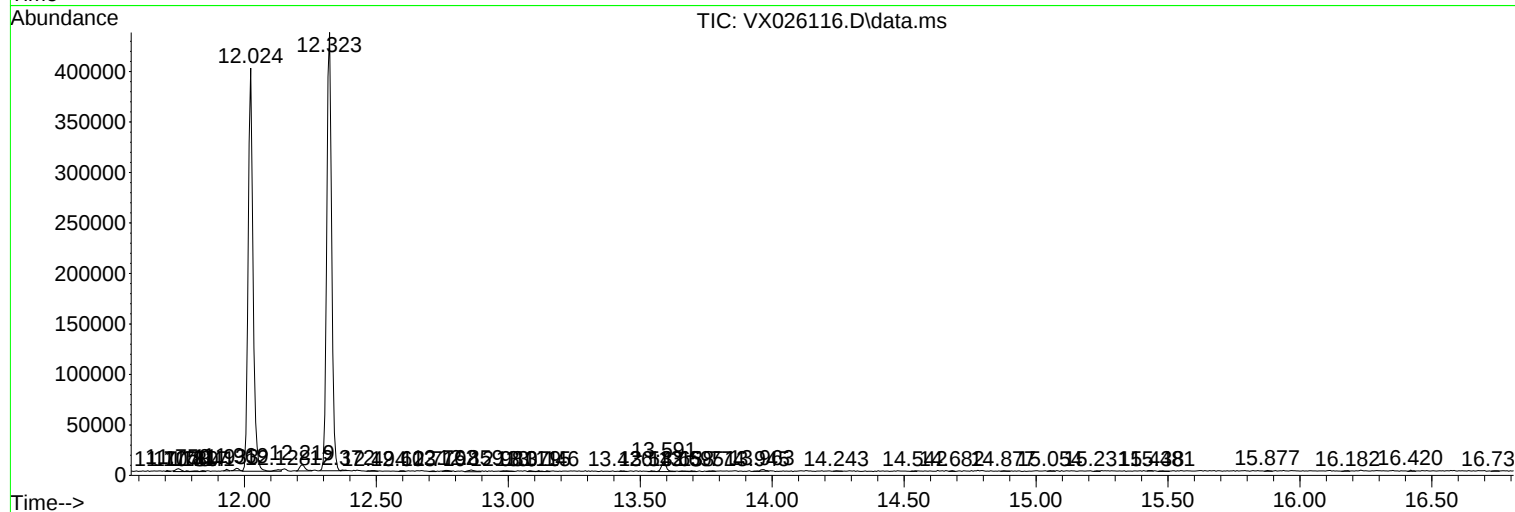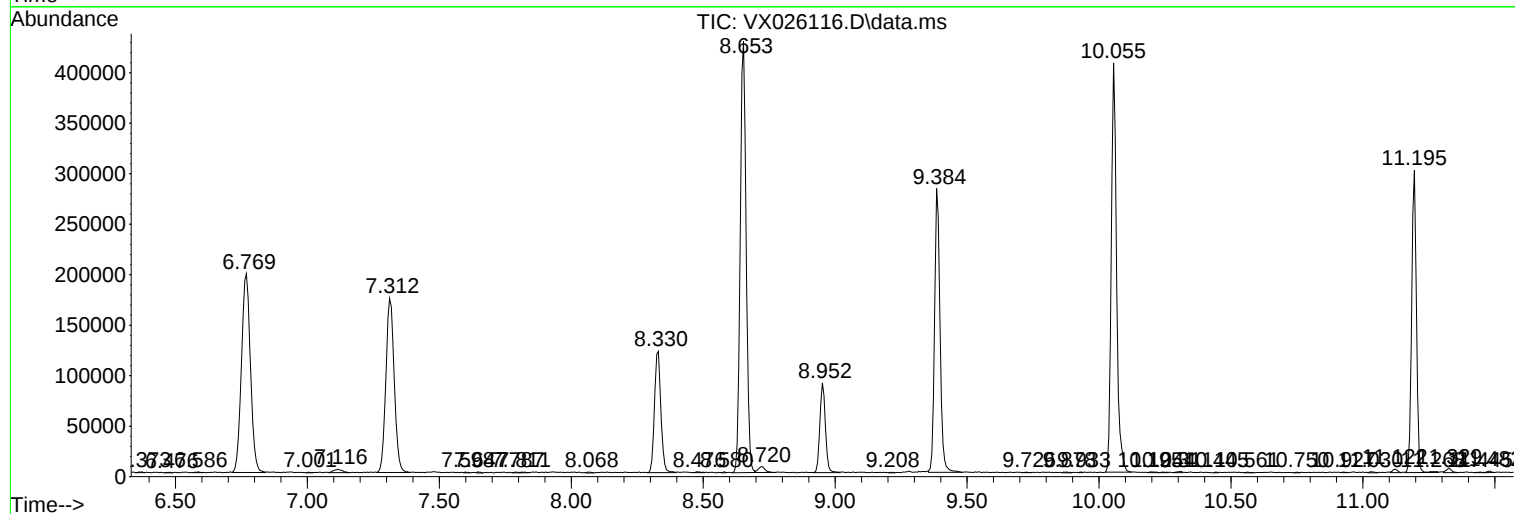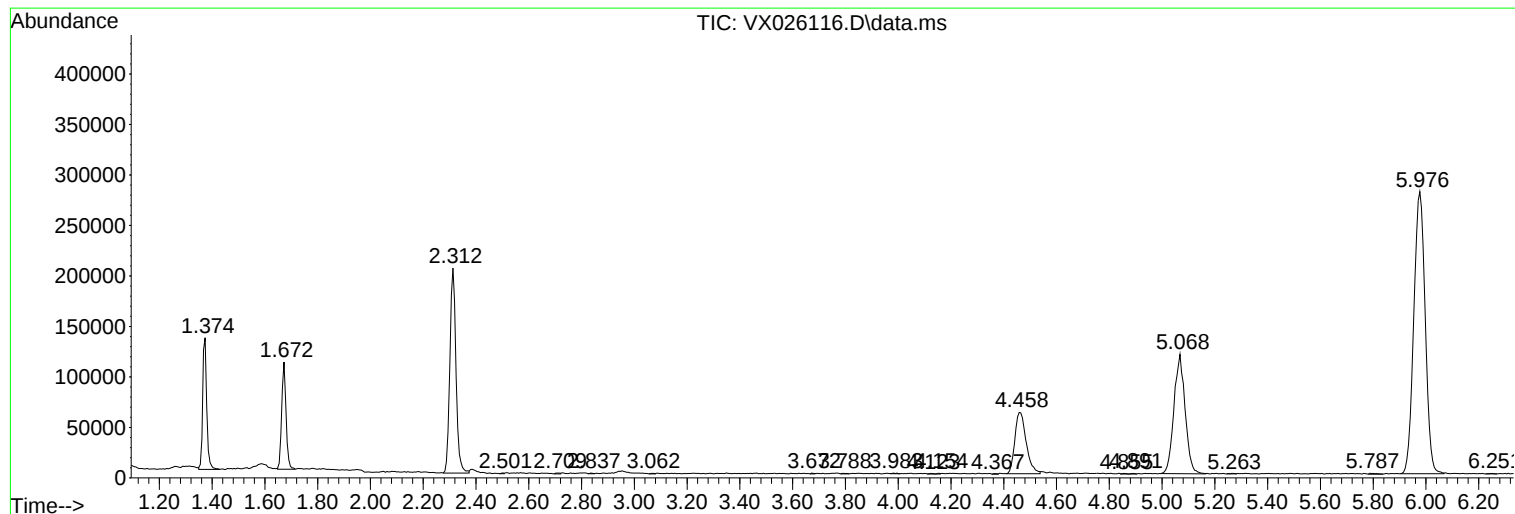

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026116.D
Acq On : 28 Dec 2021 22:42
Operator : JC/MD
Sample : M5216-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026116.D
Acq On : 28 Dec 2021 22:42
Operator : JC/MD
Sample : M5216-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc