
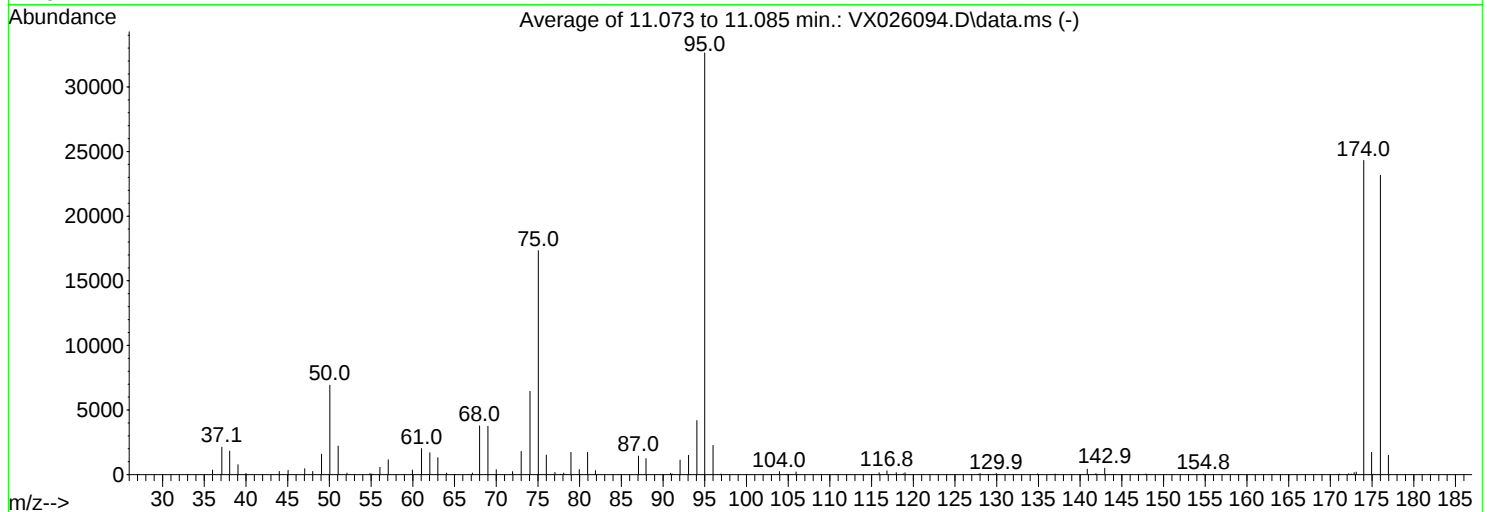


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122821\
Data File : VX026094.D
Acq On : 28 Dec 2021 12:28
Operator : JC/MD
Sample : BFB632
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB632

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Title : VOC Analysis
Last Update : Thu Dec 30 02:39:24 2021

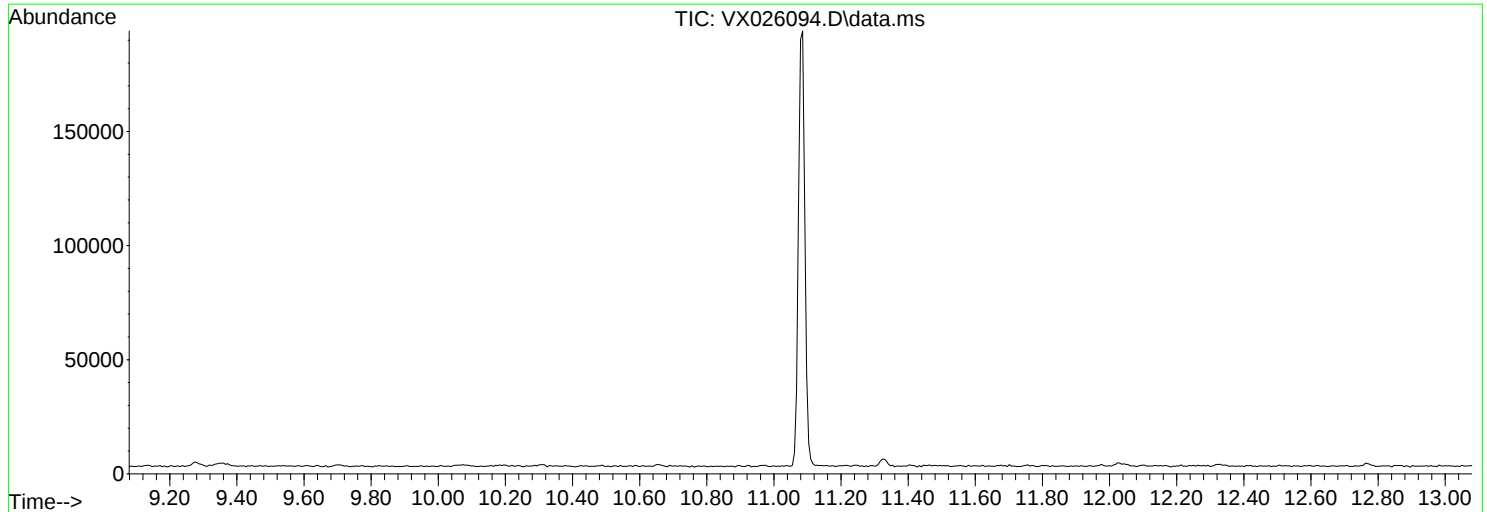

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	6923	PASS
75	95	30	80	53.1	17334	PASS
95	95	100	100	100.0	32637	PASS
96	95	5	9	6.9	2267	PASS
173	174	0.00	2	0.8	205	PASS
174	95	50	120	74.5	24312	PASS
175	174	5	9	7.1	1718	PASS
176	174	95	101	95.3	23167	PASS
177	176	5	9	6.5	1502	PASS

m/z	Abundance
40.00	3200.0
44.00	315.0

Instrument :
MSVOA_X
ClientSampleId :
BFB632

m/z	Abundance
36.00	286.0
37.10	1746.0
38.00	1554.0
39.00	683.0
40.00	3192.0
44.00	527.0
45.00	202.0
47.10	373.0
48.00	273.0
49.00	1177.0
50.00	5151.0
51.00	1757.0
52.10	113.0
54.80	73.0
55.20	83.0
56.10	317.0
57.10	937.0
60.00	276.0
61.00	1479.0
62.00	1345.0
63.00	801.0
64.20	114.0
67.20	91.0
68.00	2765.0
69.00	2567.0
70.00	333.0
71.90	211.0
73.00	1472.0
74.10	4765.0
75.00	12954.0
76.00	1254.0
77.10	149.0
78.10	210.0
79.00	1171.0
79.90	353.0
81.00	1265.0
81.90	252.0
87.10	1111.0
88.00	1057.0
90.90	106.0
92.10	781.0
93.10	1063.0
94.10	2883.0
95.00	23600.0
96.00	1706.0
96.90	67.0
103.90	172.0
105.90	212.0
115.90	100.0
116.80	233.0
118.00	100.0
118.80	174.0
140.90	324.0
143.00	304.0
171.10	51.0
172.30	92.0
172.90	163.0
174.00	14561.0
174.90	1081.0
176.00	12854.0
176.90	972.0

Instrument :
MSVOA_X
ClientSampleId :
BFB632

m/z	Abundance
36.00	399.0
37.10	2532.0
38.10	2192.0
39.00	823.0
40.00	3201.0
44.10	548.0
45.10	400.0
47.10	649.0
48.00	223.0
49.10	1880.0
50.00	8070.0
51.10	2606.0
52.10	147.0
54.90	137.0
56.00	696.0
57.00	1258.0
60.00	430.0
61.10	2344.0
62.10	1958.0
63.00	1652.0
64.00	134.0
67.10	154.0
68.00	4436.0
69.00	4557.0
70.10	450.0
72.00	263.0
73.00	1934.0
74.00	7751.0
75.10	20072.0
76.00	1774.0
77.10	230.0
78.10	143.0
78.90	2048.0
79.90	398.0
81.00	1981.0
82.00	337.0
87.00	1557.0
88.00	1394.0
91.10	155.0
92.10	1314.0
93.00	1590.0
94.10	4858.0
95.00	37416.0
96.00	2665.0
103.90	247.0
104.80	70.0
105.90	189.0
110.80	58.0
115.90	191.0
116.90	308.0
117.80	158.0
119.00	242.0
127.80	106.0
130.00	123.0
134.90	107.0
137.00	94.0
140.90	482.0
142.00	152.0
143.00	592.0
147.90	68.0
171.10	52.0
172.50	149.0
173.10	280.0
174.00	27344.0
175.00	1905.0
176.00	25904.0
177.00	1692.0

Instrument :
MSVOA_X
ClientSampleId :
BFB632

m/z	Abundance
36.00	400.0
37.10	2095.0
38.10	1722.0
39.10	788.0
40.00	3506.0
44.00	635.0
45.10	392.0
47.00	356.0
48.00	259.0
49.00	1705.0
50.10	7548.0
51.00	2303.0
52.10	116.0
55.00	184.0
56.00	716.0
57.00	1255.0
59.90	356.0
61.00	2249.0
62.00	1782.0
63.00	1483.0
63.90	134.0
65.10	57.0
67.20	134.0
68.00	4127.0
69.00	4093.0
69.90	391.0
72.00	249.0
73.00	1968.0
74.00	6823.0
75.00	18976.0
76.00	1497.0
76.90	145.0
77.70	126.0
79.00	1960.0
80.00	455.0
80.90	1949.0
81.80	360.0
87.00	1660.0
87.90	1265.0
90.90	225.0
92.00	1296.0
93.00	1854.0
94.00	4819.0
95.00	36896.0
96.00	2430.0
97.00	99.0
104.00	274.0
104.90	55.0
106.00	232.0
115.90	167.0
116.90	335.0
118.00	238.0
119.00	213.0
128.00	254.0
129.90	175.0
134.90	100.0
137.00	74.0
140.80	445.0
141.80	116.0
142.90	602.0
147.90	129.0
154.80	134.0
171.10	66.0
172.10	121.0
172.80	335.0
173.10	335.0
174.00	31032.0
175.00	2167.0
176.00	30744.0
177.00	1842.0

Instrument :
MSVOA_X
ClientSampleId :
BFB632