

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
 Data File : VX039516.D
 Acq On : 28 Dec 2023 15:09
 Operator : JC/MD
 Sample : 06015-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MR-317-0-2

Quant Time: Dec 28 22:51:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	95653	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	200984	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	201272	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	86614	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	85400	48.736	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.480%		
35) Dibromofluoromethane	5.385	113	65944	47.493	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.980%		
50) Toluene-d8	8.647	98	253580	49.193	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	98.380%		
62) 4-Bromofluorobenzene	11.079	95	103478	48.653	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.300%		
Target Compounds						Qvalue
5) Bromomethane	1.611	94	203	0.255	ug/l #	3
6) Chloroethane	1.697	64	536	0.642	ug/l #	43
11) Tert butyl alcohol	2.946	59	3140	7.136	ug/l #	78
16) Acetone	2.386	43	49150	27.419	ug/l	94
18) Methyl Acetate	2.709	43	2301	0.607	ug/l	99
20) Methylene Chloride	2.788	84	6166	4.221	ug/l	99
25) 2-Butanone	4.574	43	5634	3.726	ug/l	97
29) Tetrahydrofuran	5.031	42	601	0.720	ug/l #	78
31) Cyclohexane	5.544	56	2772	1.225	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	9306	4.247	ug/l #	50
37) Ethyl Acetate	4.733	43	5057	1.868	ug/l #	84
38) Carbon Tetrachloride	5.550	117	10881	5.204	ug/l #	16
41) Methacrylonitrile	5.025	41	533	0.369	ug/l #	40
43) Isopropyl Acetate	6.342	43	85532	19.430	ug/l	99
48) Methyl methacrylate	7.641	41	2885	1.121	ug/l #	38
51) 4-Methyl-2-Pentanone	8.549	43	71044	25.330	ug/l #	47
54) cis-1,3-Dichloropropene	8.549	75	28609	10.802	ug/l #	60
57) 1,3-Dichloropropane	9.482	76	2117	0.784	ug/l #	42
59) 2-Hexanone	9.378	43	94411	39.004	ug/l #	26
67) Ethyl Benzene	10.195	91	1753	0.214	ug/l	96
68) m/p-Xylenes	10.311	106	1778	0.606	ug/l	88
69) o-Xylene	10.646	106	812	0.286	ug/l	90
76) 1,2,3-Trichloropropane	11.079	75	56923	25.402	ug/l #	38
78) n-propylbenzene	11.305	91	1963	0.238	ug/l	100
79) 2-Chlorotoluene	11.384	91	1525	0.306	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	3051	0.536	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	56923	71.660	ug/l #	5
83) tert-Butylbenzene	11.756	119	1124	0.207	ug/l #	42
84) 1,2,4-Trimethylbenzene	11.756	105	10691	1.831	ug/l	98
95) Naphthalene	13.780	128	1539	0.243	ug/l #	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039516.D
Acq On : 28 Dec 2023 15:09
Operator : JC/MD
Sample : 06015-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2

Quant Time: Dec 28 22:51:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




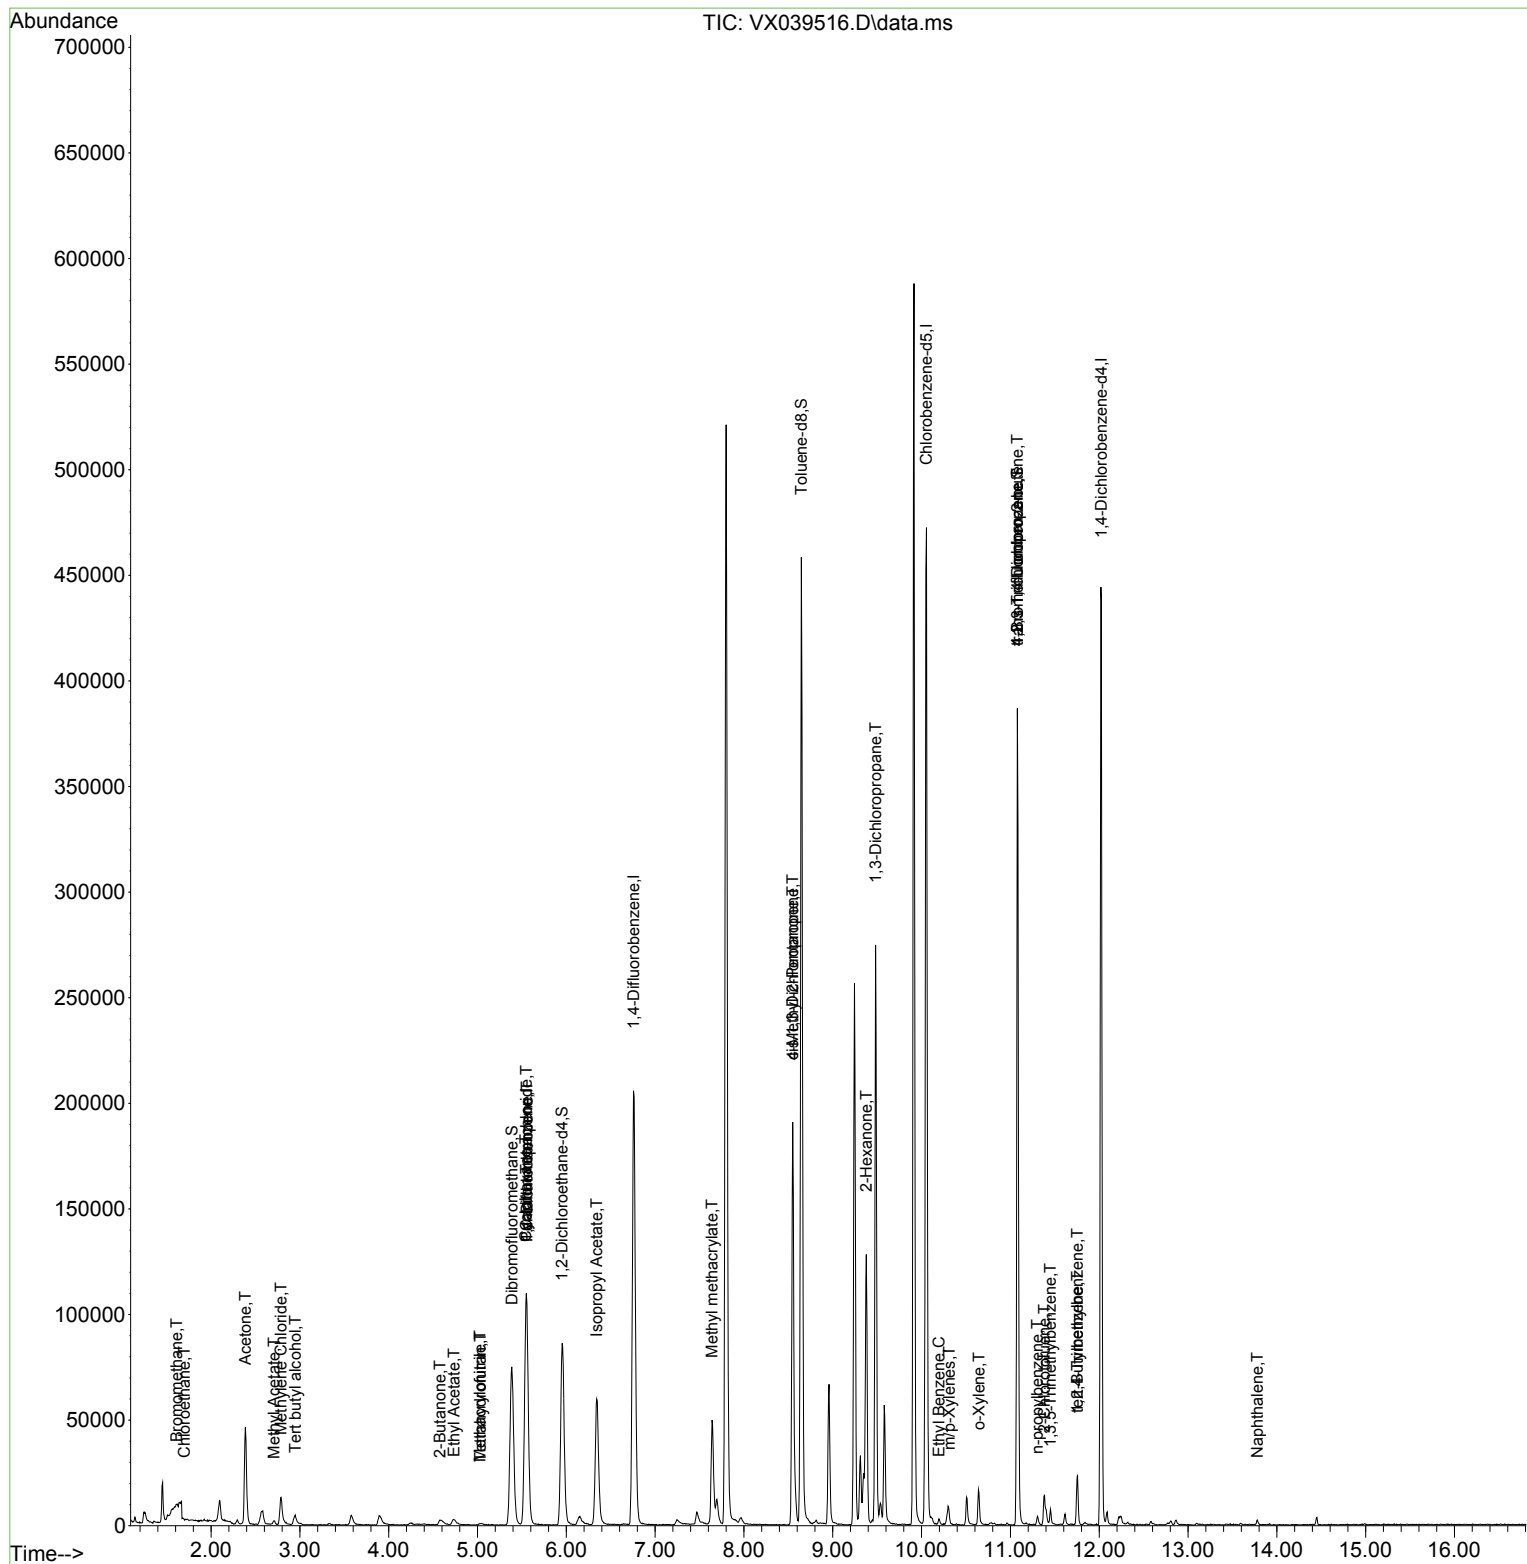




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion:168 Resp: 95653
Ion Ratio Lower Upper
168 100
99 64.5 56.6 85.0

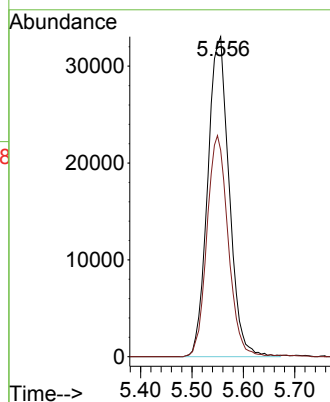

#5
Bromomethane
Concen: 0.255 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 94 Resp: 203
Ion Ratio Lower Upper
94 100
96 0.0 74.6 111.8#







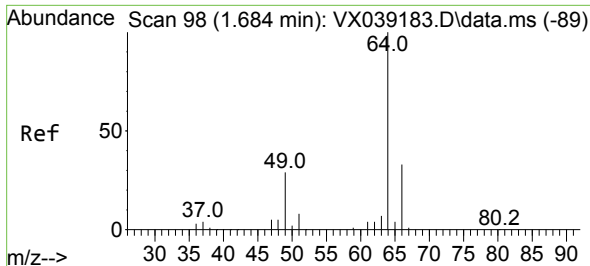

#6
Chloroethane
Concen: 0.642 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.012 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 64 Resp: 536
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

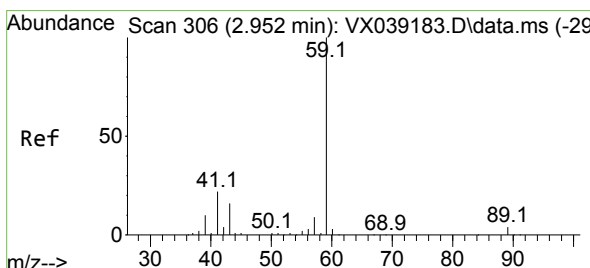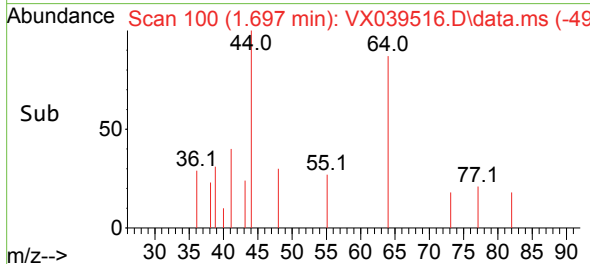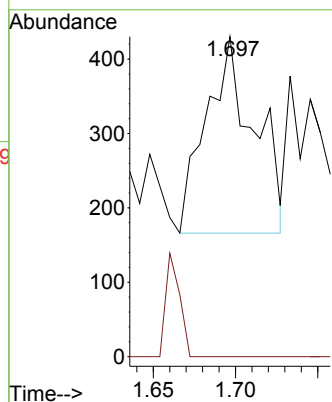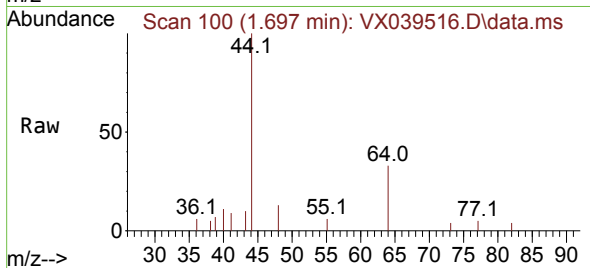

#11
Tert butyl alcohol
Concen: 7.136 ug/l
RT: 2.946 min Scan# 305
Delta R.T. -0.006 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 59 Resp: 3140
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#


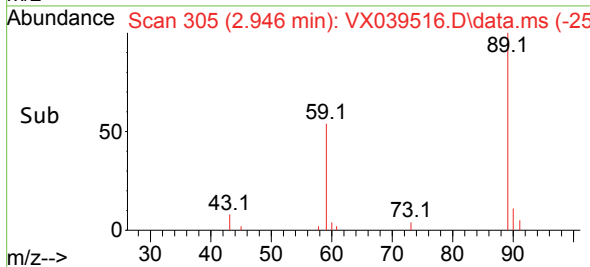
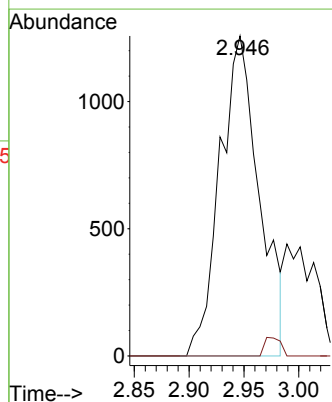
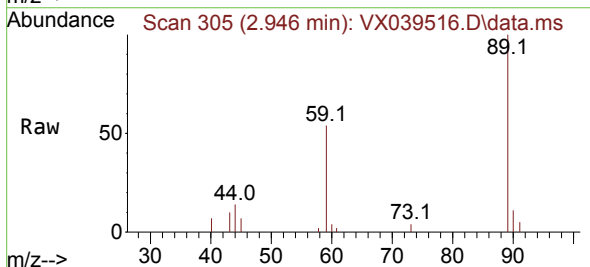


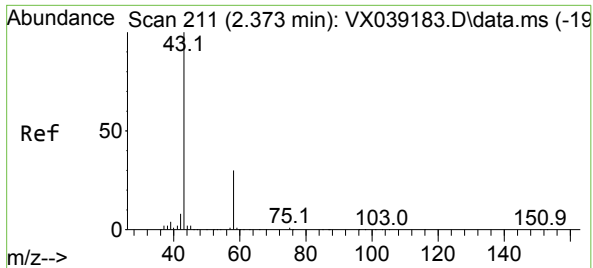

#16
Acetone
Concen: 27.419 ug/l
RT: 2.386 min Scan# 211
Delta R.T. 0.013 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 43 Resp: 49150
Ion Ratio Lower Upper
43 100
58 30.5 21.9 32.9

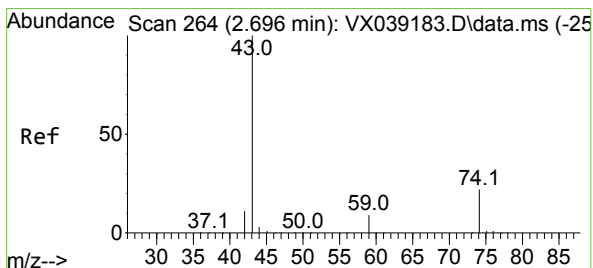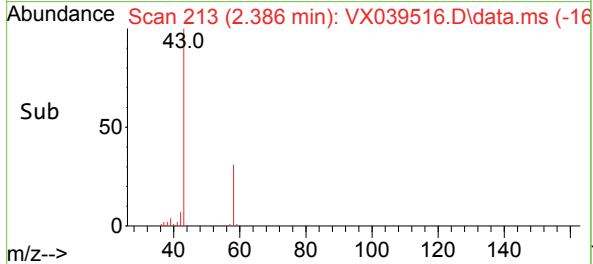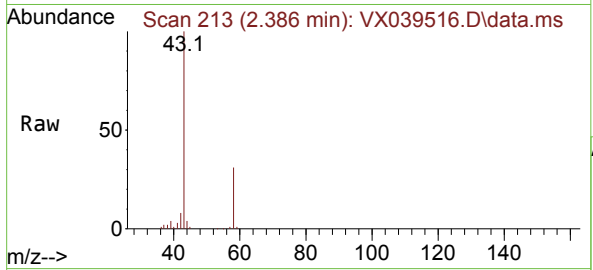

#18
Methyl Acetate
Concen: 0.607 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.012 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 43 Resp: 2301
Ion Ratio Lower Upper
43 100
74 21.9 17.8 26.8


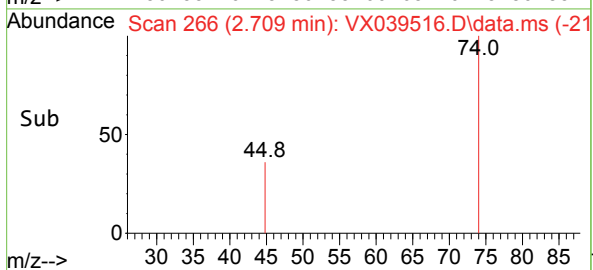

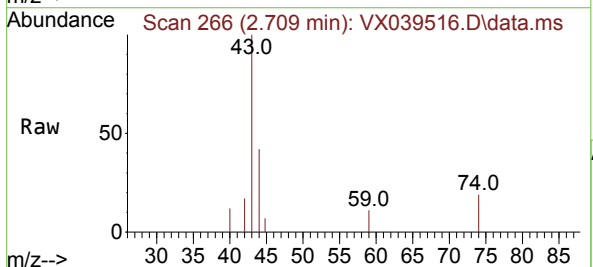




#20
Methylene Chloride
Concen: 4.221 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion:	84	Resp:	6166
Ion	Ratio	Lower	Upper
84	100		
49	131.6	103.6	155.4
51	41.2	33.8	50.6
86	62.1	49.4	74.0



#25
2-Butanone
Concen: 3.726 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.025 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion:	43	Resp:	5634
Ion	Ratio	Lower	Upper
43	100		
72	25.7	19.4	29.2

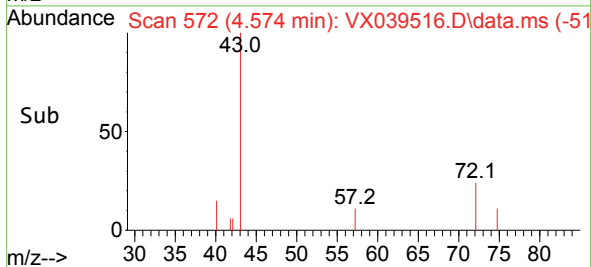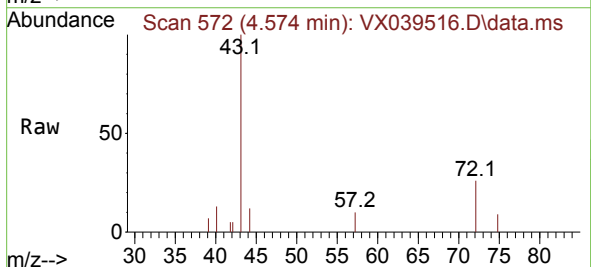



#29

Tetrahydrofuran

Concen: 0.720 ug/l

RT: 5.031 min Scan# 641

Delta R.T. 0.037 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :

MR-317-0-2





Tgt Ion: 42 Resp: 601

Ion Ratio Lower Upper

42 100

72 35.9 34.2 51.4

71 19.6 32.2 48.2#

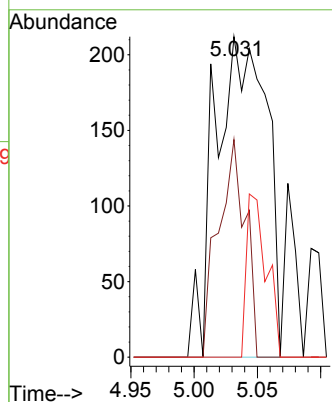

#31

Cyclohexane

Concen: 1.225 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.067 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09




Tgt Ion: 56 Resp: 2772


Ion Ratio Lower Upper

56 100

69 139.1 23.4 35.2#

84 145.4 65.9 98.9#

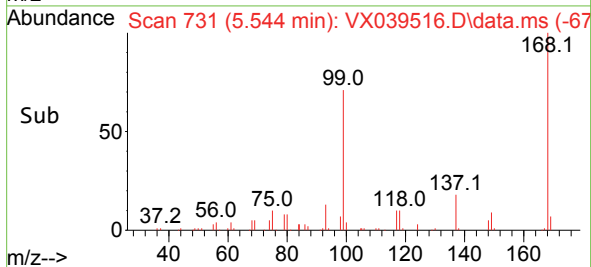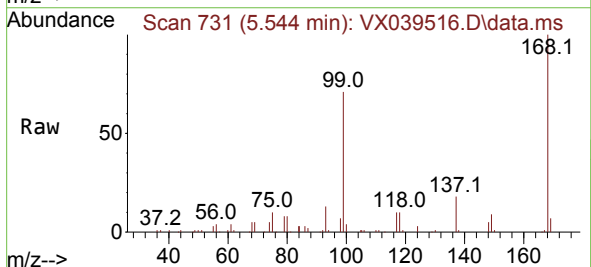



#33

1,2-Dichloroethane-d4

Concen: 48.736 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion: 65 Resp: 85400

Ion Ratio Lower Upper

65 100

67 52.3 0.0 100.2

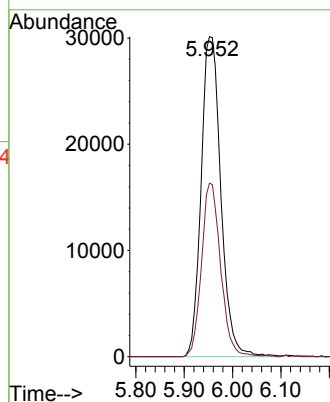

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.006 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09




Tgt Ion: 114 Resp: 200984


Ion Ratio Lower Upper

114 100

63 23.5 0.0 45.0

88 17.5 0.0 36.6



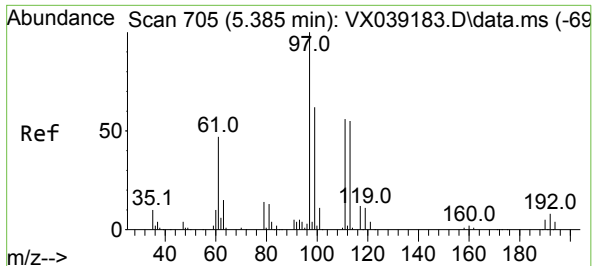

#35

Dibromofluoromethane

Concen: 47.493 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :

MR-317-0-2





Tgt Ion:113 Resp: 65944

Ion Ratio Lower Upper

113 100

111 103.6 82.9 124.3

192 15.6 13.3 19.9

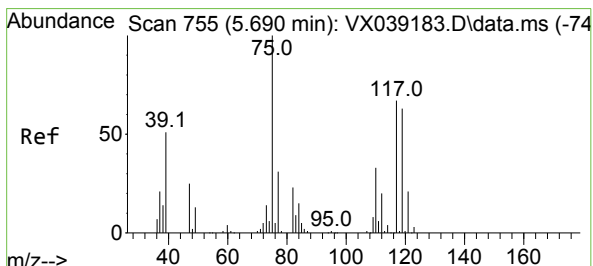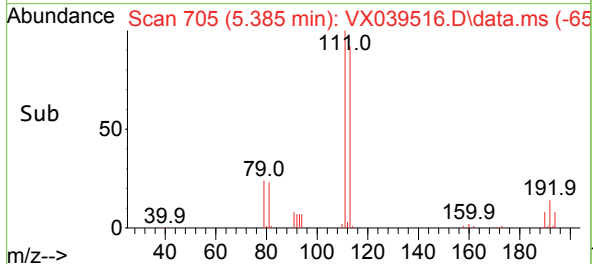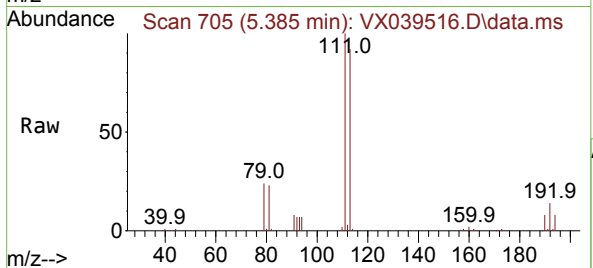

#36

1,1-Dichloropropene

Concen: 4.247 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.134 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09




Tgt Ion: 75 Resp: 9306


Ion Ratio Lower Upper

75 100

110 8.6 17.0 50.9#

77 0.0 24.7 37.1#

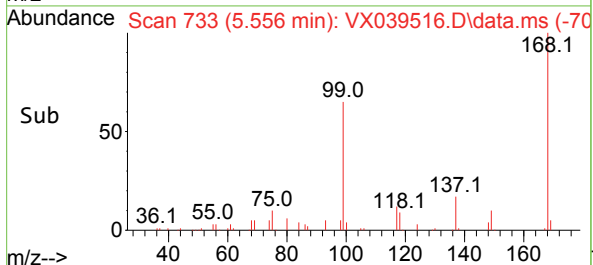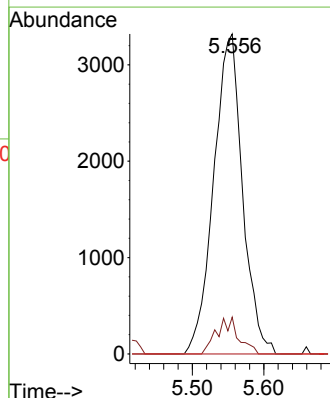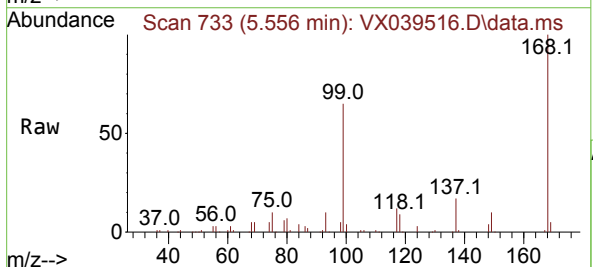



#37

Ethyl Acetate

Concen: 1.868 ug/l

RT: 4.733 min Scan# 51

Delta R.T. 0.025 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :

MR-317-0-2





Tgt Ion: 43 Resp: 5057

Ion Ratio Lower Upper

43 100

61 16.0 10.6 16.0

70 0.0 8.3 12.5#

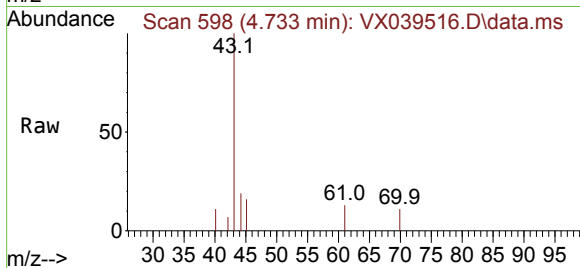

#38

Carbon Tetrachloride

Concen: 5.204 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.128 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09




Tgt Ion: 117 Resp: 10881


Ion Ratio Lower Upper

117 100

119 5.7 78.2 117.2#

121 0.0 24.4 36.6#


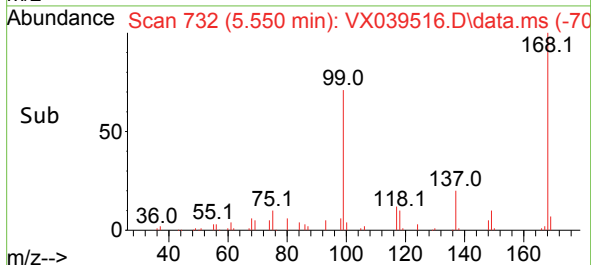
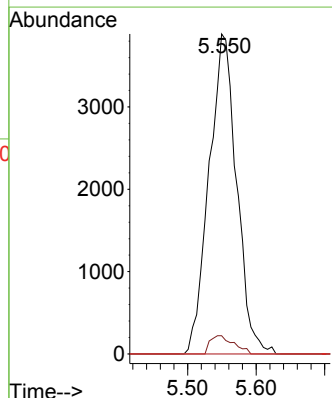
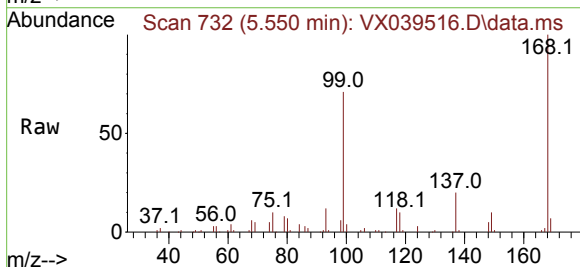




#41
Methacrylonitrile
Concen: 0.369 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.110 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 41	Resp: 533
Ion Ratio	Lower Upper
41 100	
39 30.6	45.2 67.8#
67 0.0	52.6 78.8#
52 0.0	22.7 34.1#



#43
Isopropyl Acetate
Concen: 19.430 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.006 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 43	Resp: 85532
Ion Ratio	Lower Upper
43 100	
61 18.3	15.2 22.8
87 12.2	9.8 14.6









#48
Methyl methacrylate
Concen: 1.121 ug/l
RT: 7.641 min Scan# 1083
Delta R.T. -0.049 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 41 Resp: 2885
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 82.4 47.7 71.5#

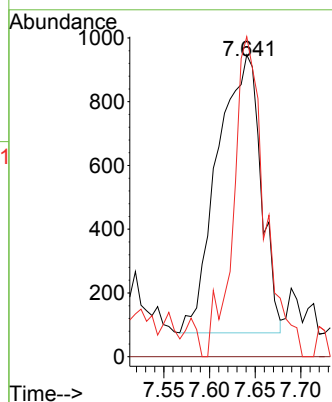

#50
Toluene-d8
Concen: 49.193 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 98 Resp: 253580
Ion Ratio Lower Upper
98 100
100 63.6 53.1 79.7


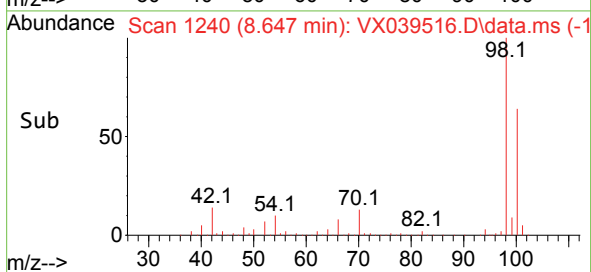
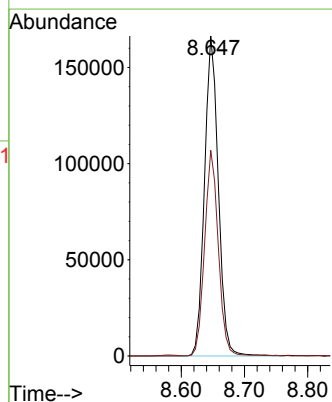
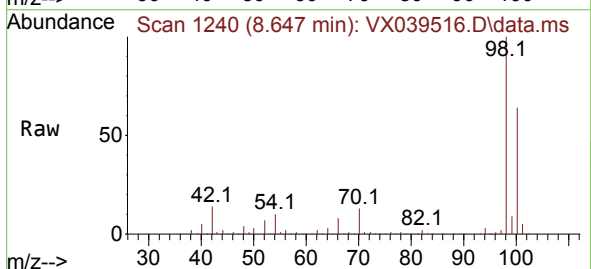




#51
4-Methyl-2-Pentanone
Concen: 25.330 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 43 Resp: 71044
Ion Ratio Lower Upper
43 100
58 6.1 30.4 45.6#

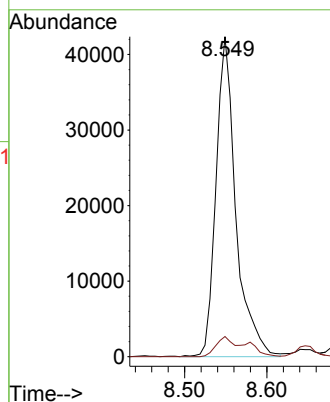

#54
cis-1,3-Dichloropropene
Concen: 10.802 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.183 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 75 Resp: 28609
Ion Ratio Lower Upper
75 100
77 0.7 25.3 37.9#
39 34.5 46.7 70.1#

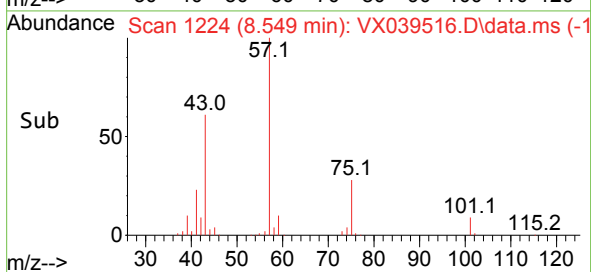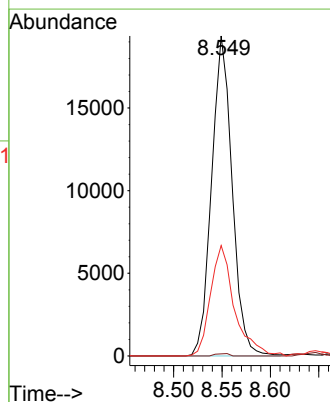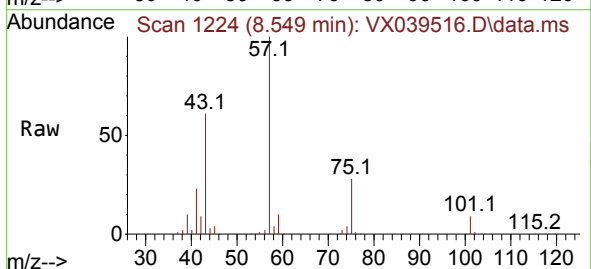



#57

1,3-Dichloropropane

Concen: 0.784 ug/l

RT: 9.482 min Scan# 1

Delta R.T. 0.177 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion: 76 Resp: 2117

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

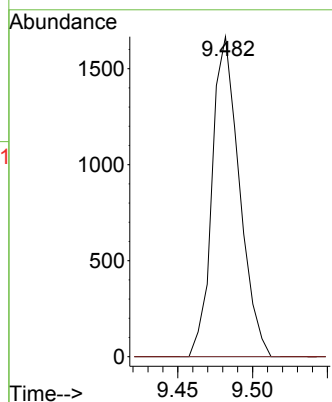

#59

2-Hexanone

Concen: 39.004 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.049 min

Lab File: VX039516.D




Acq: 28 Dec 2023 15:09


Tgt Ion: 43 Resp: 94411

Ion Ratio Lower Upper

43 100

58 0.0 26.2 78.5#









#62
4-Bromofluorobenzene
Concen: 48.653 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 95 Resp: 103478
Ion Ratio Lower Upper
95 100
174 64.3 0.0 135.6
176 61.6 0.0 131.0

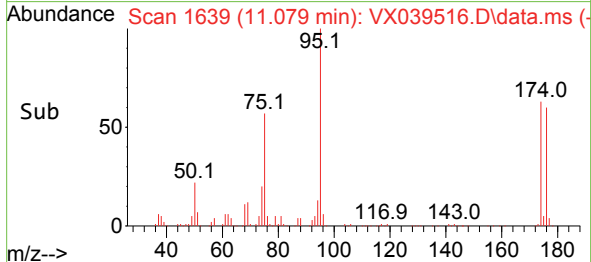

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 117 Resp: 201272
Ion Ratio Lower Upper
117 100
82 59.2 46.2 69.4
119 31.9 25.5 38.3

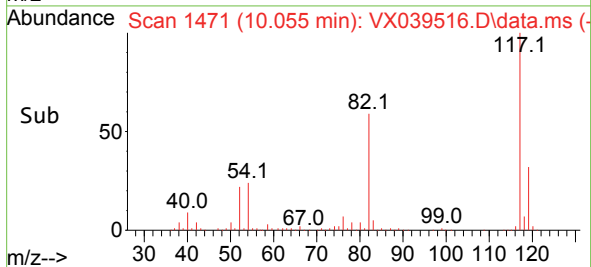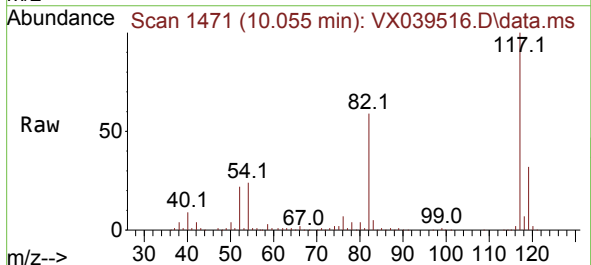



#67

Ethyl Benzene

Concen: 0.214 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion: 91 Resp: 1753

Ion Ratio Lower Upper

91 100

106 28.6 24.9 37.3

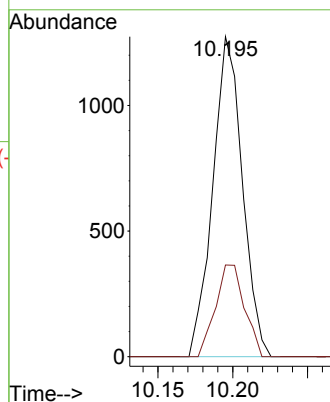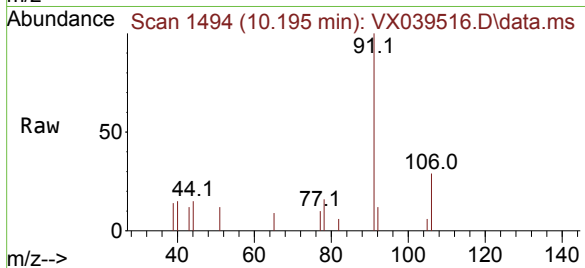

#68

m/p-Xylenes

Concen: 0.606 ug/l

RT: 10.311 min Scan# 1513

Delta R.T. 0.012 min

Lab File: VX039516.D




Acq: 28 Dec 2023 15:09


Tgt Ion: 106 Resp: 1778

Ion Ratio Lower Upper

106 100

91 225.9 165.5 248.3

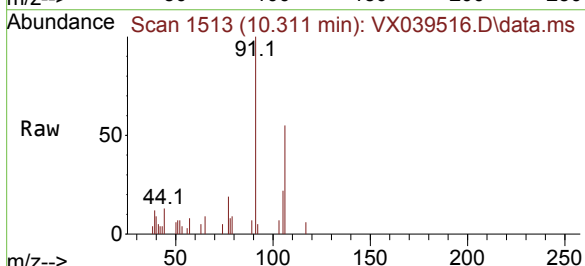



#69

o-Xylene

Concen: 0.286 ug/l

RT: 10.646 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion:106 Resp: 812

Ion Ratio Lower Upper

106 100

91 233.4 108.9 326.8



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09




Tgt Ion:152 Resp: 86614


Ion Ratio Lower Upper

152 100

115 66.5 43.3 129.9

150 156.2 0.0 345.0

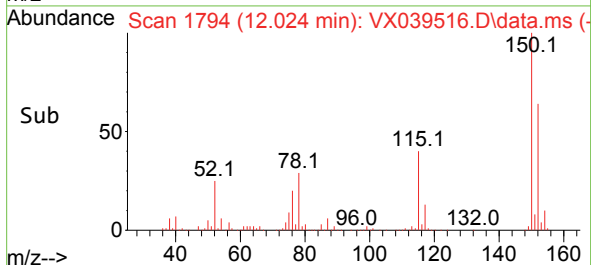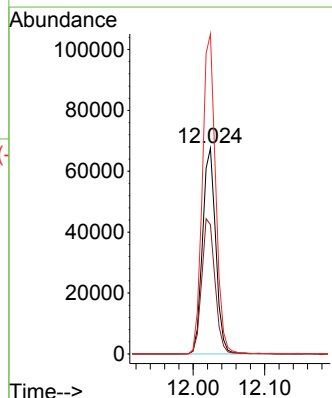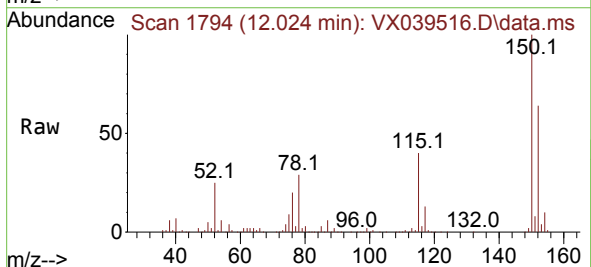



#76

1,2,3-Trichloropropane

Concen: 25.402 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion: 75 Resp: 56923

Ion Ratio Lower Upper

75 100

77 1.1 19.1 57.5#

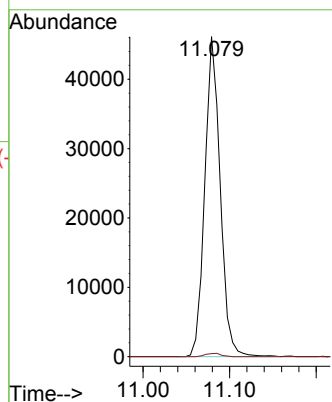

#78

n-propylbenzene

Concen: 0.238 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX039516.D




Acq: 28 Dec 2023 15:09


Tgt Ion: 91 Resp: 1963

Ion Ratio Lower Upper

91 100

120 23.0 11.5 34.4





#79

2-Chlorotoluene

Concen: 0.306 ug/l

RT: 11.384 min Scan# 1

Delta R.T. 0.025 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion: 91 Resp: 1525

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#

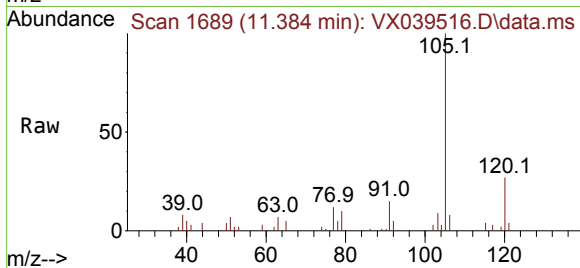

#80

1,3,5-Trimethylbenzene

Concen: 0.536 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX039516.D




Acq: 28 Dec 2023 15:09


Tgt Ion: 105 Resp: 3051

Ion Ratio Lower Upper

105 100

120 48.6 24.1 72.3


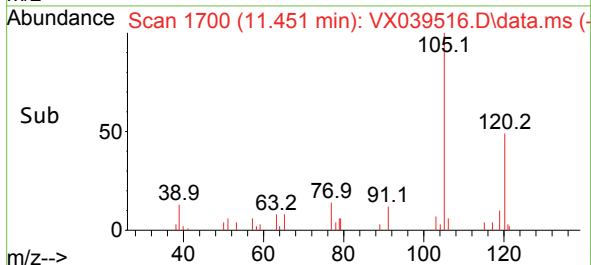

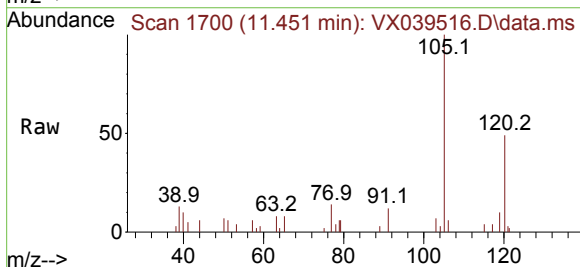




#81
trans-1,4-Dichloro-2-butene
Concen: 71.660 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09




Instrument :
MSVOA_X
ClientSampleId :
MR-317-0-2


Tgt Ion: 75 Resp: 56923
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

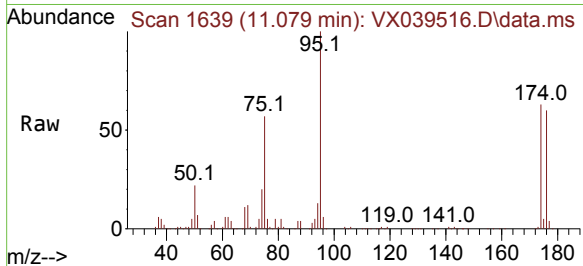

#83
tert-Butylbenzene
Concen: 0.207 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.043 min
Lab File: VX039516.D
Acq: 28 Dec 2023 15:09

Tgt Ion: 119 Resp: 1124
Ion Ratio Lower Upper
119 100
91 109.6 31.2 93.6#
134 0.0 11.7 35.0#

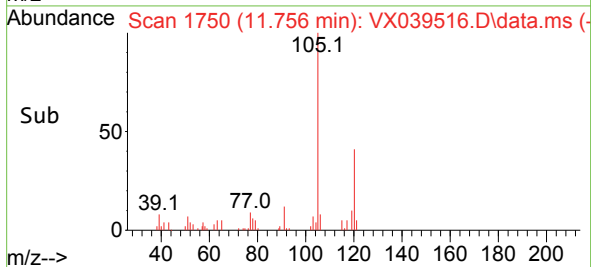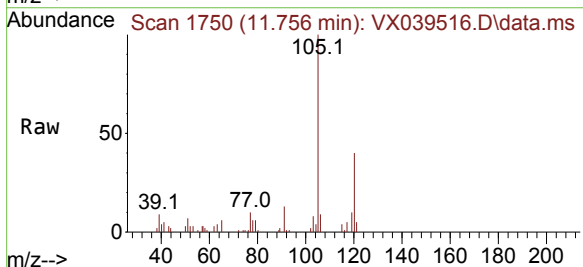



#84

1,2,4-Trimethylbenzene

Concen: 1.831 ug/l

RT: 11.756 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Instrument :

MSVOA_X

ClientSampleId :





MR-317-0-2

Tgt Ion:105 Resp: 10691

Ion Ratio Lower Upper

105 100

120 43.5 21.2 63.6

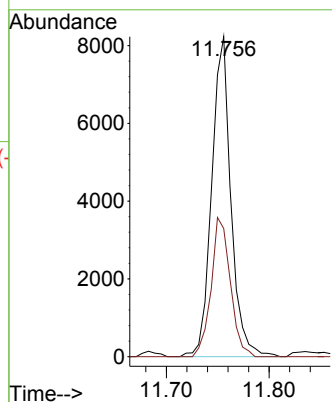

#95

Naphthalene

Concen: 0.243 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.006 min

Lab File: VX039516.D

Acq: 28 Dec 2023 15:09

Tgt Ion:128 Resp: 1539

Ion Ratio Lower Upper

128 100

127 8.7 10.3 15.5#

129 10.3 8.8 13.2

