

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
 Data File : VX039524.D
 Acq On : 28 Dec 2023 18:12
 Operator : JC/MD
 Sample : 06025-01 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50200

Quant Time: Dec 28 22:55:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	83692	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	177240	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	165197	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	67130	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	73868	48.180	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.360%
35) Dibromofluoromethane	5.385	113	56796	46.385	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.760%
50) Toluene-d8	8.647	98	218767	48.125	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.240%
62) 4-Bromofluorobenzene	11.079	95	83950	44.759	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.520%


Target Compounds					Qvalue
16) Acetone	2.386	43	25390	5.701	ug/l 91
18) Methyl Acetate	2.709	43	1621	0.489	ug/l # 89
19) Methyl tert-butyl Ether	3.117	73	12897	3.313	ug/l # 84
20) Methylene Chloride	2.788	84	877	0.686	ug/l # 71
22) Diisopropyl ether	3.770	45	1063	0.268	ug/l # 67
25) 2-Butanone	4.581	43	5602	4.234	ug/l 96
31) Cyclohexane	5.471	56	1598	0.807	ug/l 91
37) Ethyl Acetate	4.721	43	28672	12.011	ug/l 97
40) Benzene	6.031	78	166635	30.487	ug/l 97
52) Toluene	8.714	92	162312	49.201	ug/l 95
67) Ethyl Benzene	10.195	91	21256	3.167	ug/l 99
68) m/p-Xylenes	10.299	106	25114	10.436	ug/l 98
69) o-Xylene	10.640	106	11738	5.045	ug/l 91
78) n-propylbenzene	11.311	91	1511	0.237	ug/l 86
80) 1,3,5-Trimethylbenzene	11.451	105	2575	0.584	ug/l 92
84) 1,2,4-Trimethylbenzene	11.756	105	10134	2.240	ug/l 98
95) Naphthalene	13.780	128	5284	1.076	ug/l 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039524.D
Acq On : 28 Dec 2023 18:12
Operator : JC/MD
Sample : 06025-01 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50200

Quant Time: Dec 28 22:55:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




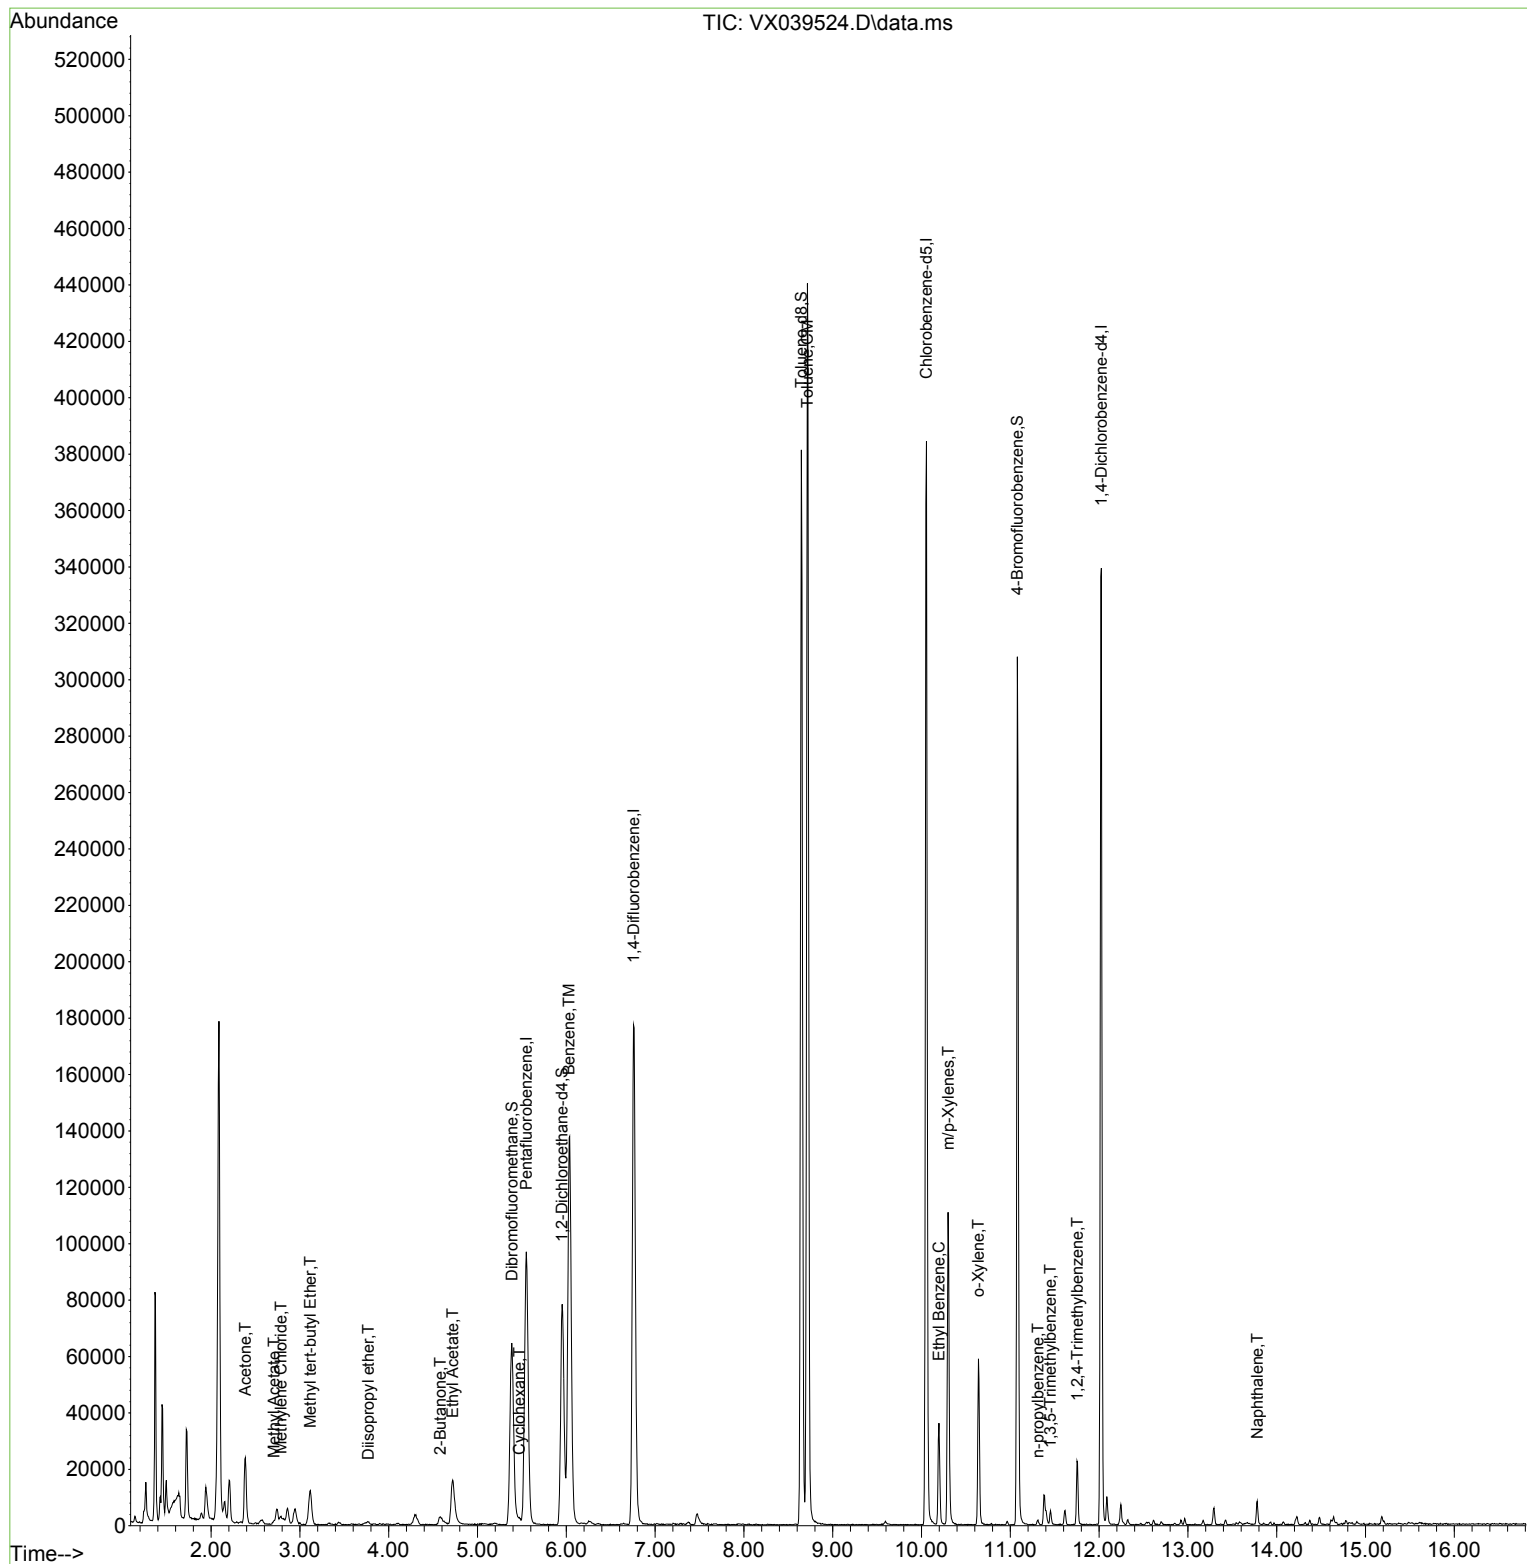


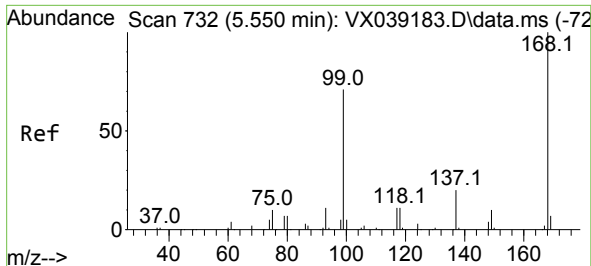

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion:168 Resp: 83692
Ion Ratio Lower Upper
168 100
99 70.6 56.6 85.0

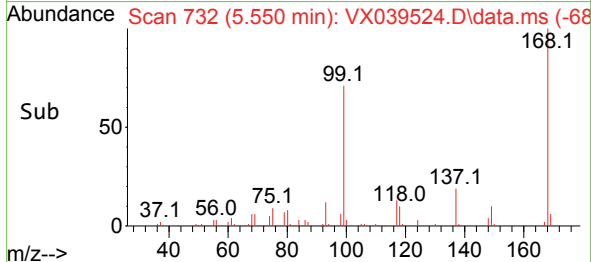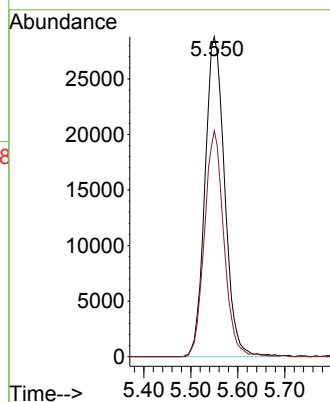

#16
Acetone
Concen: 5.701 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.013 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion: 43 Resp: 25390
Ion Ratio Lower Upper
43 100
58 32.1 21.9 32.9


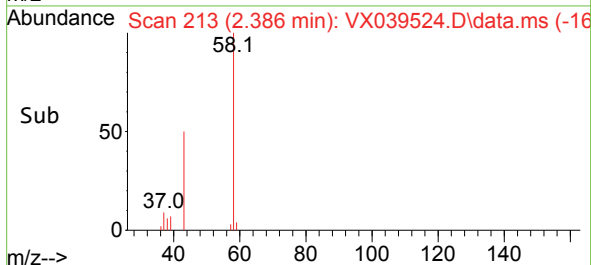
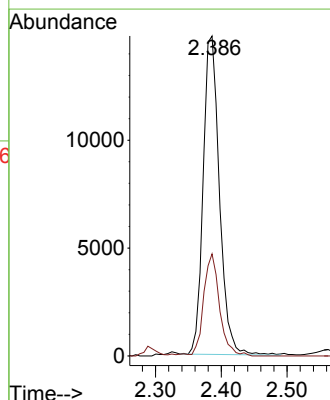
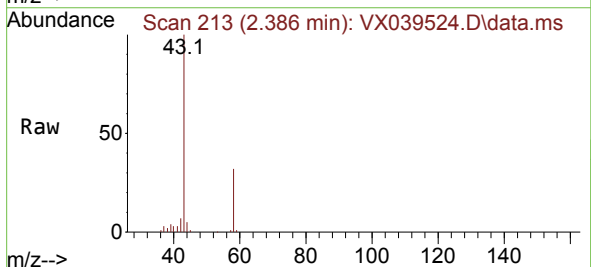


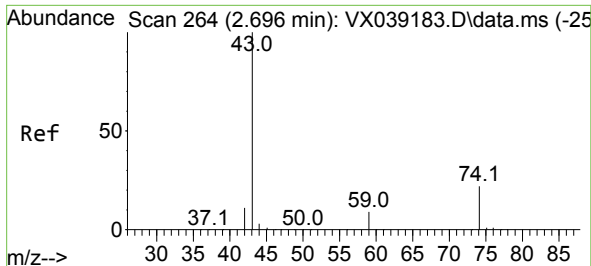

#18
Methyl Acetate
Concen: 0.489 ug/l
RT: 2.709 min Scan# 21
Delta R.T. 0.013 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion: 43 Resp: 1621
Ion Ratio Lower Upper
43 100
74 17.0 17.8 26.8#

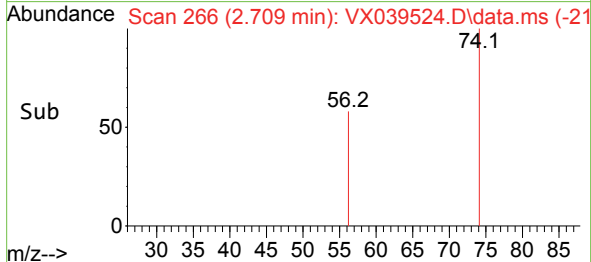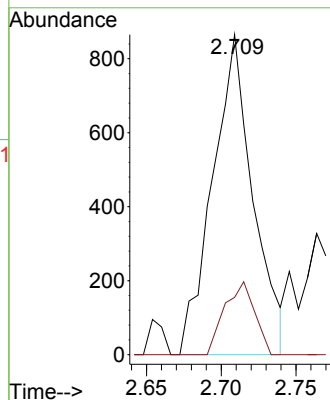

#19
Methyl tert-butyl Ether
Concen: 3.313 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.006 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12


Tgt Ion: 73 Resp: 12897
Ion Ratio Lower Upper
73 100
57 29.1 17.3 25.9#

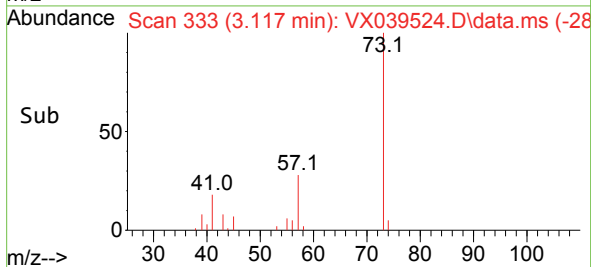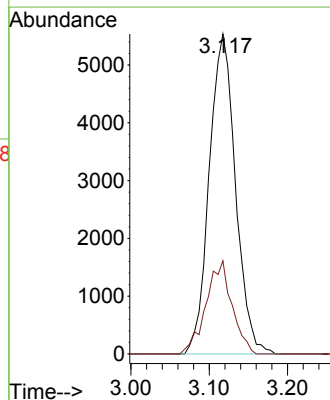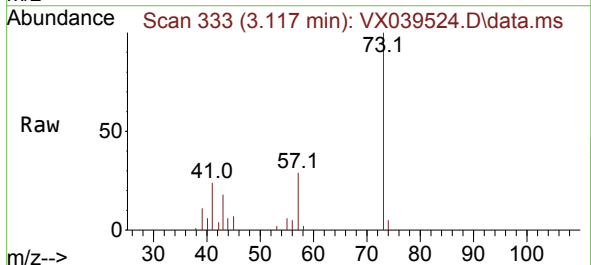



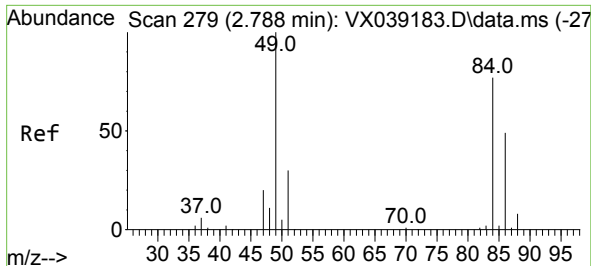


#20
Methylene Chloride
Concen: 0.686 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12


Instrument :
MSVOA_X
ClientSampleId :
50200





Tgt Ion: 84	Resp: 877
Ion Ratio	Lower Upper
84 100	
49 153.9	103.6 155.4
51 45.4	33.8 50.6
86 108.0	49.4 74.0#

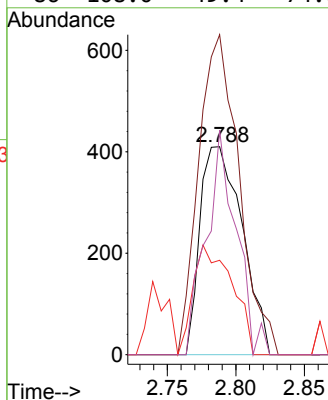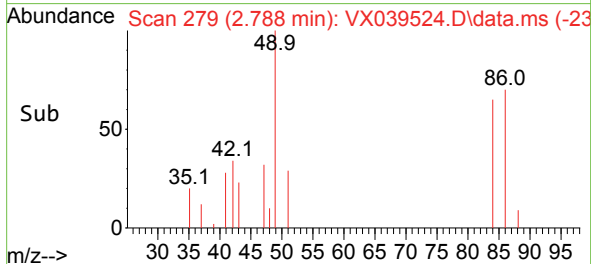


#22
Diisopropyl ether
Concen: 0.268 ug/l
RT: 3.770 min Scan# 440
Delta R.T. 0.013 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

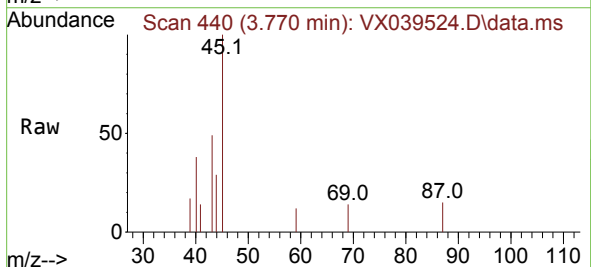

Tgt Ion: 45	Resp: 1063
Ion Ratio	Lower Upper
45 100	
43 49.5	69.7 104.5#
87 15.2	20.8 31.2#
59 12.3	9.0 13.4



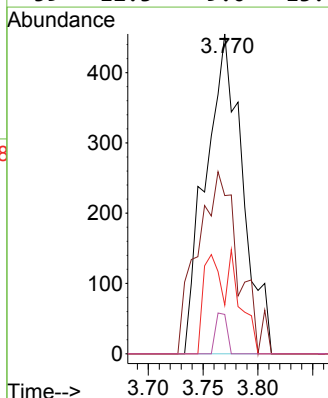





#25
2-Butanone
Concen: 4.234 ug/l
RT: 4.581 min Scan# 51
Delta R.T. 0.031 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion: 43 Resp: 5602
Ion Ratio Lower Upper
43 100
72 26.1 19.4 29.2

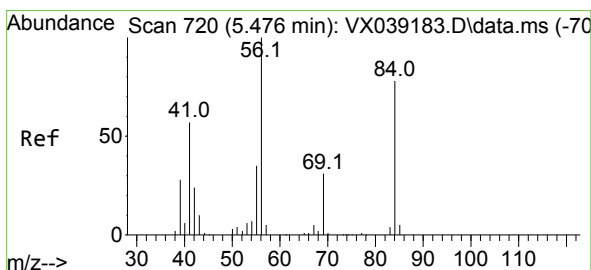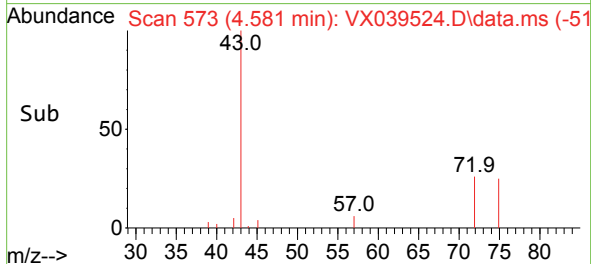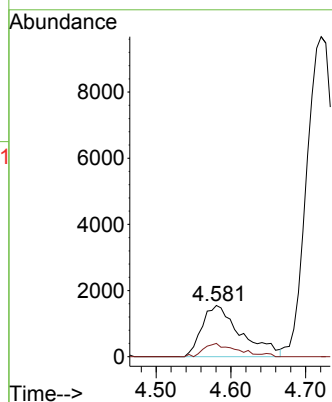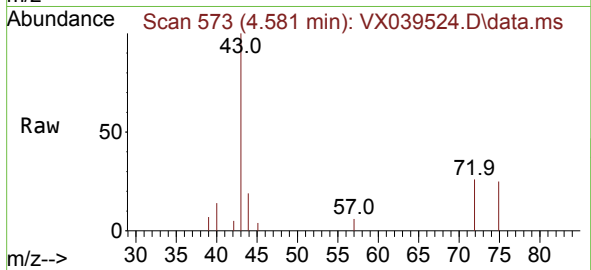

#31
Cyclohexane
Concen: 0.807 ug/l
RT: 5.471 min Scan# 719
Delta R.T. -0.006 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion: 56 Resp: 1598
Ion Ratio Lower Upper
56 100
69 27.9 23.4 35.2
84 71.8 65.9 98.9


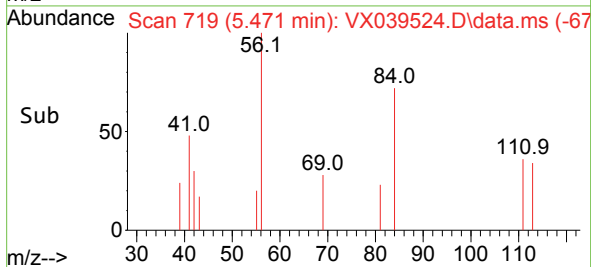
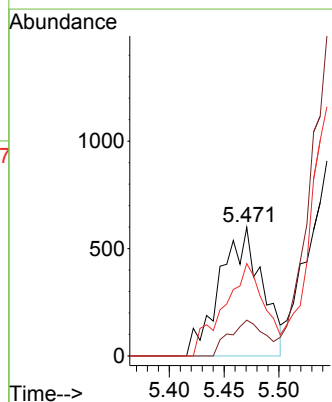
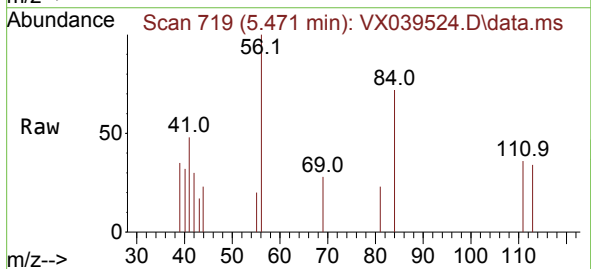


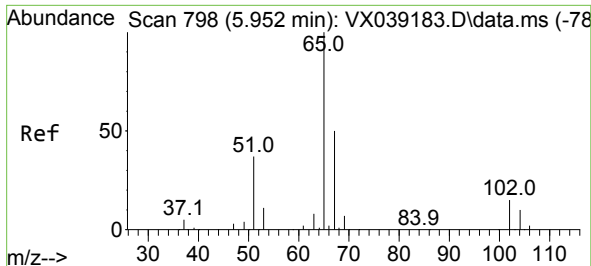

#33
1,2-Dichloroethane-d4
Concen: 48.180 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion: 65 Resp: 73868
Ion Ratio Lower Upper
65 100
67 52.9 0.0 100.2

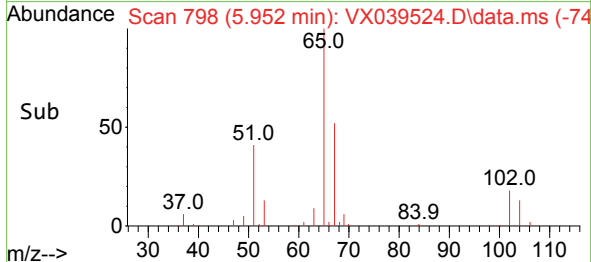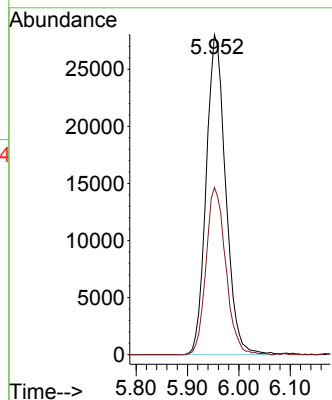

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.006 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion: 114 Resp: 177240
Ion Ratio Lower Upper
114 100
63 23.6 0.0 45.0
88 16.9 0.0 36.6


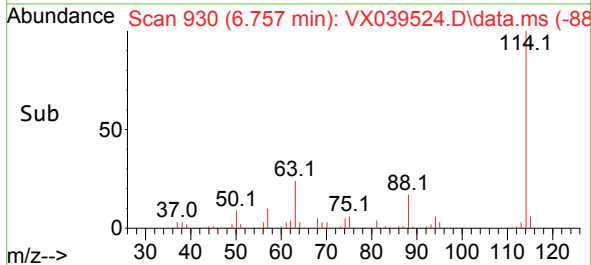
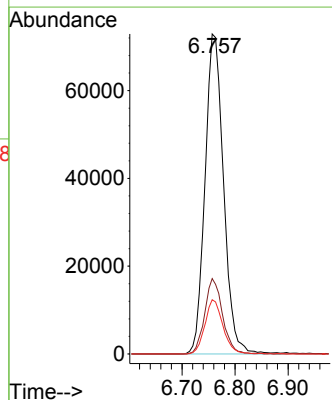
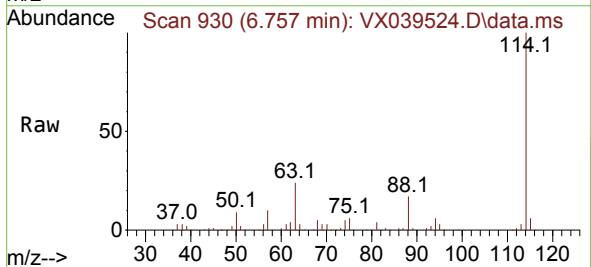


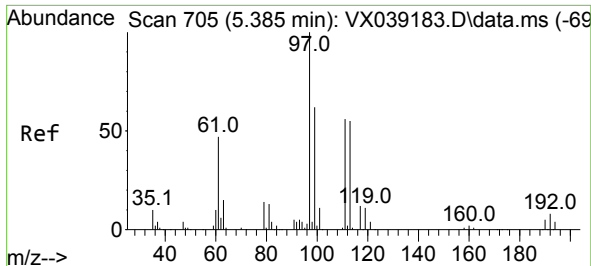

#35
Dibromofluoromethane
Concen: 46.385 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion:113 Resp: 56796
Ion Ratio Lower Upper
113 100
111 102.7 82.9 124.3
192 15.7 13.3 19.9

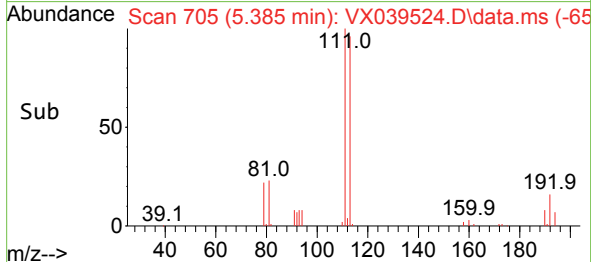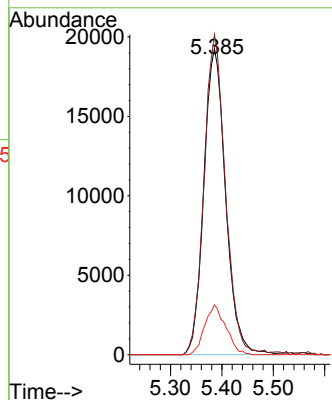

#37
Ethyl Acetate
Concen: 12.011 ug/l
RT: 4.721 min Scan# 596
Delta R.T. 0.013 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion: 43 Resp: 28672
Ion Ratio Lower Upper
43 100
61 14.5 10.6 16.0
70 11.3 8.3 12.5


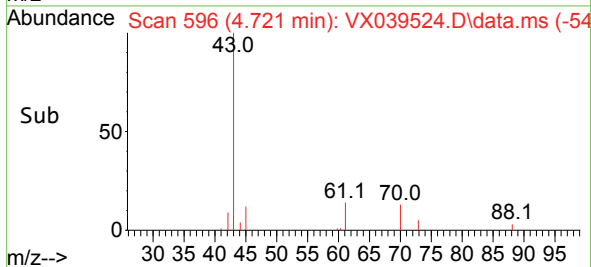
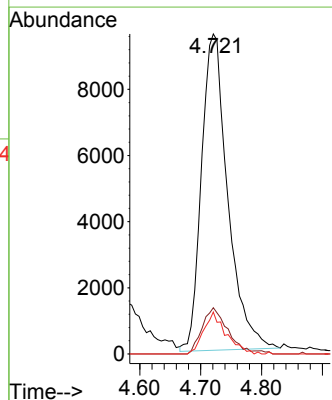
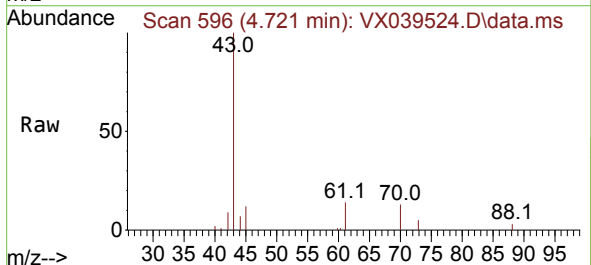


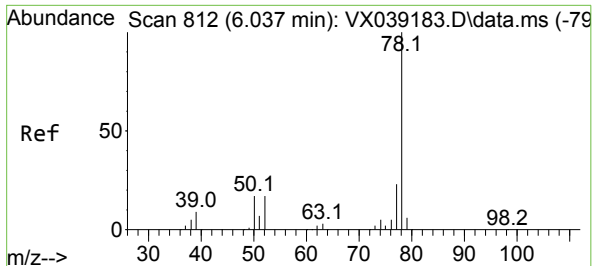

#40
Benzene
Concen: 30.487 ug/l
RT: 6.031 min Scan# 812
Delta R.T. -0.006 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion: 78 Resp: 166635
Ion Ratio Lower Upper
78 100
77 22.6 19.3 28.9

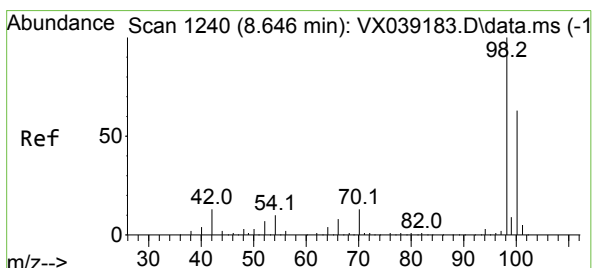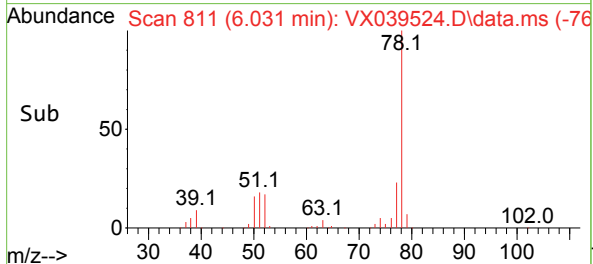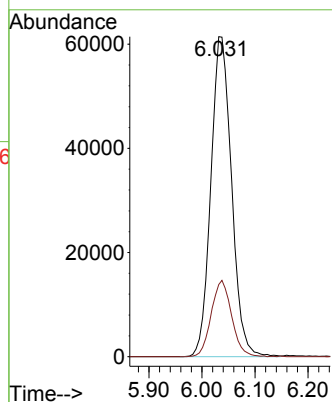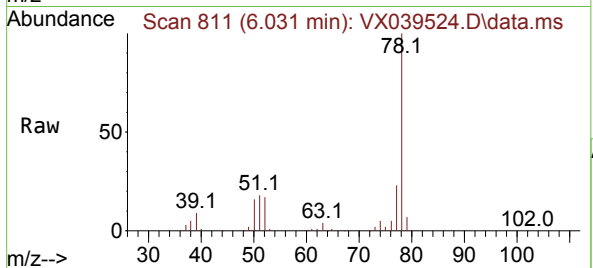

#50
Toluene-d8
Concen: 48.125 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion: 98 Resp: 218767
Ion Ratio Lower Upper
98 100
100 63.5 53.1 79.7


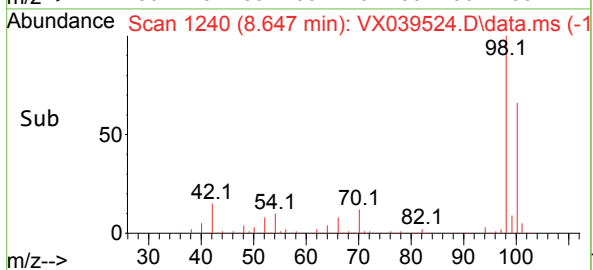
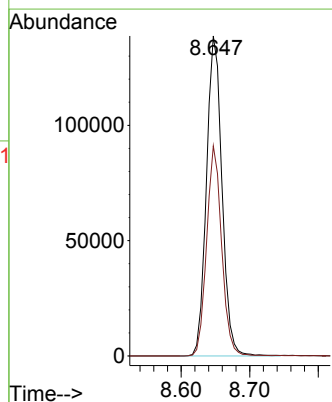
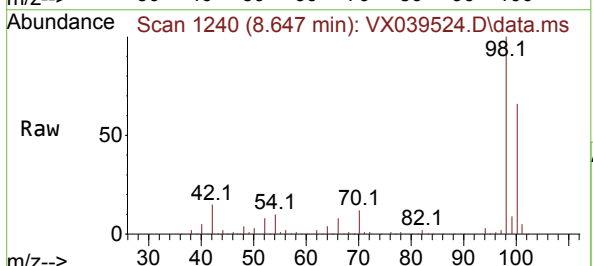


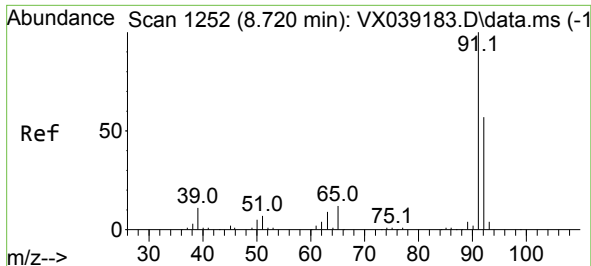

#52
Toluene
Concen: 49.201 ug/l
RT: 8.714 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion: 92 Resp: 162312
Ion Ratio Lower Upper
92 100
91 174.7 134.2 201.2

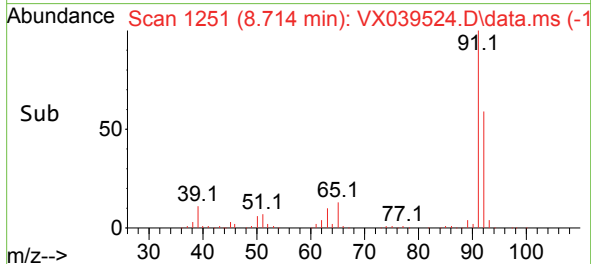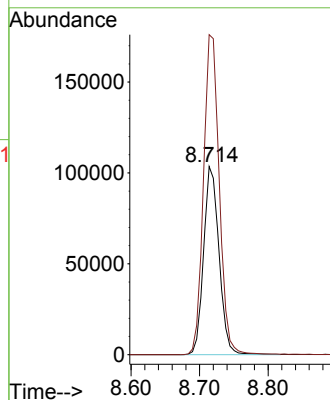

#62
4-Bromofluorobenzene
Concen: 44.759 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion: 95 Resp: 83950
Ion Ratio Lower Upper
95 100
174 64.7 0.0 135.6
176 62.0 0.0 131.0

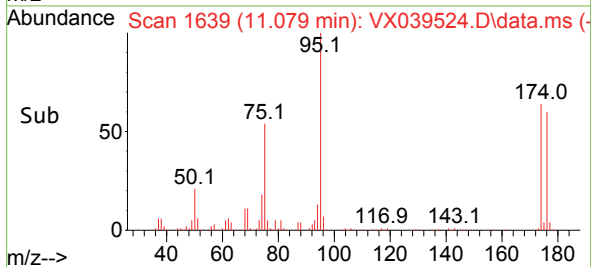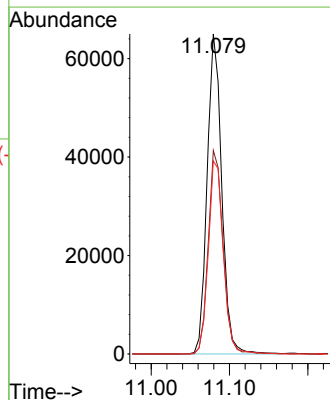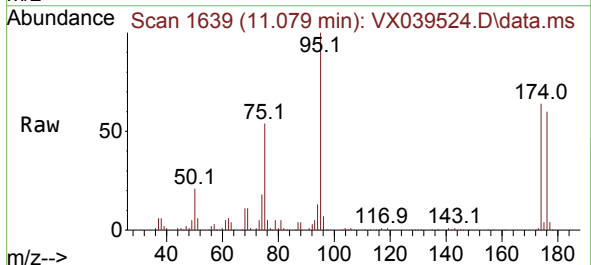



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX039524.D

Acq: 28 Dec 2023 18:12

Instrument :

MSVOA_X

ClientSampleId :

50200





Tgt Ion:117 Resp: 165197

Ion Ratio Lower Upper

117 100

82 60.9 46.2 69.4

119 32.6 25.5 38.3

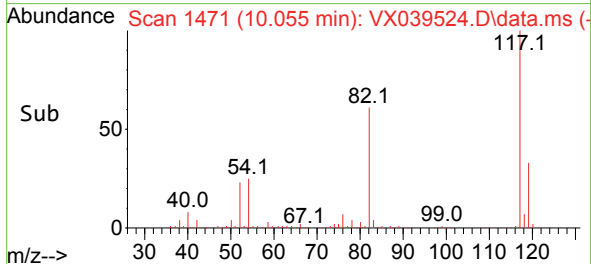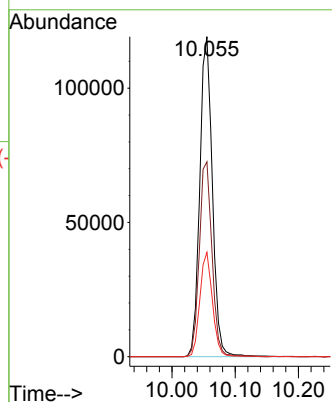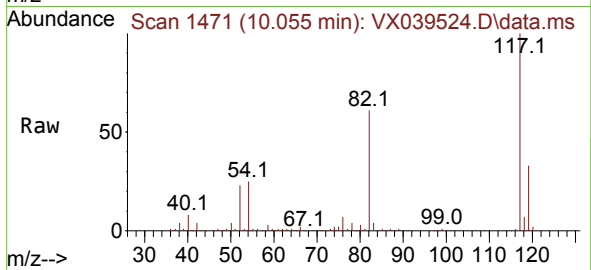

#67

Ethyl Benzene

Concen: 3.167 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX039524.D




Acq: 28 Dec 2023 18:12


Tgt Ion: 91 Resp: 21256

Ion Ratio Lower Upper

91 100

106 30.6 24.9 37.3


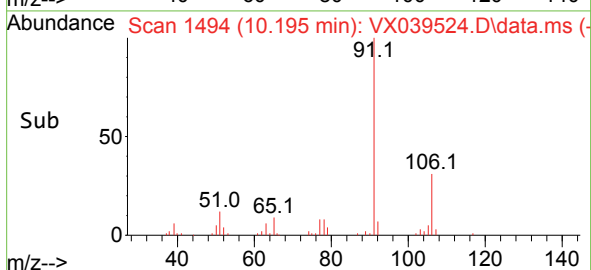
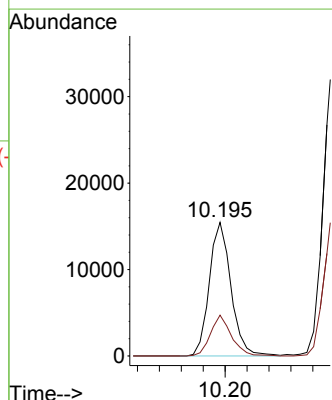
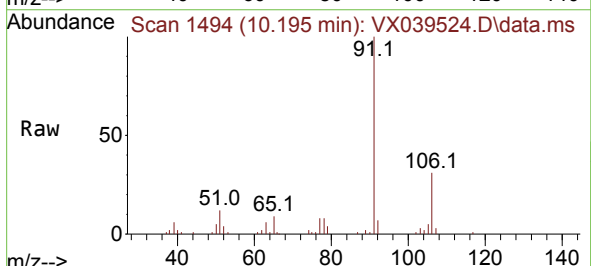


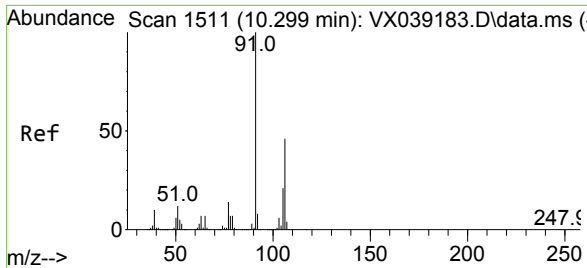

#68
m/p-Xylenes
Concen: 10.436 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12




Instrument :
MSVOA_X
ClientSampleId :
50200


Tgt Ion:106 Resp: 25114
Ion Ratio Lower Upper
106 100
91 210.3 165.5 248.3

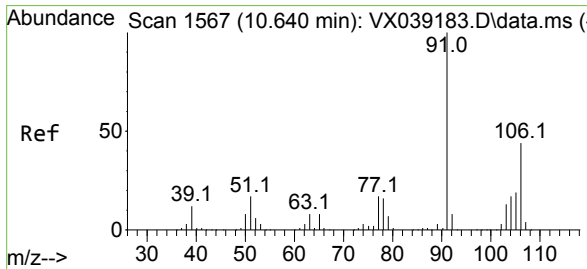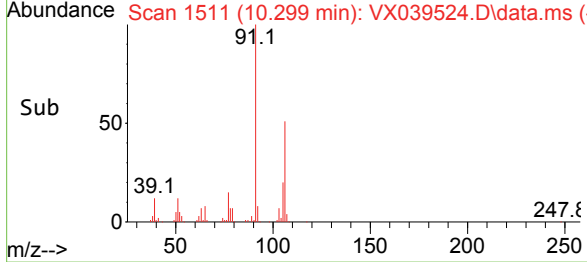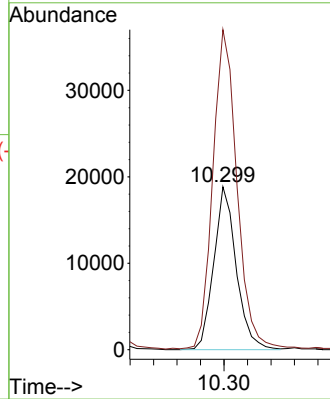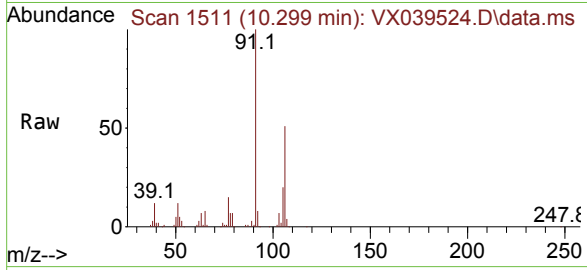

#69
o-Xylene
Concen: 5.045 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX039524.D
Acq: 28 Dec 2023 18:12

Tgt Ion:106 Resp: 11738
Ion Ratio Lower Upper
106 100
91 232.7 108.9 326.8

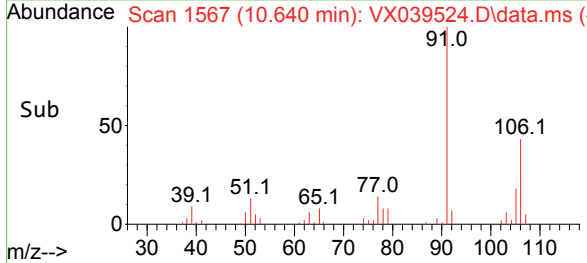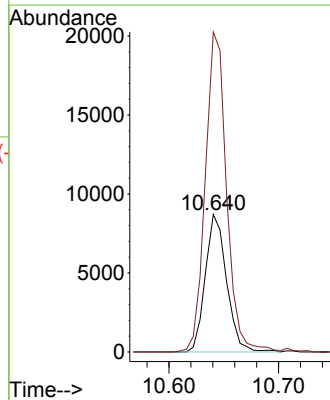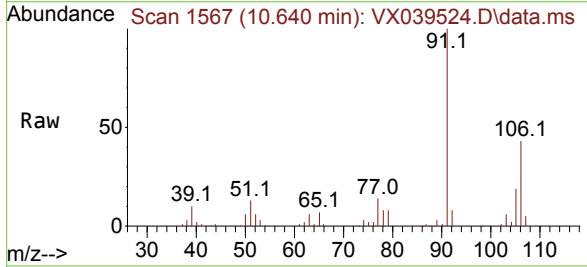



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX039524.D

Acq: 28 Dec 2023 18:12

Instrument :

MSVOA_X

ClientSampleId :

50200





Tgt Ion:152 Resp: 67130

Ion Ratio Lower Upper

152 100

115 64.9 43.3 129.9

150 154.8 0.0 345.0

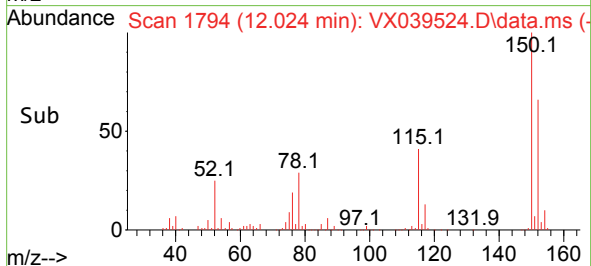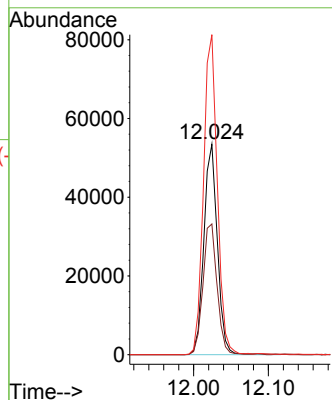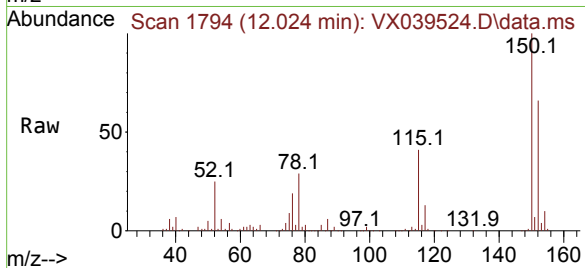

#78

n-propylbenzene

Concen: 0.237 ug/l

RT: 11.311 min Scan# 1677

Delta R.T. 0.006 min

Lab File: VX039524.D




Acq: 28 Dec 2023 18:12


Tgt Ion: 91 Resp: 1511

Ion Ratio Lower Upper

91 100

120 16.1 11.5 34.4

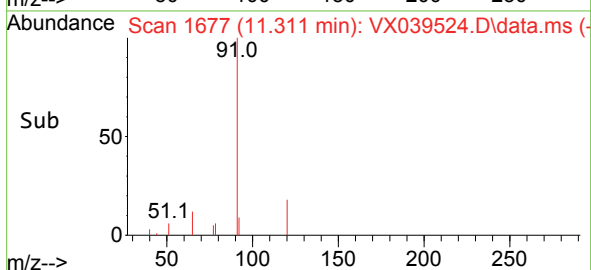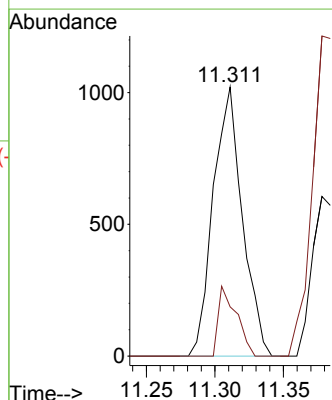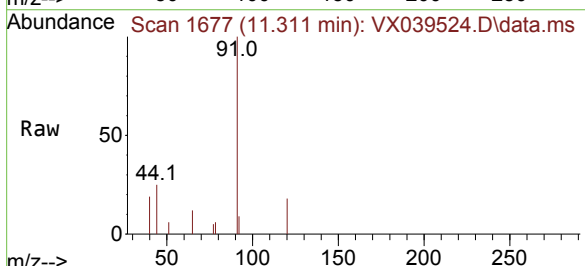



#80

1,3,5-Trimethylbenzene

Concen: 0.584 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX039524.D

Acq: 28 Dec 2023 18:12

Instrument :

MSVOA_X

ClientSampleId :





50200

Tgt Ion:105 Resp: 2575

Ion Ratio Lower Upper

105 100

120 42.8 24.1 72.3

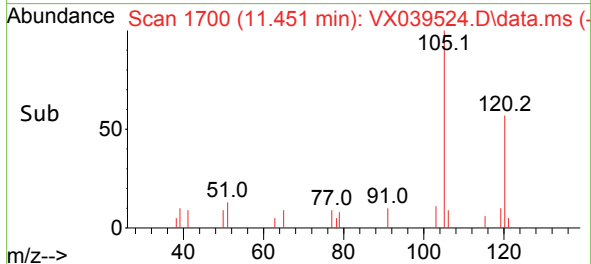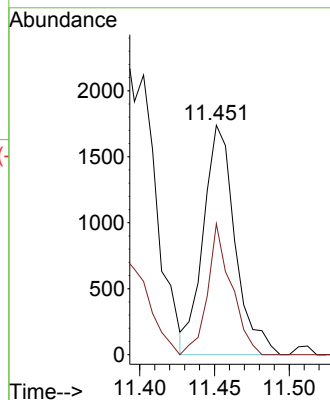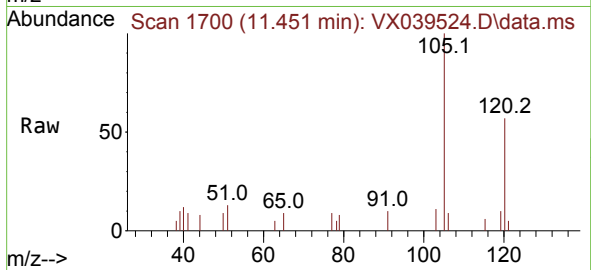

#84

1,2,4-Trimethylbenzene

Concen: 2.240 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min

Lab File: VX039524.D




Acq: 28 Dec 2023 18:12


Tgt Ion:105 Resp: 10134

Ion Ratio Lower Upper

105 100

120 43.5 21.2 63.6

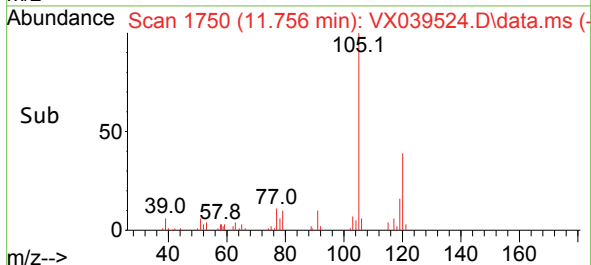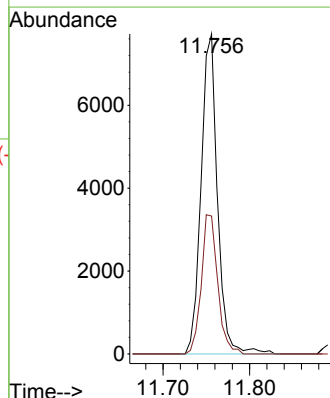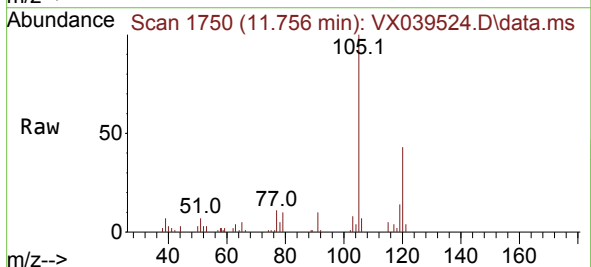



#95

Naphthalene

Concen: 1.076 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX039524.D


Acq: 28 Dec 2023 18:12

Instrument :

MSVOA_X

ClientSampleId :

50200

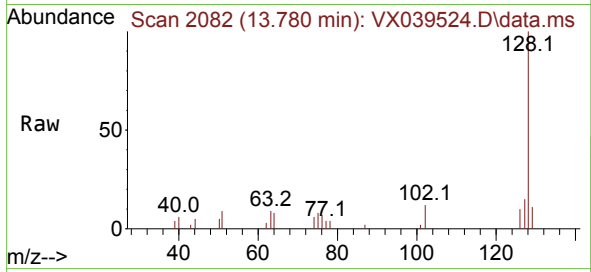

Tgt Ion:128 Resp: 5284

Ion Ratio Lower Upper

128 100

127 13.1 10.3 15.5

129 10.4 8.8 13.2

