

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
 Data File : VX039510.D
 Acq On : 28 Dec 2023 12:52
 Operator : JC/MD
 Sample : 06025-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50200

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Title : SW846 8260

Signal : TIC: VX039510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV	4877	6046	1.10%	0.191%
2	1.374	41	47	50	rBV	12109	13794	2.52%	0.435%
3	1.581	70	81	82	rBV7	6380	17447	3.19%	0.550%
4	1.727	100	105	109	rVB3	4306	5996	1.10%	0.189%
5	2.087	156	164	172	rBV	18062	30432	5.56%	0.959%
6	2.203	180	183	191	rVB4	3459	6523	1.19%	0.206%
7	2.940	298	304	317	rVB	7925	17251	3.15%	0.544%
8	5.385	694	705	719	rBV2	58211	171506	31.33%	5.406%
9	5.550	721	732	750	rVB2	86884	246990	45.12%	7.785%
10	5.958	788	799	807	rBV	70966	185574	33.90%	5.849%
11	6.031	807	811	826	rVB2	13335	37995	6.94%	1.198%
12	6.757	921	930	948	rBV	159485	391729	71.56%	12.347%
13	8.647	1234	1240	1247	rBV	344231	547439	100.00%	17.255%
14	8.720	1247	1252	1261	rVB	43767	70762	12.93%	2.230%
15	10.055	1465	1471	1482	rBV	372234	519871	94.96%	16.386%
16	10.305	1506	1512	1519	rBV	9936	15503	2.83%	0.489%
17	10.640	1564	1567	1577	rVB	5624	7640	1.40%	0.241%
18	11.079	1634	1639	1653	rBV	300173	390813	71.39%	12.318%
19	12.024	1788	1794	1802	rBV	353584	470839	86.01%	14.841%
20	15.487	2355	2362	2367	rBV4	3629	6391	1.17%	0.201%
21	16.377	2501	2508	2514	rBV2	6707	12044	2.20%	0.380%




Sum of corrected areas: 3172585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039510.D
Acq On : 28 Dec 2023 12:52
Operator : JC/MD
Sample : 06025-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

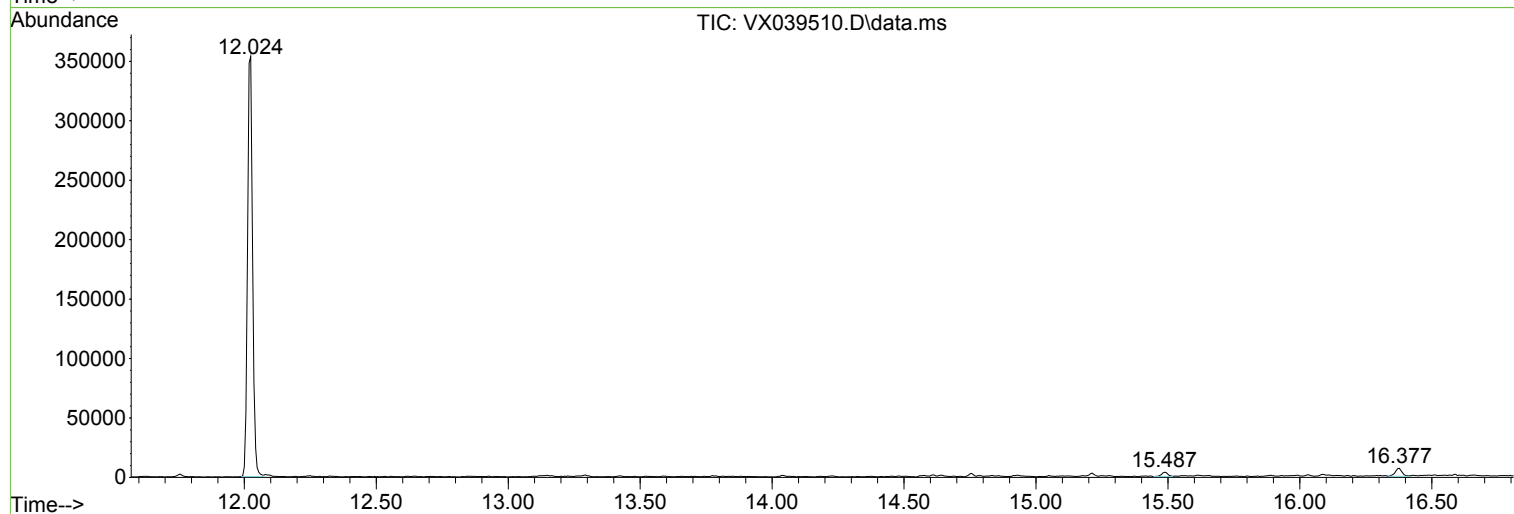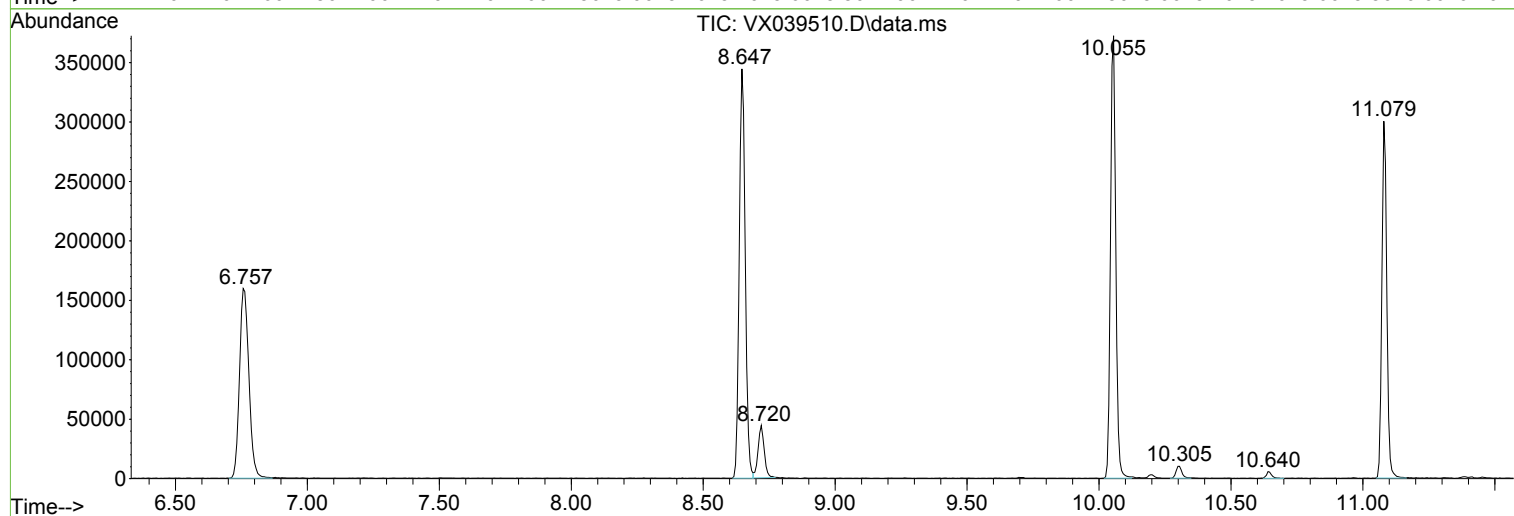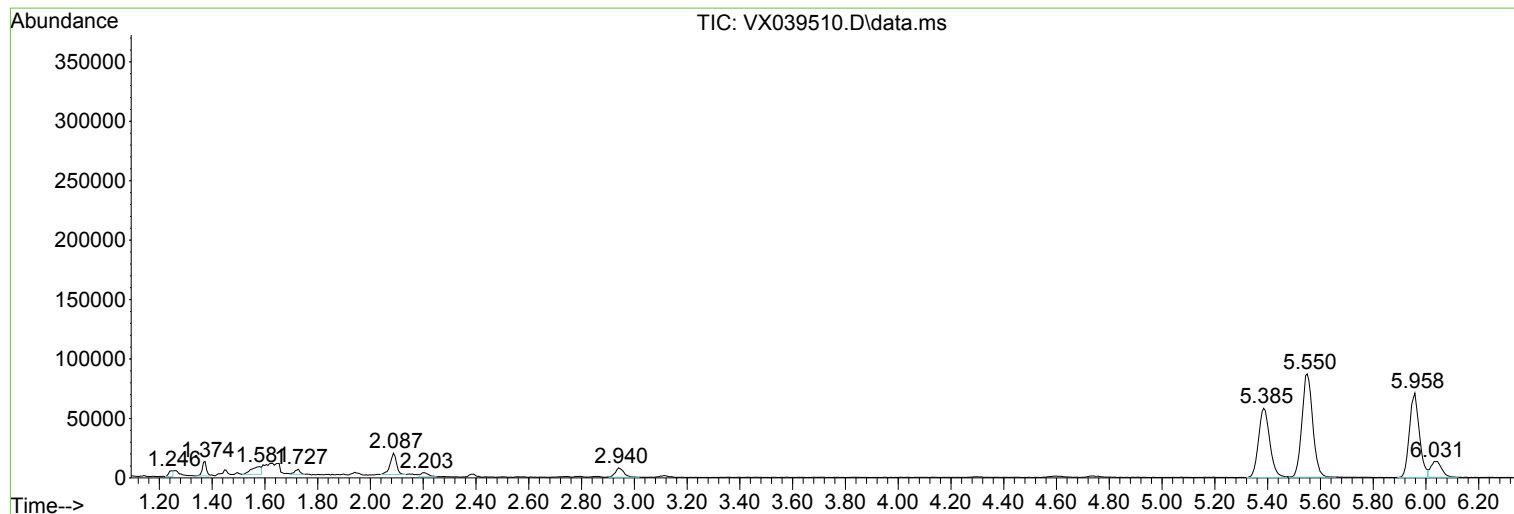

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039510.D
Acq On : 28 Dec 2023 12:52
Operator : JC/MD
Sample : 06025-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039510.D
Acq On : 28 Dec 2023 12:52
Operator : JC/MD
Sample : 06025-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50200

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc