

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
 Data File : VX039511.D
 Acq On : 28 Dec 2023 13:15
 Operator : JC/MD
 Sample : 06025-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50230

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Title : SW846 8260

Signal : TIC: VX039511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	27	rBV	4719	5849	1.05%	0.181%
2	1.264	27	29	39	rVV4	4802	7932	1.42%	0.246%
3	1.374	42	47	51	rVV	6156	6825	1.22%	0.211%
4	1.453	56	60	65	rVV	11763	14109	2.53%	0.437%
5	1.569	71	79	80	rBV2	5385	10301	1.85%	0.319%
6	2.087	156	164	171	rBV	29199	50252	9.01%	1.556%
7	2.392	209	214	223	rVB2	3131	5748	1.03%	0.178%
8	2.940	296	304	318	rBV	7127	17116	3.07%	0.530%
9	4.727	587	597	606	rBV2	3374	10937	1.96%	0.339%
10	5.385	695	705	722	rBV2	60623	175122	31.42%	5.423%
11	5.550	722	732	747	rVV2	88963	249957	44.84%	7.741%
12	5.958	790	799	807	rBV	69480	188250	33.77%	5.830%
13	6.037	807	812	822	rVB	14957	40269	7.22%	1.247%
14	6.763	922	931	948	rBV	165394	398681	71.52%	12.346%
15	8.647	1233	1240	1247	rBV	351006	557427	100.00%	17.262%
16	8.720	1247	1252	1263	rVB	46258	78134	14.02%	2.420%
17	10.055	1465	1471	1483	rBV	376205	525203	94.22%	16.264%
18	10.299	1507	1511	1519	rBV	10539	16262	2.92%	0.504%
19	10.646	1562	1568	1574	rBV	5646	7811	1.40%	0.242%
20	11.079	1634	1639	1651	rBV	297725	393405	70.58%	12.183%
21	12.024	1788	1794	1802	rBV	355698	469614	84.25%	14.543%




Sum of corrected areas: 3229204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039511.D
Acq On : 28 Dec 2023 13:15
Operator : JC/MD
Sample : 06025-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

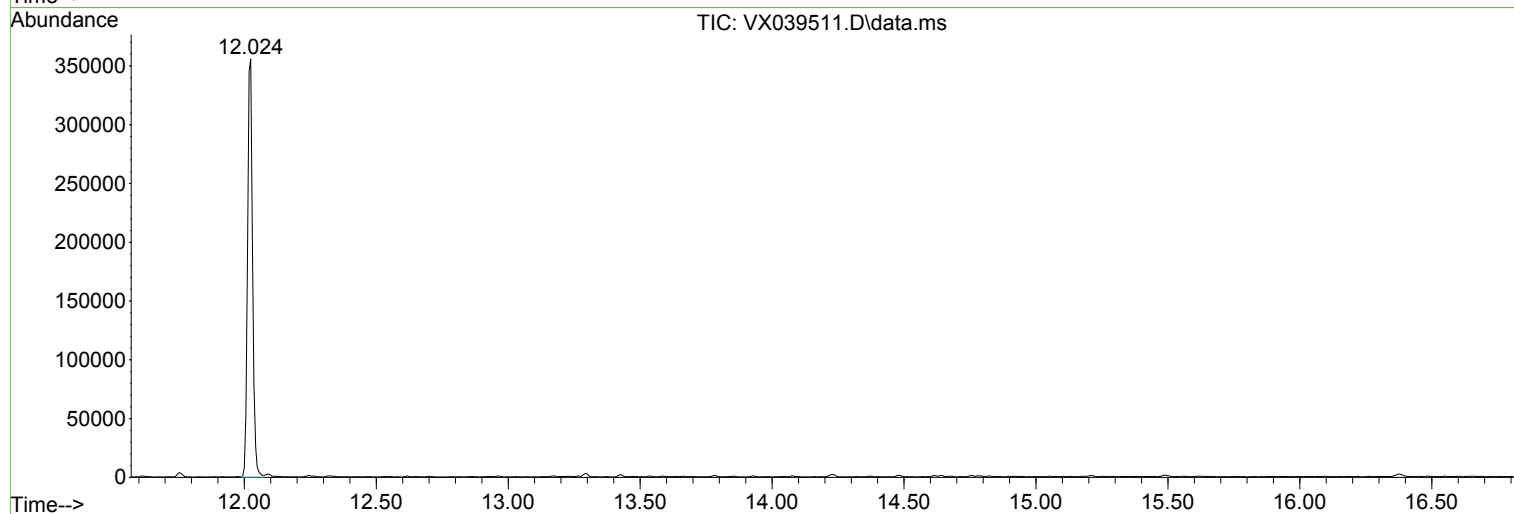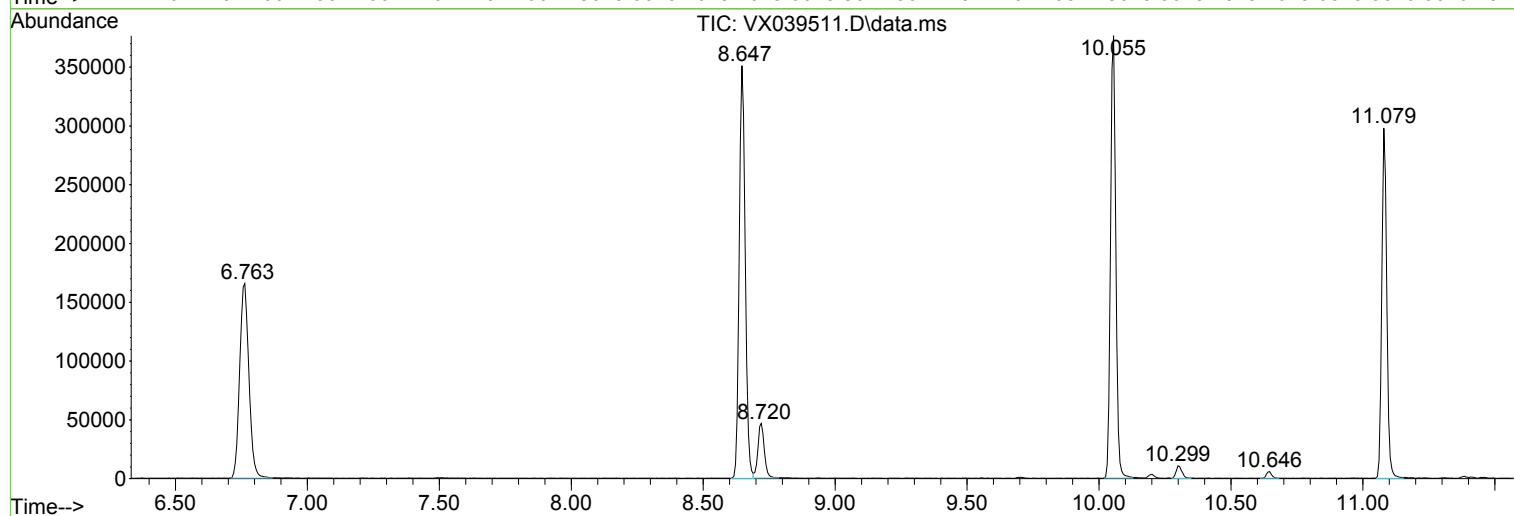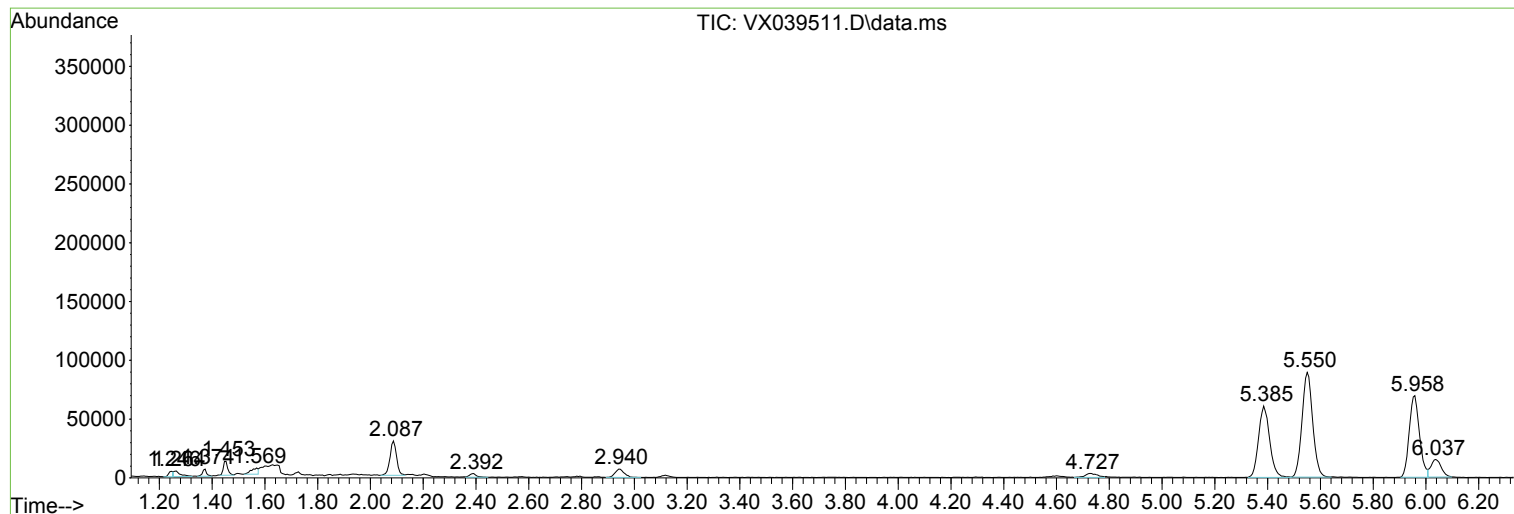

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039511.D
Acq On : 28 Dec 2023 13:15
Operator : JC/MD
Sample : 06025-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50230










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.087 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.087	10.05 ug/l	50252	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethanol			46	C2H6O	000064-17-5	43
2	Dimethyl ether			46	C2H6O	000115-10-6	5
3	Formic acid			46	CH2O2	000064-18-6	4
4	Methane, nitroso-			45	CH3NO	000865-40-7	4
5	Oxalic acid			90	C2H2O4	000144-62-7	4

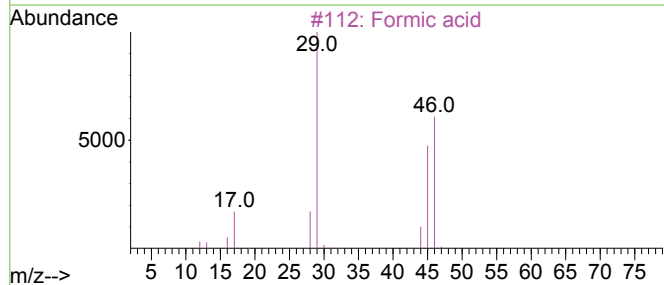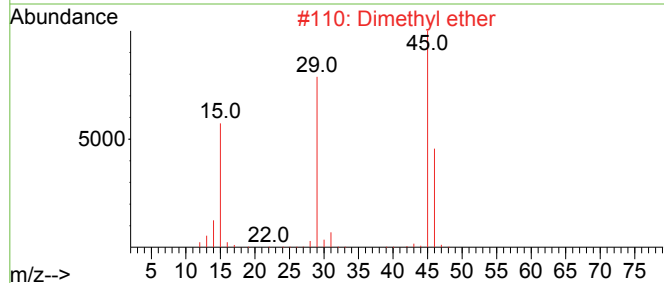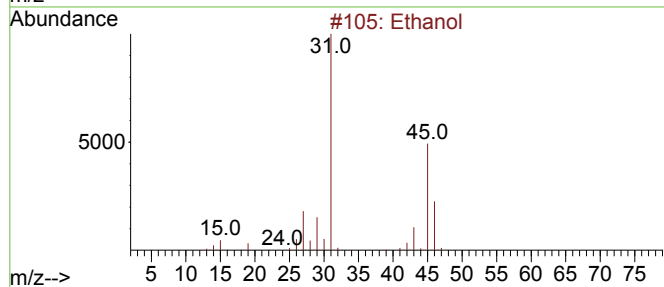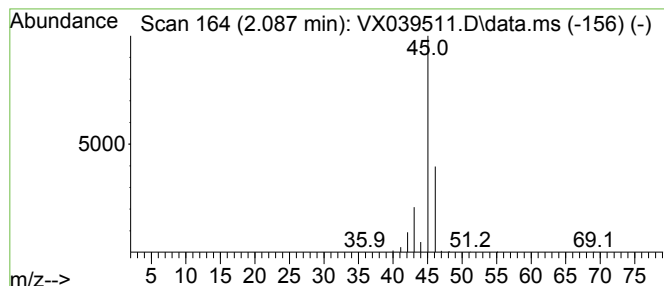

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039511.D
Acq On : 28 Dec 2023 13:15
Operator : JC/MD
Sample : 06025-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50230

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.087	2.087	10.1	ug/l	50252	1	5.556	249957	50.0