
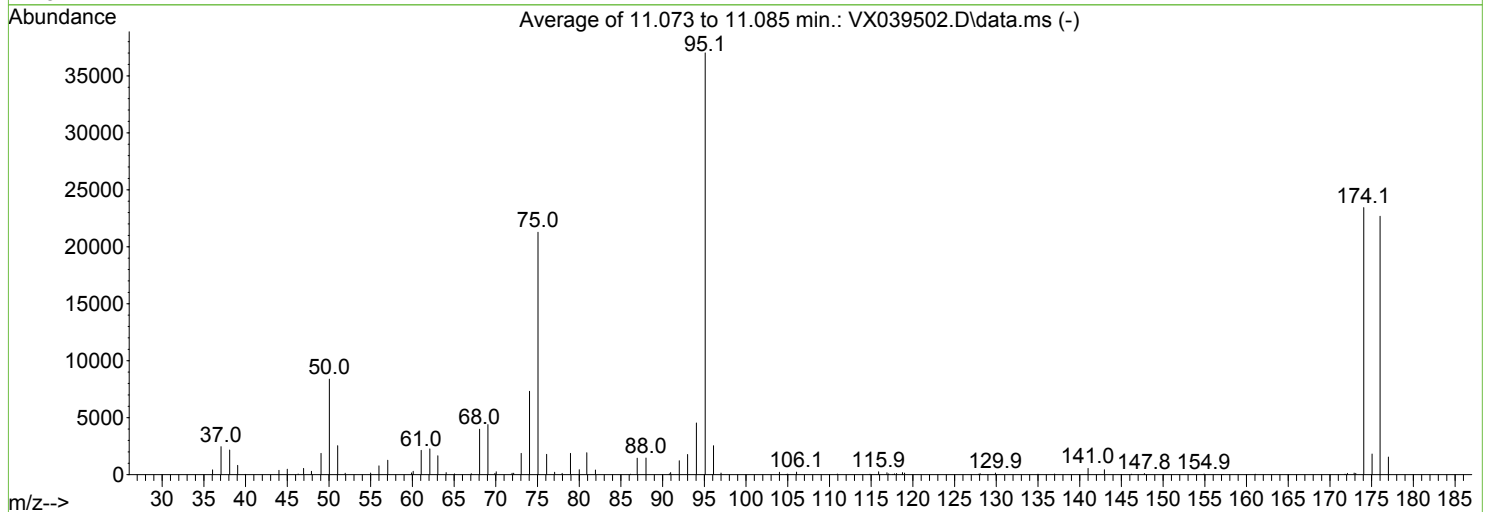


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122823\
Data File : VX039502.D
Acq On : 28 Dec 2023 09:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Title : SW846 8260
Last Update : Thu Dec 14 01:28:15 2023

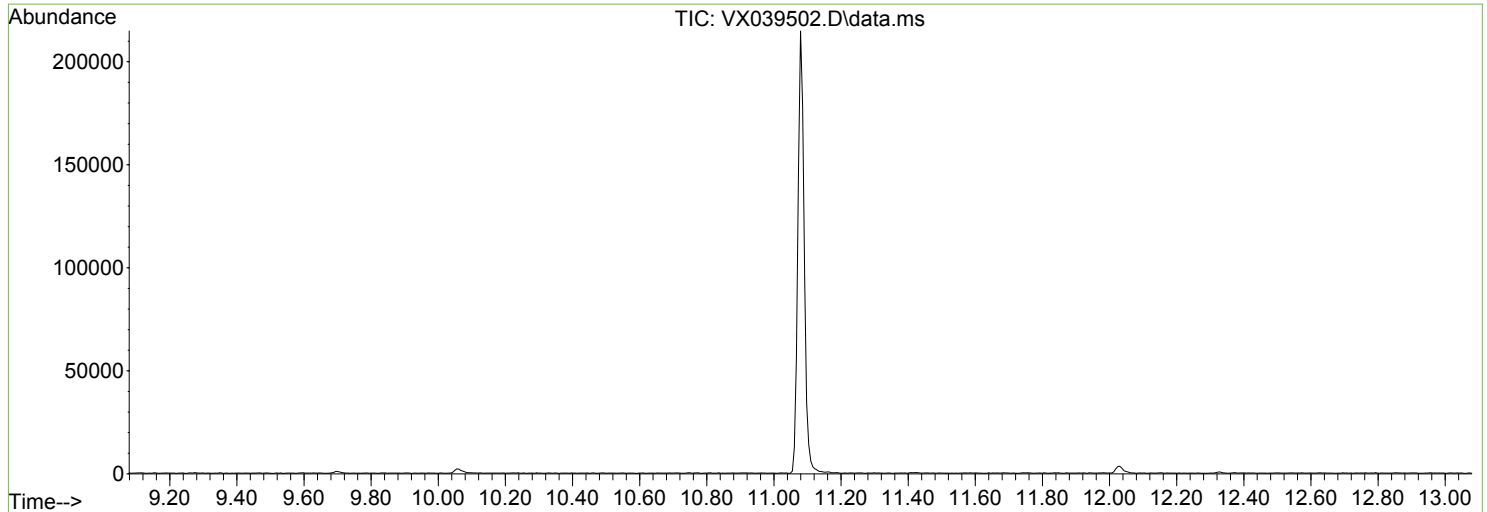

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	8389	PASS
75	95	30	60	57.5	21277	PASS
95	95	100	100	100.0	37019	PASS
96	95	5	9	6.9	2542	PASS
173	174	0.00	2	0.6	143	PASS
174	95	50	100	63.3	23434	PASS
175	174	5	9	7.7	1806	PASS
176	174	95	101	96.8	22684	PASS
177	176	5	9	6.8	1544	PASS