

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026136.D
 Acq On : 29 Dec 2021 14:11
 Operator : JC/MD
 Sample : M5216-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB9

Quant Time: Dec 30 02:41:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 30 02:39:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	191148	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	164150	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	76570	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.374	65	70936	47.814	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 95.620%			
7) Chloroethane-d5	1.672	69	56414	52.307	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 104.620%			
11) 1,1-Dichloroethene-d2	2.313	63	104677	38.654	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.300%			
21) 2-Butanone-d5	4.465	46	108325	105.667	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 105.670%			
24) Chloroform-d	5.062	84	123972	49.204	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.400%			
26) 1,2-Dichloroethane-d4	5.964	65	85723	52.487	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.980%			
32) Benzene-d6	5.983	84	245634	51.903	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.800%			
36) 1,2-Dichloropropane-d6	7.318	67	78736	53.780	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 107.560%			
41) Toluene-d8	8.653	98	234506	54.333	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.660%			
43) trans-1,3-Dichloroprop...	8.952	79	37773	52.854	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 105.700%			
47) 2-Hexanone-d5	9.384	63	77911	114.106	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 114.110%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	107292	55.065	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 110.120%			
66) 1,2-Dichlorobenzene-d4	12.323	152	79202	54.225	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.460%			
Target Compounds					Qvalue	
13) Acetone	2.386	43	5076	5.228	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026136.D
Acq On : 29 Dec 2021 14:11
Operator : JC/MD
Sample : M5216-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB9

Quant Time: Dec 30 02:41:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 30 02:39:24 2021
Response via : Initial Calibration

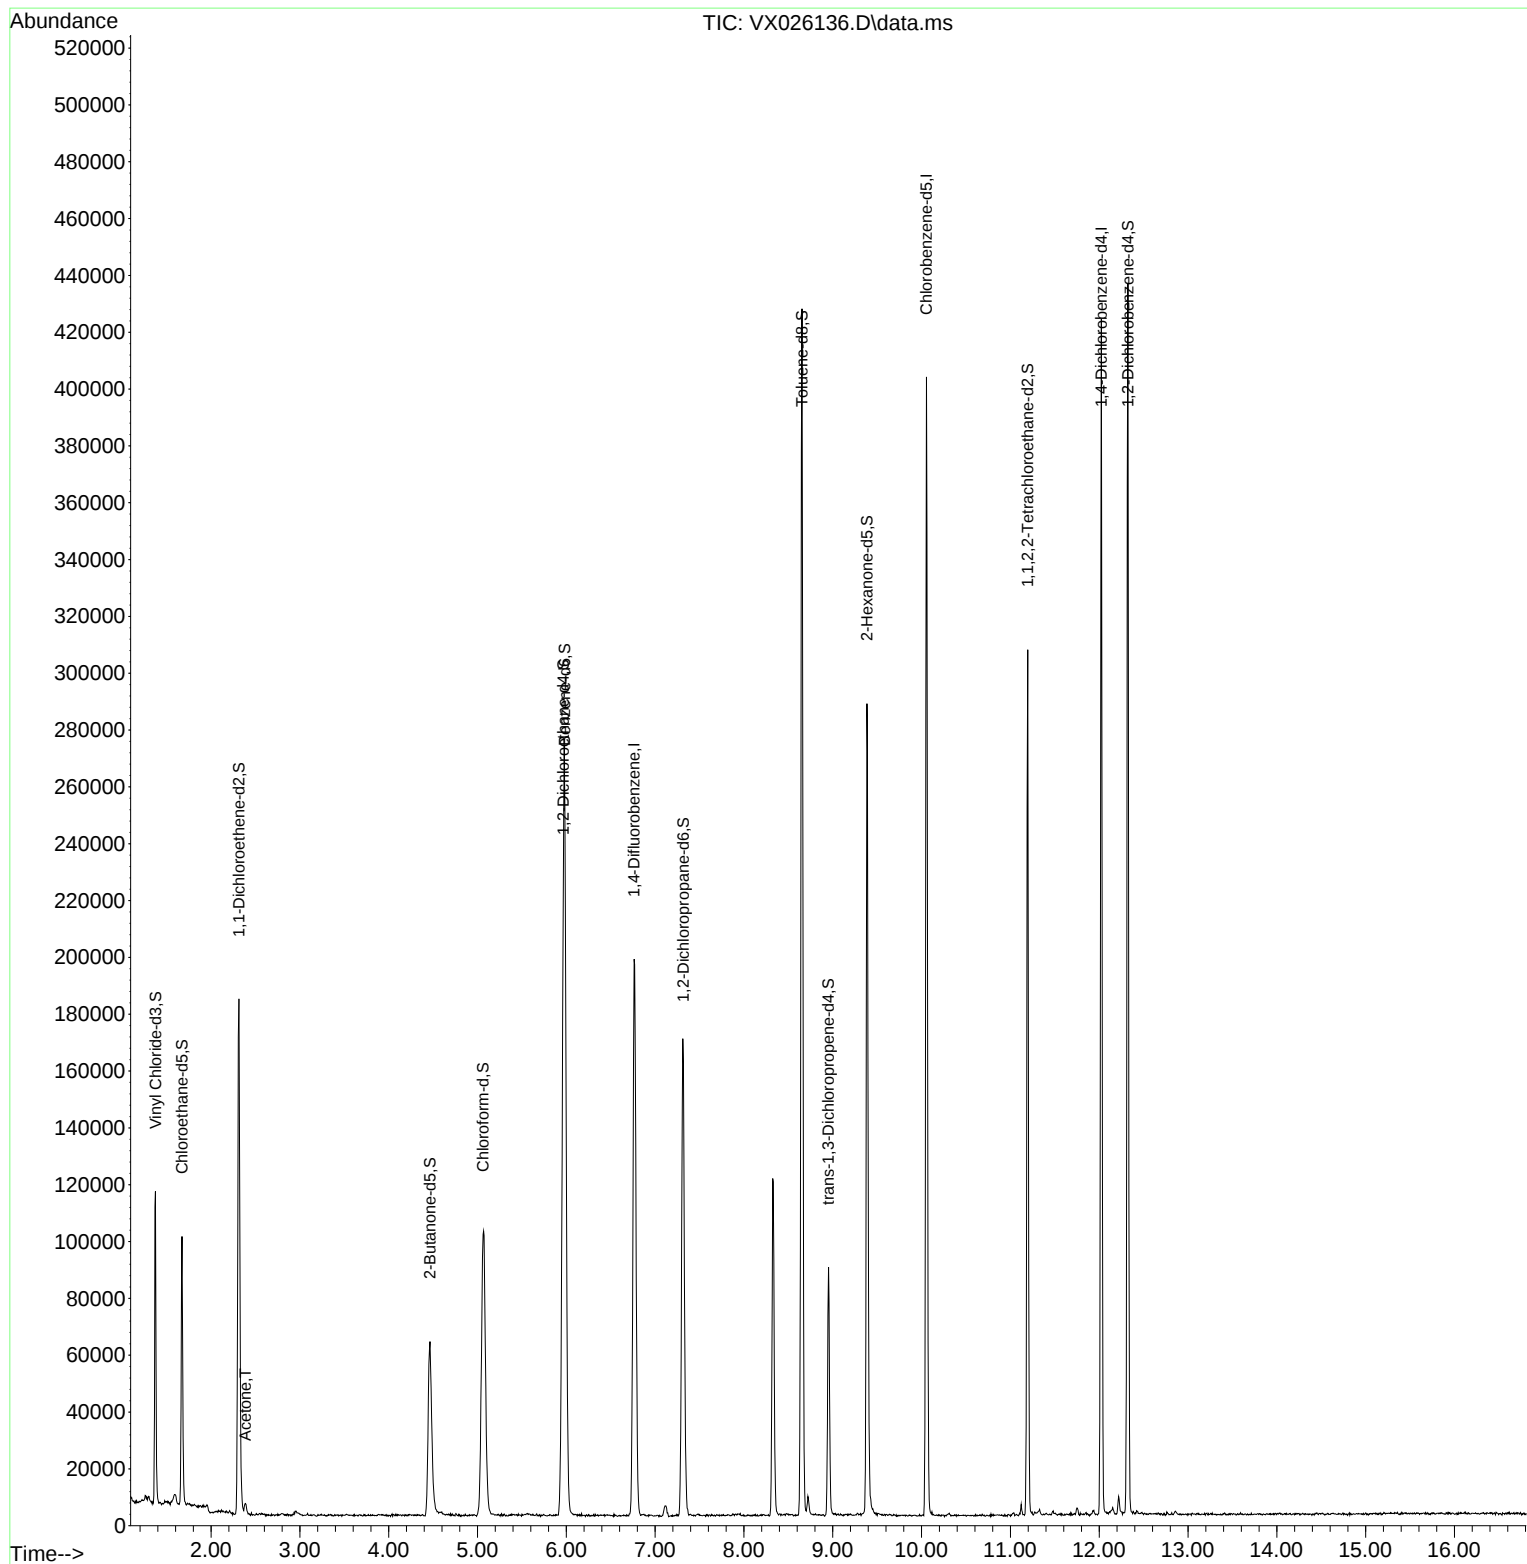

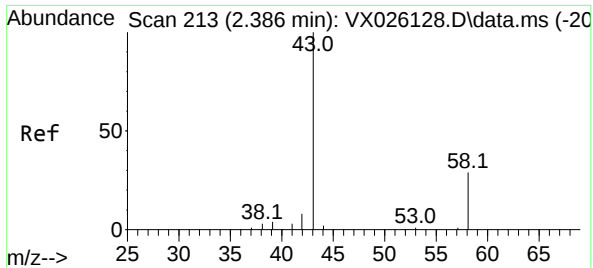

#13
 Acetone
 Concen: 5.228 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX026136.D
 Acq: 29 Dec 2021 14:11

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB9

Tgt Ion: 43 Resp: 5076
 Ion Ratio Lower Upper
 43 100
 58 25.2 0.0 58.2

