

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026131.D
 Acq On : 29 Dec 2021 12:15
 Operator : JC/MD
 Sample : M5232-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M

Title : VOC Analysis

Signal : TIC: VX026131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	54	rVB	115072	125760	15.02%	1.919%
2	1.672	92	96	103	rVB	99828	118961	14.21%	1.815%
3	2.313	194	201	217	rVB	194132	318345	38.02%	4.857%
4	2.453	222	224	226	rBV	572	595	0.07%	0.009%
5	2.672	259	260	261	rBV	675	306	0.04%	0.005%
6	2.733	268	270	271	rVB	271	155	0.02%	0.002%
7	2.794	276	280	284	rVB4	1971	3087	0.37%	0.047%
8	2.867	289	292	294	rBV2	651	914	0.11%	0.014%
9	3.312	363	365	368	rVB	755	713	0.09%	0.011%
10	3.343	368	370	373	rBV2	413	475	0.06%	0.007%
11	3.373	373	375	377	rVB	531	381	0.05%	0.006%
12	3.428	382	384	387	rVB2	582	645	0.08%	0.010%
13	3.568	405	407	410	rVV	498	432	0.05%	0.007%
14	3.599	410	412	414	rVB2	601	464	0.06%	0.007%
15	3.697	427	428	429	rVB	580	212	0.03%	0.003%
16	3.867	455	456	460	rBV2	596	670	0.08%	0.010%
17	3.916	462	464	467	rBV2	496	641	0.08%	0.010%
18	4.001	476	478	480	rBV2	504	365	0.04%	0.006%
19	4.050	485	486	488	rVB	546	381	0.05%	0.006%
20	4.068	488	489	490	rBV	627	259	0.03%	0.004%
21	4.129	497	499	503	rVB	578	642	0.08%	0.010%
22	4.166	503	505	508	rBV	364	383	0.05%	0.006%
23	4.245	517	518	519	rBV	171	65	0.01%	0.001%
24	4.324	529	531	532	rVB2	531	290	0.03%	0.004%
25	4.343	532	534	538	rVB2	657	694	0.08%	0.011%
26	4.379	538	540	542	rBV	443	307	0.04%	0.005%
27	4.459	545	553	567	rBV	60125	175922	21.01%	2.684%
28	4.702	588	593	594	rBV	810	1024	0.12%	0.016%
29	4.782	604	606	609	rBV	352	434	0.05%	0.007%
30	4.843	612	616	618	rVB	773	888	0.11%	0.014%
31	4.861	618	619	622	rBV2	449	484	0.06%	0.007%
32	5.062	640	652	668	rBV	108563	340744	40.69%	5.198%
33	5.172	668	670	672	rBV	565	468	0.06%	0.007%
34	5.446	713	715	717	rBV	428	424	0.05%	0.006%
35	5.525	725	728	729	rBV2	684	797	0.10%	0.012%
36	5.544	729	731	732	rBV2	849	668	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026131.D
 Acq On : 29 Dec 2021 12:15
 Operator : JC/MD
 Sample : M5232-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	5.629	744	745	746	rBV	703	384	0.05%	0.006%
38	5.696	754	756	757	rBV	413	361	0.04%	0.006%
39	5.727	759	761	763	rBV2	524	459	0.05%	0.007%
40	5.849	780	781	782	rBV	569	236	0.03%	0.004%

41	5.971	789	801	819	rBV2	281126	837389	100.00%	12.775%
42	6.117	823	825	826	rBV	671	349	0.04%	0.005%
43	6.178	833	835	837	rBV	363	341	0.04%	0.005%
44	6.257	847	848	849	rBV	362	161	0.02%	0.002%
45	6.275	849	851	855	rVB2	676	561	0.07%	0.009%

46	6.336	859	861	863	rBV	508	542	0.06%	0.008%
47	6.397	870	871	872	rVB	617	226	0.03%	0.003%
48	6.416	872	874	878	rBV	274	330	0.04%	0.005%
49	6.452	878	880	882	rBV2	468	640	0.08%	0.010%
50	6.489	885	886	888	rBV	589	528	0.06%	0.008%

51	6.763	922	931	947	rVB	231065	545920	65.19%	8.329%
52	6.873	947	949	952	rBV2	813	779	0.09%	0.012%
53	6.952	961	962	963	rVB	630	231	0.03%	0.004%
54	6.970	963	965	967	rBV	556	683	0.08%	0.010%
55	7.037	973	976	978	rBV2	775	942	0.11%	0.014%

56	7.111	982	988	996	rVB3	4504	9827	1.17%	0.150%
57	7.184	999	1000	1003	rBV	590	637	0.08%	0.010%
58	7.312	1012	1021	1034	rVB2	188006	411556	49.15%	6.279%
59	8.055	1139	1143	1144	rBV2	508	756	0.09%	0.012%
60	8.324	1181	1187	1196	rBV	130923	218733	26.12%	3.337%

61	8.580	1228	1229	1230	rVB	741	271	0.03%	0.004%
62	8.604	1230	1233	1234	rBV	673	614	0.07%	0.009%
63	8.653	1234	1241	1248	rVV	435975	696673	83.20%	10.629%
64	8.720	1249	1252	1258	rVB	6677	9702	1.16%	0.148%
65	8.952	1285	1290	1301	rVB	94691	138049	16.49%	2.106%

66	9.281	1342	1344	1345	rVB	784	384	0.05%	0.006%
67	9.385	1356	1361	1375	rVB	294982	416165	49.70%	6.349%
68	9.976	1456	1458	1459	rVB	561	294	0.04%	0.004%
69	9.994	1459	1461	1463	rBV	690	538	0.06%	0.008%
70	10.055	1465	1471	1485	rVB	464114	620595	74.11%	9.468%

71	10.470	1538	1539	1540	rBV	500	251	0.03%	0.004%
72	10.543	1550	1551	1554	rBV	714	691	0.08%	0.011%
73	10.604	1559	1561	1564	rBV	569	670	0.08%	0.010%
74	10.890	1607	1608	1613	rBV	614	953	0.11%	0.015%
75	11.122	1642	1646	1652	rBV3	3593	4923	0.59%	0.075%

76	11.195	1652	1658	1666	rBV	301267	390849	46.67%	5.963%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026131.D
 Acq On : 29 Dec 2021 12:15
 Operator : JC/MD
 Sample : M5232-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	11.750	1746	1749	1753	rVB3	3671	4706	0.56%	0.072%
78	11.787	1753	1755	1756	rBV	439	295	0.04%	0.005%
79	12.024	1788	1794	1804	rVB	455641	558953	66.75%	8.527%
80	12.323	1836	1843	1850	rBV	442012	570119	68.08%	8.698%
81	12.421	1857	1859	1865	rVB3	1076	1770	0.21%	0.027%
82	12.530	1875	1877	1878	rBB	569	212	0.03%	0.003%
83	13.055	1961	1963	1964	rVB	1442	768	0.09%	0.012%
84	13.189	1983	1985	1987	rVB	690	439	0.05%	0.007%
85	13.207	1987	1988	1989	rBV	539	303	0.04%	0.005%
86	13.280	1996	2000	2002	rBV	1059	1085	0.13%	0.017%
87	13.426	2023	2024	2025	rVB	637	233	0.03%	0.004%
88	14.262	2159	2161	2163	rBV	556	612	0.07%	0.009%
89	14.304	2167	2168	2169	rBV	468	261	0.03%	0.004%
90	14.451	2190	2192	2194	rBV2	485	310	0.04%	0.005%
91	14.585	2212	2214	2216	rBV	622	471	0.06%	0.007%
92	14.780	2244	2246	2247	rBV2	497	332	0.04%	0.005%
93	14.890	2263	2264	2267	rBV2	532	575	0.07%	0.009%
94	15.188	2310	2313	2316	rBV3	785	1107	0.13%	0.017%




Sum of corrected areas: 6554739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026131.D
Acq On : 29 Dec 2021 12:15
Operator : JC/MD
Sample : M5232-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

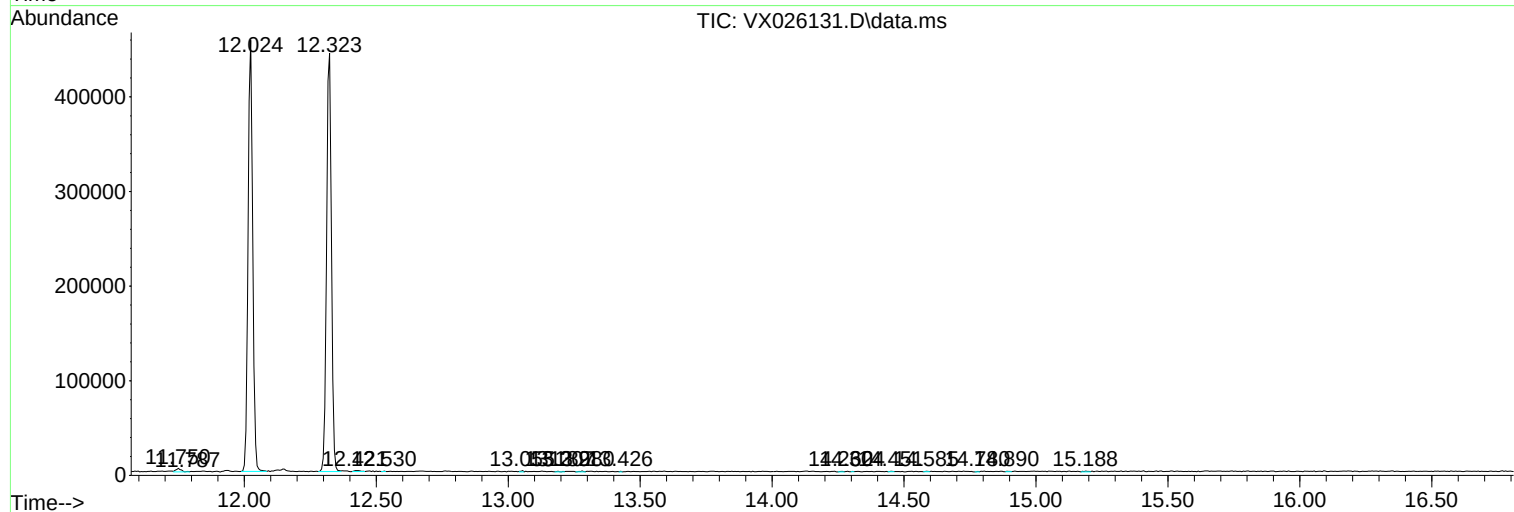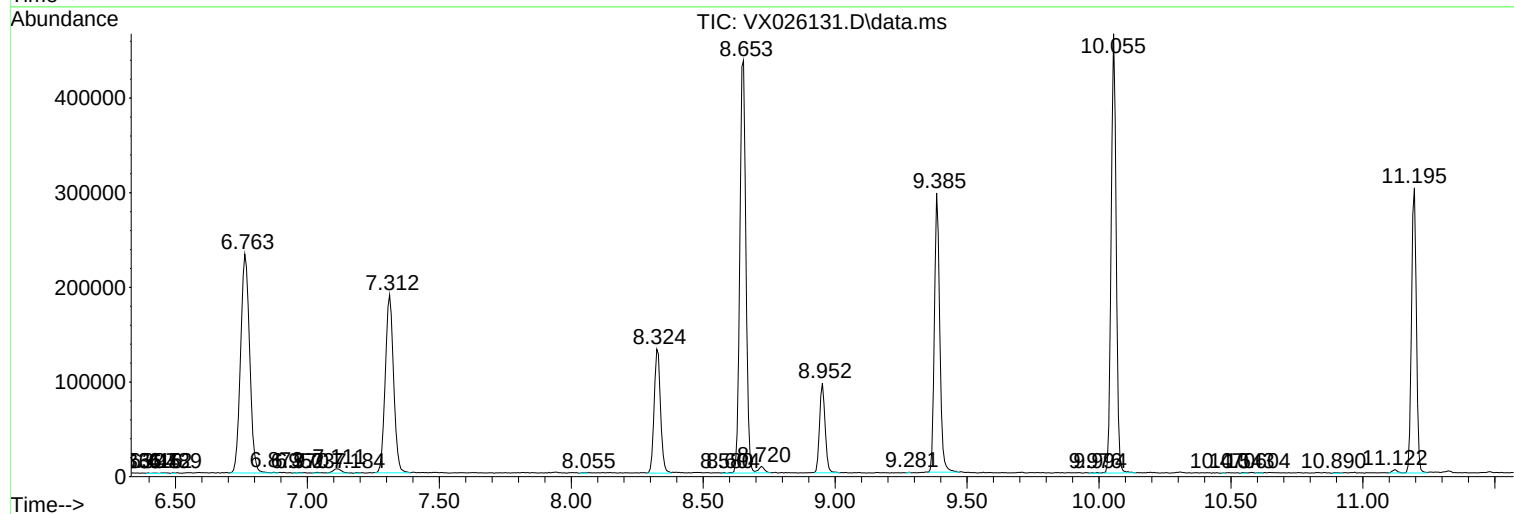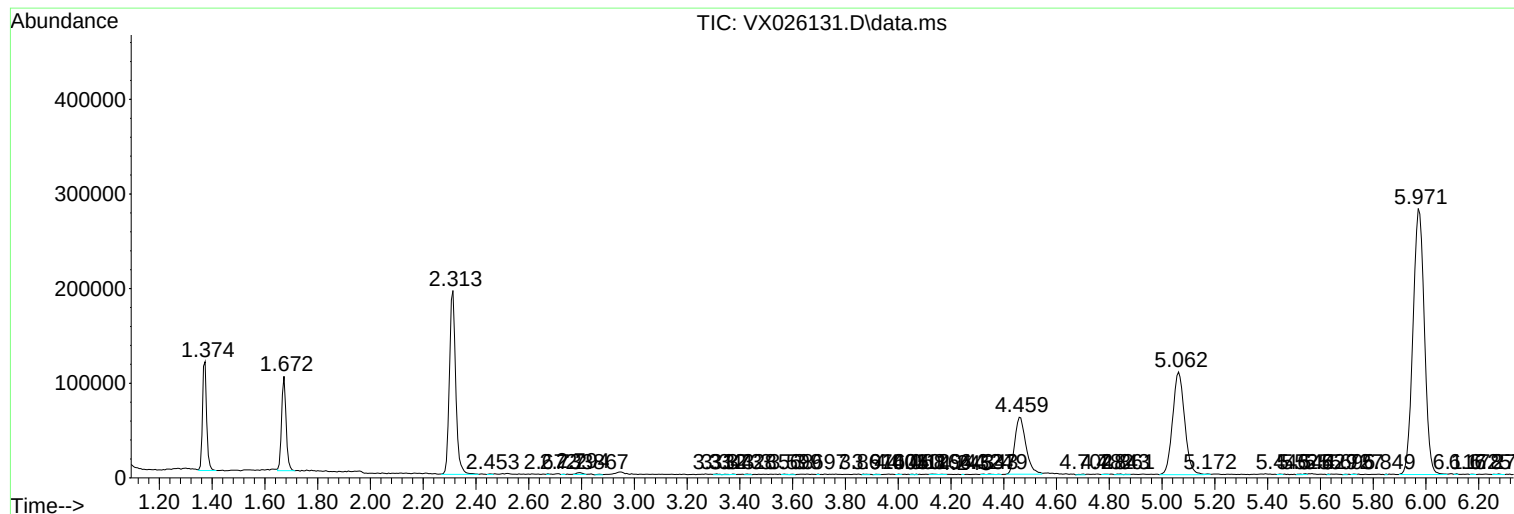

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026131.D
Acq On : 29 Dec 2021 12:15
Operator : JC/MD
Sample : M5232-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026131.D
Acq On : 29 Dec 2021 12:15
Operator : JC/MD
Sample : M5232-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc