

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026132.D
 Acq On : 29 Dec 2021 12:38
 Operator : JC/MD
 Sample : M5216-02DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	57	rVB	119868	128106	6.17%	1.290%
2	1.672	92	96	105	rVB	98832	121033	5.83%	1.219%
3	2.313	194	201	210	rBV	200093	321615	15.50%	3.238%
4	2.520	233	235	238	rVB2	934	899	0.04%	0.009%
5	2.544	238	239	241	rBV	818	551	0.03%	0.006%
6	2.666	257	259	260	rVB	746	451	0.02%	0.005%
7	2.691	260	263	265	rBV2	592	847	0.04%	0.009%
8	2.794	276	280	286	rVB4	2553	4774	0.23%	0.048%
9	2.940	299	304	315	rVB2	4329	9704	0.47%	0.098%
10	3.172	341	342	345	rBV2	622	575	0.03%	0.006%
11	3.221	348	350	352	rVB	608	559	0.03%	0.006%
12	3.428	380	384	385	rBV2	374	471	0.02%	0.005%
13	3.471	390	391	392	rBV	974	542	0.03%	0.005%
14	3.849	451	453	455	rVB	708	444	0.02%	0.004%
15	3.977	472	474	476	rBV	759	685	0.03%	0.007%
16	4.263	520	521	524	rVB2	657	592	0.03%	0.006%
17	4.312	524	529	532	rBV3	829	1574	0.08%	0.016%
18	4.379	539	540	542	rBV	459	412	0.02%	0.004%
19	4.458	544	553	566	rBV	66817	193055	9.30%	1.944%
20	4.702	591	593	595	rVV3	531	442	0.02%	0.004%
21	4.977	635	638	639	rBV	538	552	0.03%	0.006%
22	5.062	641	652	669	rVB	118659	358069	17.25%	3.605%
23	5.300	688	691	692	rVB	502	421	0.02%	0.004%
24	5.330	694	696	700	rVV2	353	517	0.02%	0.005%
25	5.379	702	704	710	rVV2	748	1432	0.07%	0.014%
26	5.519	726	727	729	rBV	560	489	0.02%	0.005%
27	5.544	729	731	733	rVB2	651	703	0.03%	0.007%
28	5.611	740	742	745	rBV	561	742	0.04%	0.007%
29	5.672	750	752	753	rBV	681	655	0.03%	0.007%
30	5.775	767	769	771	rVB2	690	447	0.02%	0.005%
31	5.977	788	802	809	rBV2	296735	897046	43.22%	9.031%
32	6.409	869	873	874	rBV	599	619	0.03%	0.006%
33	6.458	879	881	884	rBV3	637	847	0.04%	0.009%
34	6.519	889	891	893	rBV	738	612	0.03%	0.006%
35	6.672	914	916	919	rVV	406	580	0.03%	0.006%
36	6.763	922	931	942	rBV	206511	501233	24.15%	5.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026132.D
 Acq On : 29 Dec 2021 12:38
 Operator : JC/MD
 Sample : M5216-02DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

37	7.117	983	989	997	rVB3	4327	9833	0.47%	0.099%
38	7.312	1012	1021	1034	rBV	187227	409775	19.75%	4.125%
39	7.525	1054	1056	1059	rBV2	439	628	0.03%	0.006%
40	7.824	1103	1105	1107	rVB	915	592	0.03%	0.006%
41	7.860	1107	1111	1112	rBV	923	763	0.04%	0.008%
42	7.927	1119	1122	1124	rBV4	937	1161	0.06%	0.012%
43	8.330	1181	1188	1195	rVV	126554	214772	10.35%	2.162%
44	8.482	1211	1213	1218	rVB2	1105	1247	0.06%	0.013%
45	8.653	1234	1241	1249	rBV	446278	706398	34.04%	7.112%
46	8.720	1249	1252	1258	rVV3	6995	11148	0.54%	0.112%
47	8.769	1258	1260	1261	rVB	1000	528	0.03%	0.005%
48	8.811	1264	1267	1268	rBV	449	460	0.02%	0.005%
49	8.903	1281	1282	1284	rBV	823	567	0.03%	0.006%
50	8.952	1284	1290	1298	rVV	98701	140255	6.76%	1.412%
51	9.128	1317	1319	1321	rBV2	447	493	0.02%	0.005%
52	9.281	1340	1344	1347	rBV	863	1257	0.06%	0.013%
53	9.348	1353	1355	1356	rBV2	975	748	0.04%	0.008%
54	9.384	1356	1361	1376	rVB	306352	434912	20.96%	4.378%
55	9.689	1409	1411	1412	rBV	658	622	0.03%	0.006%
56	9.756	1421	1422	1425	rBV2	680	736	0.04%	0.007%
57	9.909	1444	1447	1448	rBV	464	423	0.02%	0.004%
58	10.079	1465	1475	1490	rVB2	1137435	2075332	100.00%	20.893%
59	10.195	1490	1494	1498	rVB4	1039	1844	0.09%	0.019%
60	10.293	1509	1510	1512	rBV2	997	927	0.04%	0.009%
61	10.433	1530	1533	1535	rVB2	659	851	0.04%	0.009%
62	10.518	1545	1547	1550	rBV2	334	443	0.02%	0.004%
63	10.634	1564	1566	1567	rBV	520	413	0.02%	0.004%
64	10.732	1581	1582	1586	rBV	727	709	0.03%	0.007%
65	10.762	1586	1587	1591	rVB2	610	505	0.02%	0.005%
66	10.866	1602	1604	1608	rVB	422	450	0.02%	0.005%
67	10.902	1608	1610	1612	rVV	534	416	0.02%	0.004%
68	10.933	1614	1615	1618	rVV2	853	841	0.04%	0.008%
69	10.970	1618	1621	1623	rVB	646	829	0.04%	0.008%
70	11.079	1636	1639	1640	rBV	586	544	0.03%	0.005%
71	11.122	1642	1646	1650	rVV3	3749	4976	0.24%	0.050%
72	11.195	1652	1658	1665	rVV	316915	398521	19.20%	4.012%
73	11.408	1692	1693	1696	rVB2	472	419	0.02%	0.004%
74	11.451	1696	1700	1701	rBV2	728	850	0.04%	0.009%
75	11.476	1702	1704	1710	rVB3	1288	1688	0.08%	0.017%
76	11.750	1745	1749	1754	rVB3	3139	4723	0.23%	0.048%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026132.D
 Acq On : 29 Dec 2021 12:38
 Operator : JC/MD
 Sample : M5216-02DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COHB5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	11.829	1761	1762	1763	rBV	810	544	0.03%	0.005%
78	11.927	1775	1778	1781	rBV3	1792	2729	0.13%	0.027%
79	11.969	1781	1785	1789	rVV	65519	81029	3.90%	0.816%
80	12.043	1789	1797	1805	rVB2	582187	1198191	57.73%	12.063%
81	12.152	1813	1815	1822	rVB2	3371	3902	0.19%	0.039%
82	12.213	1822	1825	1827	rVB2	704	846	0.04%	0.009%
83	12.335	1837	1845	1857	rVV2	791523	1449938	69.87%	14.597%
84	12.427	1857	1860	1864	rVB4	1438	1854	0.09%	0.019%
85	12.616	1889	1891	1894	rVB2	621	615	0.03%	0.006%
86	12.731	1908	1910	1913	rBV	583	720	0.03%	0.007%
87	12.878	1929	1934	1935	rVV2	543	802	0.04%	0.008%
88	12.920	1939	1941	1946	rBV3	971	1460	0.07%	0.015%
89	13.042	1959	1961	1963	rBV2	855	954	0.05%	0.010%
90	13.158	1979	1980	1982	rBV2	497	477	0.02%	0.005%
91	13.402	2018	2020	2023	rBV	449	476	0.02%	0.005%
92	13.591	2046	2051	2058	rBV	122247	157925	7.61%	1.590%
93	13.914	2102	2104	2107	rBV	420	426	0.02%	0.004%
94	13.963	2107	2112	2118	rVV	30552	37787	1.82%	0.380%
95	14.743	2237	2240	2242	rBV2	671	919	0.04%	0.009%
96	14.792	2244	2248	2250	rBV2	1076	1534	0.07%	0.015%
97	14.975	2277	2278	2280	rBV	899	584	0.03%	0.006%
98	15.249	2320	2323	2327	rVB5	2320	3261	0.16%	0.033%
99	15.402	2346	2348	2349	rBV	799	613	0.03%	0.006%
100	16.322	2497	2499	2500	rBV	611	447	0.02%	0.005%




Sum of corrected areas: 9932927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026132.D
Acq On : 29 Dec 2021 12:38
Operator : JC/MD
Sample : M5216-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

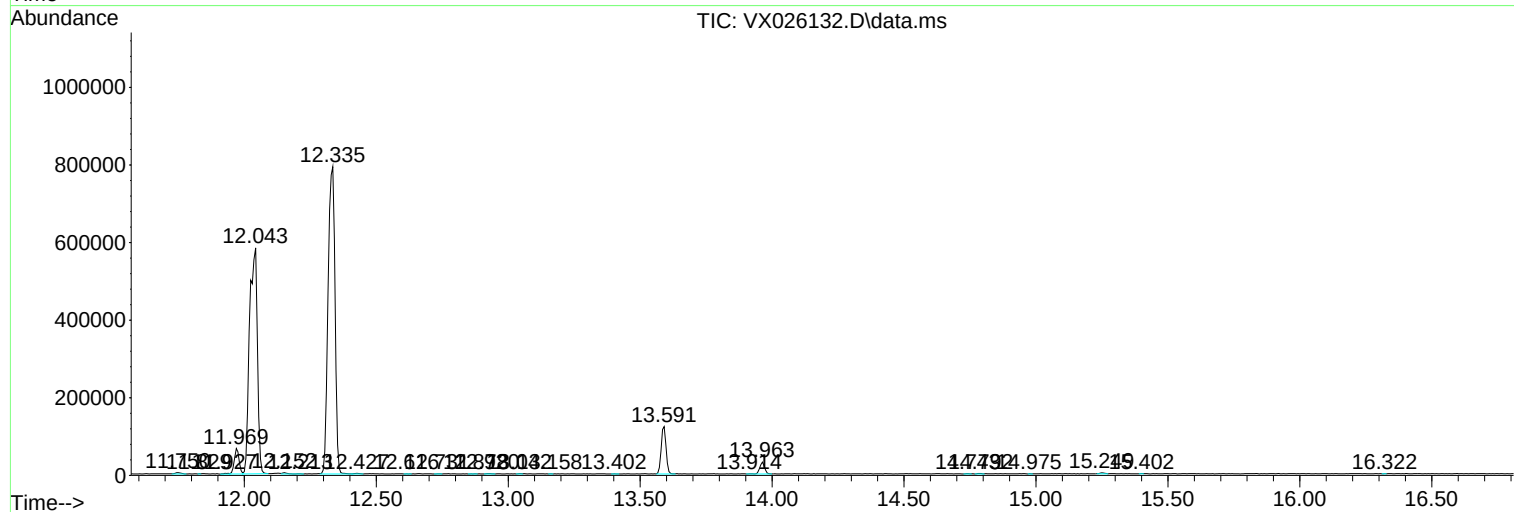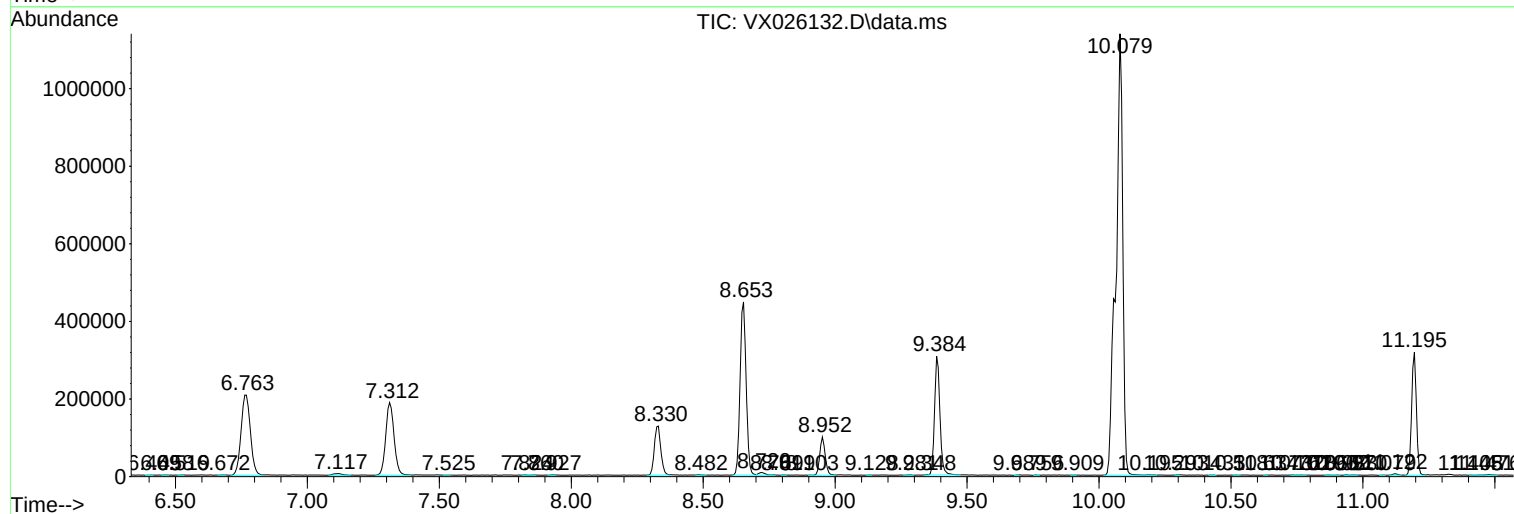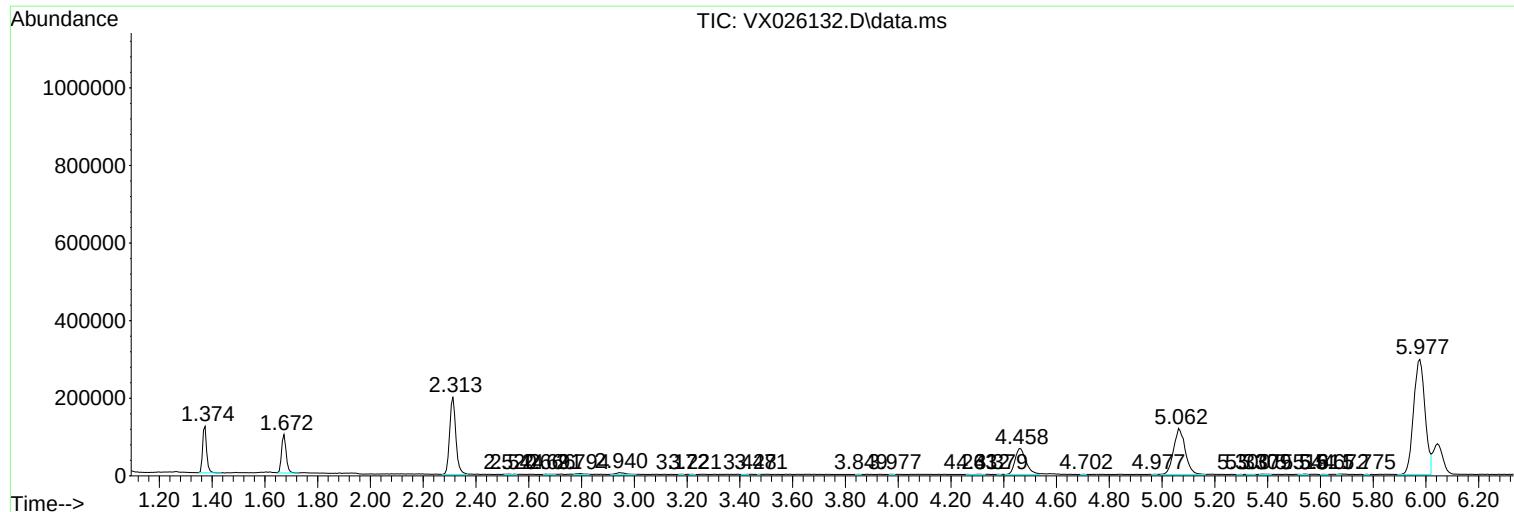

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026132.D
Acq On : 29 Dec 2021 12:38
Operator : JC/MD
Sample : M5216-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026132.D
Acq On : 29 Dec 2021 12:38
Operator : JC/MD
Sample : M5216-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COHB5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc