

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026139.D
 Acq On : 29 Dec 2021 15:20
 Operator : JC/MD
 Sample : VIBLK623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

Signal : TIC: VX026139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	53	rVB	113508	119486	14.93%	1.964%
2	1.672	92	96	104	rVB	90860	112943	14.11%	1.856%
3	2.246	188	190	194	rVB	537	543	0.07%	0.009%
4	2.313	194	201	211	rBV	190694	299452	37.42%	4.922%
5	2.569	239	243	244	rVB	730	733	0.09%	0.012%
6	2.593	244	247	250	rBV	557	720	0.09%	0.012%
7	2.697	261	264	265	rBV2	609	714	0.09%	0.012%
8	2.794	277	280	286	rVB3	2010	3295	0.41%	0.054%
9	2.873	291	293	298	rBV2	685	821	0.10%	0.013%
10	2.947	301	305	311	rVB5	2096	4494	0.56%	0.074%
11	3.069	322	325	326	rBV	605	590	0.07%	0.010%
12	3.087	326	328	332	rVV3	470	671	0.08%	0.011%
13	3.349	368	371	372	rBV	695	707	0.09%	0.012%
14	3.928	463	466	469	rVB	612	838	0.10%	0.014%
15	3.971	471	473	476	rVV	451	502	0.06%	0.008%
16	4.032	479	483	485	rBV	511	559	0.07%	0.009%
17	4.142	497	501	504	rBV	820	848	0.11%	0.014%
18	4.166	504	505	507	rVV	805	475	0.06%	0.008%
19	4.367	534	538	540	rBV	424	709	0.09%	0.012%
20	4.465	545	554	570	rBV	63177	183720	22.96%	3.020%
21	4.654	583	585	589	rBV2	1032	1536	0.19%	0.025%
22	4.824	609	613	615	rBV	428	576	0.07%	0.009%
23	4.904	625	626	629	rBV2	535	522	0.07%	0.009%
24	5.068	642	653	671	rVB	101289	324320	40.53%	5.331%
25	5.202	671	675	678	rBV	461	710	0.09%	0.012%
26	5.245	680	682	683	rBV2	789	542	0.07%	0.009%
27	5.312	689	693	697	rBV	1000	1520	0.19%	0.025%
28	5.379	702	704	706	rBV	540	692	0.09%	0.011%
29	5.751	763	765	767	rBV2	777	717	0.09%	0.012%
30	5.769	767	768	771	rVV	550	518	0.06%	0.009%
31	5.977	789	802	816	rBV2	269567	800296	100.00%	13.154%
32	6.147	829	830	833	rBV2	463	468	0.06%	0.008%
33	6.769	922	932	942	rBV	196122	461421	57.66%	7.584%
34	7.043	975	977	983	rVB	792	781	0.10%	0.013%
35	7.117	983	989	995	rBV4	3796	8649	1.08%	0.142%
36	7.202	1000	1003	1006	rBV	592	892	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026139.D
 Acq On : 29 Dec 2021 15:20
 Operator : JC/MD
 Sample : VIBLK623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1035	rBV	168392	364953	45.60%	5.999%
38	7.488	1046	1050	1052	rVV4	863	1353	0.17%	0.022%
39	7.562	1060	1062	1067	rVB2	606	561	0.07%	0.009%
40	7.598	1067	1068	1070	rBV	860	519	0.06%	0.009%
41	7.927	1120	1122	1126	rVV2	661	1028	0.13%	0.017%
42	8.123	1152	1154	1158	rVV2	582	828	0.10%	0.014%
43	8.183	1162	1164	1167	rBV	762	562	0.07%	0.009%
44	8.330	1181	1188	1199	rVB	114647	187179	23.39%	3.077%
45	8.592	1229	1231	1234	rVB2	569	555	0.07%	0.009%
46	8.653	1234	1241	1248	rBV	407742	649078	81.10%	10.669%
47	8.720	1250	1252	1260	rVB3	5796	9239	1.15%	0.152%
48	8.818	1266	1268	1271	rBV2	479	553	0.07%	0.009%
49	8.848	1271	1273	1279	rVB2	725	1211	0.15%	0.020%
50	8.897	1279	1281	1283	rBV	710	722	0.09%	0.012%
51	8.952	1285	1290	1296	rBV	88937	126390	15.79%	2.077%
52	9.049	1304	1306	1307	rVB	930	570	0.07%	0.009%
53	9.074	1307	1310	1312	rBV2	1007	924	0.12%	0.015%
54	9.122	1315	1318	1319	rBV2	690	782	0.10%	0.013%
55	9.159	1322	1324	1326	rBV2	496	519	0.06%	0.009%
56	9.281	1340	1344	1345	rBV	826	732	0.09%	0.012%
57	9.384	1356	1361	1373	rVB	280748	405156	50.63%	6.659%
58	9.586	1392	1394	1395	rBV	700	568	0.07%	0.009%
59	9.641	1402	1403	1406	rBV2	590	537	0.07%	0.009%
60	9.701	1409	1413	1415	rBV2	941	1489	0.19%	0.024%
61	9.756	1421	1422	1425	rBV	619	540	0.07%	0.009%
62	9.823	1431	1433	1437	rVB	714	723	0.09%	0.012%
63	9.933	1450	1451	1454	rVB	600	534	0.07%	0.009%
64	10.055	1465	1471	1484	rBV	399980	528573	66.05%	8.688%
65	10.311	1508	1513	1516	rVB4	1262	2111	0.26%	0.035%
66	10.403	1527	1528	1530	rBV2	646	559	0.07%	0.009%
67	10.445	1533	1535	1539	rVV	688	777	0.10%	0.013%
68	10.500	1539	1544	1545	rVV	573	761	0.10%	0.013%
69	10.579	1555	1557	1560	rVB	424	467	0.06%	0.008%
70	10.610	1560	1562	1564	rBV	677	551	0.07%	0.009%
71	10.878	1605	1606	1610	rVB	594	612	0.08%	0.010%
72	11.122	1643	1646	1650	rVB3	3144	4171	0.52%	0.069%
73	11.195	1652	1658	1665	rBV	283715	362602	45.31%	5.960%
74	11.250	1665	1667	1669	rBV2	705	554	0.07%	0.009%
75	11.280	1670	1672	1675	rVV2	877	582	0.07%	0.010%
76	11.427	1694	1696	1697	rBV	606	538	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
 Data File : VX026139.D
 Acq On : 29 Dec 2021 15:20
 Operator : JC/MD
 Sample : VIBLK623
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK623

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
 Title : VOC Analysis

77	11.549	1714	1716	1718	rBV2	786	822	0.10%	0.014%
78	11.573	1718	1720	1721	rVV	903	604	0.08%	0.010%
79	11.658	1733	1734	1737	rBV	727	771	0.10%	0.013%
80	11.750	1745	1749	1753	rVV4	2976	4642	0.58%	0.076%
81	11.835	1761	1763	1764	rVV	749	536	0.07%	0.009%
82	11.933	1777	1779	1783	rVB2	1670	1703	0.21%	0.028%
83	12.024	1789	1794	1800	rBV	410382	501326	62.64%	8.240%
84	12.262	1831	1833	1835	rBV	907	700	0.09%	0.012%
85	12.323	1837	1843	1850	rVV	444705	555365	69.39%	9.128%
86	12.658	1896	1898	1899	rBV	694	550	0.07%	0.009%
87	12.774	1913	1917	1919	rVB2	899	1132	0.14%	0.019%
88	12.799	1919	1921	1923	rBV	706	612	0.08%	0.010%
89	12.981	1950	1951	1953	rBV	761	638	0.08%	0.010%
90	13.292	2001	2002	2005	rBV	654	628	0.08%	0.010%
91	13.780	2079	2082	2086	rVB3	906	1113	0.14%	0.018%
92	14.006	2115	2119	2121	rBV	811	802	0.10%	0.013%
93	14.158	2142	2144	2146	rBV	668	710	0.09%	0.012%
94	14.579	2210	2213	2214	rBV	623	536	0.07%	0.009%
95	14.597	2214	2216	2219	rBV2	517	581	0.07%	0.010%
96	14.640	2219	2223	2230	rVV2	6000	6998	0.87%	0.115%
97	14.786	2243	2247	2250	rBV	1881	2434	0.30%	0.040%
98	15.201	2313	2315	2318	rBV3	769	1008	0.13%	0.017%
99	15.304	2330	2332	2335	rBV	897	1273	0.16%	0.021%
100	16.578	2538	2541	2542	rBV2	940	797	0.10%	0.013%




Sum of corrected areas: 6083924

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026139.D
Acq On : 29 Dec 2021 15:20
Operator : JC/MD
Sample : VIBLK623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

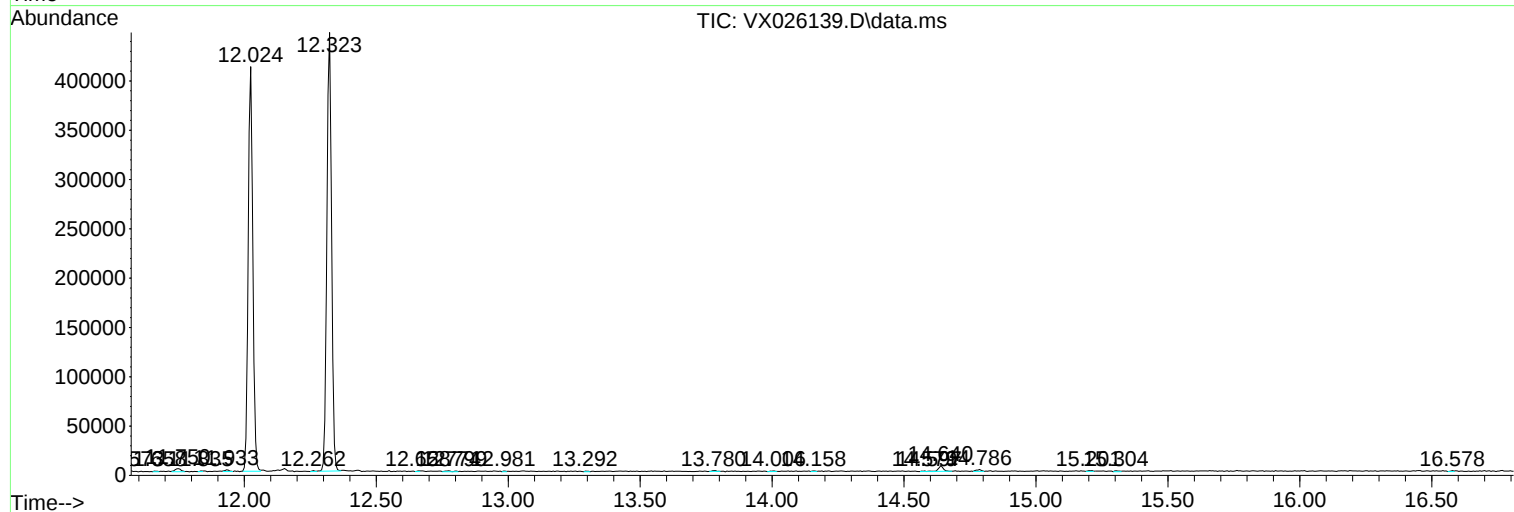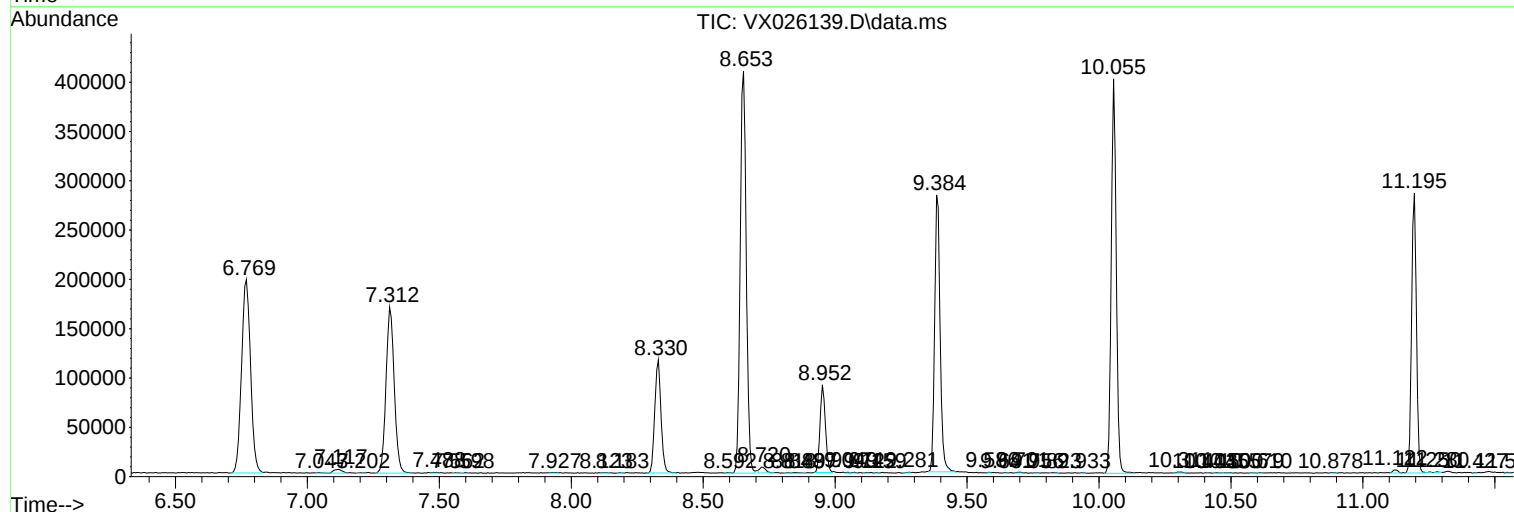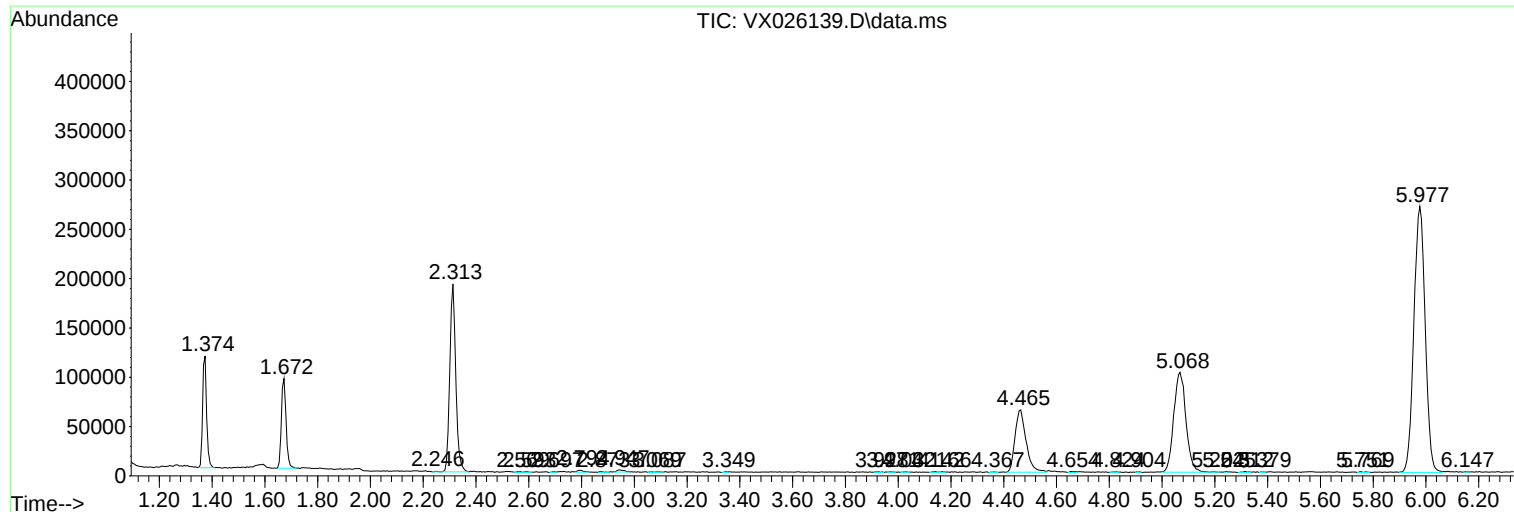

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026139.D
Acq On : 29 Dec 2021 15:20
Operator : JC/MD
Sample : VIBLK623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026139.D
Acq On : 29 Dec 2021 15:20
Operator : JC/MD
Sample : VIBLK623
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML122821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc