
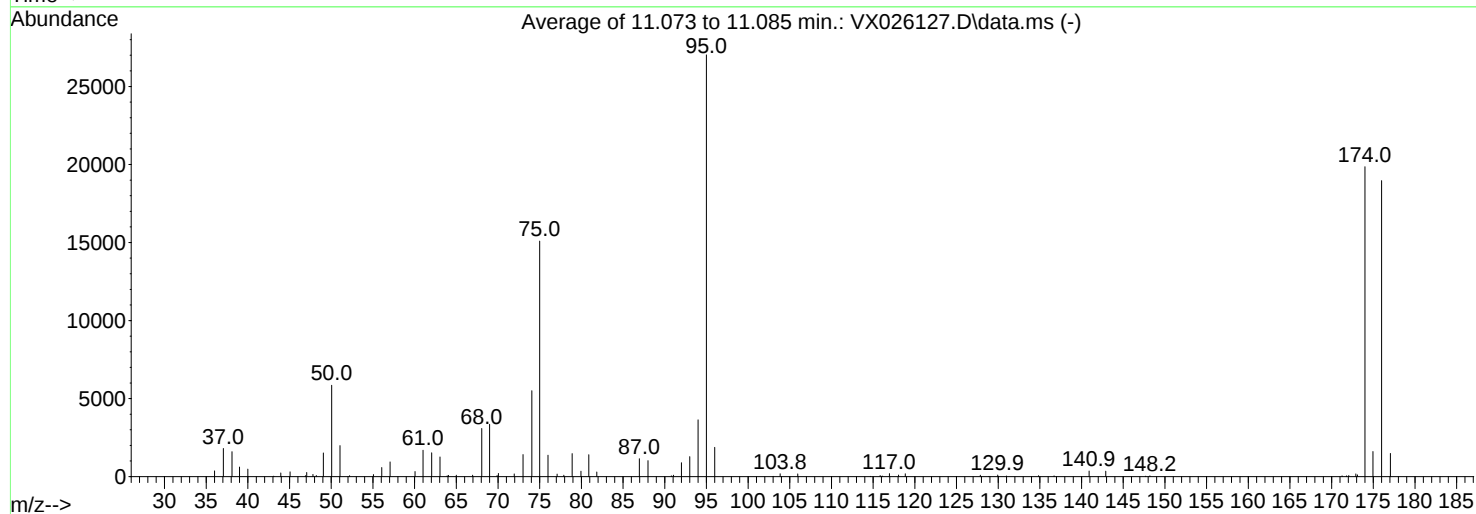


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122921\
Data File : VX026127.D
Acq On : 29 Dec 2021 09:21
Operator : JC/MD
Sample : BFB633
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB633

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM122821WMA.M
Title : VOC Analysis
Last Update : Thu Dec 30 02:39:24 2021

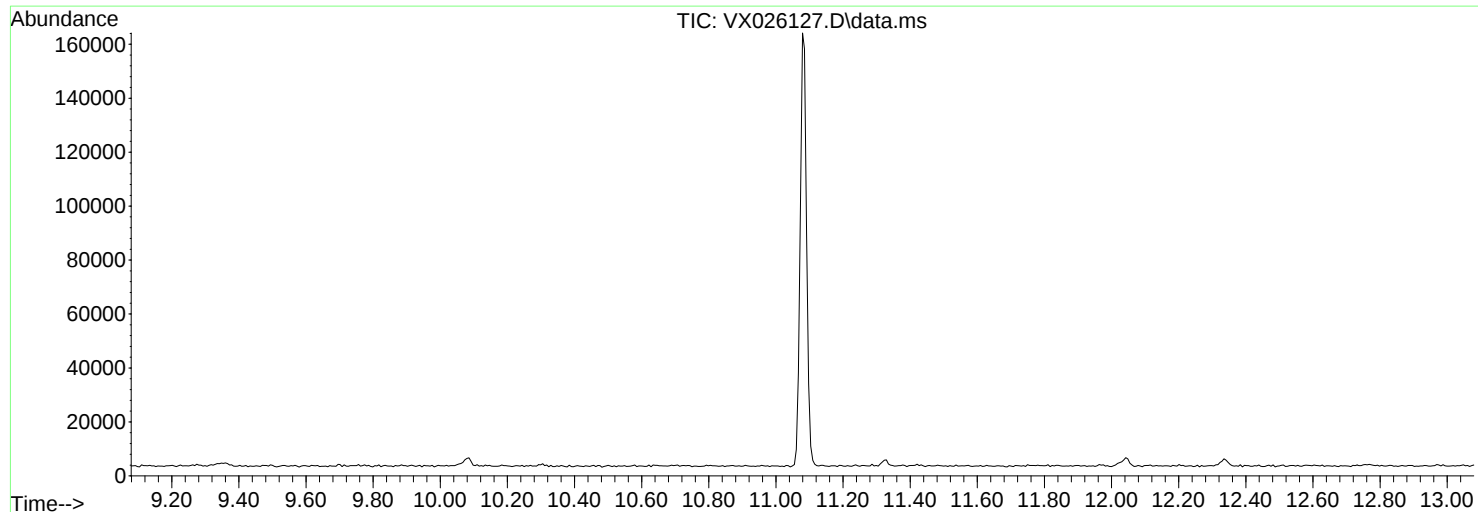

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	5856	PASS
75	95	30	80	55.8	15093	PASS
95	95	100	100	100.0	27027	PASS
96	95	5	9	6.9	1875	PASS
173	174	0.00	2	0.9	179	PASS
174	95	50	120	73.5	19862	PASS
175	174	5	9	8.1	1606	PASS
176	174	95	101	95.5	18964	PASS
177	176	5	9	7.9	1492	PASS

m/z	Abundance
40.00	3083.0
43.90	231.0

Instrument :
MSVOA_X
ClientSampleId :
BFB633

m/z	Abundance
36.00	329.0
37.10	1647.0
38.10	1221.0
39.00	461.0
40.00	3509.0
44.00	430.0
45.10	257.0
46.90	181.0
48.20	204.0
49.10	1189.0
50.00	5001.0
51.10	1529.0
52.20	64.0
55.10	81.0
56.10	458.0
57.00	714.0
60.00	302.0
61.00	1320.0
62.00	1148.0
63.00	947.0
63.90	163.0
65.00	117.0
68.00	2541.0
69.00	2687.0
69.90	207.0
72.00	108.0
73.00	1162.0
74.00	4199.0
75.00	11623.0
76.00	1139.0
77.10	160.0
78.00	69.0
78.90	1048.0
80.00	261.0
80.90	903.0
81.80	172.0
86.90	884.0
88.00	767.0
91.10	86.0
92.00	608.0
93.00	979.0
94.00	2682.0
95.00	19384.0
96.00	1519.0
103.90	119.0
106.00	143.0
115.90	103.0
117.10	103.0
118.10	74.0
118.80	127.0
127.90	80.0
128.90	55.0
131.00	60.0
134.90	82.0
141.00	278.0
142.90	259.0
171.30	52.0
172.10	104.0
172.90	162.0
174.00	11697.0
174.90	1082.0
176.00	11060.0
177.10	836.0

Instrument :
MSVOA_X
ClientSampleId :
BFB633

m/z	Abundance
36.00	438.0
37.10	2003.0
38.10	2036.0
39.00	646.0
40.00	3269.0
43.10	77.0
44.00	469.0
45.00	271.0
47.10	484.0
47.90	253.0
49.00	1786.0
50.00	6802.0
51.00	2364.0
52.20	62.0
55.10	197.0
55.90	617.0
57.10	1121.0
60.10	347.0
61.00	1971.0
62.00	1757.0
63.00	1428.0
64.10	134.0
65.00	97.0
66.90	189.0
68.00	3623.0
69.00	3792.0
70.10	361.0
71.90	247.0
73.00	1623.0
74.10	6386.0
75.00	17752.0
76.00	1777.0
77.10	190.0
77.90	129.0
78.90	1744.0
79.90	409.0
80.90	1979.0
81.90	398.0
87.00	1420.0
88.00	1278.0
91.00	187.0
92.00	1107.0
93.00	1532.0
94.00	4163.0
95.00	31704.0
96.00	2176.0
103.80	172.0
105.90	240.0
116.10	129.0
116.90	267.0
118.00	118.0
118.90	222.0
127.90	109.0
129.90	186.0
134.80	107.0
136.70	74.0
140.90	373.0
142.90	317.0
148.20	78.0
171.20	100.0
171.80	146.0
173.10	327.0
174.00	22752.0
175.00	1841.0
176.00	21968.0
177.00	1852.0

Instrument :
MSVOA_X
ClientSampleId :
BFB633

m/z	Abundance
36.00	356.0
37.00	1775.0
38.10	1527.0
39.00	745.0
40.00	3913.0
44.00	506.0
45.00	402.0
47.00	316.0
47.70	190.0
49.10	1567.0
50.10	5766.0
51.10	2068.0
52.20	73.0
54.90	118.0
56.10	668.0
57.00	1007.0
60.00	349.0
61.00	1791.0
62.10	1684.0
63.10	1412.0
64.00	117.0
64.90	61.0
67.00	85.0
68.10	3100.0
69.00	3569.0
70.00	257.0
71.90	165.0
73.00	1449.0
74.00	5945.0
75.00	15905.0
76.00	1199.0
77.10	147.0
77.80	87.0
78.90	1650.0
80.00	373.0
80.90	1320.0
81.90	334.0
86.90	1134.0
88.00	1033.0
90.80	146.0
92.00	965.0
93.00	1320.0
94.00	4067.0
95.00	29992.0
96.00	1931.0
103.00	53.0
103.80	264.0
105.90	132.0
114.70	58.0
115.80	126.0
117.00	221.0
118.00	106.0
118.90	216.0
127.80	92.0
130.00	132.0
131.00	59.0
136.70	74.0
140.80	429.0
142.90	472.0
147.70	77.0
148.20	62.0
172.00	102.0
172.90	375.0
174.00	25136.0
175.00	1894.0
176.00	23864.0
177.00	1789.0

Instrument :
MSVOA_X
ClientSampleId :
BFB633