

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122923\
 Data File : VX039535.D
 Acq On : 29 Dec 2023 11:19
 Operator : JC/MD
 Sample : 06017-06
 Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB32-1-20231222-10.0-11.0

Quant Time: Dec 30 01:55:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	83560	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	171492	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	165638	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	71957	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	70115	45.804	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	91.600%		
35) Dibromofluoromethane	5.385	113	52600	44.398	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.800%		
50) Toluene-d8	8.647	98	214729	48.820	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.640%		
62) 4-Bromofluorobenzene	11.085	95	85391	47.053	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	94.100%		
Target Compounds						Qvalue
5) Bromomethane	1.599	94	365	0.524	ug/l #	69
10) Methyl Iodide	2.422	142	306	0.274	ug/l #	53
11) Tert butyl alcohol	2.947	59	2195	5.710	ug/l #	78
16) Acetone	2.361	43	131	Below Cal	#	47
17) Carbon Disulfide	2.483	76	703	0.224	ug/l #	76
20) Methylene Chloride	2.782	84	1357	1.063	ug/l	97
25) 2-Butanone	4.654	43	383	0.290	ug/l #	51
29) Tetrahydrofuran	5.087	42	568	0.779	ug/l #	65
31) Cyclohexane	5.489	56	1551	0.784	ug/l #	56
36) 1,1-Dichloropropene	5.538	75	8079	4.321	ug/l #	51
38) Carbon Tetrachloride	5.544	117	9359	5.246	ug/l #	14
39) Methylcyclohexane	7.367	83	2754	1.226	ug/l	92
48) Methyl methacrylate	7.647	41	920	0.419	ug/l	89
51) 4-Methyl-2-Pentanone	8.604	43	2455	1.026	ug/l #	77
55) 1,1,2-Trichloroethane	9.092	97	2266	1.700	ug/l #	19
56) Ethyl methacrylate	9.098	69	751	0.462	ug/l #	1
59) 2-Hexanone	9.385	43	3336	1.615	ug/l #	27
73) Isopropylbenzene	10.970	105	1948	0.351	ug/l	87
74) N-amyl acetate	10.854	43	1298	0.462	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.195	83	556	0.269	ug/l #	91
76) 1,2,3-Trichloropropane	11.079	75	46687	25.078	ug/l #	39
78) n-propylbenzene	11.305	91	6314	0.923	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	46687	70.746	ug/l #	6
85) sec-Butylbenzene	11.890	105	2292	0.400	ug/l	89
89) n-Butylbenzene	12.335	91	4330	0.916	ug/l	89
90) Hexachloroethane	12.616	117	1641	1.890	ug/l #	17
93) 1,2,4-Trichlorobenzene	13.585	180	424	0.281	ug/l #	24
95) Naphthalene	13.780	128	2488	0.473	ug/l #	96
96) 1,2,3-Trichlorobenzene	13.963	180	329	0.226	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122923\
Data File : VX039535.D
Acq On : 29 Dec 2023 11:19
Operator : JC/MD
Sample : 06017-06
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0

Quant Time: Dec 30 01:55:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration

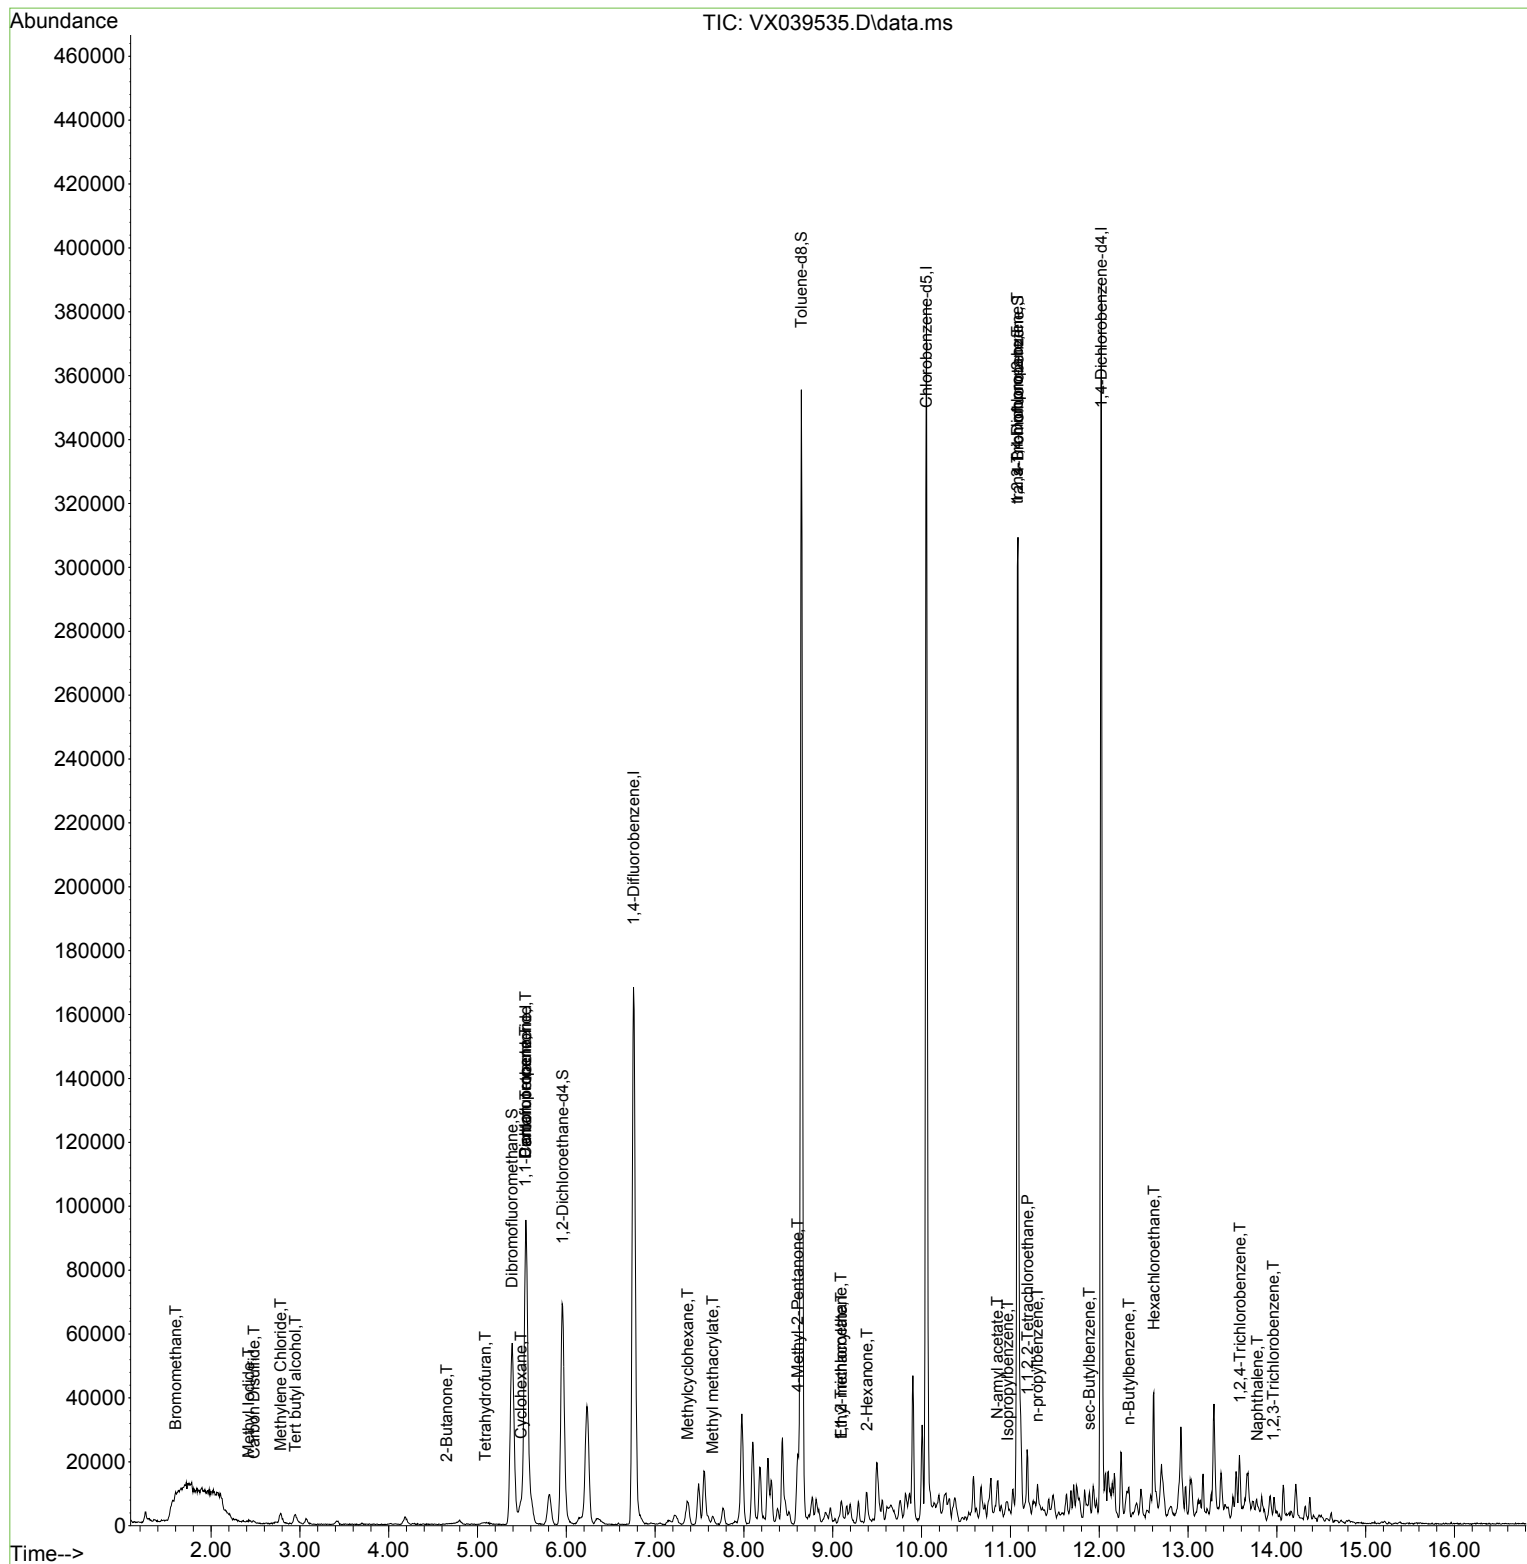



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.544 min Scan# 71

Delta R.T. -0.006 min

Lab File: VX039535.D

Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :





SB32-1-20231222-10.0-11.0

Tgt Ion:168 Resp: 83560

Ion Ratio Lower Upper

168 100

99 65.7 56.6 85.0

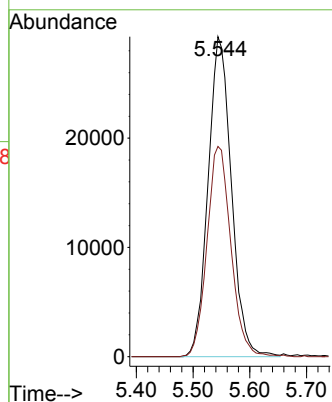

#5

Bromomethane

Concen: 0.524 ug/l

RT: 1.599 min Scan# 84

Delta R.T. 0.000 min

Lab File: VX039535.D




Acq: 29 Dec 2023 11:19


Tgt Ion: 94 Resp: 365

Ion Ratio Lower Upper

94 100


96 63.7 74.6 111.8#

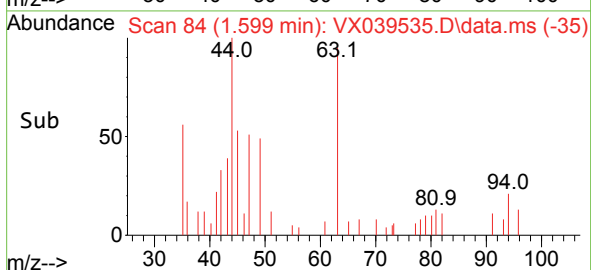






#10
Methyl Iodide
Concen: 0.274 ug/l
RT: 2.422 min Scan# 21
Delta R.T. -0.030 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0



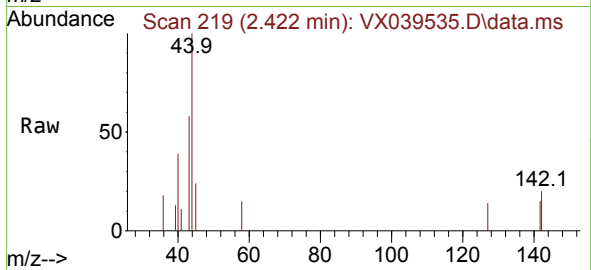



Tgt Ion:142 Resp: 306
Ion Ratio Lower Upper
142 100
127 16.7 41.6 62.4#
141 0.0 11.6 17.4#

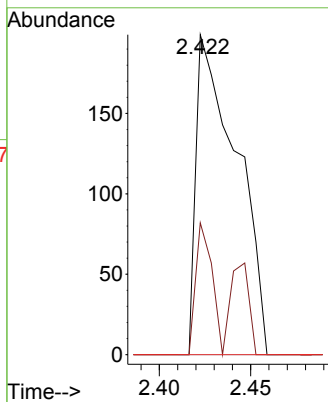

#11
Tert butyl alcohol
Concen: 5.710 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.006 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 59 Resp: 2195
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#


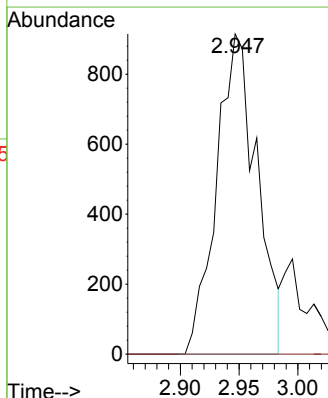




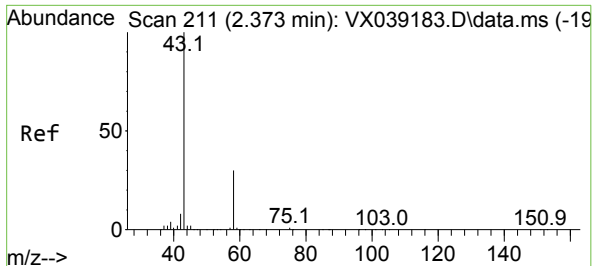

#16
Acetone
Concen: Below Cal
RT: 2.361 min Scan# 209
Delta R.T. -0.012 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion: 43 Resp: 131
Ion Ratio Lower Upper
43 100
58 0.0 21.9 32.9#

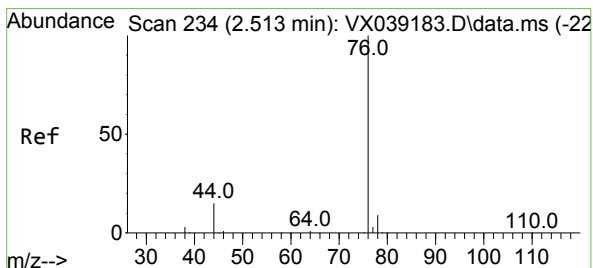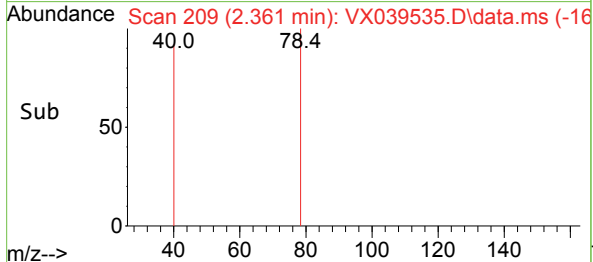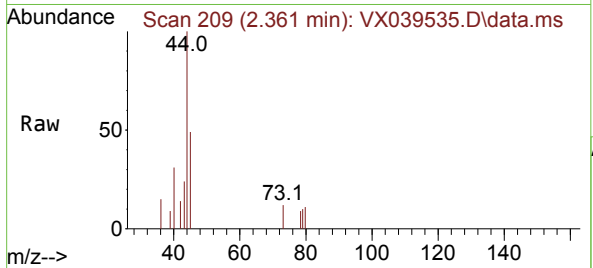

#17
Carbon Disulfide
Concen: 0.224 ug/l
RT: 2.483 min Scan# 229
Delta R.T. -0.030 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19


Tgt Ion: 76 Resp: 703
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#

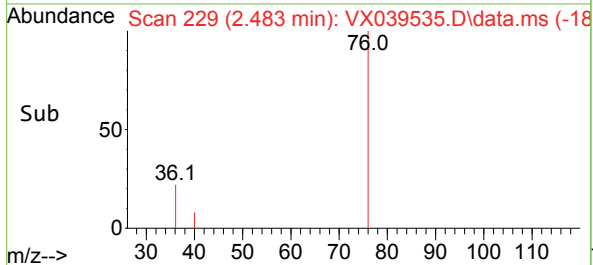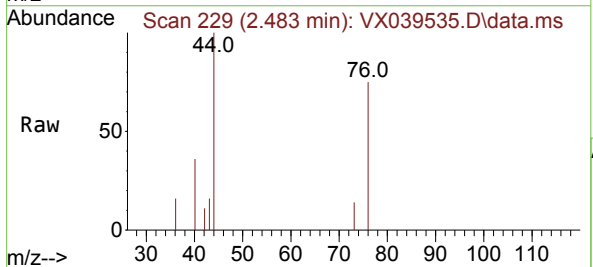






#20
Methylene Chloride
Concen: 1.063 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0







Tgt Ion: 84	Resp: 1357
Ion Ratio	Lower Upper
84 100	
49 130.8	103.6 155.4
51 39.0	33.8 50.6
86 56.2	49.4 74.0



#25
2-Butanone
Concen: 0.290 ug/l
RT: 4.654 min Scan# 585
Delta R.T. 0.104 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 43	Resp: 383		
Ion Ratio	Lower	Upper	
43 100			
72 0.0	19.4	29.2#	

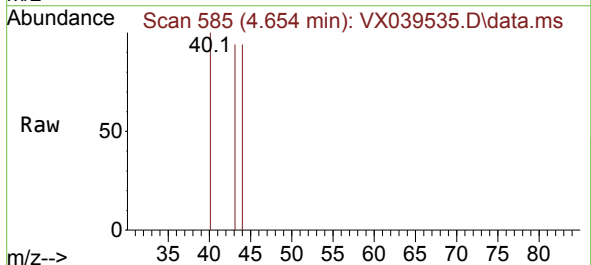

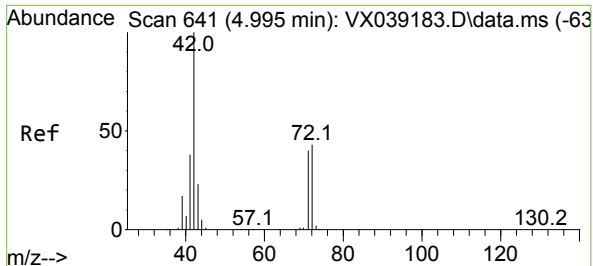

#29

Tetrahydrofuran

Concen: 0.779 ug/l

RT: 5.087 min Scan# 61

Delta R.T. 0.092 min

Lab File: VX039535.D


Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :

SB32-1-20231222-10.0-11.0

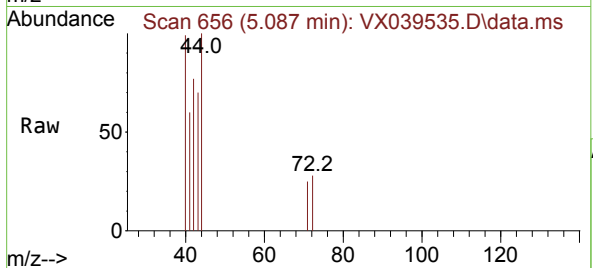




Tgt Ion: 42 Resp: 568

Ion Ratio Lower Upper

42 100

72 29.4 34.2 51.4#

71 9.5 32.2 48.2#

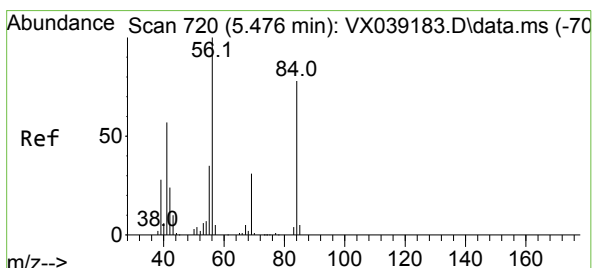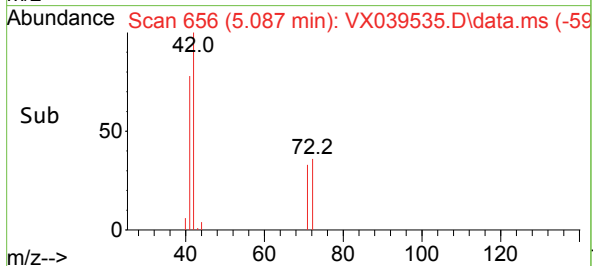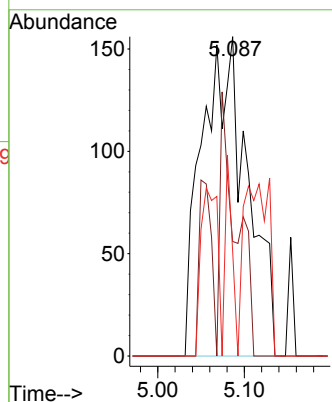

#31

Cyclohexane

Concen: 0.784 ug/l

RT: 5.489 min Scan# 722

Delta R.T. 0.013 min

Lab File: VX039535.D

Acq: 29 Dec 2023 11:19




Tgt Ion: 56 Resp: 1551


Ion Ratio Lower Upper

56 100

69 12.7 23.4 35.2#

84 38.4 65.9 98.9#


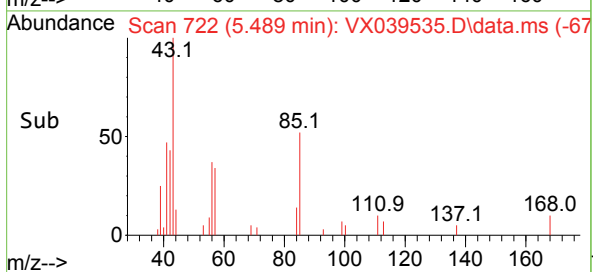
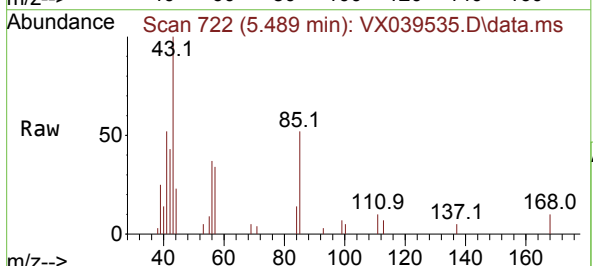
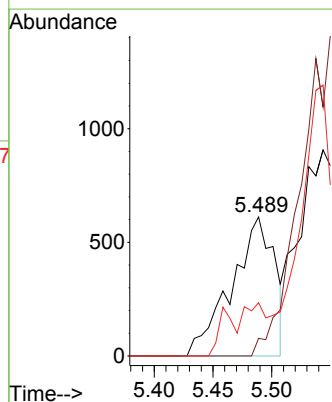




#33
 1,2-Dichloroethane-d4
 Concen: 45.804 ug/l
 RT: 5.958 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX039535.D
 Acq: 29 Dec 2023 11:19




Instrument :
 MSVOA_X
 ClientSampleId :
 SB32-1-20231222-10.0-11.0


Tgt Ion: 65 Resp: 70115
 Ion Ratio Lower Upper
 65 100
 67 52.6 0.0 100.2

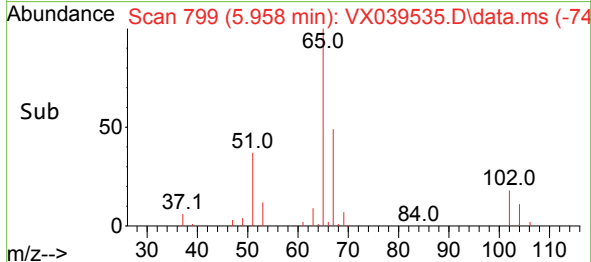

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. -0.006 min
 Lab File: VX039535.D
 Acq: 29 Dec 2023 11:19


Tgt Ion: 114 Resp: 171492
 Ion Ratio Lower Upper
 114 100
 63 23.6 0.0 45.0
 88 16.5 0.0 36.6

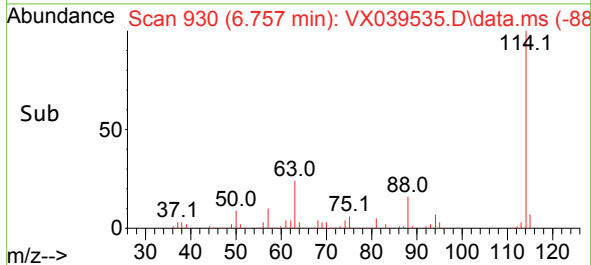






#35
Dibromofluoromethane
Concen: 44.398 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0







Tgt Ion:113 Resp: 52600
Ion Ratio Lower Upper
113 100
111 102.5 82.9 124.3
192 15.9 13.3 19.9



#36
1,1-Dichloropropene
Concen: 4.321 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.152 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19


Tgt Ion: 75 Resp: 8079
Ion Ratio Lower Upper
75 100
110 9.7 17.0 50.9#
77 0.0 24.7 37.1#

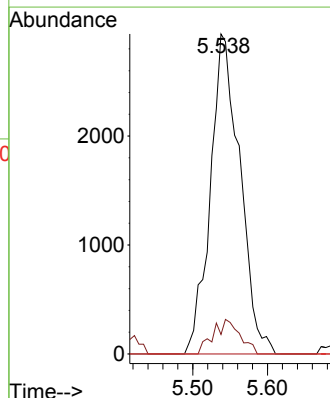






#38
Carbon Tetrachloride
Concen: 5.246 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0



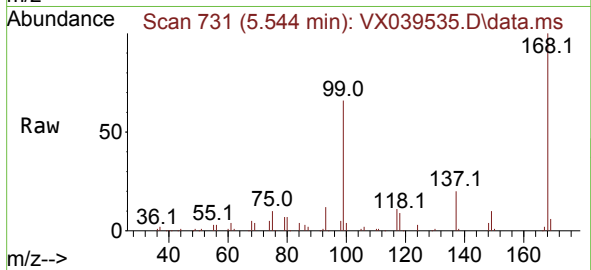



Tgt Ion:117 Resp: 9359
Ion Ratio Lower Upper
117 100
119 3.2 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 1.226 ug/l
RT: 7.367 min Scan# 1030
Delta R.T. -0.012 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 83 Resp: 2754
Ion Ratio Lower Upper
83 100
55 86.8 64.6 97.0
98 38.7 36.7 55.1

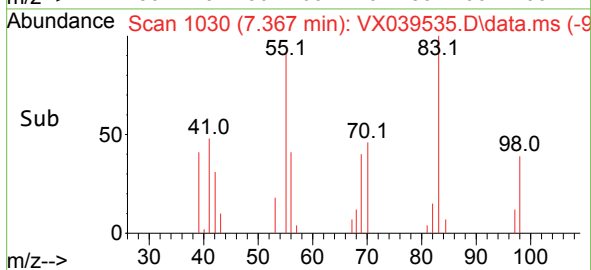



#48

Methyl methacrylate

Concen: 0.419 ug/l

RT: 7.647 min Scan# 1083

Delta R.T. -0.042 min

Lab File: VX039535.D

Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :

SB32-1-20231222-10.0-11.0





Tgt Ion: 41 Resp: 920

Ion Ratio Lower Upper

41 100

69 87.2 59.2 88.8

39 56.1 47.7 71.5



#50

Toluene-d8

Concen: 48.820 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX039535.D




Acq: 29 Dec 2023 11:19


Tgt Ion: 98 Resp: 214729

Ion Ratio Lower Upper

98 100

100 63.8 53.1 79.7


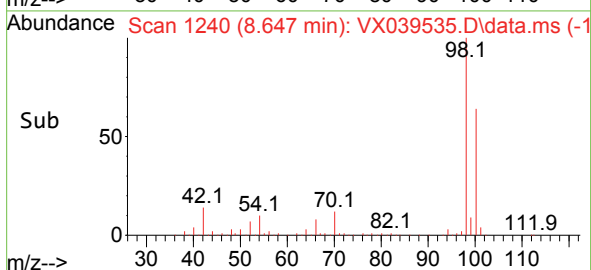






#51
4-Methyl-2-Pentanone
Concen: 1.026 ug/l
RT: 8.604 min Scan# 11
Delta R.T. 0.031 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion: 43 Resp: 2455
Ion Ratio Lower Upper
43 100
58 24.3 30.4 45.6#

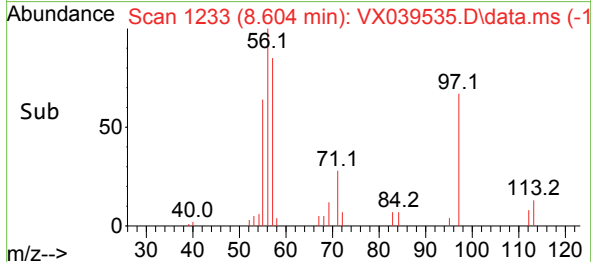

#55
1,1,2-Trichloroethane
Concen: 1.700 ug/l
RT: 9.092 min Scan# 1313
Delta R.T. -0.061 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 97 Resp: 2266
Ion Ratio Lower Upper
97 100
83 4.0 65.8 98.8#
85 0.0 41.6 62.4#
99 0.0 47.8 71.8#


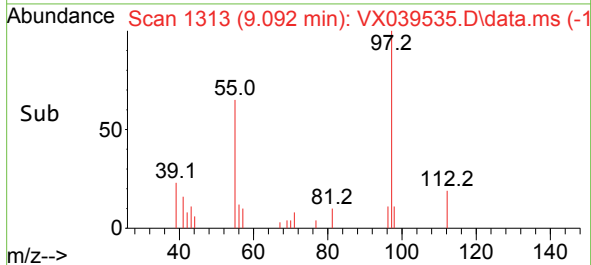






#56
Ethyl methacrylate
Concen: 0.462 ug/l
RT: 9.098 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion: 69 Resp: 751
Ion Ratio Lower Upper
69 100
41 161.1 56.8 85.2#
39 145.4 32.0 48.0#

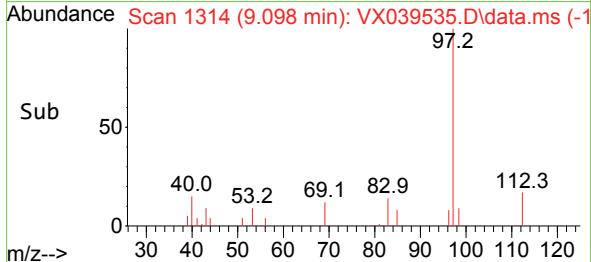

#59
2-Hexanone
Concen: 1.615 ug/l
RT: 9.385 min Scan# 1361
Delta R.T. -0.042 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 43 Resp: 3336
Ion Ratio Lower Upper
43 100
58 0.8 26.2 78.5#




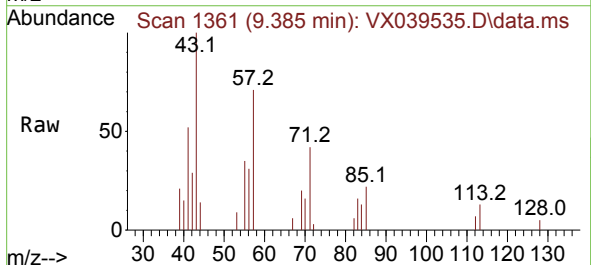




#62
4-Bromofluorobenzene
Concen: 47.053 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion: 95 Resp: 85391
Ion Ratio Lower Upper
95 100
174 64.0 0.0 135.6
176 62.1 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 117 Resp: 165638
Ion Ratio Lower Upper
117 100
82 59.7 46.2 69.4
119 31.7 25.5 38.3

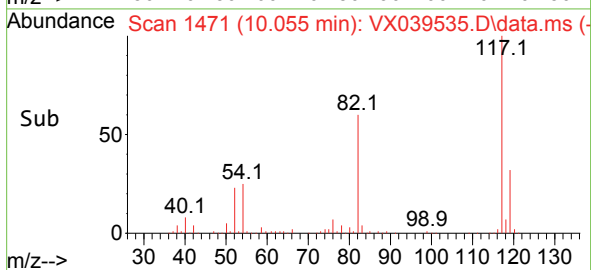



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX039535.D

Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :

SB32-1-20231222-10.0-11.0





Tgt Ion:152 Resp: 71957

Ion Ratio Lower Upper

152 100

115 68.0 43.3 129.9

150 156.4 0.0 345.0

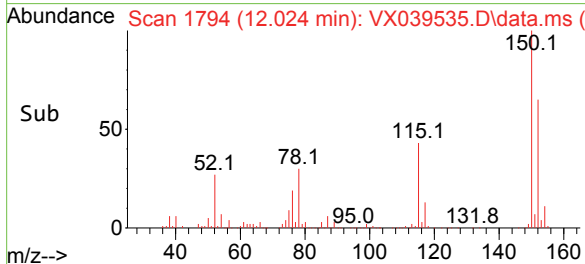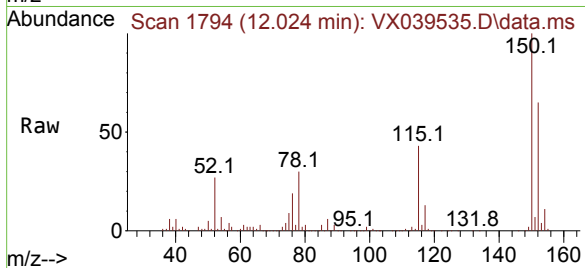

#73

Isopropylbenzene

Concen: 0.351 ug/l

RT: 10.970 min Scan# 1621

Delta R.T. 0.006 min

Lab File: VX039535.D




Acq: 29 Dec 2023 11:19


Tgt Ion:105 Resp: 1948

Ion Ratio Lower Upper

105 100

120 19.1 12.9 38.6


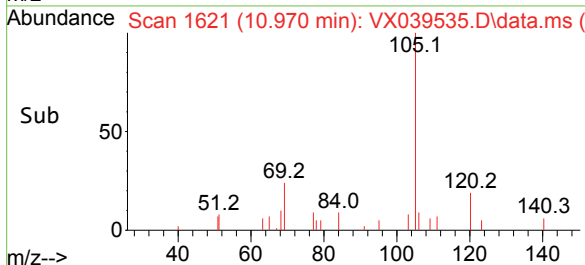
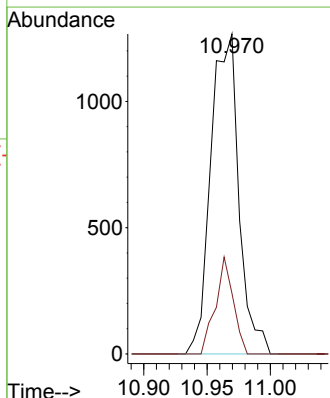
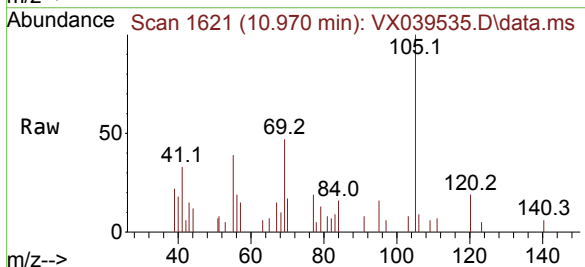




#74
N-amy1 acetate
Concen: 0.462 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.013 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion: 43	Resp: 1298
Ion Ratio	Lower Upper
43 100	
70 40.4	32.9 49.3
55 205.0	19.3 28.9#
61 0.0	18.8 28.2#

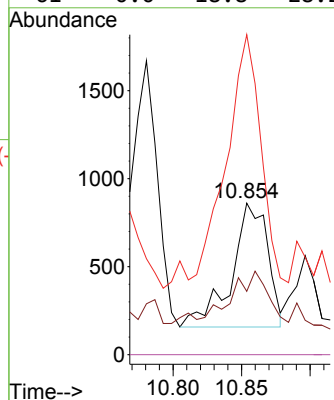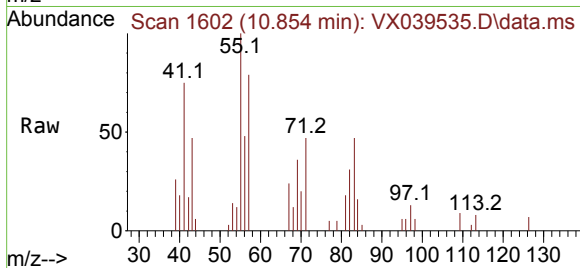

#75
1,1,2,2-Tetrachloroethane
Concen: 0.269 ug/l
RT: 11.195 min Scan# 1658
Delta R.T. -0.018 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 83	Resp: 556
Ion Ratio	Lower Upper
83 100	
131 0.0	5.3 15.8#
85 68.7	32.0 96.2

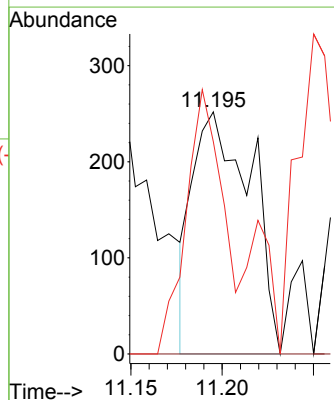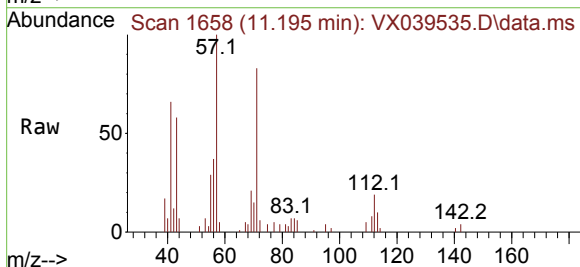



#76

1,2,3-Trichloropropane

Concen: 25.078 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX039535.D

Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :





SB32-1-20231222-10.0-11.0

Tgt Ion: 75 Resp: 46687

Ion Ratio Lower Upper

75 100

77 1.6 19.1 57.5#

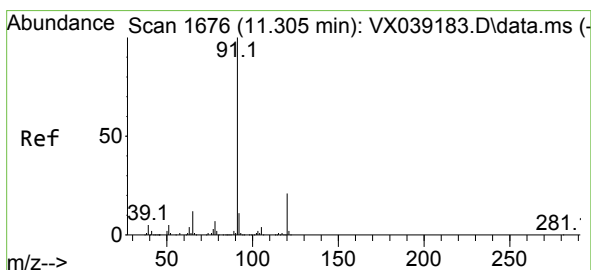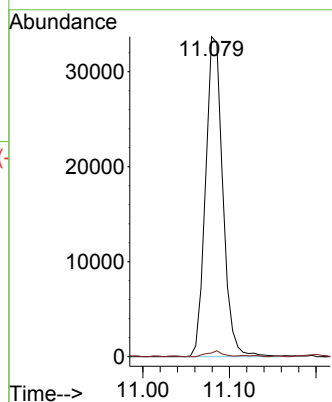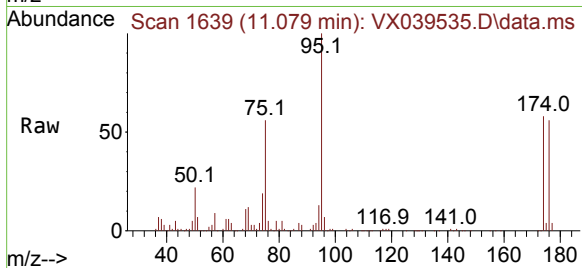

#78

n-propylbenzene

Concen: 0.923 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX039535.D




Acq: 29 Dec 2023 11:19


Tgt Ion: 91 Resp: 6314

Ion Ratio Lower Upper

91 100

120 19.3 11.5 34.4



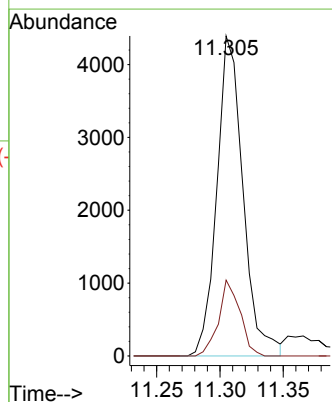
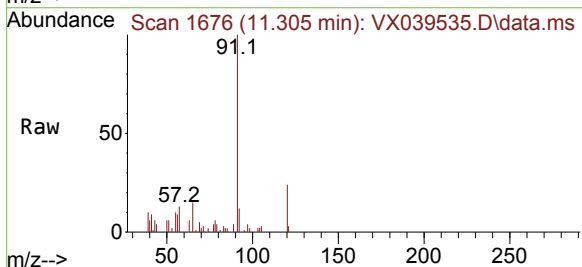




#81
trans-1,4-Dichloro-2-butene
Concen: 70.746 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion: 75 Resp: 46687
Ion Ratio Lower Upper
75 100
53 1.1 90.5 135.7#
89 0.0 36.9 55.3#

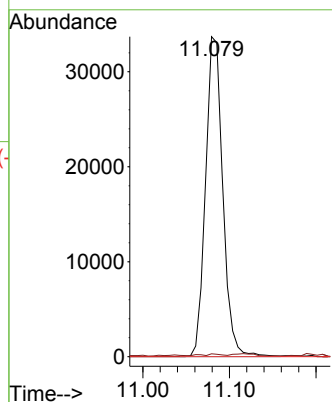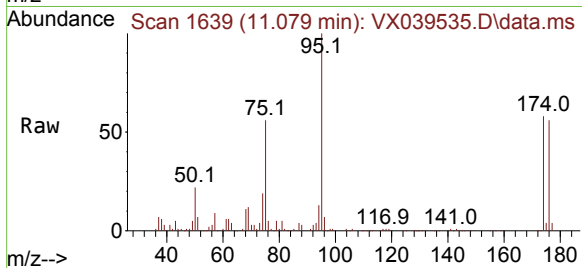

#85
sec-Butylbenzene
Concen: 0.400 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion: 105 Resp: 2292
Ion Ratio Lower Upper
105 100
134 14.6 9.8 29.4

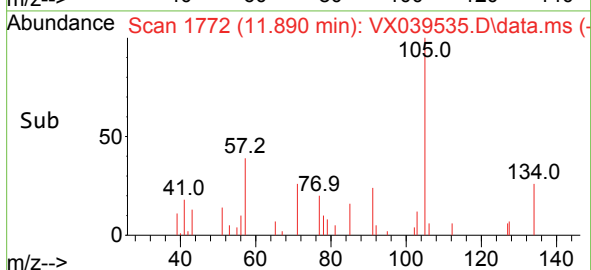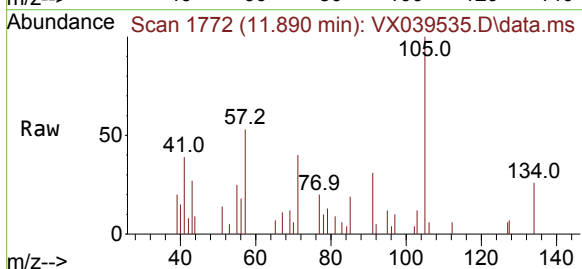



#89

n-Butylbenzene

Concen: 0.916 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.006 min

Lab File: VX039535.D

Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :

SB32-1-20231222-10.0-11.0





Tgt Ion: 91 Resp: 4330

Ion Ratio Lower Upper

91 100

92 48.7 27.4 82.0

134 34.2 12.6 37.8



#90

Hexachloroethane

Concen: 1.890 ug/l

RT: 12.616 min Scan# 1891

Delta R.T. 0.080 min

Lab File: VX039535.D




Acq: 29 Dec 2023 11:19


Tgt Ion:117 Resp: 1641

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#


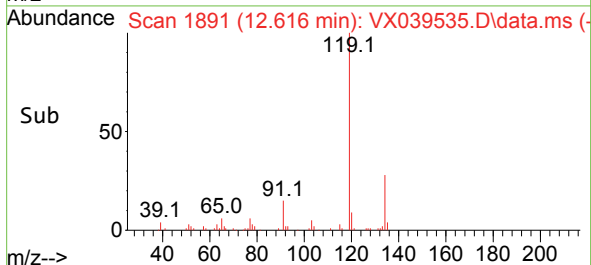






#93
1,2,4-Trichlorobenzene
Concen: 0.281 ug/l
RT: 13.585 min Scan# 2050
Delta R.T. 0.000 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19




Instrument :
MSVOA_X
ClientSampleId :
SB32-1-20231222-10.0-11.0


Tgt Ion:180 Resp: 424
Ion Ratio Lower Upper
180 100
182 78.3 48.3 144.8
145 170.8 18.0 54.0#

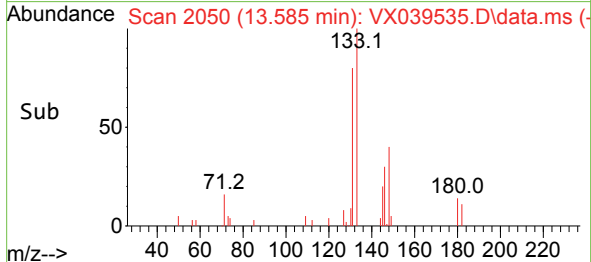

#95
Naphthalene
Concen: 0.473 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX039535.D
Acq: 29 Dec 2023 11:19

Tgt Ion:128 Resp: 2488
Ion Ratio Lower Upper
128 100
127 13.3 10.3 15.5
129 7.8 8.8 13.2#

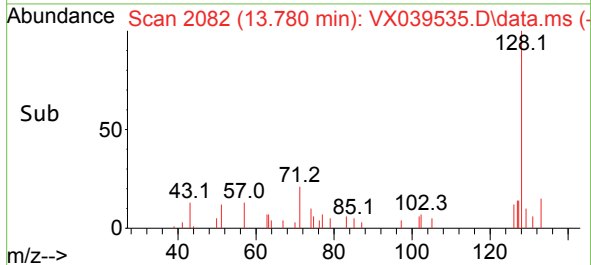



#96

1,2,3-Trichlorobenzene

Concen: 0.226 ug/l

RT: 13.963 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX039535.D


Acq: 29 Dec 2023 11:19

Instrument :

MSVOA_X

ClientSampleId :

SB32-1-20231222-10.0-11.0

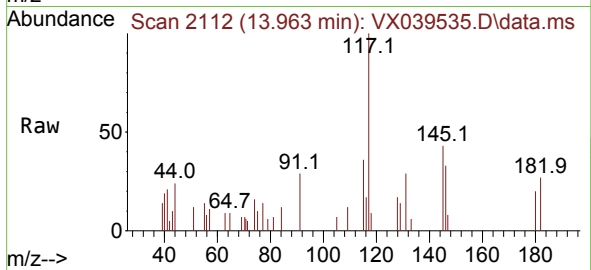

Tgt Ion:180 Resp: 329

Ion Ratio Lower Upper

180 100

182 99.4 46.9 140.6

145 256.5 17.8 53.5#

