

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122923\
 Data File : VX039547.D
 Acq On : 29 Dec 2023 15:54
 Operator : JC/MD
 Sample : 06038-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 T-703

Quant Time: Dec 30 02:03:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	87810	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	180475	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	179514	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	75396	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	78895	49.045	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.100%		
35) Dibromofluoromethane	5.385	113	58564	46.971	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	93.940%		
50) Toluene-d8	8.647	98	232501	50.229	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	100.460%		
62) 4-Bromofluorobenzene	11.079	95	94443	49.451	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.900%		
Target Compounds						Qvalue
5) Bromomethane	1.599	94	301	0.411	ug/l #	45
6) Chloroethane	1.666	64	356	0.464	ug/l #	43
11) Tert butyl alcohol	2.983	59	5640	13.962	ug/l	97
13) Acrolein	2.246	56	357	1.108	ug/l #	69
16) Acetone	2.380	43	27389	6.581	ug/l	94
18) Methyl Acetate	2.703	43	2560	0.736	ug/l	97
20) Methylene Chloride	2.788	84	6356	4.740	ug/l	98
25) 2-Butanone	4.568	43	17433	12.559	ug/l	97
29) Tetrahydrofuran	5.044	42	989	1.290	ug/l #	60
31) Cyclohexane	5.556	56	2643	1.272	ug/l #	21
36) 1,1-Dichloropropene	5.550	75	8690	4.417	ug/l #	50
37) Ethyl Acetate	4.733	43	3181	1.309	ug/l #	85
38) Carbon Tetrachloride	5.550	117	10087	5.372	ug/l #	15
40) Benzene	6.044	78	7406	1.331	ug/l	96
43) Isopropyl Acetate	6.342	43	114219	28.896	ug/l	99
48) Methyl methacrylate	7.598	41	4595	1.988	ug/l #	16
49) 1,4-Dioxane	7.799	88	111	3.563	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	84221	33.441	ug/l #	46
52) Toluene	8.714	92	939	0.280	ug/l	86
53) t-1,3-Dichloropropene	8.952	75	600	0.271	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	33172	13.948	ug/l #	62
57) 1,3-Dichloropropane	9.482	76	4322	1.783	ug/l #	42
59) 2-Hexanone	9.439	43	6327	2.911	ug/l	91
67) Ethyl Benzene	10.195	91	12579	1.725	ug/l	96
68) m/p-Xylenes	10.299	106	1686	0.645	ug/l	99
69) o-Xylene	10.647	106	734	0.290	ug/l	82
74) N-amyl acetate	10.854	43	3199	1.087	ug/l #	38
76) 1,2,3-Trichloropropane	11.079	75	53011	27.176	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	53011	76.664	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	3703	0.729	ug/l	82
85) sec-Butylbenzene	11.756	105	3703	0.617	ug/l #	57
90) Hexachloroethane	12.695	117	442	0.486	ug/l #	17
95) Naphthalene	13.774	128	129901	23.558	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
T-703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122923\
Data File : VX039547.D
Acq On : 29 Dec 2023 15:54
Operator : JC/MD
Sample : 06038-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T-703

Quant Time: Dec 30 02:03:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




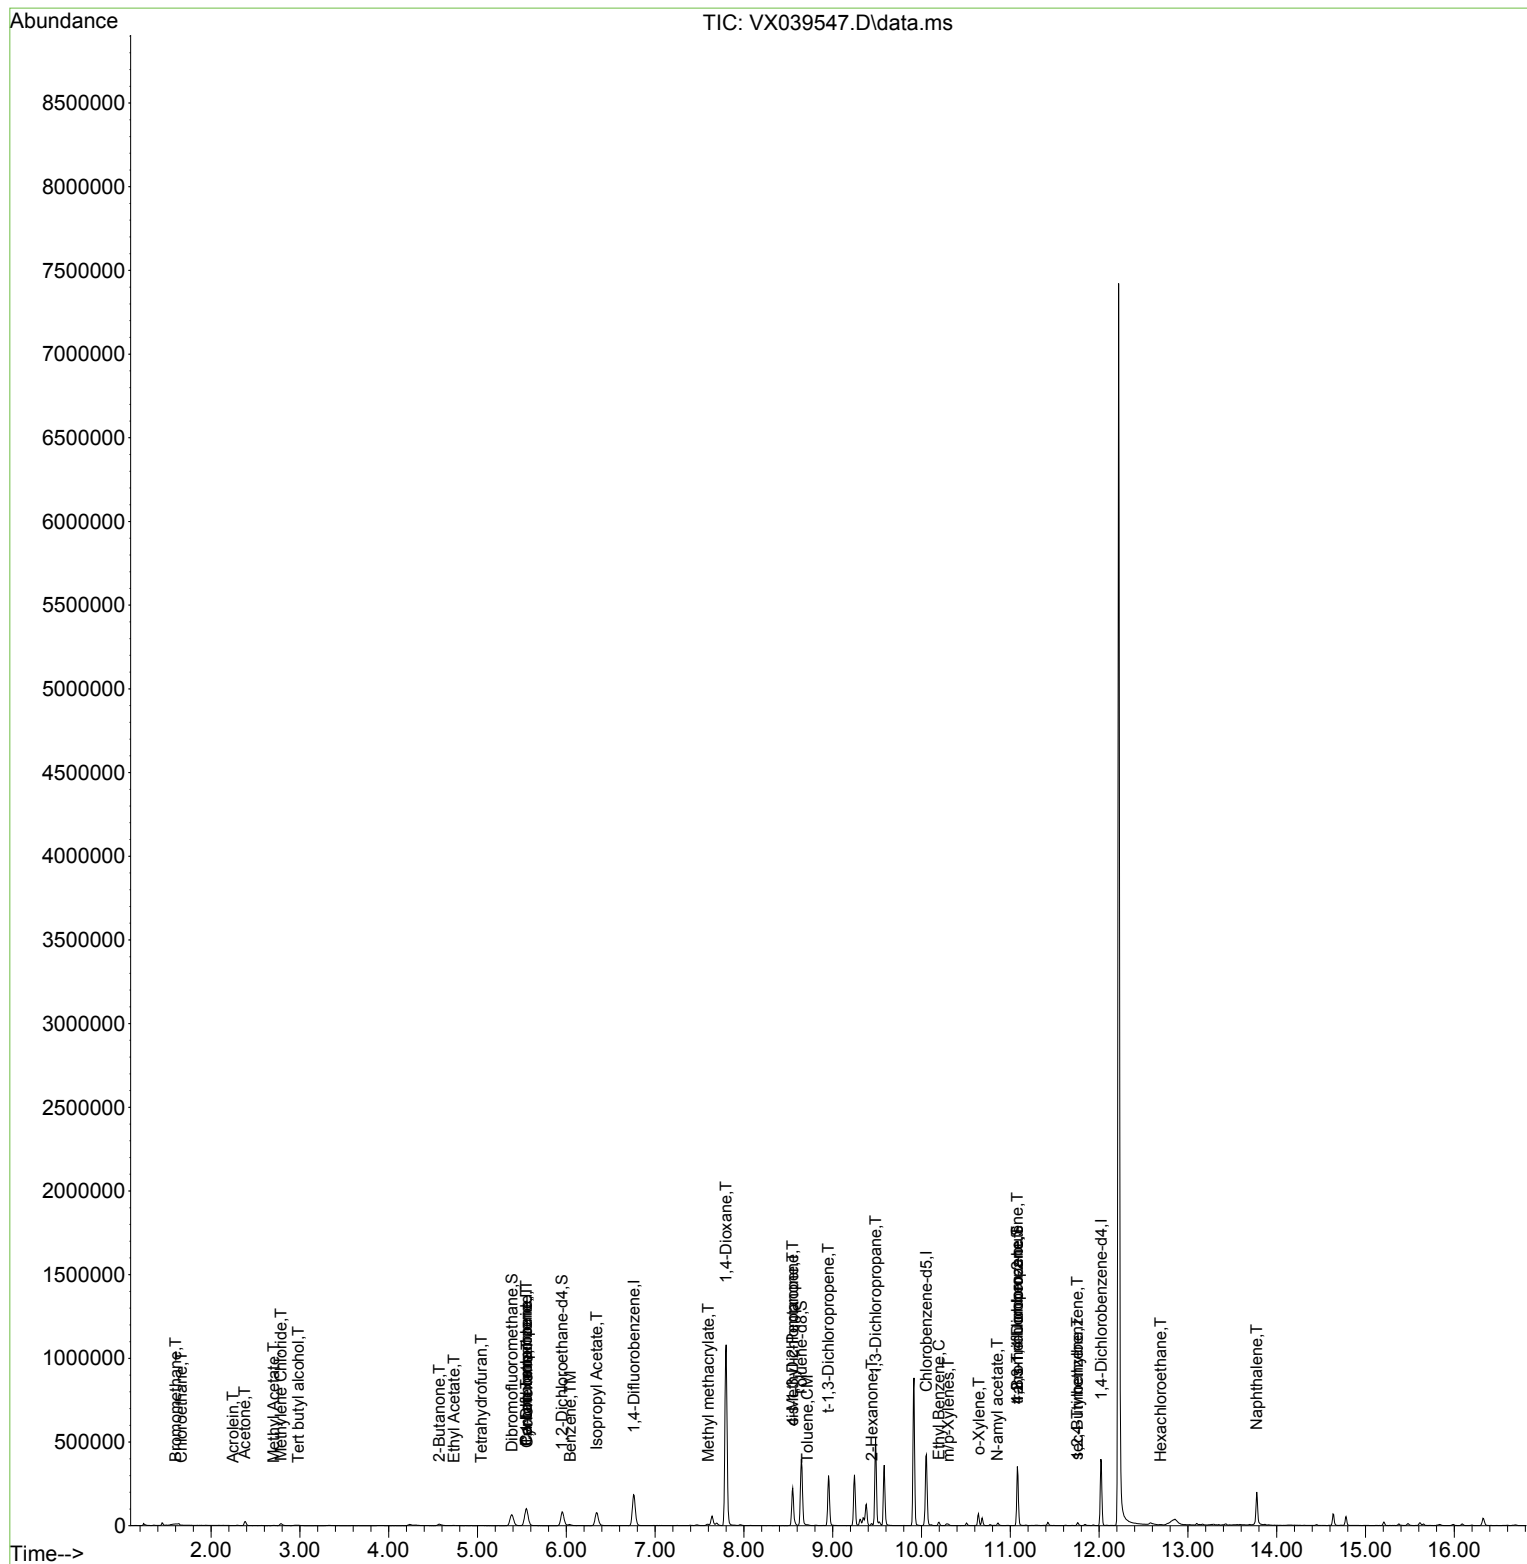




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion:168 Resp: 87810
Ion Ratio Lower Upper
168 100
99 71.0 56.6 85.0

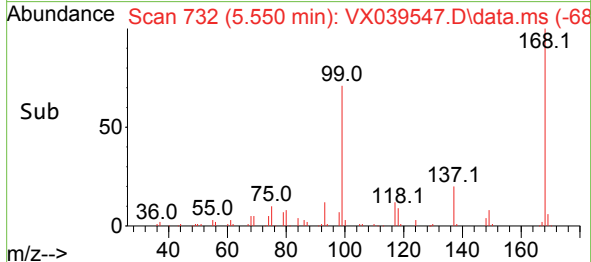

#5
Bromomethane
Concen: 0.411 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 94 Resp: 301
Ion Ratio Lower Upper
94 100
96 40.4 74.6 111.8#


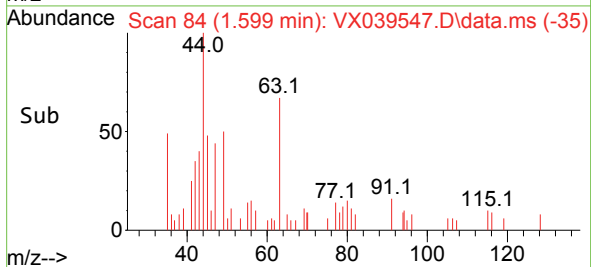

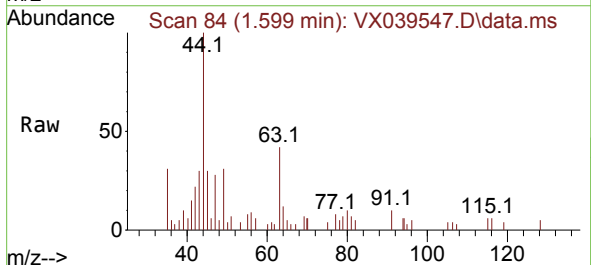


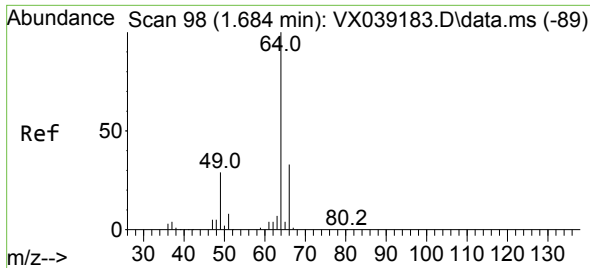

#6
Chloroethane
Concen: 0.464 ug/l
RT: 1.666 min Scan# 91
Delta R.T. -0.018 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 64 Resp: 356
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

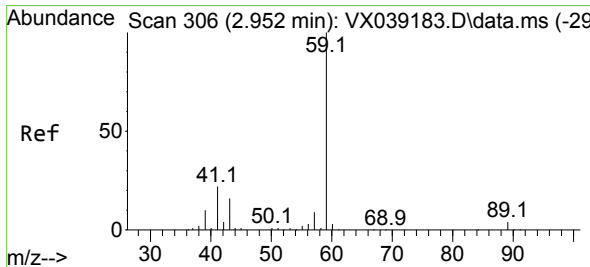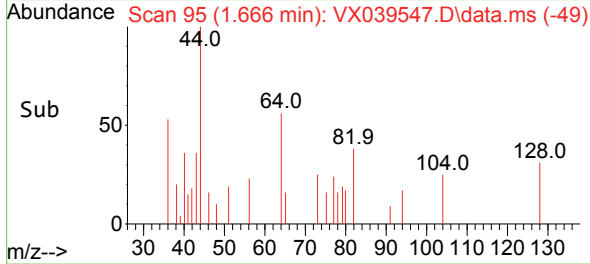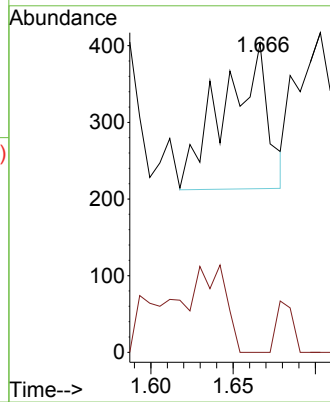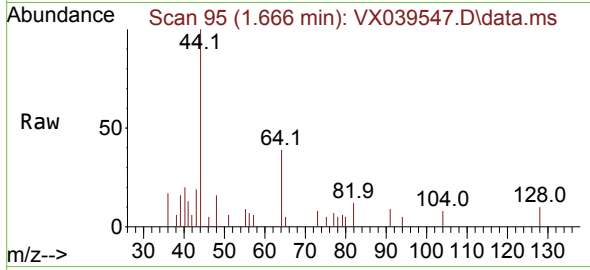

#11
Tert butyl alcohol
Concen: 13.962 ug/l
RT: 2.983 min Scan# 311
Delta R.T. 0.031 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 59 Resp: 5640
Ion Ratio Lower Upper
59 100
57 8.5 6.0 9.0

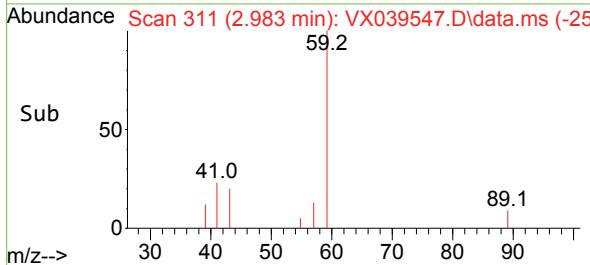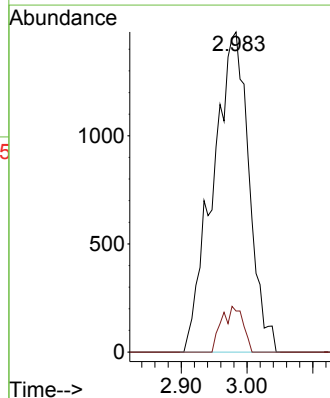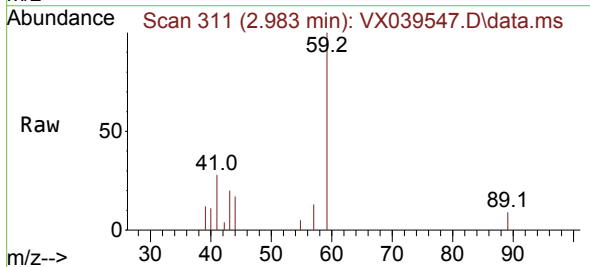

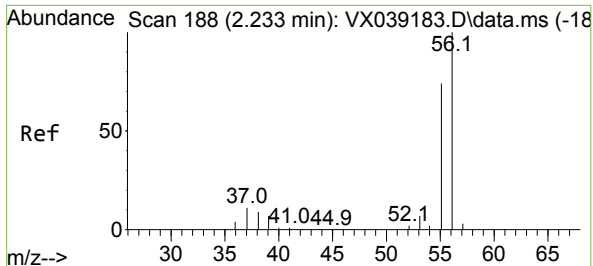

#13

Acrolein

Concen: 1.108 ug/l

RT: 2.246 min Scan# 190

Delta R.T. 0.013 min

Lab File: VX039547.D

Acq: 29 Dec 2023 15:54

Instrument :

MSVOA_X

ClientSampleId :





T-703

Tgt Ion: 56 Resp: 357

Ion Ratio Lower Upper

56 100

55 97.2 57.1 85.7#

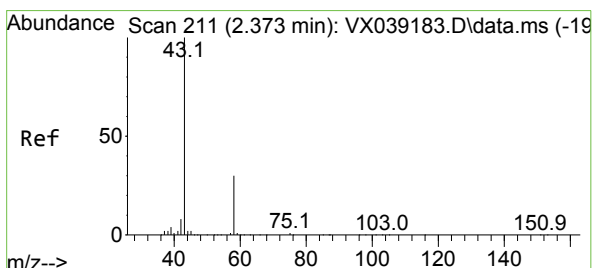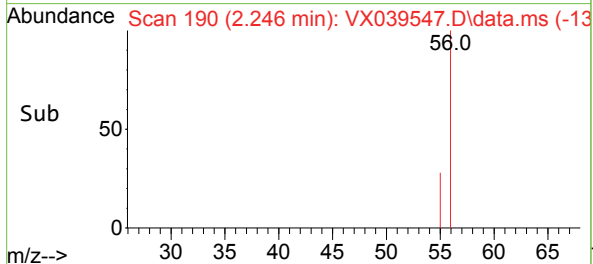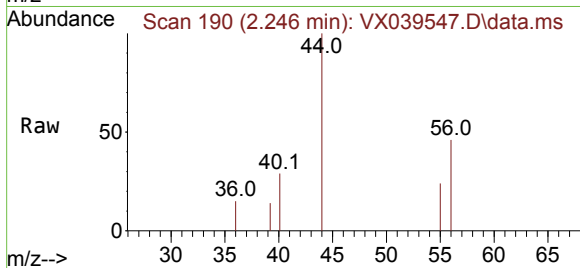

#16

Acetone

Concen: 6.581 ug/l

RT: 2.380 min Scan# 212

Delta R.T. 0.007 min

Lab File: VX039547.D




Acq: 29 Dec 2023 15:54


Tgt Ion: 43 Resp: 27389

Ion Ratio Lower Upper

43 100

58 30.7 21.9 32.9


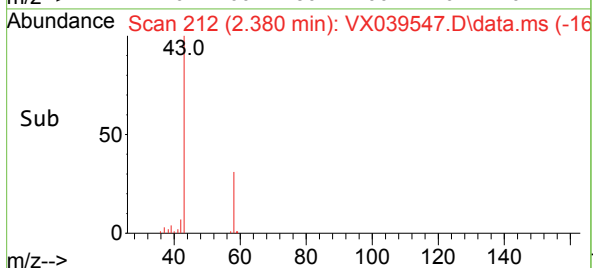

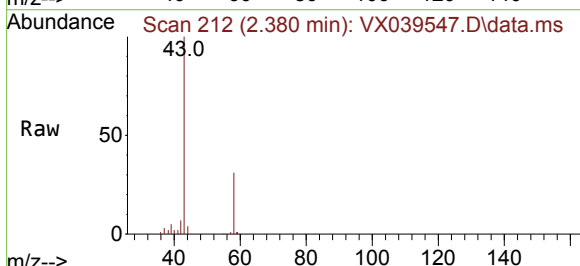




#18
Methyl Acetate
Concen: 0.736 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 43 Resp: 2560
Ion Ratio Lower Upper
43 100
74 23.6 17.8 26.8

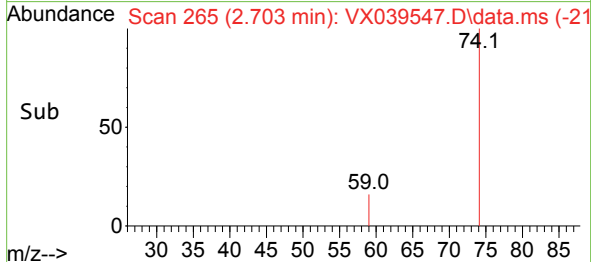

#20
Methylene Chloride
Concen: 4.740 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 84 Resp: 6356
Ion Ratio Lower Upper
84 100
49 129.3 103.6 155.4
51 41.5 33.8 50.6
86 65.6 49.4 74.0


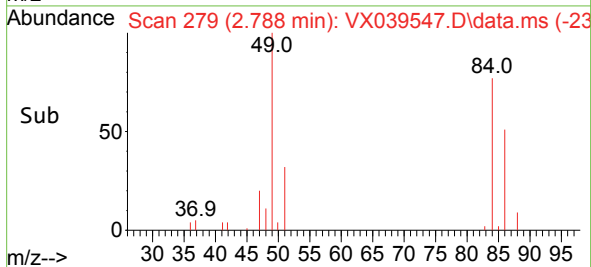

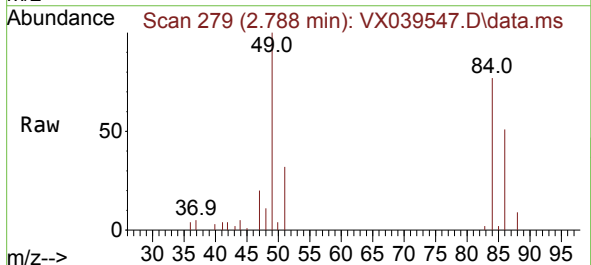


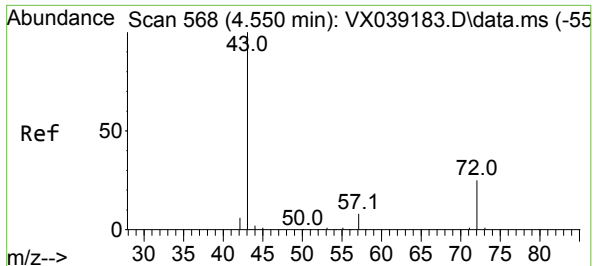

#25
2-Butanone
Concen: 12.559 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.019 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 43 Resp: 17433
Ion Ratio Lower Upper
43 100
72 22.8 19.4 29.2

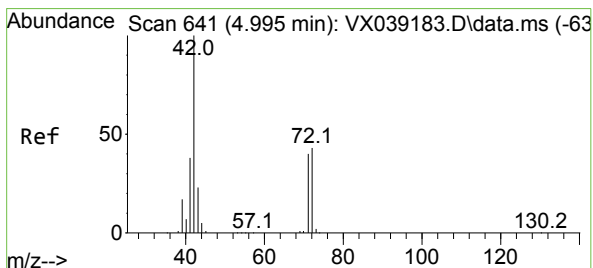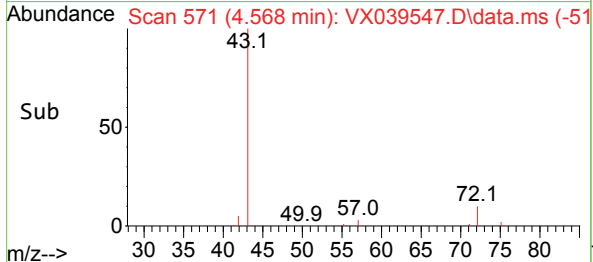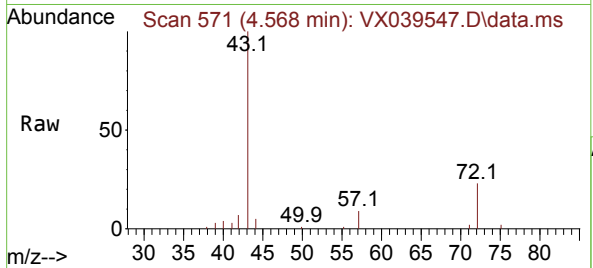

#29
Tetrahydrofuran
Concen: 1.290 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.049 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 42 Resp: 989
Ion Ratio Lower Upper
42 100
72 6.1 34.2 51.4#
71 26.6 32.2 48.2#


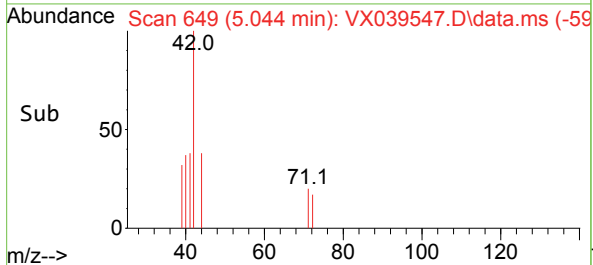

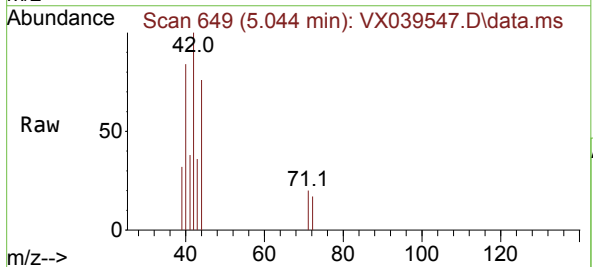


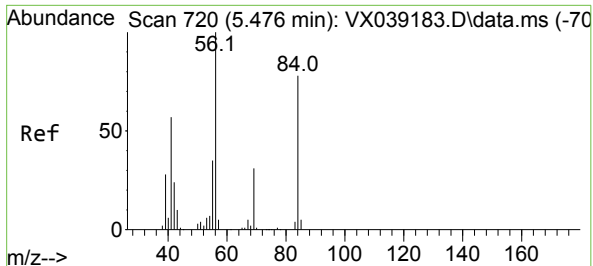

#31
Cyclohexane
Concen: 1.272 ug/l
RT: 5.556 min Scan# 713
Delta R.T. 0.080 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 56 Resp: 2643
Ion Ratio Lower Upper
56 100
69 137.9 23.4 35.2#
84 113.8 65.9 98.9#

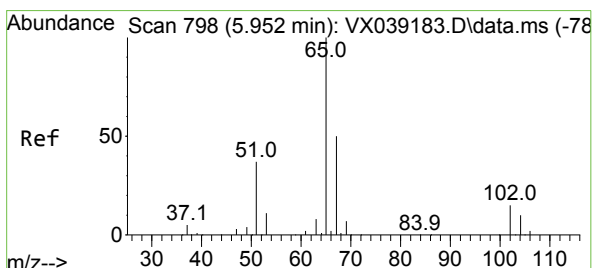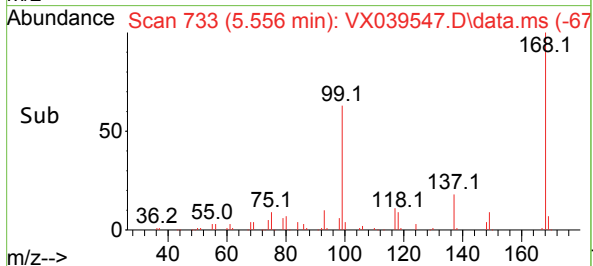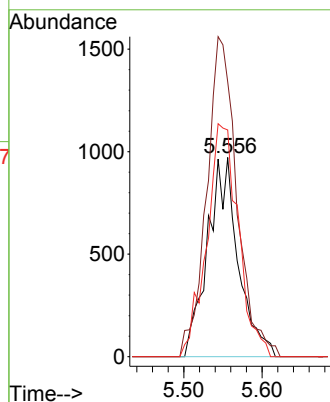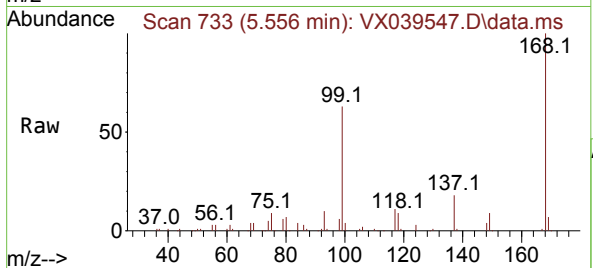

#33
1,2-Dichloroethane-d4
Concen: 49.045 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 65 Resp: 78895
Ion Ratio Lower Upper
65 100
67 51.5 0.0 100.2


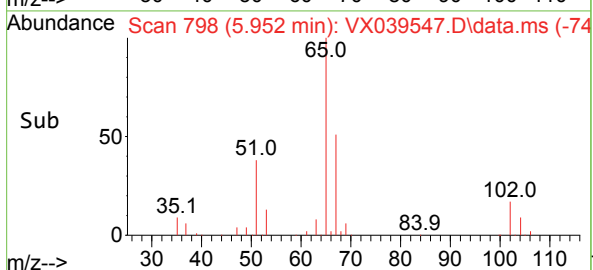

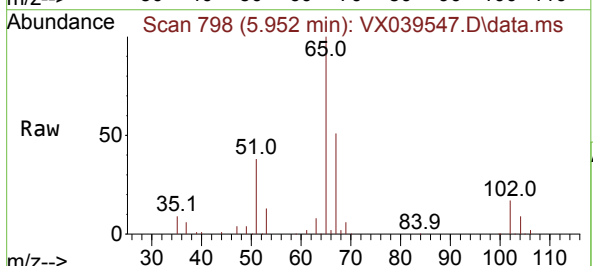




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion:114 Resp: 180475
Ion Ratio Lower Upper
114 100
63 23.0 0.0 45.0
88 17.3 0.0 36.6

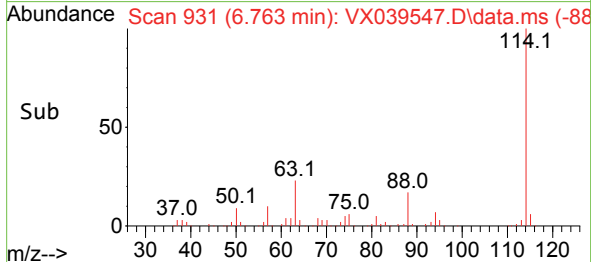

#35
Dibromofluoromethane
Concen: 46.971 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion:113 Resp: 58564
Ion Ratio Lower Upper
113 100
111 103.1 82.9 124.3
192 16.0 13.3 19.9


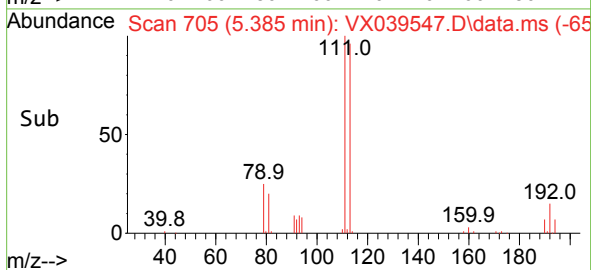






#36
1,1-Dichloropropene
Concen: 4.417 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 75 Resp: 8690
Ion Ratio Lower Upper
75 100
110 8.7 17.0 50.9#
77 0.0 24.7 37.1#

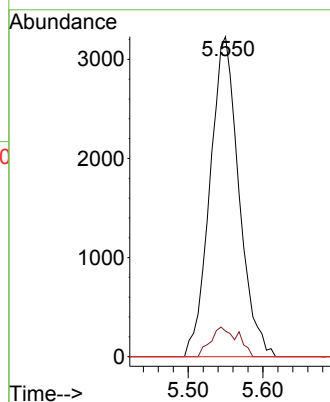

#37
Ethyl Acetate
Concen: 1.309 ug/l
RT: 4.733 min Scan# 598
Delta R.T. 0.025 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 43 Resp: 3181
Ion Ratio Lower Upper
43 100
61 9.4 10.6 16.0#
70 2.3 8.3 12.5#


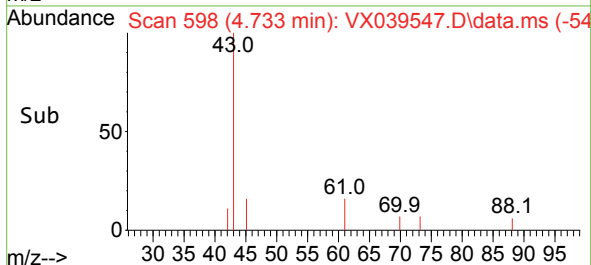

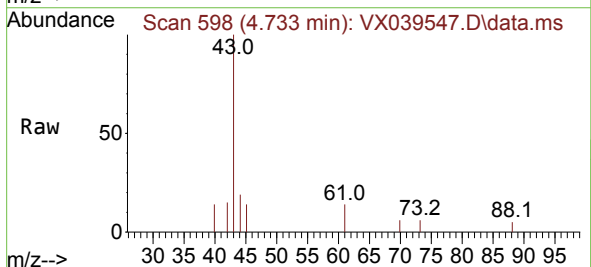


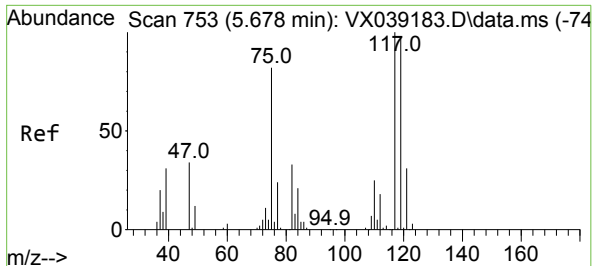

#38
Carbon Tetrachloride
Concen: 5.372 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion:117 Resp: 10087
Ion Ratio Lower Upper
117 100
119 4.9 78.2 117.2#
121 0.0 24.4 36.6#

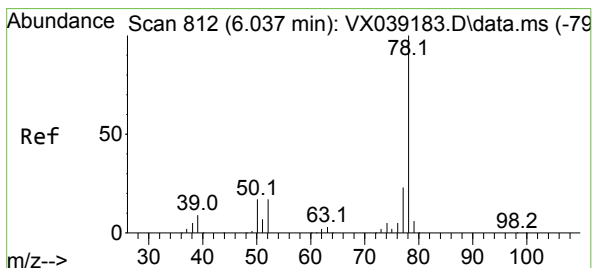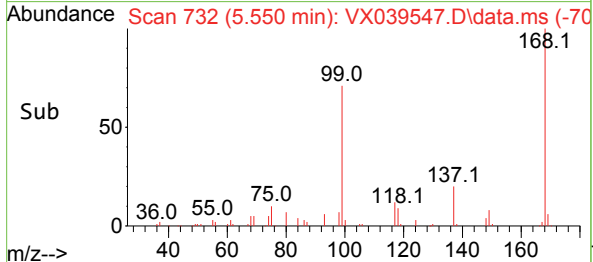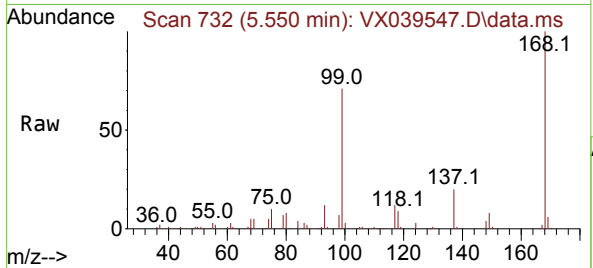

#40
Benzene
Concen: 1.331 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 78 Resp: 7406
Ion Ratio Lower Upper
78 100
77 22.0 19.3 28.9


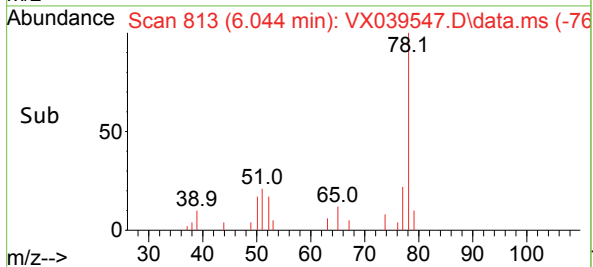

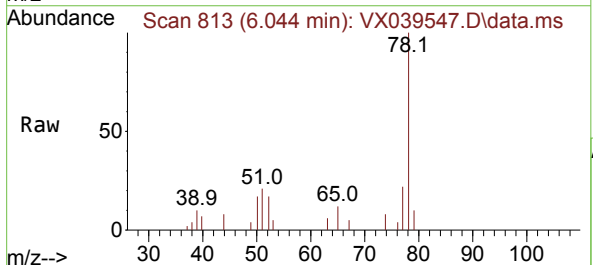




#43
Isopropyl Acetate
Concen: 28.896 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.006 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 43 Resp: 114219
Ion Ratio Lower Upper
43 100
61 18.3 15.2 22.8
87 11.7 9.8 14.6



#48
Methyl methacrylate
Concen: 1.988 ug/l
RT: 7.598 min Scan# 1068
Delta R.T. -0.091 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 41 Resp: 4595
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 0.0 47.7 71.5#


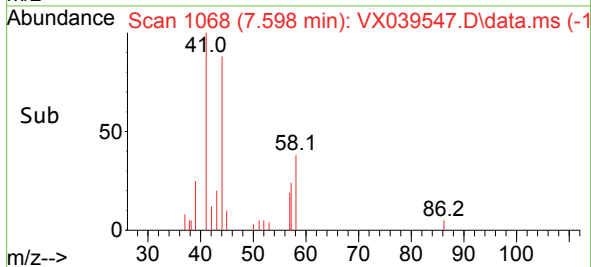

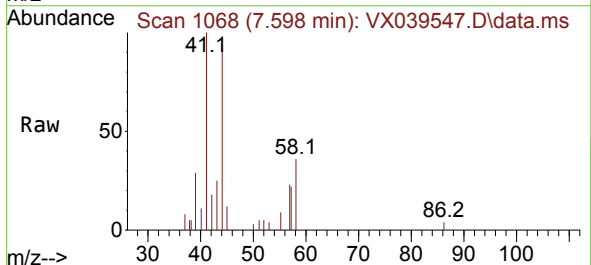




#49
1,4-Dioxane
Concen: 3.563 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.147 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 88 Resp: 111
Ion Ratio Lower Upper
88 100
43 926011.7 0.0 0.0#
58 3997.3 60.1 90.1#



#50
Toluene-d8
Concen: 50.229 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 98 Resp: 232501
Ion Ratio Lower Upper
98 100
100 63.5 53.1 79.7

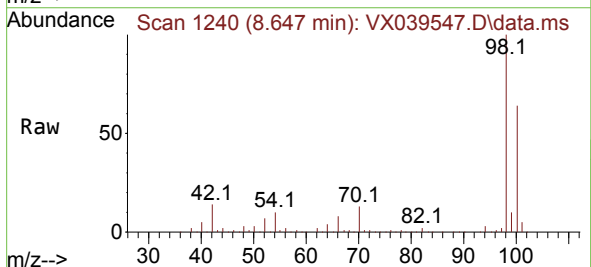



#51

4-Methyl-2-Pentanone

Concen: 33.441 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX039547.D

Acq: 29 Dec 2023 15:54

Instrument :

MSVOA_X

ClientSampleId :





T-703

Tgt Ion: 43 Resp: 84221

Ion Ratio Lower Upper

43 100

58 5.2 30.4 45.6#

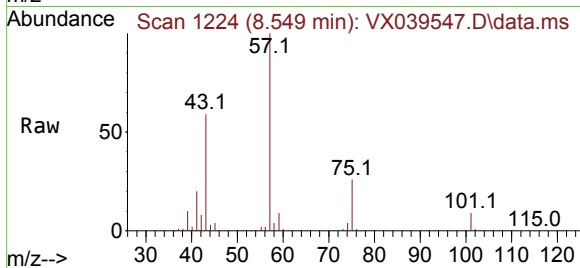

#52

Toluene

Concen: 0.280 ug/l

RT: 8.714 min Scan# 1251

Delta R.T. -0.006 min

Lab File: VX039547.D




Acq: 29 Dec 2023 15:54


Tgt Ion: 92 Resp: 939

Ion Ratio Lower Upper

92 100

91 186.2 134.2 201.2


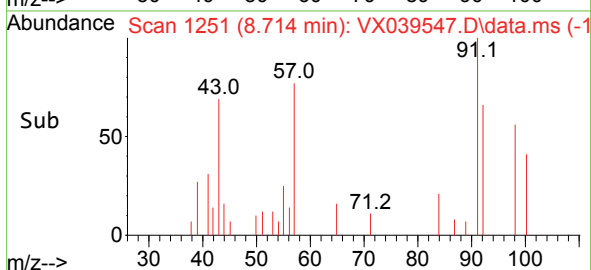

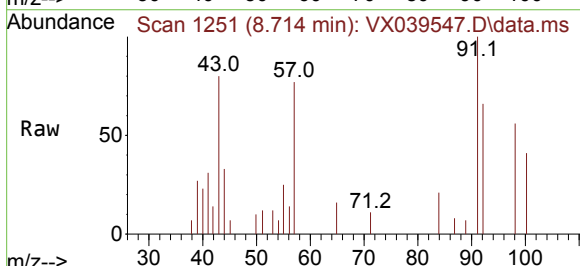




#53
 t-1,3-Dichloropropene
 Concen: 0.271 ug/l
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX039547.D
 Acq: 29 Dec 2023 15:54




Instrument :
 MSVOA_X
 ClientSampleId :
 T-703


Tgt Ion: 75 Resp: 600
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#



#54
 cis-1,3-Dichloropropene
 Concen: 13.948 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.183 min
 Lab File: VX039547.D
 Acq: 29 Dec 2023 15:54

Tgt Ion: 75 Resp: 33172
 Ion Ratio Lower Upper
 75 100
 77 0.4 25.3 37.9#
 39 37.4 46.7 70.1#

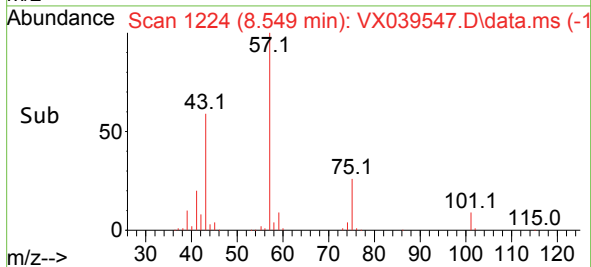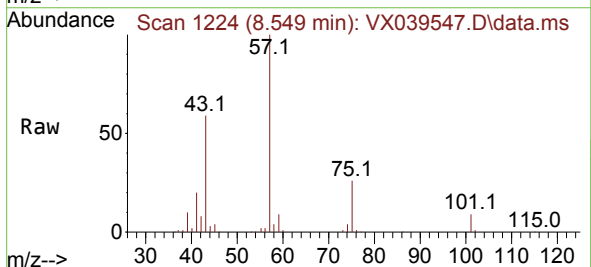



#57

1,3-Dichloropropane

Concen: 1.783 ug/l

RT: 9.482 min Scan# 11

Delta R.T. 0.177 min

Lab File: VX039547.D

Acq: 29 Dec 2023 15:54

Instrument :

MSVOA_X

ClientSampleId :





T-703

Tgt Ion: 76 Resp: 4322

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

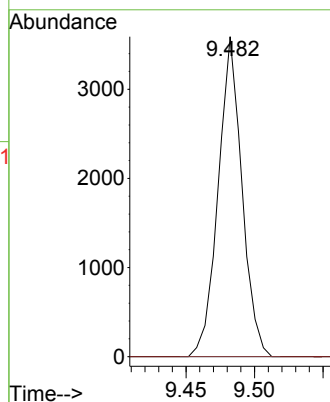

#59

2-Hexanone

Concen: 2.911 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.013 min

Lab File: VX039547.D




Acq: 29 Dec 2023 15:54


Tgt Ion: 43 Resp: 6327

Ion Ratio Lower Upper

43 100

58 58.6 26.2 78.5


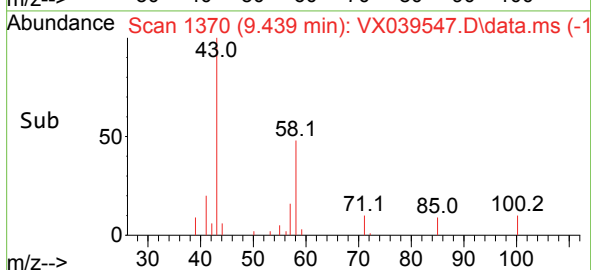






#62
4-Bromofluorobenzene
Concen: 49.451 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 95 Resp: 94443
Ion Ratio Lower Upper
95 100
174 64.9 0.0 135.6
176 62.4 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 117 Resp: 179514
Ion Ratio Lower Upper
117 100
82 59.9 46.2 69.4
119 31.5 25.5 38.3



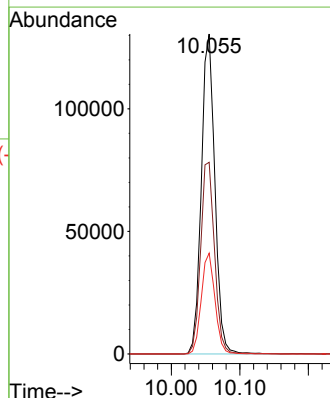



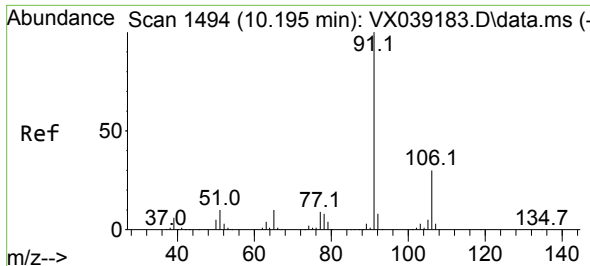

#67
Ethyl Benzene
Concen: 1.725 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 91 Resp: 12579
Ion Ratio Lower Upper
91 100
106 29.1 24.9 37.3

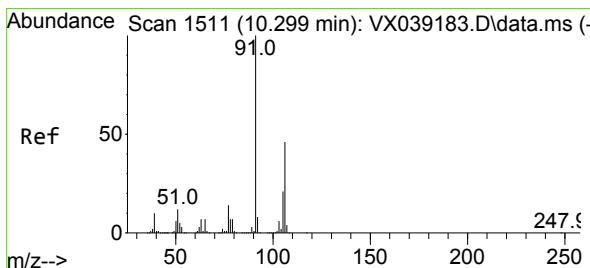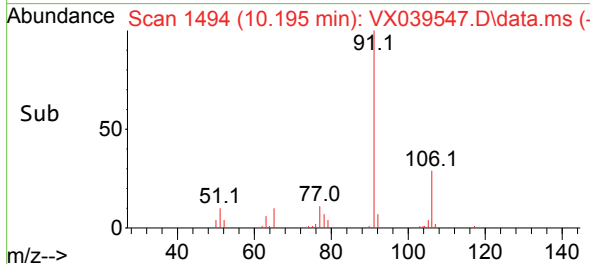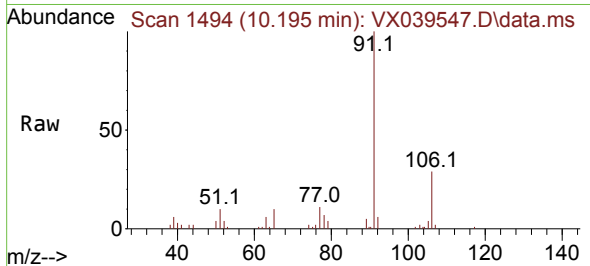

#68
m/p-Xylenes
Concen: 0.645 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 106 Resp: 1686
Ion Ratio Lower Upper
106 100
91 209.2 165.5 248.3


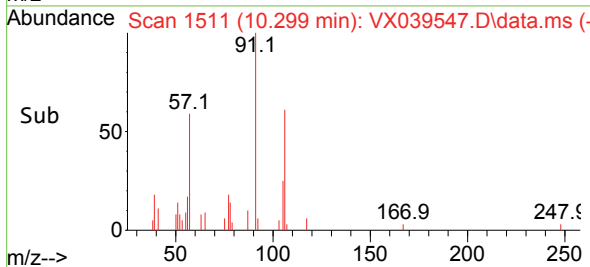

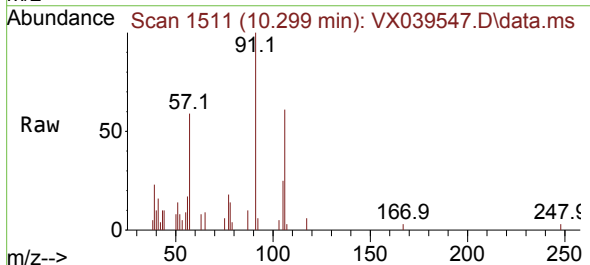




#69
o-Xylene
Concen: 0.290 ug/l
RT: 10.647 min Scan# 1567
Delta R.T. 0.006 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion:106 Resp: 734
Ion Ratio Lower Upper
106 100
91 246.3 108.9 326.8



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion:152 Resp: 75396
Ion Ratio Lower Upper
152 100
115 65.8 43.3 129.9
150 157.8 0.0 345.0



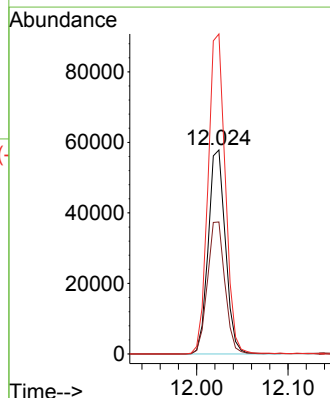
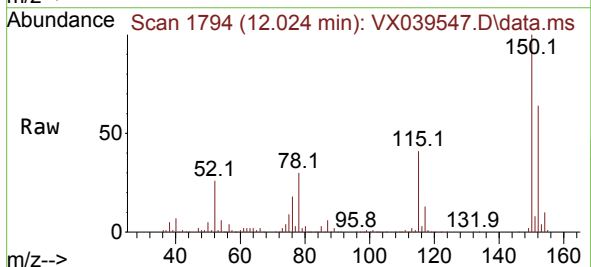




#74
N-amy1 acetate
Concen: 1.087 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.013 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 43 Resp: 3199
Ion Ratio Lower Upper
43 100
70 77.3 32.9 49.3#
55 65.3 19.3 28.9#
61 0.0 18.8 28.2#

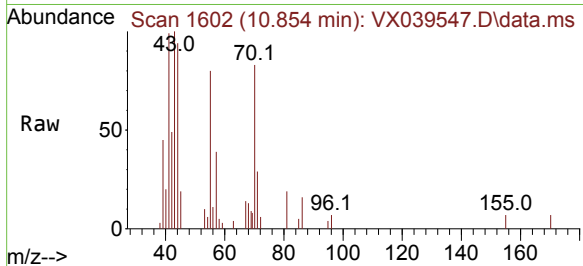

#76
1,2,3-Trichloropropane
Concen: 27.176 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 75 Resp: 53011
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#




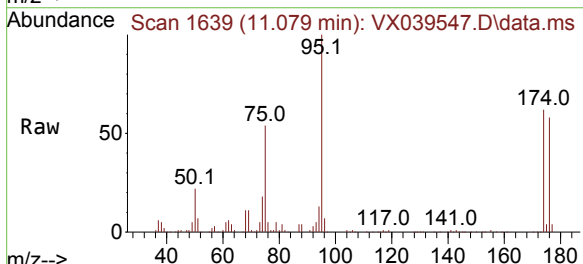




#81
trans-1,4-Dichloro-2-butene
Concen: 76.664 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54




Instrument :
MSVOA_X
ClientSampleId :
T-703


Tgt Ion: 75 Resp: 53011
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

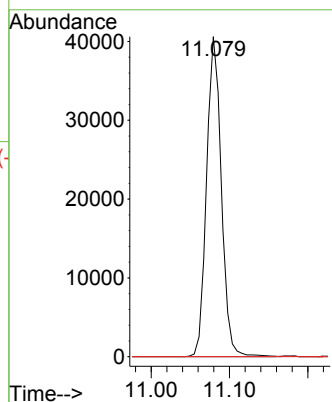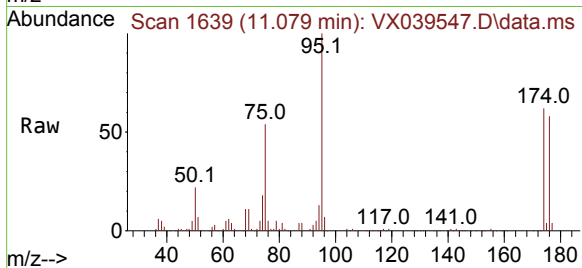

#84
1,2,4-Trimethylbenzene
Concen: 0.729 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Tgt Ion: 105 Resp: 3703
Ion Ratio Lower Upper
105 100
120 30.9 21.2 63.6

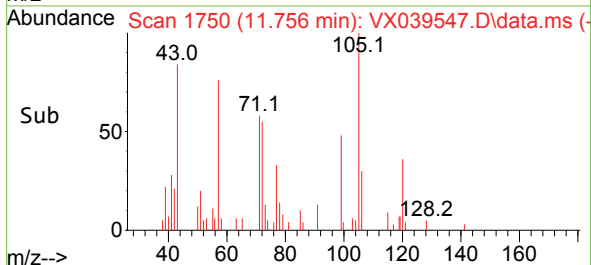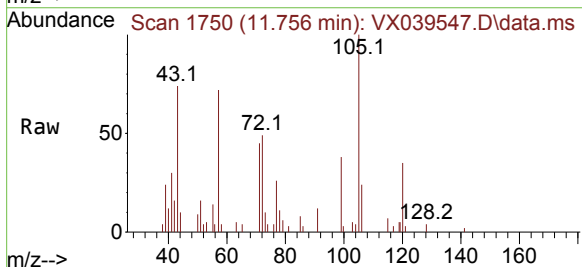

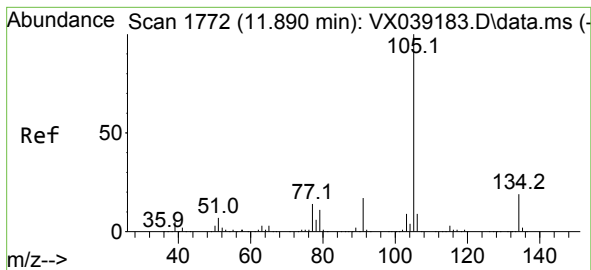

#85

sec-Butylbenzene

Concen: 0.617 ug/l

RT: 11.756 min Scan# 11

Delta R.T. -0.134 min

Lab File: VX039547.D

Acq: 29 Dec 2023 15:54

Instrument :

MSVOA_X

ClientSampleId :





T-703

Tgt Ion:105 Resp: 3703

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#

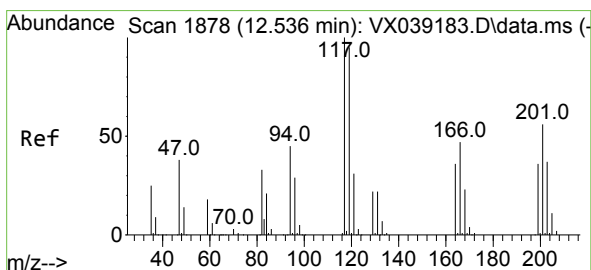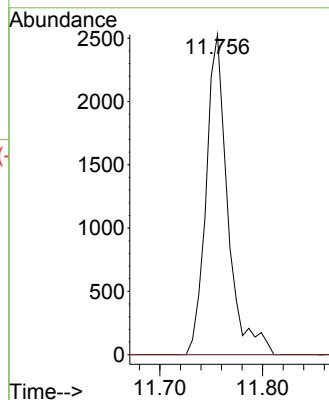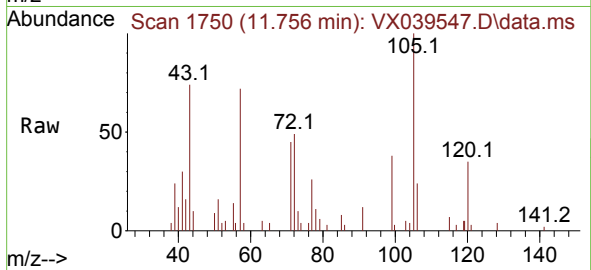

#90

Hexachloroethane

Concen: 0.486 ug/l

RT: 12.695 min Scan# 1904

Delta R.T. 0.159 min

Lab File: VX039547.D




Acq: 29 Dec 2023 15:54


Tgt Ion:117 Resp: 442

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#

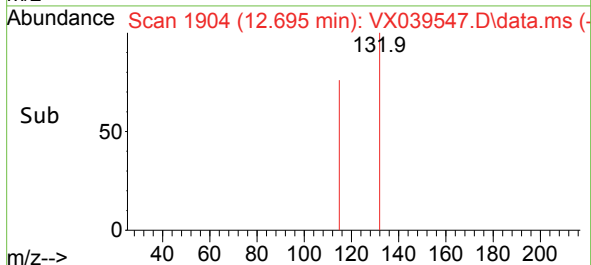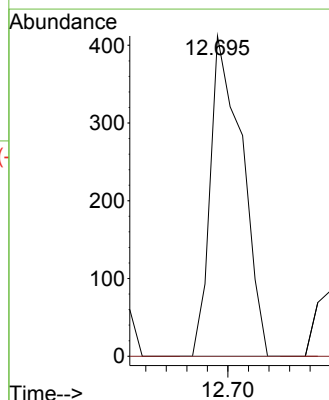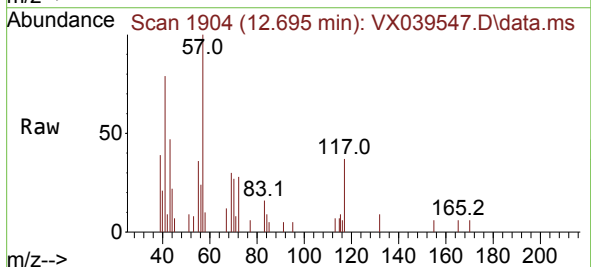



#95
Naphthalene
Concen: 23.558 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX039547.D
Acq: 29 Dec 2023 15:54

Instrument :
MSVOA_X
ClientSampleId :
T-703

Tgt Ion:128 Resp: 129901
Ion Ratio Lower Upper
128 100
127 12.2 10.3 15.5
129 10.8 8.8 13.2

