

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122923\
 Data File : VX039556.D
 Acq On : 29 Dec 2023 19:20
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Dec 30 02:07:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	83955	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	181423	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	186477	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	89490	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	76964	50.042	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	100.080%
35) Dibromofluoromethane	5.385	113	57876	46.177	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.360%
50) Toluene-d8	8.647	98	229648	49.353	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.700%
62) 4-Bromofluorobenzene	11.079	95	101348	52.789	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122923\
Data File : VX039556.D
Acq On : 29 Dec 2023 19:20
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Dec 30 02:07:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




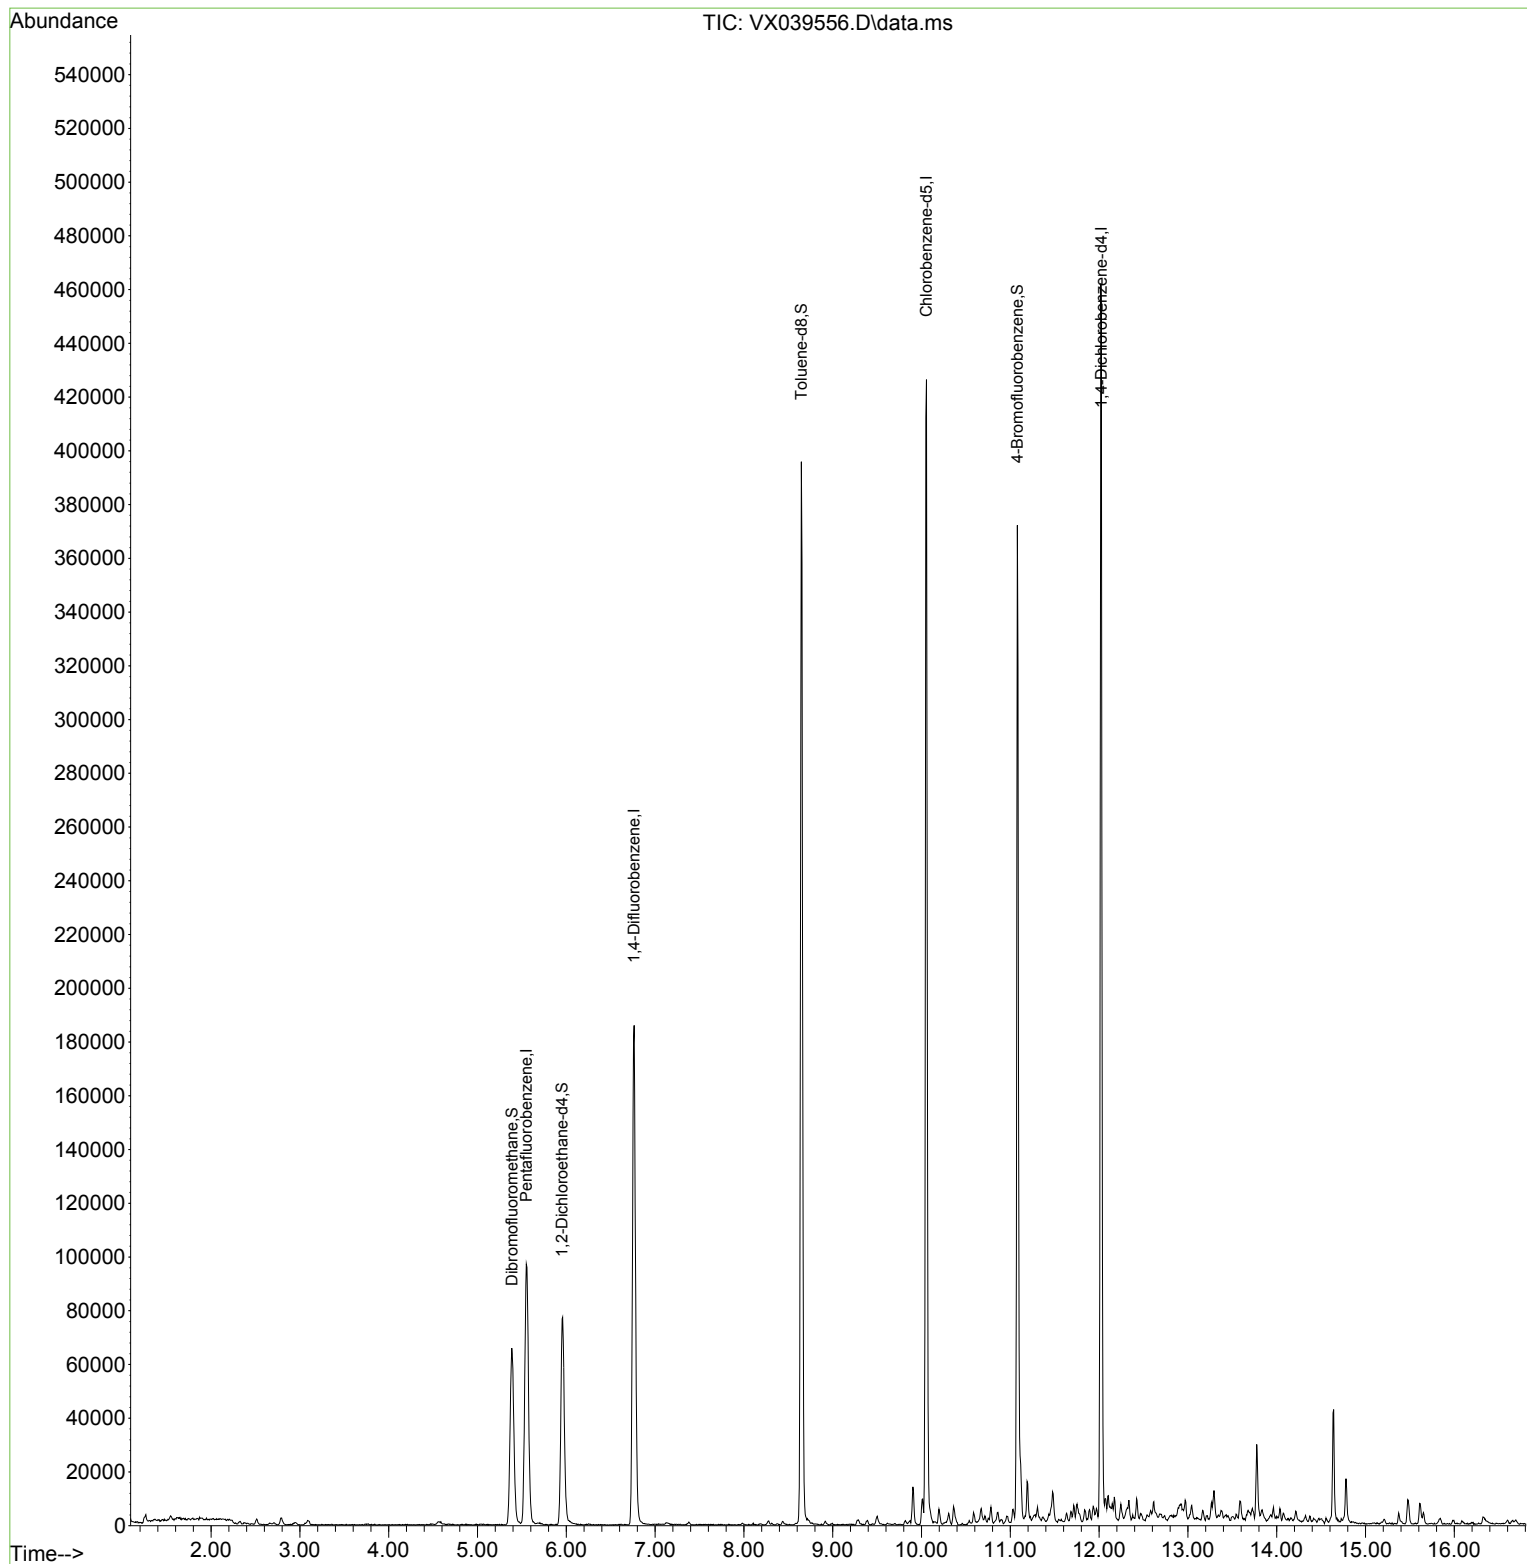


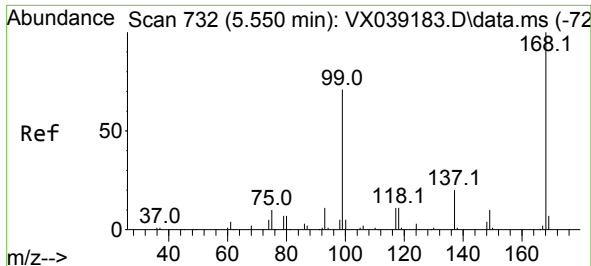

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX039556.D
Acq: 29 Dec 2023 19:20




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 83955
Ion Ratio Lower Upper
168 100
99 67.9 56.6 85.0

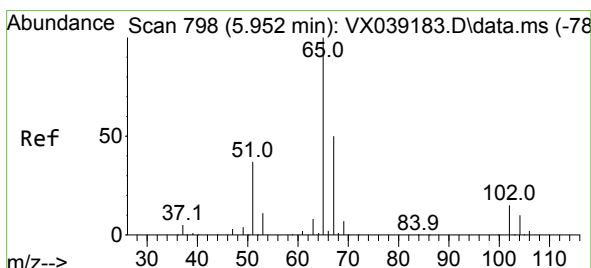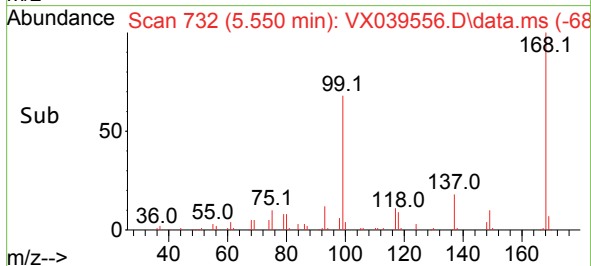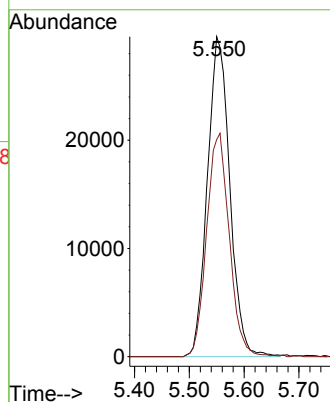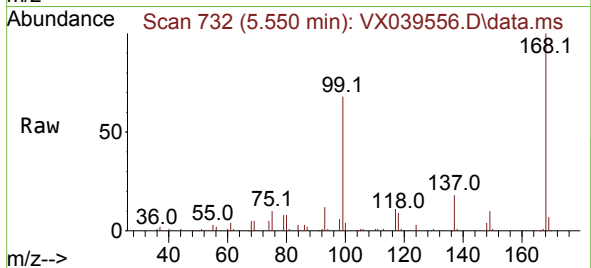

#33
1,2-Dichloroethane-d4
Concen: 50.042 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039556.D
Acq: 29 Dec 2023 19:20

Tgt Ion: 65 Resp: 76964
Ion Ratio Lower Upper
65 100
67 51.3 0.0 100.2


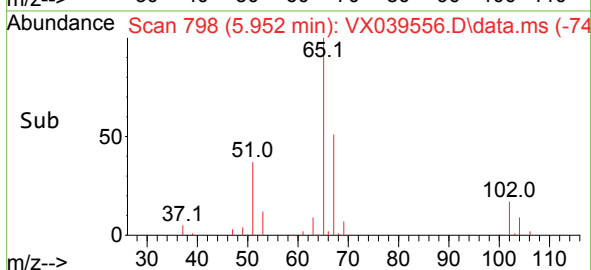
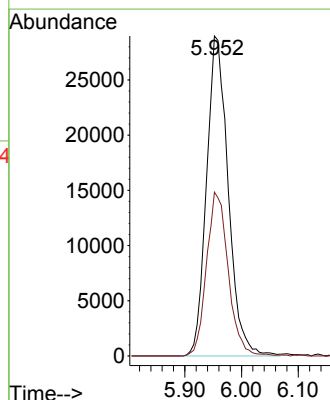
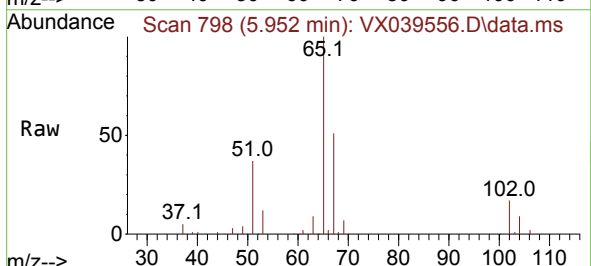


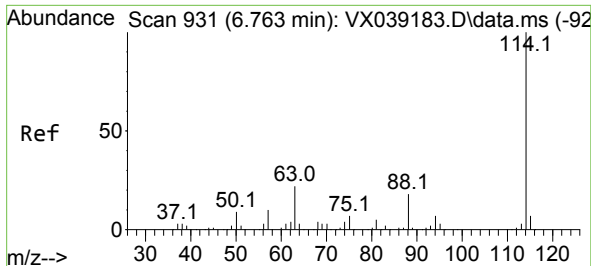

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX039556.D
Acq: 29 Dec 2023 19:20




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 181423
Ion Ratio Lower Upper
114 100
63 22.3 0.0 45.0
88 18.1 0.0 36.6

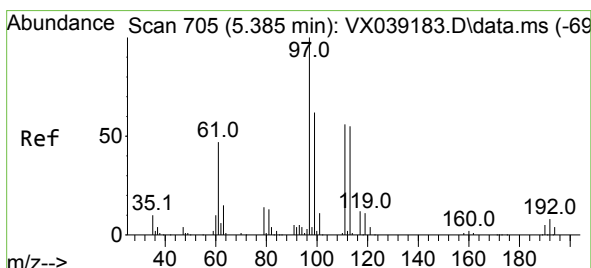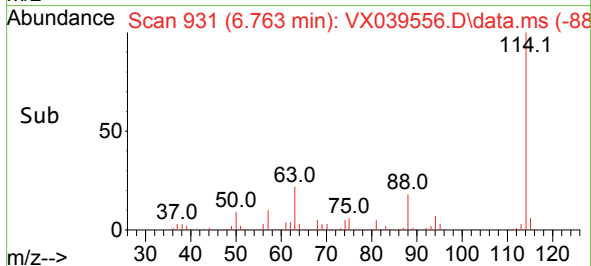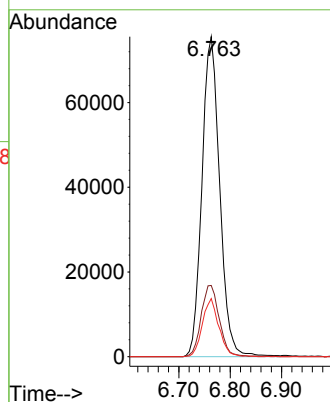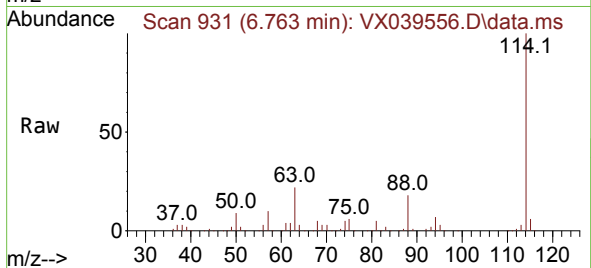

#35
Dibromofluoromethane
Concen: 46.177 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039556.D
Acq: 29 Dec 2023 19:20

Tgt Ion:113 Resp: 57876
Ion Ratio Lower Upper
113 100
111 103.7 82.9 124.3
192 16.1 13.3 19.9


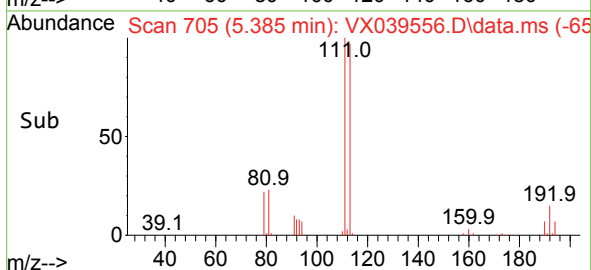
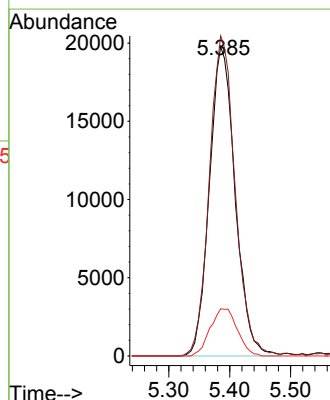
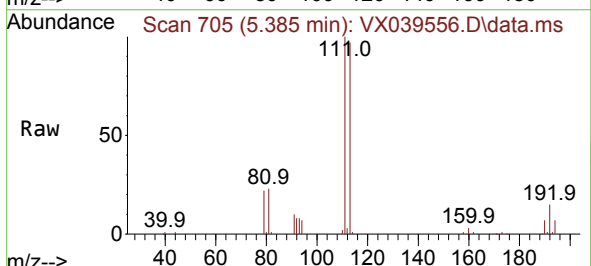


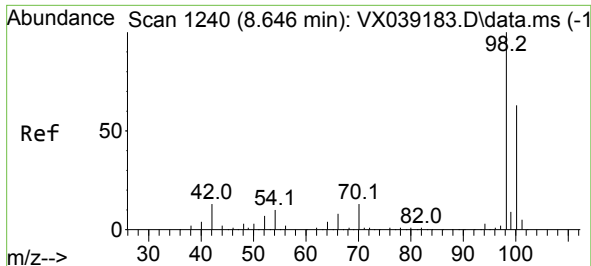

#50
Toluene-d8
Concen: 49.353 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX039556.D
Acq: 29 Dec 2023 19:20




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 229648
Ion Ratio Lower Upper
98 100
100 64.4 53.1 79.7

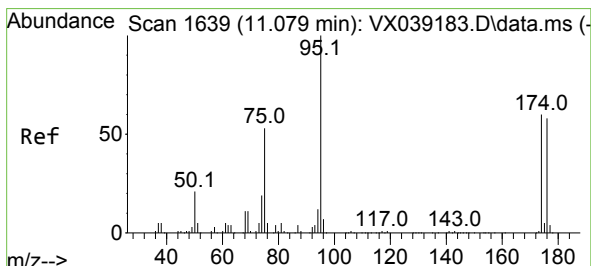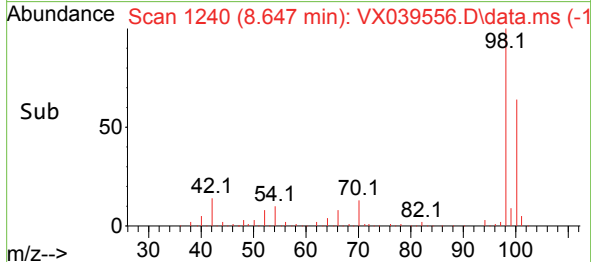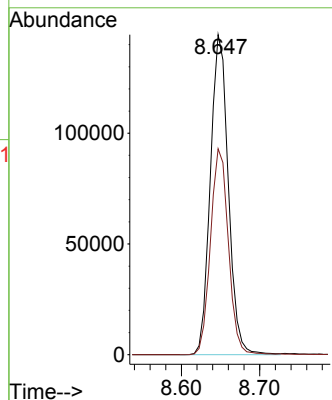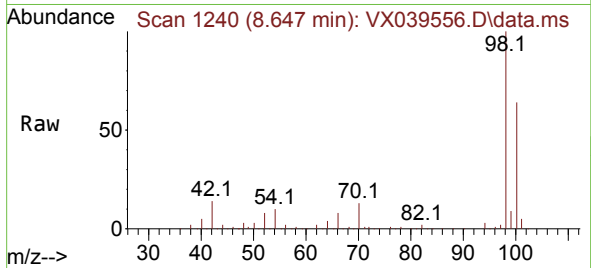

#62
4-Bromofluorobenzene
Concen: 52.789 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039556.D
Acq: 29 Dec 2023 19:20

Tgt Ion: 95 Resp: 101348
Ion Ratio Lower Upper
95 100
174 62.5 0.0 135.6
176 60.8 0.0 131.0

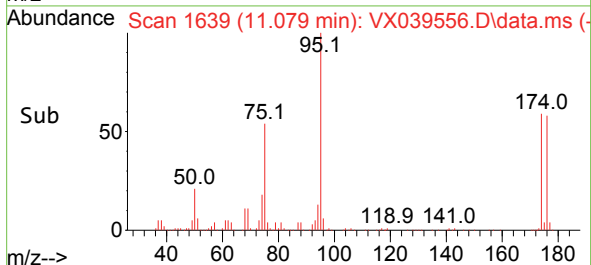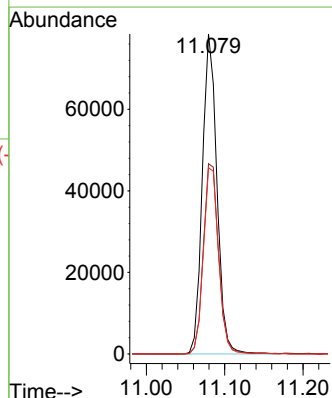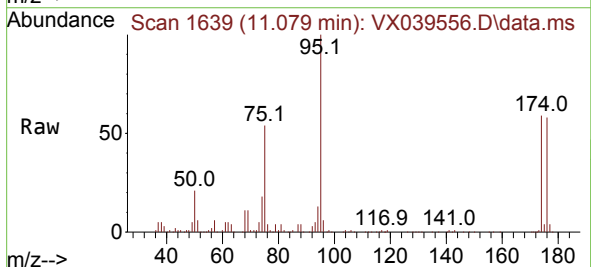

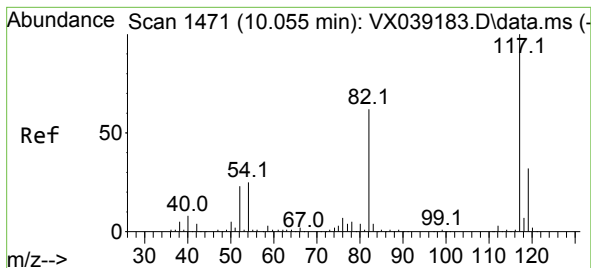

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX039556.D

Acq: 29 Dec 2023 19:20

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:117 Resp: 186477

Ion Ratio Lower Upper

117 100

82 57.6 46.2 69.4

119 31.7 25.5 38.3

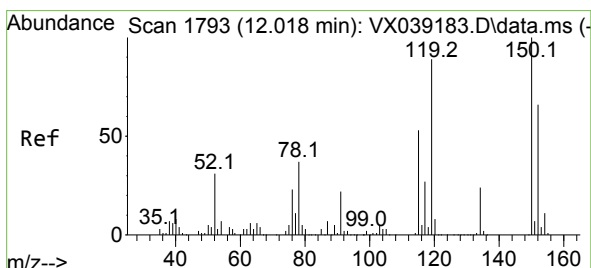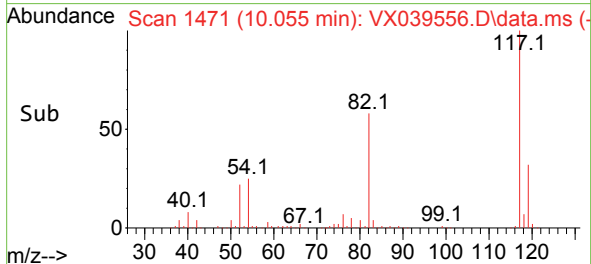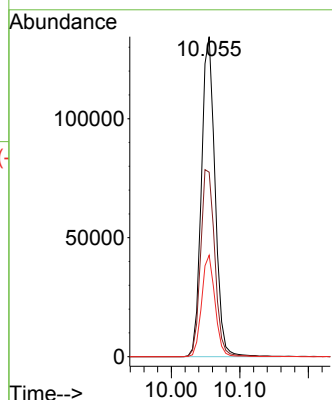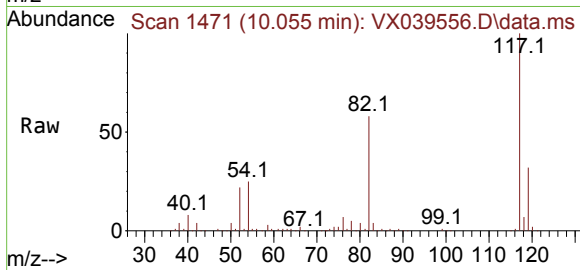

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.006 min

Lab File: VX039556.D

Acq: 29 Dec 2023 19:20

Tgt Ion:152 Resp: 89490

Ion Ratio Lower Upper

152 100

115 67.4 43.3 129.9

150 156.8 0.0 345.0

