

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX123019\
 Data File : VX014346.D
 Acq On : 30 Dec 2019 11:32
 Operator : JC/SP
 Sample : VX1230WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1230WBL02

Quant Time: Dec 31 01:36:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 17 03:01:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	542683	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	845249	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	756220	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	331507	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	305647	49.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.38%	
35) Dibromofluoromethane	5.49	113	252038	49.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.10%	
50) Toluene-d8	8.71	98	1010905	50.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.06%	
62) 4-Bromofluorobenzene	11.13	95	339316	46.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.80%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX123019\
Data File : VX014346.D
Acq On : 30 Dec 2019 11:32
Operator : JC/SP
Sample : VX1230WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1230WBL02

Quant Time: Dec 31 01:36:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 17 03:01:07 2019
Response via : Initial Calibration

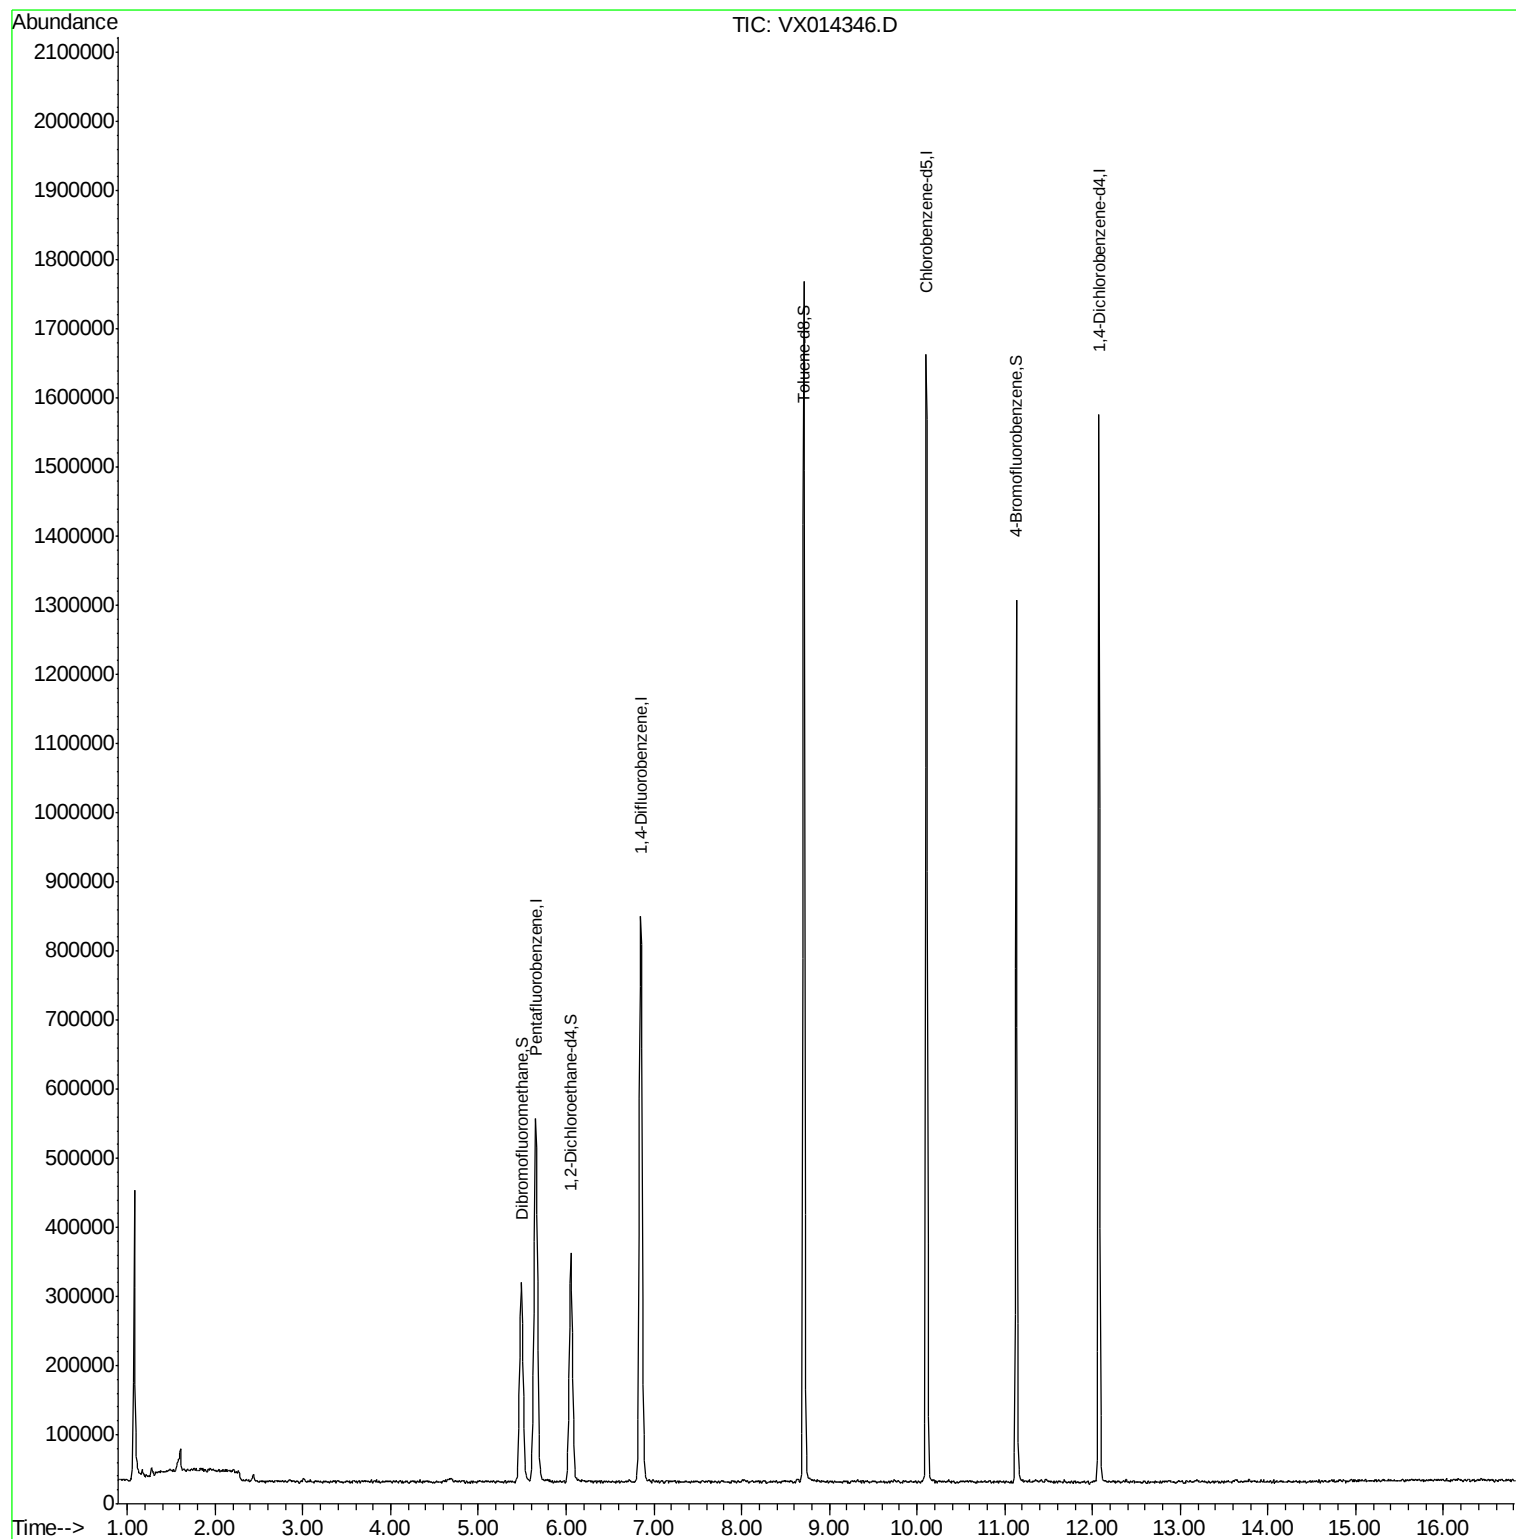

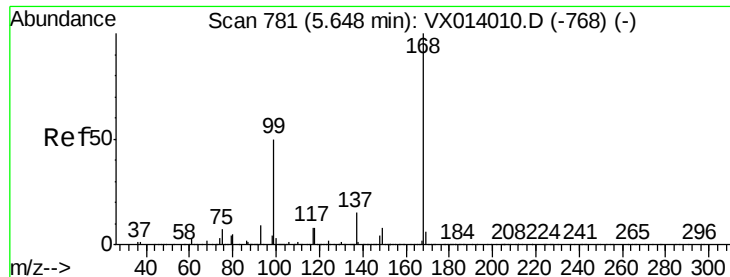

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. 0.01 min

Lab File: VX014346.D

Acq: 30 Dec 2019 11:32

Instrument :

MSVOA_X

ClientSampleId :


VX1230WBL02

Tot Ion:168 Resp: 542683

Ion Ratio Lower Upper

168 100

99 51.5 40.3 60.5

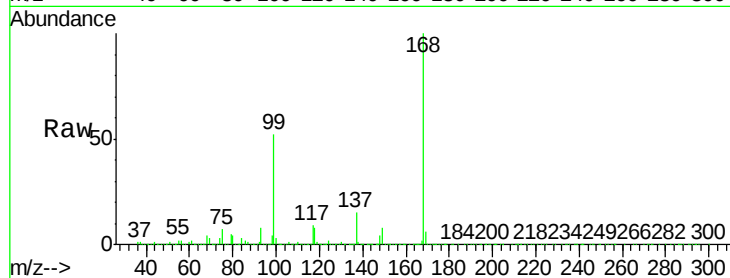

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

200000



150000

100000

50000

0

Time-->

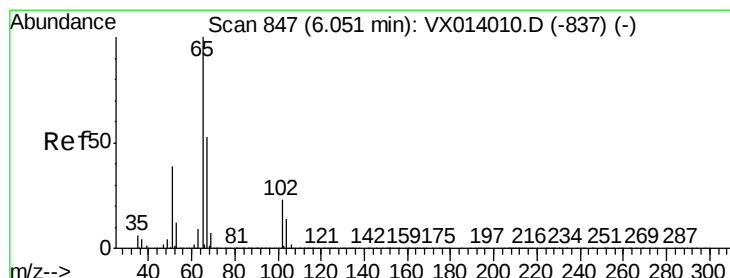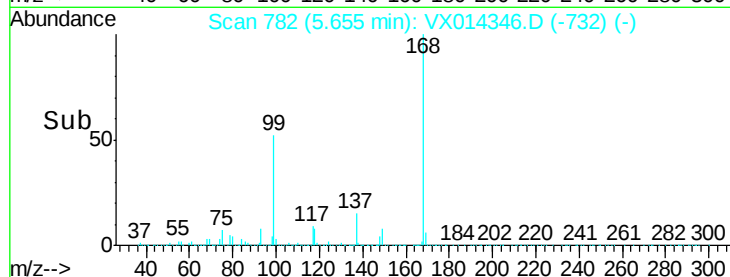

#33

1,2-Dichloroethane-d4

Concen: 49.694 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX014346.D


Acq: 30 Dec 2019 11:32

Tgt Ion: 65 Resp: 305647

Ion Ratio Lower Upper

65 100

67 53.2 0.0 106.4

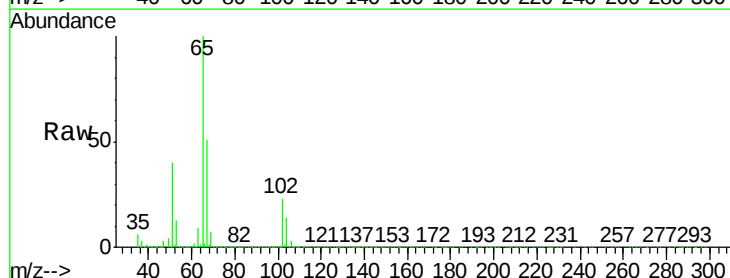

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0


6.05


100000

50000

0

Time-->

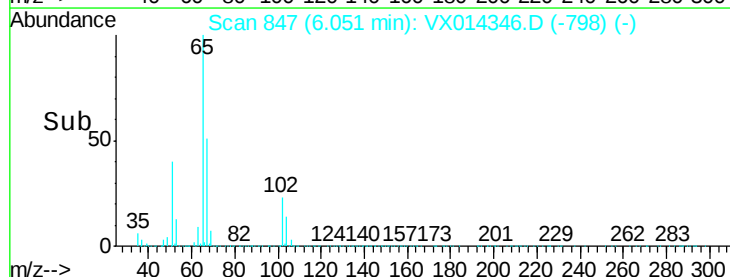

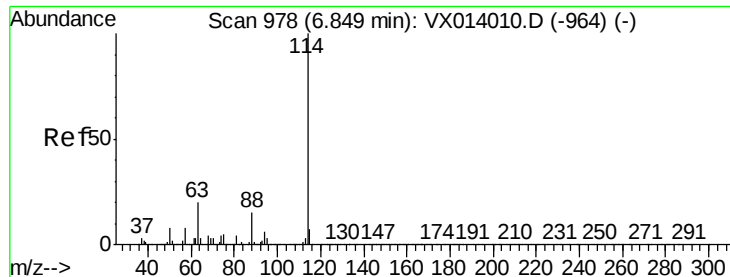

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX014346.D

Acq: 30 Dec 2019 11:32

Instrument :

MSVOA_X

ClientSampleId :

VX1230WBL02


Tot Ion:114 Resp: 845249

Ion Ratio Lower Upper

114 100

63 20.8 0.0 40.8

88 15.9 0.0 30.4

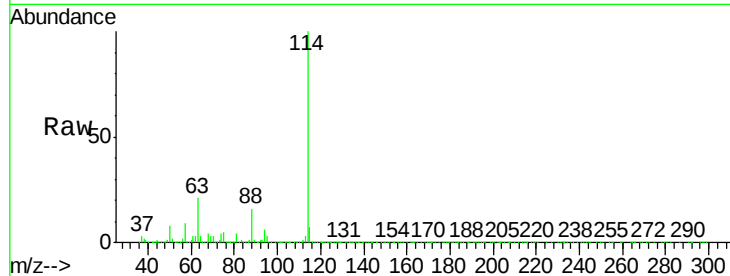

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

500000

400000

300000


200000

100000


0

6.85

6.70 6.80 6.90 7.00

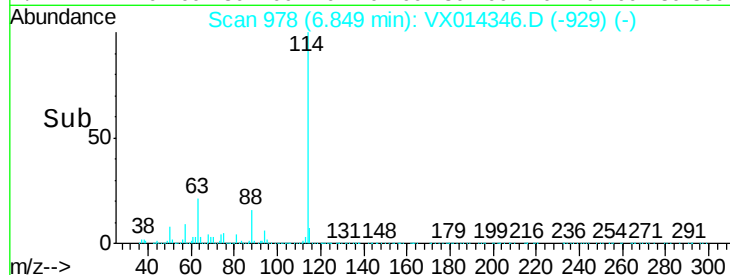

Time-->

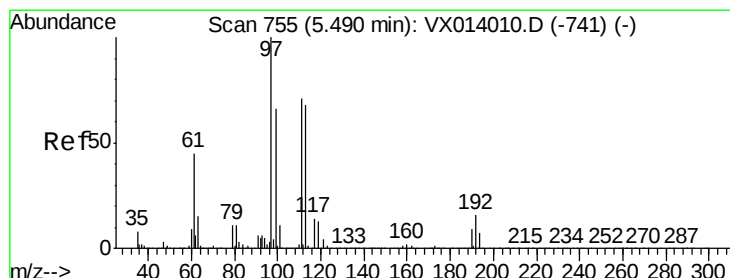

#35

Dibromofluoromethane

Concen: 49.052 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.00 min

Lab File: VX014346.D

Acq: 30 Dec 2019 11:32


Tgt Ion:113 Resp: 252038

Ion Ratio Lower Upper

113 100

111 101.9 82.0 123.0

192 23.4 19.3 28.9

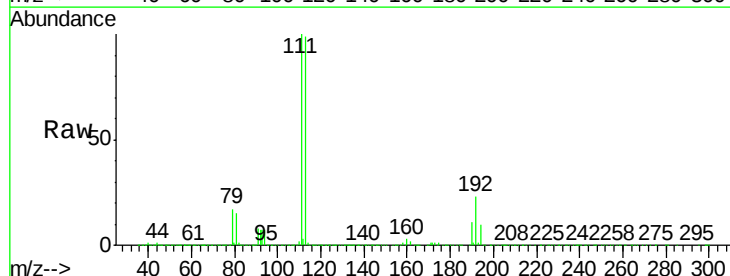

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

120000

100000

80000

60000


40000

20000

0

5.49

5.40 5.50 5.60

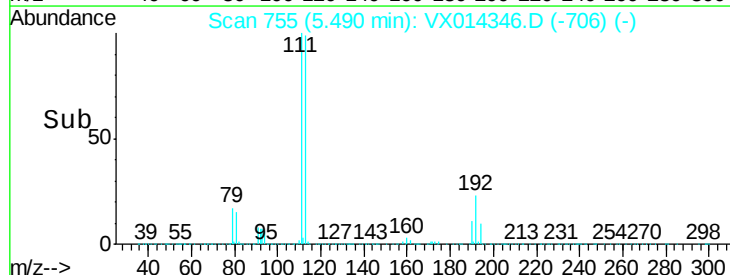

Time-->



#50

Toluene-d8

Concen: 50.535 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX014346.D

Acq: 30 Dec 2019 11:32

Instrument :

MSVOA_X

ClientSampleId :





VX1230WBL02

Tot Ion: 98 Resp: 1010905

Ion Ratio Lower Upper

98 100

100 65.5 52.9 79.3

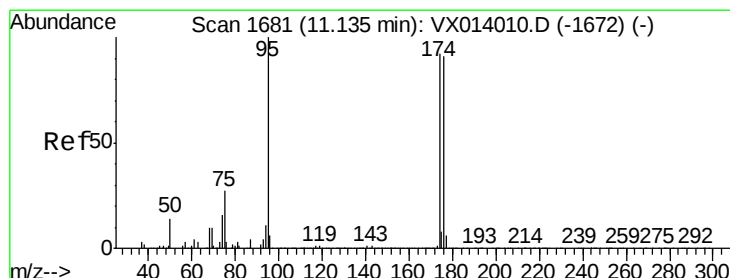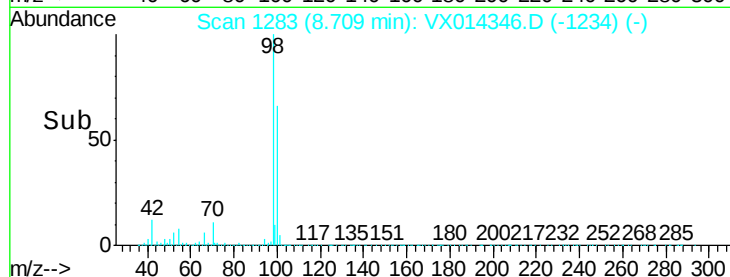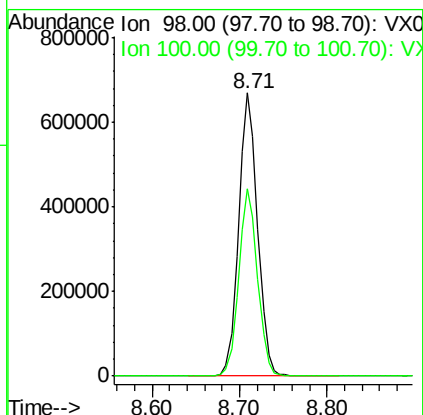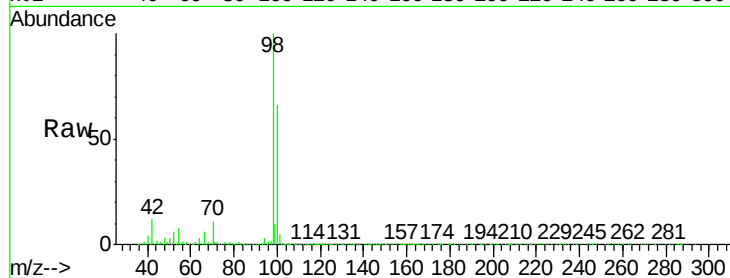

#62

4-Bromofluorobenzene

Concen: 46.403 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.01 min

Lab File: VX014346.D

Acq: 30 Dec 2019 11:32




Tgt Ion: 95 Resp: 339316


Ion Ratio Lower Upper

95 100

174 87.4 0.0 175.8

176 84.2 0.0 173.0


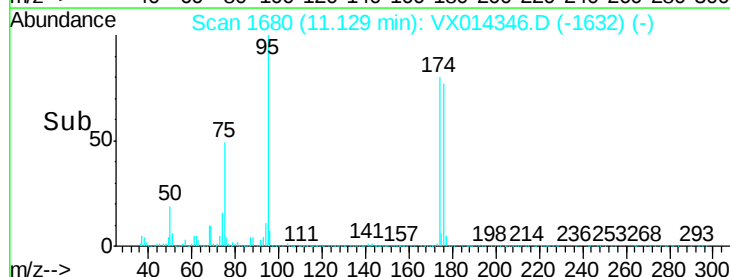
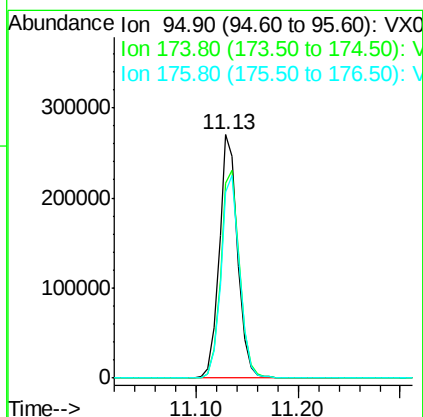
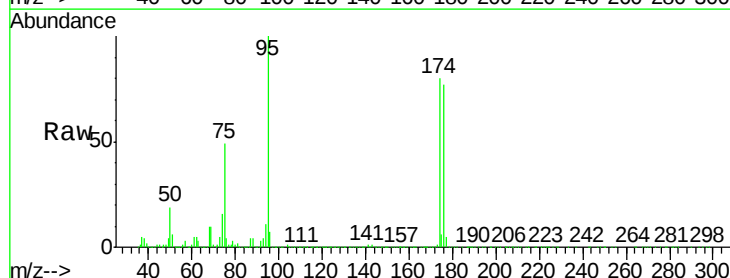


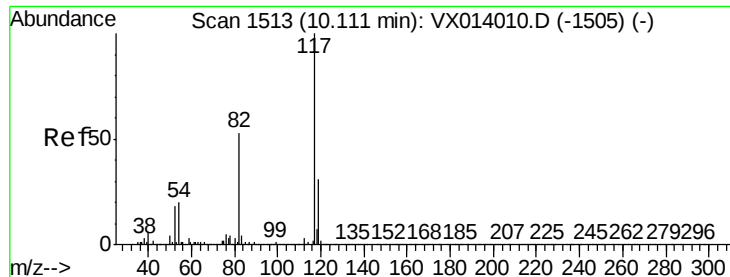

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX014346.D
Acq: 30 Dec 2019 11:32

Instrument :
MSVOA_X
ClientSampleId :
VX1230WBL02

Tot Ion	Ratio	Lower	Upper
117	100		
82	56.7	42.2	63.4
119	32.3	25.1	37.7

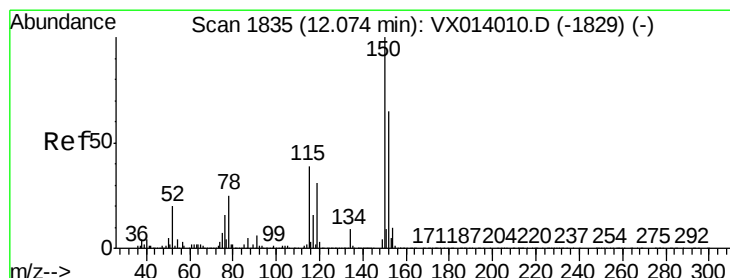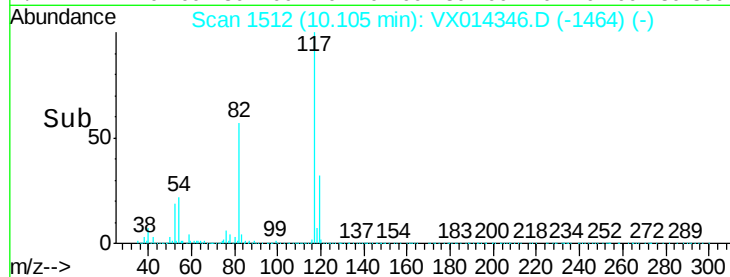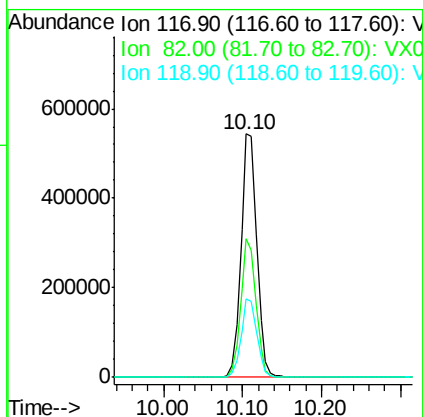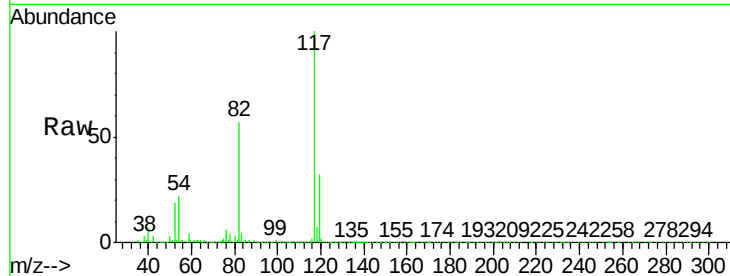

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX014346.D
Acq: 30 Dec 2019 11:32

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.0	38.3	114.9
150	157.4	0.0	345.4

