

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044536.D
 Acq On : 30 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5344-06DL 2000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Quant Time: Dec 31 01:04:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 31 01:02:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	223794	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	193329	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	80564	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	81508	39.799	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.600%		
7) Chloroethane-d5	1.648	69	75307	47.469	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.940%		
11) 1,1-Dichloroethene-d2	2.294	65	35661	40.716	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.440%		
21) 2-Butanone-d5	4.465	46	120969	96.476	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.480%		
24) Chloroform-d	5.050	84	173944	44.733	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.460%		
26) 1,2-Dichloroethane-d4	5.952	65	114952	41.803	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.600%		
32) Benzene-d6	5.970	84	317685	47.557	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.120%		
36) 1,2-Dichloropropane-d6	7.306	67	100109	48.263	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.520%		
41) Toluene-d8	8.647	98	278525	45.094	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.180%		
43) trans-1,3-Dichloroprop...	8.952	79	40379	40.509	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.020%		
47) 2-Hexanone-d5	9.384	63	79739	98.594	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.590%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	137337	49.379	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.760%		
66) 1,2-Dichlorobenzene-d4	12.317	152	95693	50.979	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.960%		
Target Compounds					Qvalue	
34) Trichloroethene	7.123	95	132082	82.405	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044536.D
Acq On : 30 Dec 2024 11:21
Operator : JC/MD
Sample : P5344-06DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Time: Dec 31 01:04:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 31 01:02:15 2024
Response via : Initial Calibration

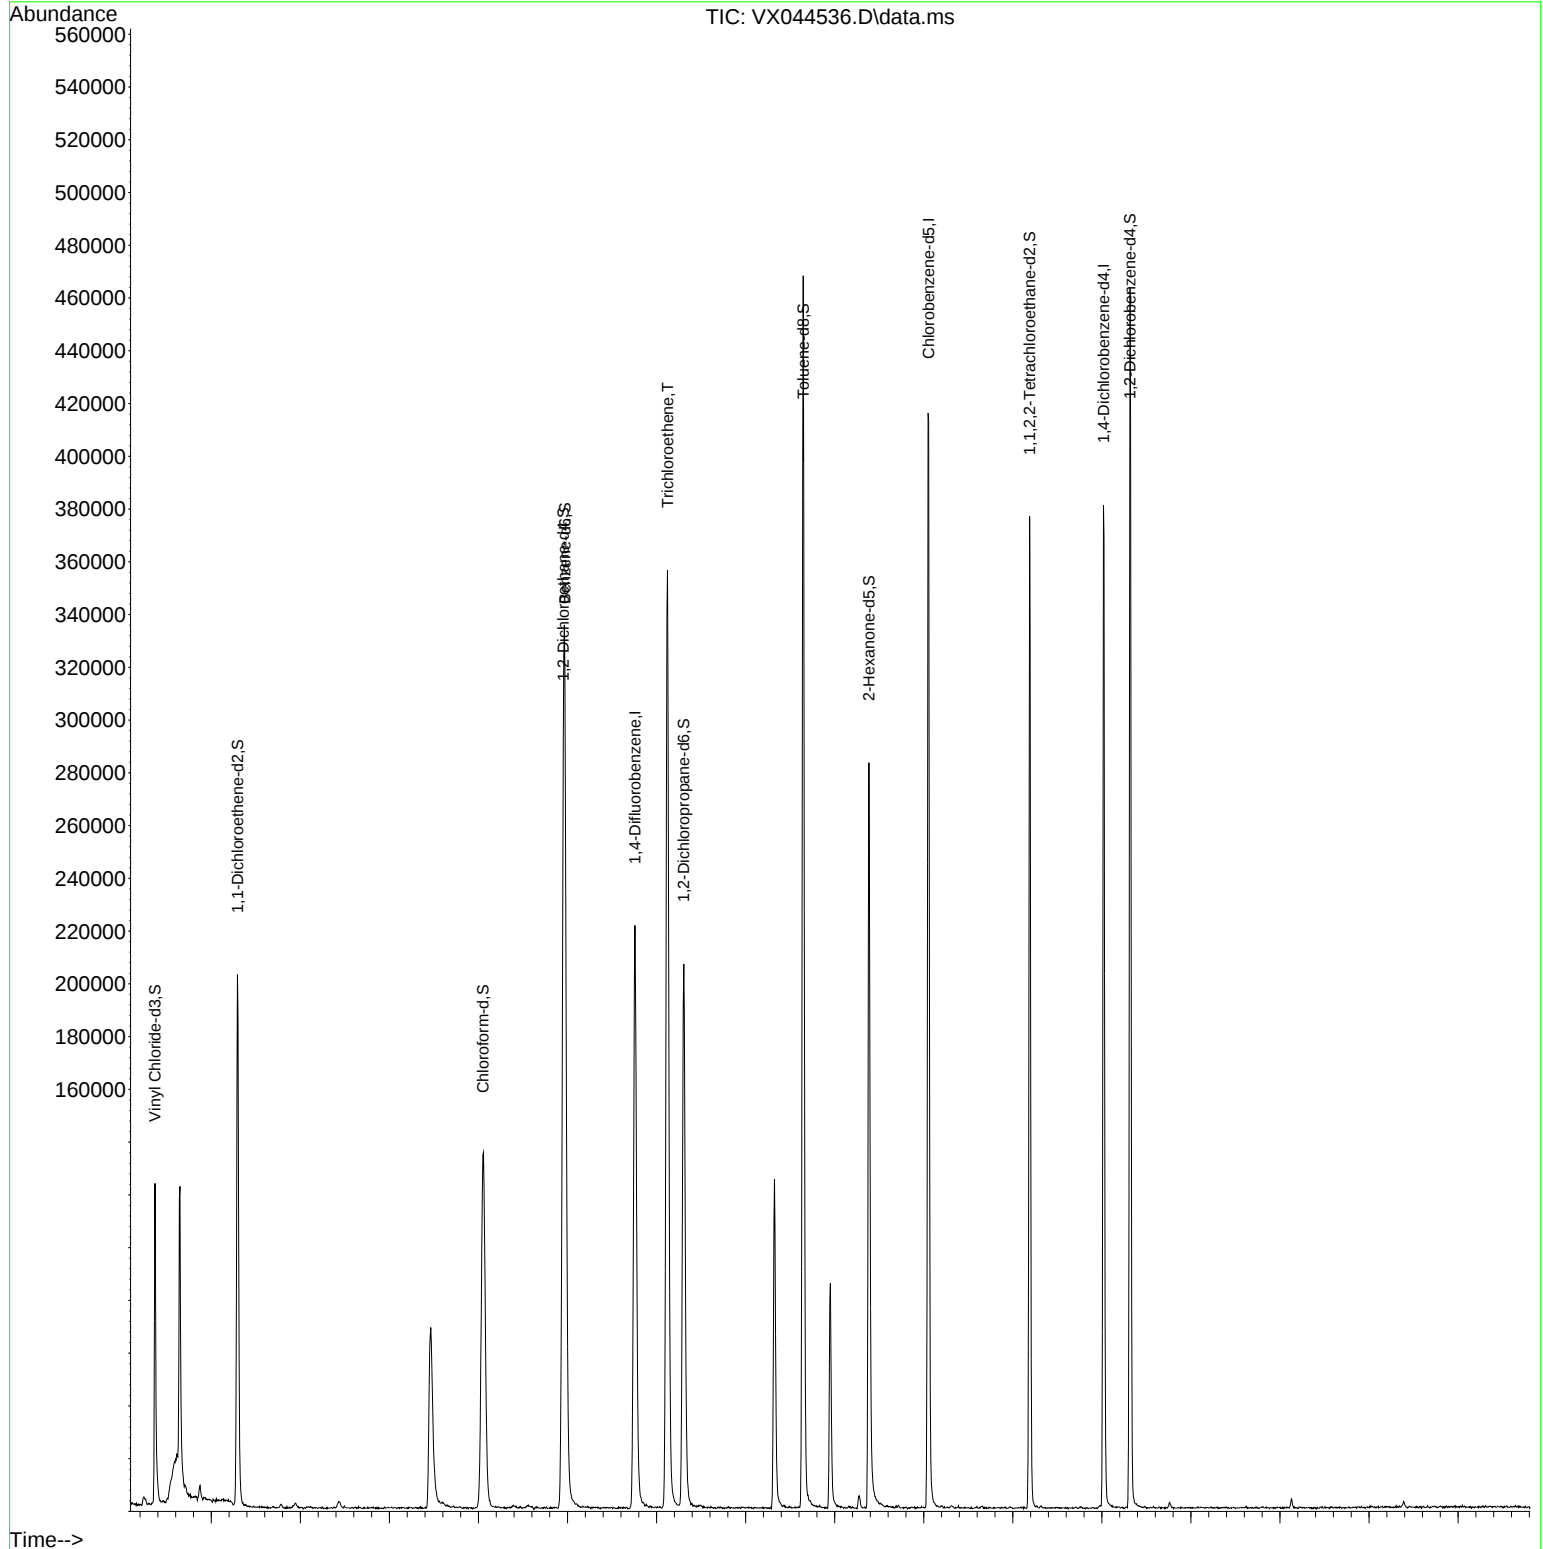

Abundance Scan 989 (7.117 min): VX044532.D\data.ms (-98

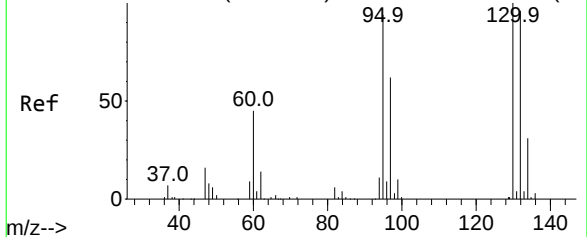

#34

Trichloroethene

Concen: 82.405 ug/L

RT: 7.123 min Scan# 99

Delta R.T. 0.006 min

Lab File: VX044536.D

Acq: 30 Dec 2024 11:21


Instrument :

MSVOA_X

ClientSampleId :

C0CE8DL

Abundance Scan 990 (7.123 min): VX044536.D\data.ms

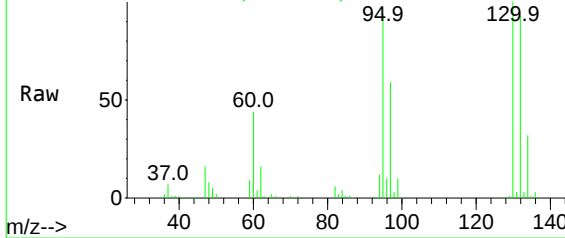

Tgt Ion: 95 Resp: 132082

Ion Ratio Lower Upper


95 100

97 63.3 45.0 83.6

132 99.5 66.6 123.8

130 106.5 72.4 134.5

Abundance

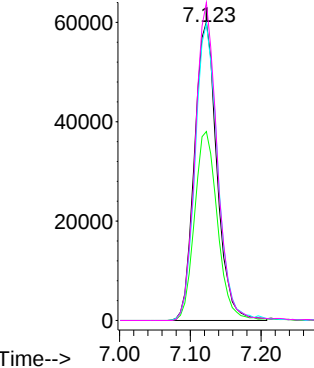

Abundance Scan 990 (7.123 min): VX044536.D\data.ms (-94

