

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044534.D
 Acq On : 30 Dec 2024 10:28
 Operator : JC/MD
 Sample : VX1230WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK749

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	23	25	28	rBV	2891	4002	0.41%	0.057%
2	1.367	42	46	56	rBV	115102	132477	13.51%	1.890%
3	1.648	88	92	100	rVB	97088	134362	13.71%	1.917%
4	2.294	192	198	212	rBV	203650	320737	32.72%	4.576%
5	2.757	272	274	275	rBV2	684	687	0.07%	0.010%
6	2.782	275	278	282	rVB5	1533	2450	0.25%	0.035%
7	2.940	298	304	311	rVB2	3629	7119	0.73%	0.102%
8	3.087	324	328	330	rBV4	1064	1760	0.18%	0.025%
9	3.324	365	367	368	rBV2	692	530	0.05%	0.008%
10	3.379	372	376	379	rVV3	778	784	0.08%	0.011%
11	3.434	381	385	391	rVV6	2235	3662	0.37%	0.052%
12	3.660	419	422	425	rBV2	660	816	0.08%	0.012%
13	3.708	428	430	433	rBV2	464	589	0.06%	0.008%
14	3.751	435	437	438	rBV	576	518	0.05%	0.007%
15	3.855	453	454	457	rVB3	664	555	0.06%	0.008%
16	3.879	457	458	460	rBV2	514	433	0.04%	0.006%
17	4.056	484	487	491	rVB3	620	1017	0.10%	0.015%
18	4.086	491	492	494	rBV2	851	470	0.05%	0.007%
19	4.190	508	509	512	rVB2	612	579	0.06%	0.008%
20	4.221	512	514	515	rBV2	658	557	0.06%	0.008%
21	4.275	521	523	525	rVB2	586	479	0.05%	0.007%
22	4.330	530	532	534	rVB2	598	458	0.05%	0.007%
23	4.397	539	543	545	rBV3	596	1027	0.10%	0.015%
24	4.458	545	553	568	rBV	68018	205072	20.92%	2.926%
25	5.050	639	650	665	rBV	131772	418057	42.65%	5.964%
26	5.257	682	684	687	rVB3	493	521	0.05%	0.007%
27	5.379	702	704	707	rBV4	979	1054	0.11%	0.015%
28	5.556	726	733	738	rBV5	1229	2799	0.29%	0.040%
29	5.659	746	750	751	rBV2	1120	1263	0.13%	0.018%
30	5.830	774	778	779	rBV2	668	690	0.07%	0.010%
31	5.958	788	799	813	rBV2	325643	980269	100.00%	13.985%
32	6.251	845	847	849	rVB2	592	515	0.05%	0.007%
33	6.623	906	908	912	rVB3	504	574	0.06%	0.008%
34	6.757	919	930	951	rBV	216463	527689	53.83%	7.528%
35	7.116	982	989	997	rBV8	4002	10862	1.11%	0.155%
36	7.305	1012	1020	1035	rBV	201926	450357	45.94%	6.425%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044534.D
 Acq On : 30 Dec 2024 10:28
 Operator : JC/MD
 Sample : VX1230WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK749

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.476	1047	1048	1054	rVB4	1186	1658	0.17%	0.024%
38	7.604	1067	1069	1072	rBV2	663	635	0.06%	0.009%
39	7.763	1094	1095	1099	rVB4	732	647	0.07%	0.009%
40	7.830	1101	1106	1111	rVV5	1060	1986	0.20%	0.028%
41	8.116	1150	1153	1155	rBV2	589	587	0.06%	0.008%
42	8.232	1169	1172	1173	rBV3	484	499	0.05%	0.007%
43	8.263	1176	1177	1181	rVB3	714	510	0.05%	0.007%
44	8.324	1181	1187	1200	rBV	124395	213527	21.78%	3.046%
45	8.409	1200	1201	1204	rVB	1326	819	0.08%	0.012%
46	8.482	1211	1213	1216	rVB4	713	634	0.06%	0.009%
47	8.586	1226	1230	1234	rBV4	1558	2991	0.31%	0.043%
48	8.647	1234	1240	1249	rBV	449443	727687	74.23%	10.382%
49	8.951	1284	1290	1301	rBV	85112	136422	13.92%	1.946%
50	9.159	1322	1324	1328	rVB3	1242	1106	0.11%	0.016%
51	9.281	1338	1344	1347	rBV4	2030	3048	0.31%	0.043%
52	9.384	1356	1361	1375	rBV	279094	434492	44.32%	6.199%
53	9.695	1408	1412	1420	rVB8	950	2247	0.23%	0.032%
54	9.890	1440	1444	1446	rVB3	498	759	0.08%	0.011%
55	10.049	1465	1470	1485	rBV	404367	601613	61.37%	8.583%
56	10.195	1490	1494	1499	rBV2	2628	4646	0.47%	0.066%
57	10.311	1509	1513	1517	rVB2	2455	3166	0.32%	0.045%
58	10.451	1534	1536	1539	rVV2	817	553	0.06%	0.008%
59	10.494	1541	1543	1546	rBV2	682	721	0.07%	0.010%
60	10.561	1553	1554	1557	rVB2	582	440	0.04%	0.006%
61	10.610	1557	1562	1564	rBV4	446	802	0.08%	0.011%
62	10.646	1564	1568	1576	rVV4	3094	6398	0.65%	0.091%
63	10.969	1616	1621	1627	rBV4	2720	4766	0.49%	0.068%
64	11.043	1630	1633	1634	rBV	536	472	0.05%	0.007%
65	11.079	1637	1639	1642	rBV4	467	549	0.06%	0.008%
66	11.189	1652	1657	1664	rBV	376161	481850	49.15%	6.875%
67	11.305	1672	1676	1679	rBV4	626	1160	0.12%	0.017%
68	11.457	1696	1701	1706	rBV3	2079	3121	0.32%	0.045%
69	11.500	1706	1708	1710	rVB2	675	559	0.06%	0.008%
70	11.536	1713	1714	1716	rBV2	539	438	0.04%	0.006%
71	11.610	1724	1726	1728	rBV3	486	578	0.06%	0.008%
72	11.756	1747	1750	1755	rVB2	2732	3077	0.31%	0.044%
73	11.841	1763	1764	1766	rVB2	813	554	0.06%	0.008%
74	11.866	1766	1768	1769	rBV	624	443	0.05%	0.006%
75	11.975	1783	1786	1788	rBV4	2102	2914	0.30%	0.042%
76	12.018	1788	1793	1806	rVV	372789	505402	51.56%	7.211%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044534.D
 Acq On : 30 Dec 2024 10:28
 Operator : JC/MD
 Sample : VX1230WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK749

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1851	rBV	466197	604569	61.67%	8.625%
78	12.768	1911	1916	1922	rVV4	2379	3700	0.38%	0.053%
79	12.939	1941	1944	1946	rBV3	605	769	0.08%	0.011%
80	13.018	1955	1957	1959	rBV2	724	594	0.06%	0.008%
81	13.121	1969	1974	1979	rBV5	2221	3886	0.40%	0.055%
82	13.445	2025	2027	2031	rVB3	701	739	0.08%	0.011%
83	13.597	2049	2052	2056	rVV4	1571	2196	0.22%	0.031%
84	13.780	2079	2082	2088	rVV2	2597	3488	0.36%	0.050%
85	13.920	2103	2105	2107	rVV2	733	499	0.05%	0.007%
86	13.963	2109	2112	2116	rVB4	1717	2334	0.24%	0.033%
87	14.127	2135	2139	2145	rBV	3327	4556	0.46%	0.065%
88	14.408	2182	2185	2189	rBV2	574	704	0.07%	0.010%
89	14.457	2189	2193	2195	rVB2	558	861	0.09%	0.012%
90	14.481	2195	2197	2200	rBV3	521	526	0.05%	0.008%
91	14.615	2217	2219	2222	rBV3	507	661	0.07%	0.009%
92	14.688	2230	2231	2233	rBV2	786	554	0.06%	0.008%
93	14.828	2253	2254	2256	rBV2	734	562	0.06%	0.008%
94	15.048	2289	2290	2292	rBV	777	598	0.06%	0.009%
95	15.255	2323	2324	2327	rVB3	891	638	0.07%	0.009%
96	15.280	2327	2328	2332	rBV3	763	1151	0.12%	0.016%
97	15.389	2344	2346	2353	rVB4	2449	3713	0.38%	0.053%
98	15.493	2361	2363	2365	rBV3	521	456	0.05%	0.007%
99	16.011	2444	2448	2449	rBV2	492	568	0.06%	0.008%
100	16.420	2513	2515	2520	rVB3	600	634	0.06%	0.009%

Sum of corrected areas: 7009222




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044534.D
Acq On : 30 Dec 2024 10:28
Operator : JC/MD
Sample : VX1230WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK749

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

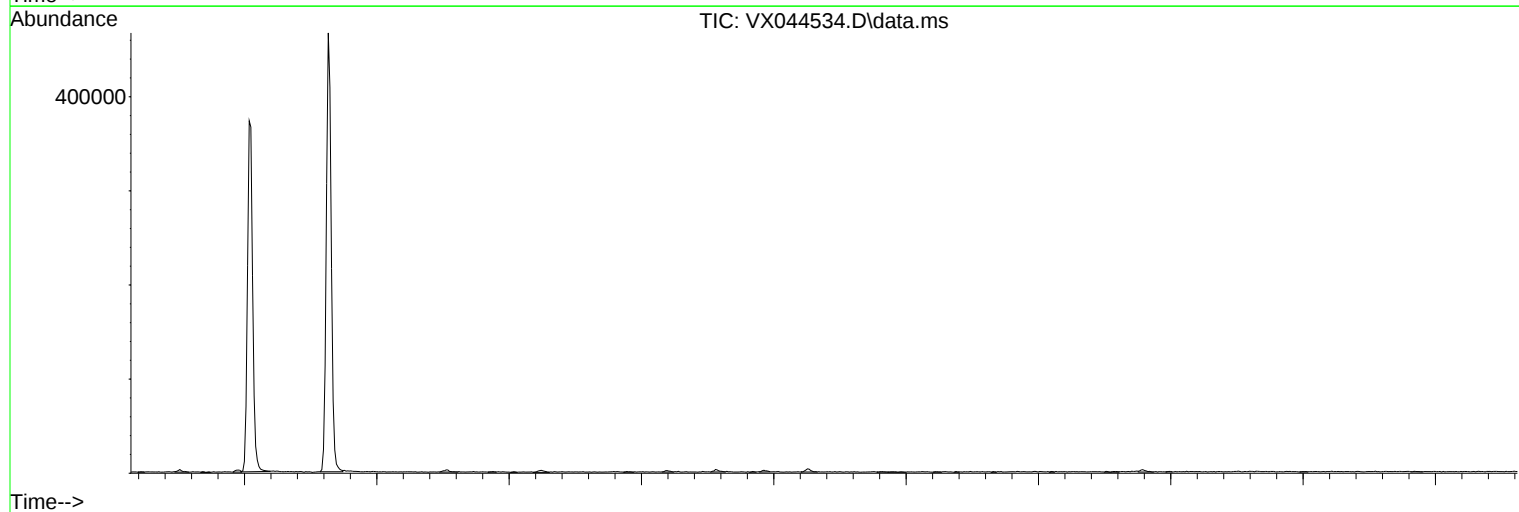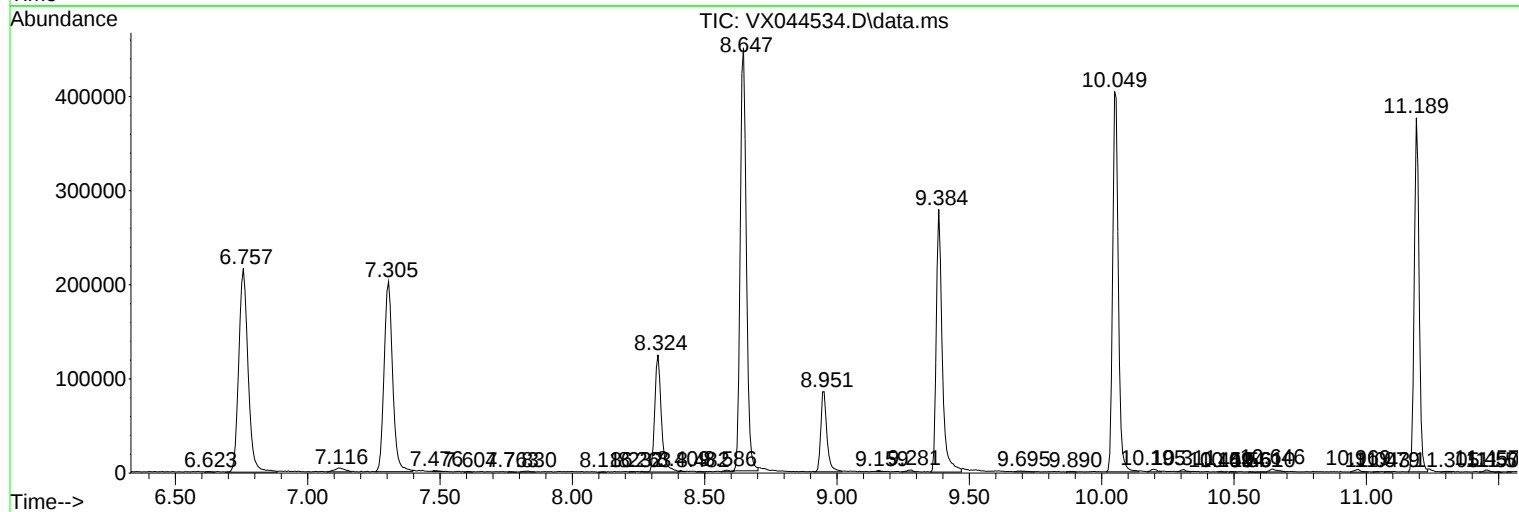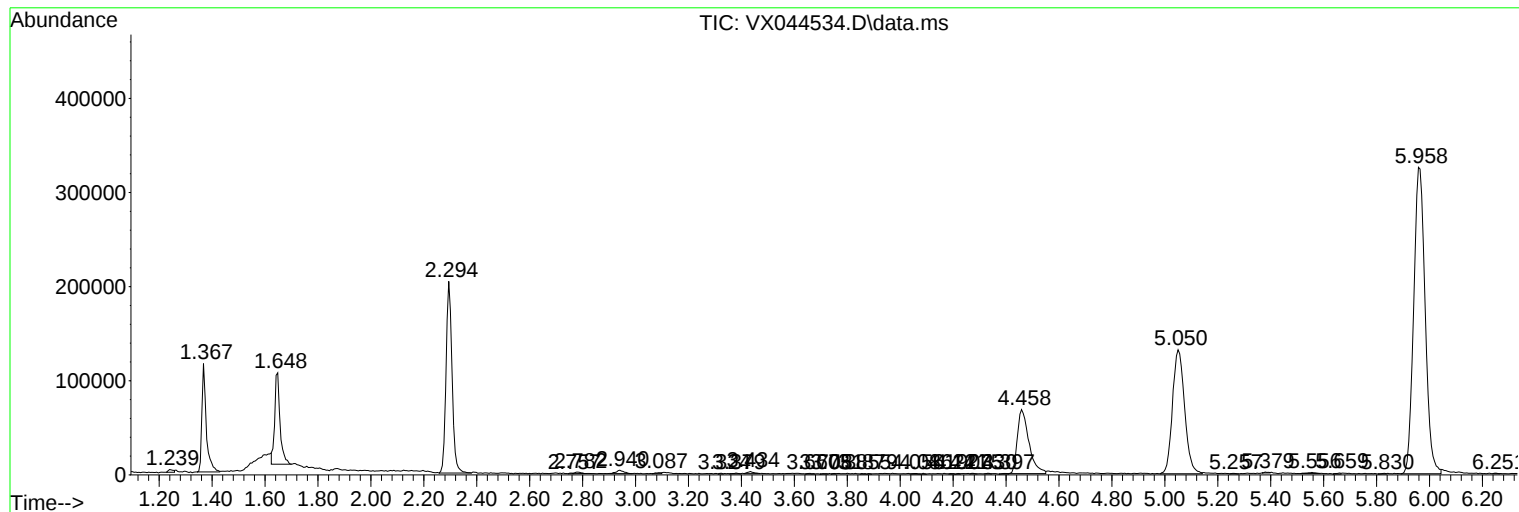

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044534.D
Acq On : 30 Dec 2024 10:28
Operator : JC/MD
Sample : VX1230WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK749

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044534.D
Acq On : 30 Dec 2024 10:28
Operator : JC/MD
Sample : VX1230WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK749

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
