

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044536.D
 Acq On : 30 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5344-06DL 2000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	28	rBV3	3206	5261	0.52%	0.067%
2	1.368	42	46	57	rBV	121142	137607	13.71%	1.759%
3	1.648	88	92	100	rVB	113903	153065	15.25%	1.957%
4	2.294	192	198	211	rVB	201285	321929	32.08%	4.116%
5	2.782	275	278	284	rVB5	1557	2593	0.26%	0.033%
6	2.873	291	293	294	rBV	436	257	0.03%	0.003%
7	2.916	298	300	301	rBV	858	630	0.06%	0.008%
8	3.044	319	321	323	rBV2	547	581	0.06%	0.007%
9	3.069	323	325	326	rBV	619	440	0.04%	0.006%
10	3.245	353	354	356	rVB2	772	533	0.05%	0.007%
11	3.270	356	358	361	rBV3	279	327	0.03%	0.004%
12	3.379	373	376	378	rBV2	597	574	0.06%	0.007%
13	3.428	380	384	393	rVB4	2491	5981	0.60%	0.076%
14	3.495	393	395	397	rBV	793	641	0.06%	0.008%
15	3.605	412	413	414	rBV	461	309	0.03%	0.004%
16	3.654	420	421	422	rBV	719	353	0.04%	0.005%
17	3.776	440	441	444	rBV2	387	471	0.05%	0.006%
18	3.843	450	452	453	rVB2	542	303	0.03%	0.004%
19	3.861	453	455	458	rBV2	630	628	0.06%	0.008%
20	3.946	467	469	470	rBV	600	396	0.04%	0.005%
21	4.337	531	533	534	rBV	530	367	0.04%	0.005%
22	4.465	545	554	568	rBV	68530	209073	20.83%	2.673%
23	4.837	613	615	616	rBV2	491	284	0.03%	0.004%
24	4.873	620	621	623	rVB	614	354	0.04%	0.005%
25	4.904	623	626	628	rBV3	584	789	0.08%	0.010%
26	4.940	631	632	635	rBV2	519	433	0.04%	0.006%
27	5.056	639	651	668	rVV	134589	423288	42.17%	5.412%
28	5.367	701	702	703	rBV	565	294	0.03%	0.004%
29	5.391	703	706	710	rVV4	950	1442	0.14%	0.018%
30	5.629	744	745	746	rBV	621	428	0.04%	0.005%
31	5.647	746	748	749	rVV2	550	408	0.04%	0.005%
32	5.763	765	767	769	rVB3	596	425	0.04%	0.005%
33	5.806	773	774	776	rVV2	568	257	0.03%	0.003%
34	5.964	787	800	821	rBV2	335058	1003675	100.00%	12.833%
35	6.275	849	851	852	rBV2	629	535	0.05%	0.007%
36	6.373	866	867	868	rBV	477	293	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044536.D
 Acq On : 30 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5344-06DL 2000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	6.574	899	900	903	rBV3	605	477	0.05%	0.006%
38	6.629	908	909	912	rBV3	568	520	0.05%	0.007%
39	6.665	912	915	917	rVB3	630	649	0.06%	0.008%
40	6.757	919	930	944	rBV	221144	524350	52.24%	6.704%
41	7.123	980	990	1011	rBV	355601	791238	78.83%	10.117%
42	7.306	1012	1020	1033	rVV	205199	448711	44.71%	5.737%
43	7.610	1068	1070	1072	rBV3	591	346	0.03%	0.004%
44	7.690	1081	1083	1085	rBV3	644	569	0.06%	0.007%
45	7.714	1085	1087	1088	rBV	504	259	0.03%	0.003%
46	7.805	1099	1102	1104	rBV3	680	627	0.06%	0.008%
47	7.952	1125	1126	1128	rBV2	594	535	0.05%	0.007%
48	8.037	1139	1140	1143	rBV2	444	413	0.04%	0.005%
49	8.098	1148	1150	1151	rBV	473	388	0.04%	0.005%
50	8.281	1178	1180	1181	rVB	554	351	0.03%	0.004%
51	8.324	1181	1187	1202	rBV	124897	213728	21.29%	2.733%
52	8.647	1234	1240	1252	rBV	466852	741697	73.90%	9.483%
53	8.909	1282	1283	1285	rBV2	384	276	0.03%	0.004%
54	8.952	1285	1290	1306	rBV	85367	136963	13.65%	1.751%
55	9.110	1314	1316	1318	rBV3	387	285	0.03%	0.004%
56	9.202	1328	1331	1332	rBV	561	415	0.04%	0.005%
57	9.275	1339	1343	1349	rBV6	4919	8579	0.85%	0.110%
58	9.384	1356	1361	1381	rBV	282638	443582	44.20%	5.672%
59	9.689	1409	1411	1413	rBV	821	584	0.06%	0.007%
60	9.830	1432	1434	1435	rBV2	429	347	0.03%	0.004%
61	9.927	1449	1450	1453	rBV2	504	342	0.03%	0.004%
62	9.976	1456	1458	1460	rBV3	628	419	0.04%	0.005%
63	10.049	1465	1470	1486	rBV	415048	606014	60.38%	7.749%
64	10.390	1524	1526	1528	rVB2	955	546	0.05%	0.007%
65	10.537	1549	1550	1552	rVB2	603	261	0.03%	0.003%
66	11.116	1643	1645	1646	rVB2	778	456	0.05%	0.006%
67	11.189	1652	1657	1668	rBV	375876	485321	48.35%	6.205%
68	11.311	1674	1677	1678	rBV2	726	662	0.07%	0.008%
69	11.628	1728	1729	1733	rBV3	499	743	0.07%	0.010%
70	11.762	1747	1751	1754	rBV5	664	1017	0.10%	0.013%
71	11.829	1760	1762	1765	rBV2	490	540	0.05%	0.007%
72	11.975	1782	1786	1788	rBV3	1118	1756	0.17%	0.022%
73	12.018	1788	1793	1810	rVB	380132	500757	49.89%	6.403%
74	12.268	1832	1834	1837	rBV3	584	831	0.08%	0.011%
75	12.317	1837	1842	1853	rBV	462595	609566	60.73%	7.794%
76	12.579	1883	1885	1889	rVV3	608	621	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044536.D
 Acq On : 30 Dec 2024 11:21
 Operator : JC/MD
 Sample : P5344-06DL 2000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CE8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.640	1893	1895	1898	rVB4	592	693	0.07%	0.009%
78	12.725	1907	1909	1910	rBV2	489	386	0.04%	0.005%
79	12.762	1910	1915	1919	rVV4	2218	3365	0.34%	0.043%
80	12.890	1935	1936	1937	rBV	574	282	0.03%	0.004%
81	13.689	2065	2067	2070	rVV3	423	345	0.03%	0.004%
82	14.128	2135	2139	2144	rBV	3536	4819	0.48%	0.062%
83	14.225	2151	2155	2157	rBV3	671	990	0.10%	0.013%
84	14.371	2177	2179	2180	rBV2	418	300	0.03%	0.004%
85	14.420	2185	2187	2188	rBV2	668	494	0.05%	0.006%
86	14.457	2190	2193	2195	rBV2	523	635	0.06%	0.008%
87	14.737	2237	2239	2240	rBV2	424	293	0.03%	0.004%
88	14.871	2259	2261	2263	rBV3	580	705	0.07%	0.009%
89	14.914	2266	2268	2270	rBV2	636	479	0.05%	0.006%
90	15.085	2295	2296	2298	rBV	411	373	0.04%	0.005%
91	15.304	2330	2332	2333	rVB	767	404	0.04%	0.005%
92	15.341	2337	2338	2340	rBV2	617	410	0.04%	0.005%
93	15.450	2354	2356	2360	rBV3	599	743	0.07%	0.010%
94	15.572	2374	2376	2379	rVB3	814	951	0.09%	0.012%
95	15.609	2379	2382	2385	rBV3	775	1107	0.11%	0.014%
96	16.048	2453	2454	2456	rBV	773	409	0.04%	0.005%
97	16.158	2471	2472	2474	rBV2	603	538	0.05%	0.007%
98	16.243	2484	2486	2488	rBV2	562	455	0.05%	0.006%
99	16.517	2529	2531	2532	rBV2	695	430	0.04%	0.005%
100	16.694	2558	2560	2561	rBV2	655	397	0.04%	0.005%

Sum of corrected areas: 7820968




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044536.D
Acq On : 30 Dec 2024 11:21
Operator : JC/MD
Sample : P5344-06DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

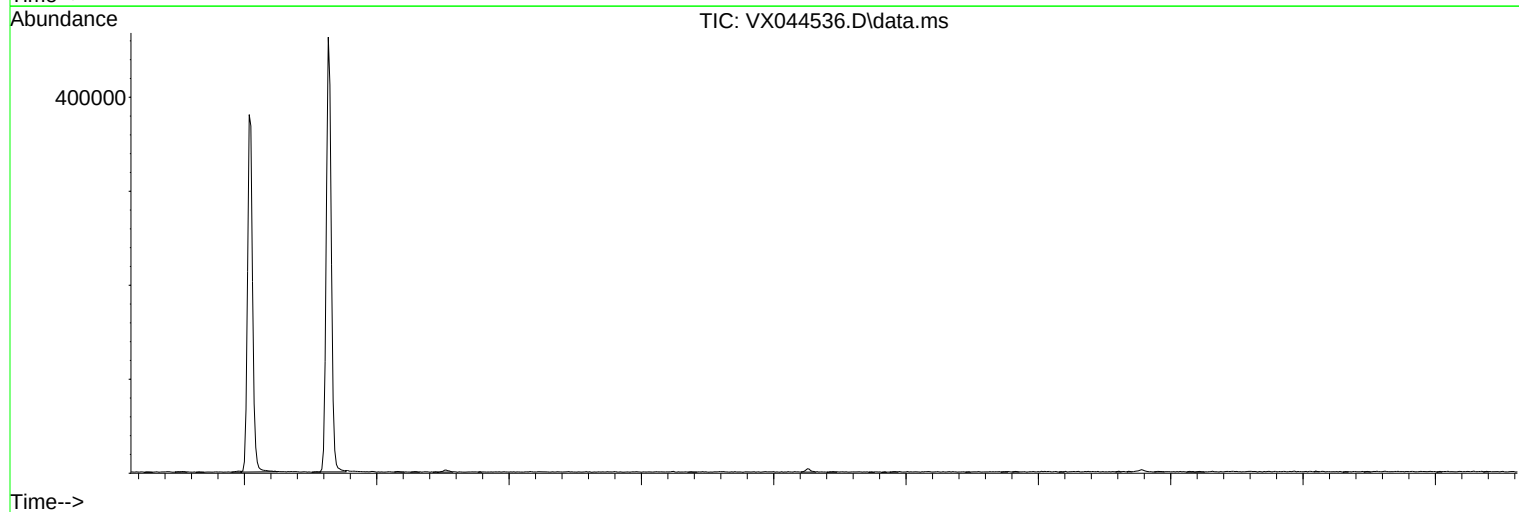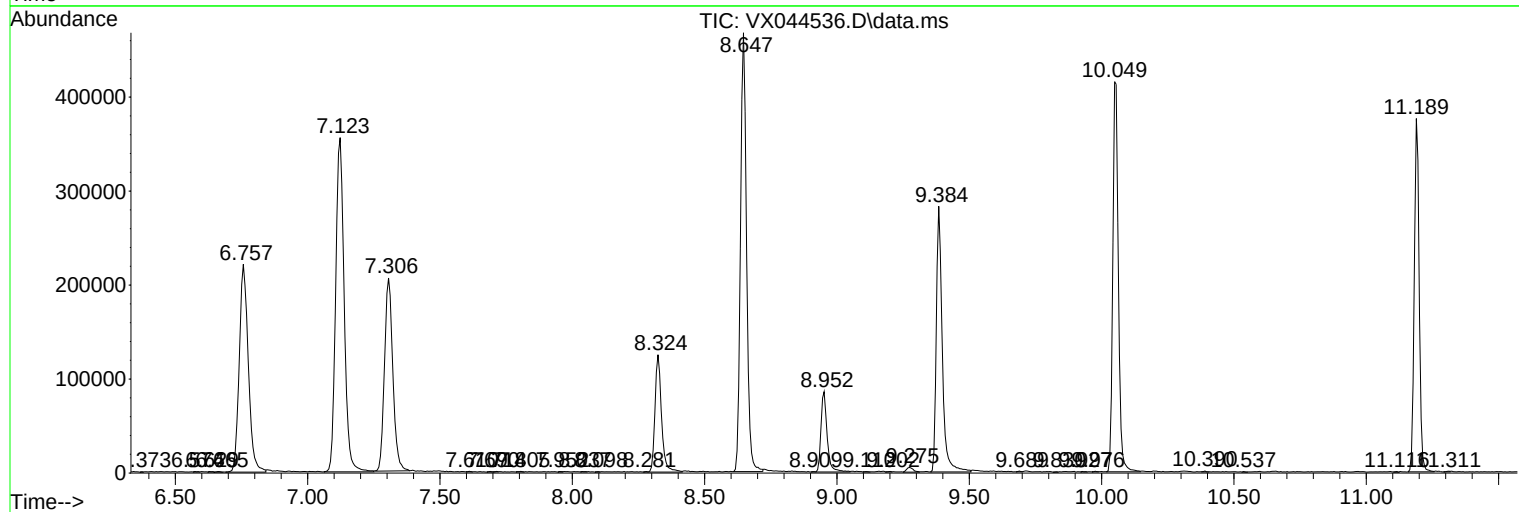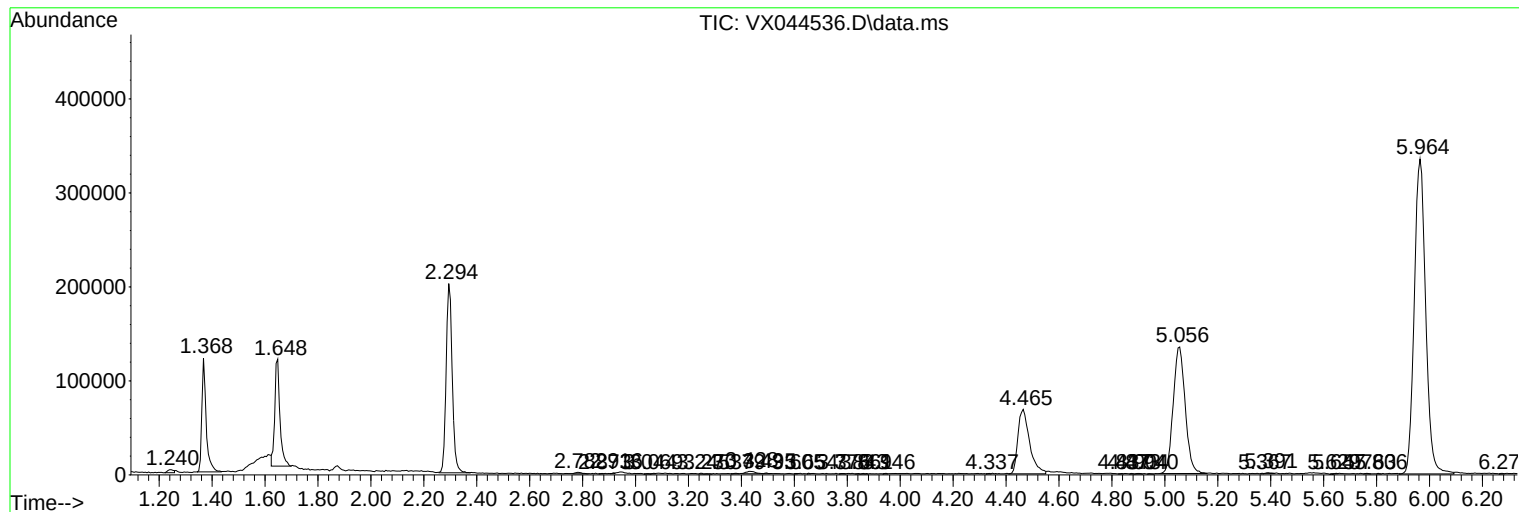

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044536.D
Acq On : 30 Dec 2024 11:21
Operator : JC/MD
Sample : P5344-06DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044536.D
Acq On : 30 Dec 2024 11:21
Operator : JC/MD
Sample : P5344-06DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CE8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
