

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044537.D
 Acq On : 30 Dec 2024 11:45
 Operator : JC/MD
 Sample : P5344-12DL 8000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M

Title : VOC Analysis

Signal : TIC: VX044537.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	27	rBV	3684	3594	0.36%	0.048%
2	1.294	32	34	37	rBV4	1449	1392	0.14%	0.019%
3	1.368	42	46	56	rBV	117947	131919	13.36%	1.767%
4	1.593	70	83	84	rBV2	15433	47294	4.79%	0.634%
5	1.648	88	92	100	rVB	107731	150524	15.25%	2.017%
6	2.294	192	198	208	rBV	203284	314476	31.86%	4.213%
7	2.782	276	278	284	rVB3	1935	2756	0.28%	0.037%
8	2.843	284	288	290	rBV2	634	1081	0.11%	0.014%
9	2.940	299	304	309	rBV5	3171	7041	0.71%	0.094%
10	3.056	319	323	325	rVB2	726	805	0.08%	0.011%
11	3.093	325	329	330	rBV2	451	496	0.05%	0.007%
12	3.105	330	331	335	rBV2	532	823	0.08%	0.011%
13	3.331	366	368	371	rBV2	595	746	0.08%	0.010%
14	3.440	380	386	394	rVV5	2961	7101	0.72%	0.095%
15	3.611	413	414	416	rBV	689	518	0.05%	0.007%
16	3.660	419	422	425	rBV3	445	633	0.06%	0.008%
17	3.757	436	438	441	rBV3	675	757	0.08%	0.010%
18	3.867	454	456	459	rBV2	465	520	0.05%	0.007%
19	4.123	496	498	500	rBV2	696	606	0.06%	0.008%
20	4.233	514	516	519	rBV2	645	516	0.05%	0.007%
21	4.410	542	545	546	rBV3	611	594	0.06%	0.008%
22	4.458	546	553	572	rBV	67664	210725	21.35%	2.823%
23	4.745	598	600	604	rBV4	640	1105	0.11%	0.015%
24	4.800	606	609	612	rBV2	567	760	0.08%	0.010%
25	4.940	630	632	638	rVB3	517	614	0.06%	0.008%
26	5.050	638	650	667	rBV	133770	421091	42.66%	5.642%
27	5.422	710	711	714	rBV2	687	736	0.07%	0.010%
28	5.684	752	754	757	rVV4	536	615	0.06%	0.008%
29	5.787	768	771	774	rBV3	564	762	0.08%	0.010%
30	5.879	780	786	789	rBV4	462	749	0.08%	0.010%
31	5.964	789	800	822	rBV3	332121	987174	100.00%	13.226%
32	6.202	837	839	842	rVB4	645	480	0.05%	0.006%
33	6.330	854	860	862	rVV3	393	765	0.08%	0.010%
34	6.361	862	865	866	rVV2	681	500	0.05%	0.007%
35	6.385	866	869	870	rVV2	545	531	0.05%	0.007%
36	6.757	921	930	949	rBV	221752	538837	54.58%	7.219%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044537.D
 Acq On : 30 Dec 2024 11:45
 Operator : JC/MD
 Sample : P5344-12DL 8000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	6.988	963	968	969	rBV3	779	800	0.08%	0.011%
38	7.123	980	990	1004	rBV	186230	420305	42.58%	5.631%
39	7.305	1012	1020	1036	rBV	203194	448903	45.47%	6.014%
40	7.574	1063	1064	1068	rBV2	513	608	0.06%	0.008%
41	8.208	1165	1168	1170	rBV3	430	550	0.06%	0.007%
42	8.324	1181	1187	1199	rBV	118778	205605	20.83%	2.755%
43	8.482	1212	1213	1217	rVB2	596	575	0.06%	0.008%
44	8.519	1217	1219	1224	rBV4	519	915	0.09%	0.012%
45	8.647	1233	1240	1251	rBV	464931	735231	74.48%	9.850%
46	8.836	1268	1271	1274	rBV4	626	917	0.09%	0.012%
47	8.952	1283	1290	1304	rBV	84735	133559	13.53%	1.789%
48	9.147	1320	1322	1327	rBV2	760	1092	0.11%	0.015%
49	9.275	1339	1343	1348	rVB3	3730	6044	0.61%	0.081%
50	9.384	1356	1361	1384	rBV	279579	447225	45.30%	5.992%
51	9.616	1397	1399	1403	rVB3	578	486	0.05%	0.007%
52	9.701	1411	1413	1417	rVB2	916	988	0.10%	0.013%
53	9.939	1447	1452	1453	rBV3	495	744	0.08%	0.010%
54	10.055	1465	1471	1491	rBV	426370	615154	62.31%	8.241%
55	10.281	1505	1508	1510	rBV3	905	1154	0.12%	0.015%
56	10.457	1533	1537	1538	rBV3	485	610	0.06%	0.008%
57	10.713	1577	1579	1581	rVV2	517	478	0.05%	0.006%
58	10.860	1602	1603	1606	rVB2	936	686	0.07%	0.009%
59	11.000	1623	1626	1628	rVB2	506	514	0.05%	0.007%
60	11.097	1638	1642	1643	rBV2	522	545	0.06%	0.007%
61	11.189	1652	1657	1667	rBV	382980	473929	48.01%	6.349%
62	11.317	1675	1678	1680	rVB4	1027	822	0.08%	0.011%
63	11.335	1680	1681	1684	rBV	498	593	0.06%	0.008%
64	11.530	1711	1713	1718	rVB3	703	685	0.07%	0.009%
65	11.573	1718	1720	1722	rBV2	426	488	0.05%	0.007%
66	11.677	1733	1737	1740	rBV4	435	732	0.07%	0.010%
67	11.719	1743	1744	1747	rVB2	773	531	0.05%	0.007%
68	11.975	1784	1786	1788	rBV3	1018	1131	0.11%	0.015%
69	12.018	1788	1793	1804	rBV	383747	499280	50.58%	6.689%
70	12.317	1837	1842	1851	rBV	462714	591121	59.88%	7.919%
71	12.451	1862	1864	1869	rBV3	423	557	0.06%	0.007%
72	12.731	1907	1910	1911	rBV2	626	632	0.06%	0.008%
73	12.762	1911	1915	1919	rVB3	2793	4114	0.42%	0.055%
74	12.878	1933	1934	1939	rBV4	613	995	0.10%	0.013%
75	13.036	1958	1960	1965	rVB4	442	795	0.08%	0.011%
76	13.097	1965	1970	1972	rBV3	391	492	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
 Data File : VX044537.D
 Acq On : 30 Dec 2024 11:45
 Operator : JC/MD
 Sample : P5344-12DL 8000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0CH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.201	1985	1987	1989	rVB2	695	515	0.05%	0.007%
78	13.365	2011	2014	2015	rBV2	473	494	0.05%	0.007%
79	13.426	2021	2024	2025	rBV2	458	505	0.05%	0.007%
80	13.457	2028	2029	2034	rVB3	729	868	0.09%	0.012%
81	13.506	2034	2037	2038	rBV2	429	497	0.05%	0.007%
82	13.676	2062	2065	2066	rBV	466	542	0.05%	0.007%
83	14.073	2127	2130	2131	rBV3	484	515	0.05%	0.007%
84	14.134	2136	2140	2144	rVV	3863	5204	0.53%	0.070%
85	14.310	2165	2169	2173	rBV4	346	497	0.05%	0.007%
86	14.414	2184	2186	2188	rVB3	776	678	0.07%	0.009%
87	14.902	2264	2266	2268	rBV3	499	516	0.05%	0.007%
88	15.078	2294	2295	2297	rBV2	757	666	0.07%	0.009%
89	15.176	2308	2311	2317	rBV4	978	1461	0.15%	0.020%
90	15.280	2326	2328	2330	rBV3	501	638	0.06%	0.009%
91	15.389	2342	2346	2350	rBV3	2091	3691	0.37%	0.049%
92	15.469	2355	2359	2360	rBV4	647	673	0.07%	0.009%
93	15.542	2367	2371	2375	rBV3	619	980	0.10%	0.013%
94	15.676	2390	2393	2397	rVV3	576	1004	0.10%	0.013%
95	15.944	2433	2437	2438	rBV2	577	519	0.05%	0.007%
96	16.164	2470	2473	2476	rVB3	700	881	0.09%	0.012%
97	16.493	2524	2527	2528	rBV3	682	610	0.06%	0.008%
98	16.529	2531	2533	2535	rBV3	799	642	0.07%	0.009%
99	16.651	2550	2553	2554	rBV2	787	762	0.08%	0.010%
100	16.670	2554	2556	2557	rBV2	1062	573	0.06%	0.008%

Sum of corrected areas: 7464152




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044537.D
Acq On : 30 Dec 2024 11:45
Operator : JC/MD
Sample : P5344-12DL 8000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

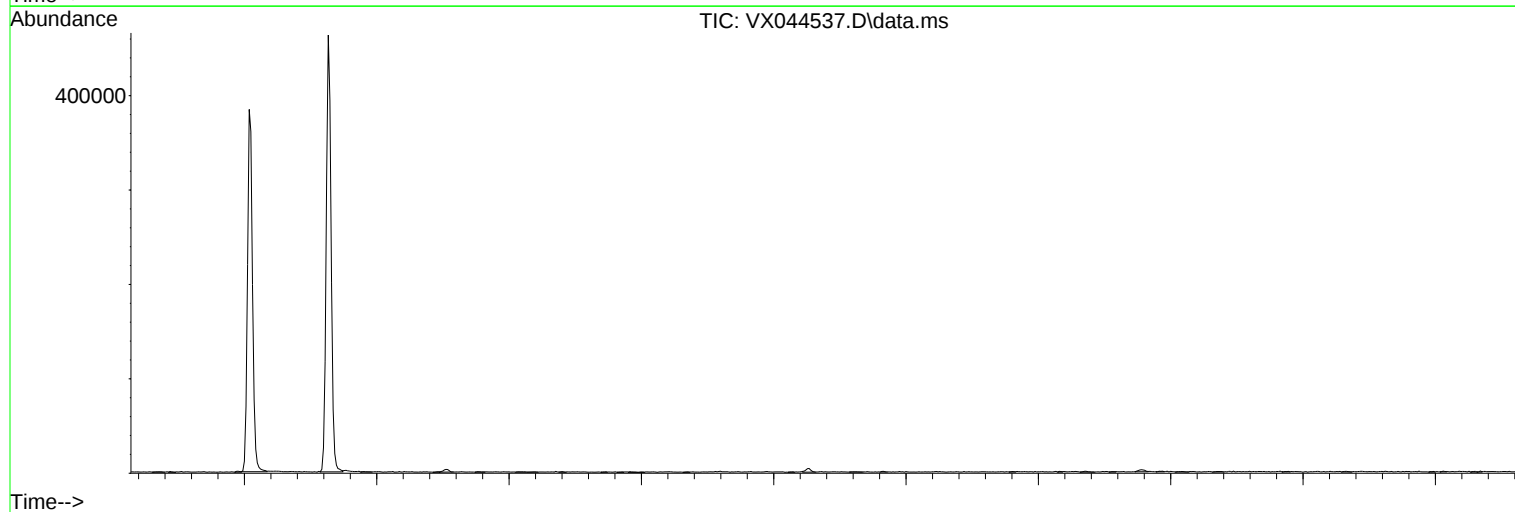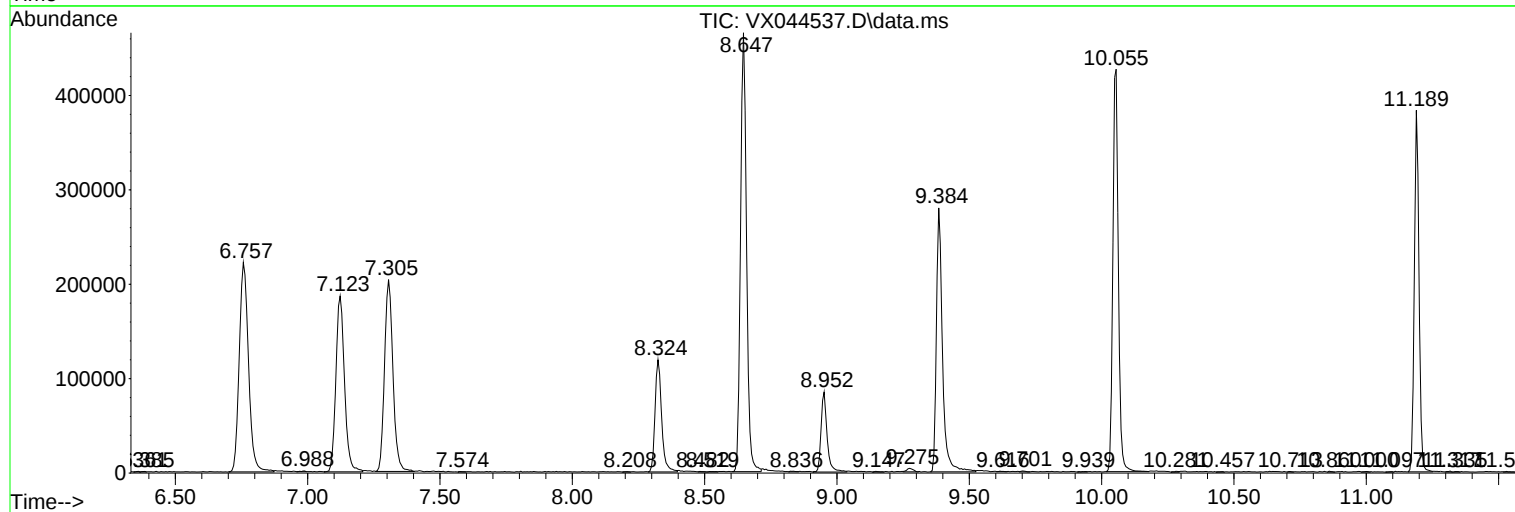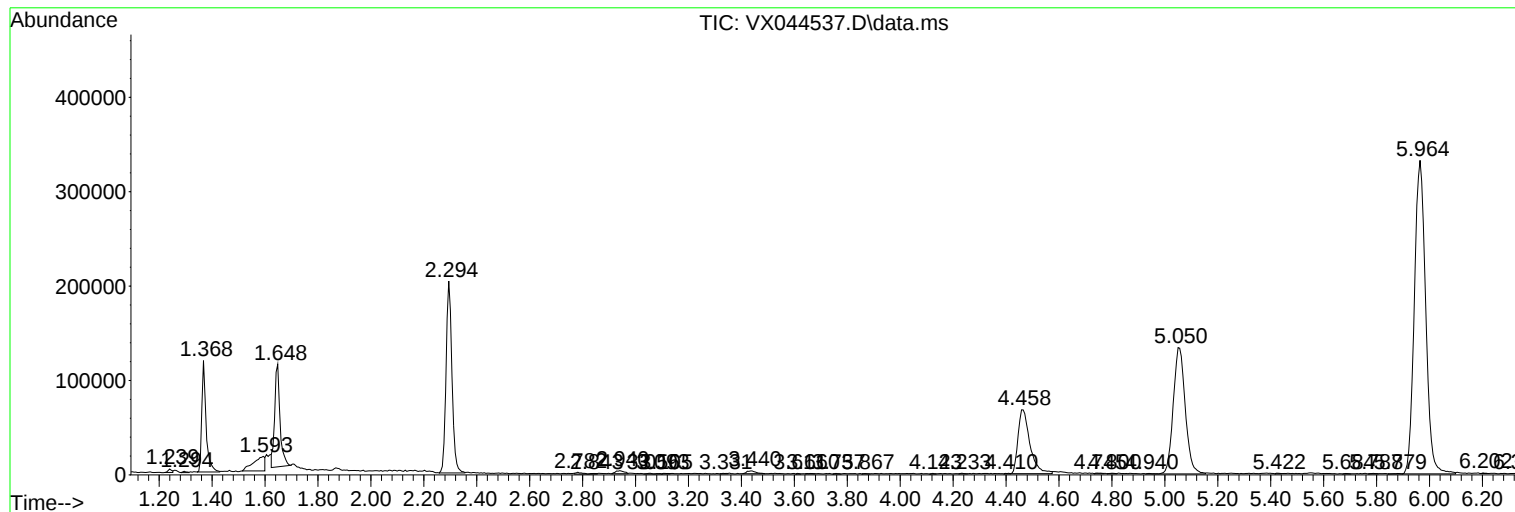

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044537.D
Acq On : 30 Dec 2024 11:45
Operator : JC/MD
Sample : P5344-12DL 8000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044537.D
Acq On : 30 Dec 2024 11:45
Operator : JC/MD
Sample : P5344-12DL 8000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0CH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc