
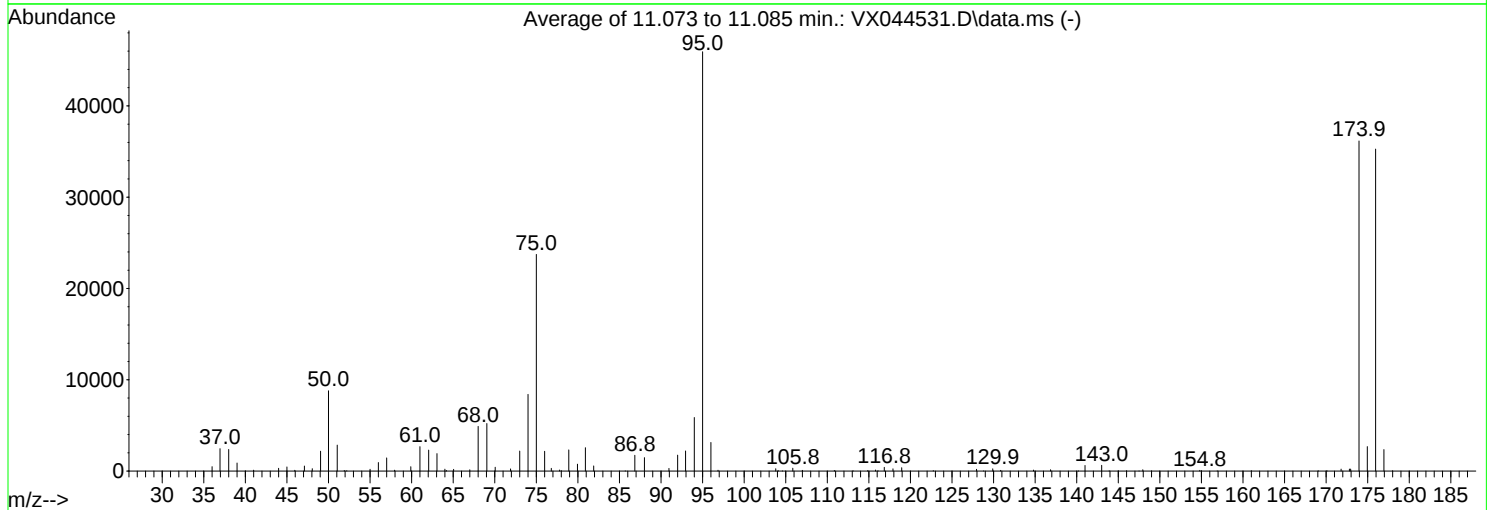


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123024\
Data File : VX044531.D
Acq On : 30 Dec 2024 08:26
Operator : JC/MD
Sample : BFB710
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB710

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Tue Dec 31 01:02:15 2024

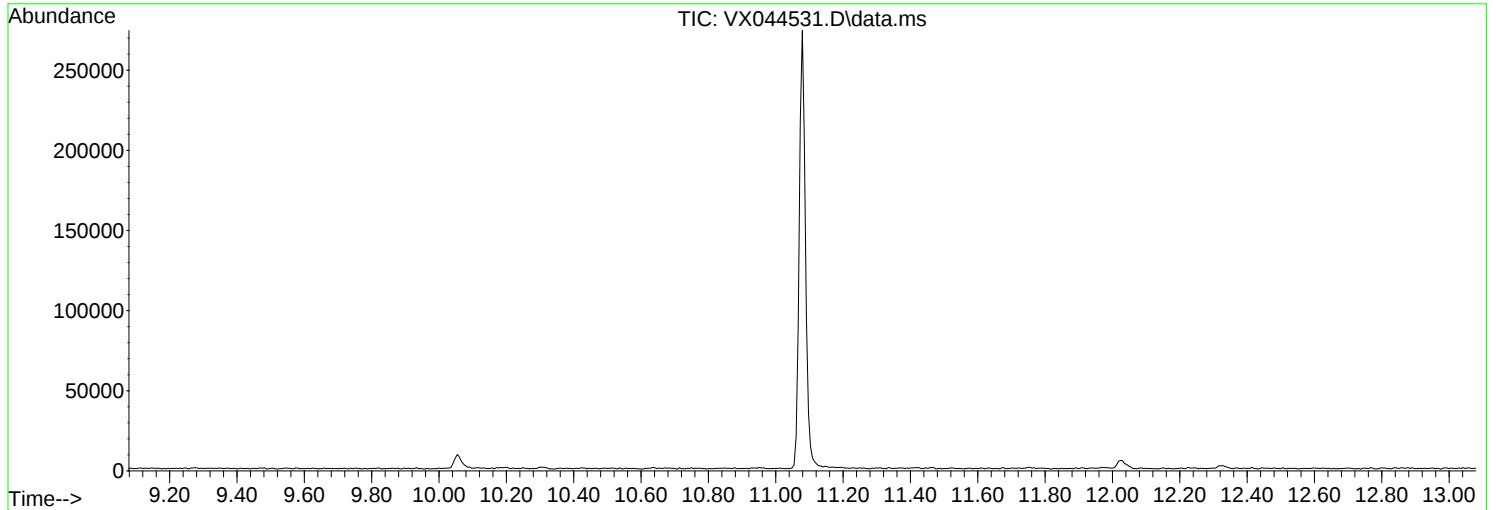

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	8794	PASS
75	95	30	80	51.7	23733	PASS
95	95	100	100	100.0	45933	PASS
96	95	5	9	6.8	3137	PASS
173	174	0.00	2	0.6	223	PASS
174	95	50	120	78.7	36160	PASS
175	174	5	9	7.4	2685	PASS
176	174	95	101	97.5	35272	PASS
177	176	5	9	6.7	2354	PASS

Scan 1633 (11.042 min): VX044531.D\data.ms
BFB710

m/z	Abundance
36.80	112.0
39.10	585.0
40.00	478.0
44.00	362.0

Instrument :
MSVOA_X
ClientSampleId :
BFB710

m/z	Abundance
35.90	629.0
37.00	2757.0
38.00	2350.0
39.00	1635.0
40.00	529.0
41.00	95.0
44.00	633.0
44.90	449.0
47.10	580.0
48.00	303.0
49.10	2193.0
50.00	9130.0
51.10	2874.0
51.90	119.0
55.00	297.0
56.00	1034.0
57.00	1693.0
57.90	113.0
59.90	573.0
61.00	2819.0
62.00	2534.0
63.00	2275.0
64.00	199.0
65.00	137.0
67.00	108.0
68.00	4982.0
69.00	5018.0
70.00	411.0
72.00	156.0
73.00	2214.0
74.00	9123.0
75.00	23648.0
76.00	2228.0
76.80	429.0
77.80	177.0
78.90	2245.0
79.90	741.0
80.90	2546.0
81.90	538.0
85.70	70.0
86.90	1954.0
88.00	1420.0
91.00	326.0
92.00	1764.0
93.00	2050.0
94.00	5394.0
95.00	43768.0
96.00	3056.0
96.80	162.0
103.80	292.0
105.80	384.0
107.00	72.0
110.90	63.0
114.90	83.0
115.80	193.0
117.00	364.0
117.90	299.0
118.90	234.0
122.80	76.0
128.00	128.0
128.80	57.0
129.80	179.0
130.80	137.0
134.80	63.0
136.80	127.0
141.00	635.0
143.00	540.0
146.00	92.0
147.50	51.0
148.00	143.0
154.80	108.0
156.90	55.0
171.90	266.0
172.80	230.0
173.00	234.0
173.90	29416.0
174.90	2126.0
175.90	29064.0
177.00	2033.0

Instrument :
MSVOA_X
ClientSampleId :
BFB710

m/z	Abundance
36.00	519.0
37.00	3078.0
38.00	2755.0
39.00	1517.0
40.00	429.0
41.10	100.0
44.10	779.0
45.00	604.0
45.90	152.0
47.10	667.0
48.10	285.0
49.10	2502.0
50.00	10503.0
51.00	3160.0
52.20	122.0
54.90	172.0
56.10	1222.0
57.00	1548.0
58.00	105.0
59.90	431.0
61.00	3115.0
62.10	2729.0
63.00	1986.0
64.00	439.0
65.10	204.0
67.00	206.0
68.00	5526.0
69.10	6346.0
70.10	504.0
71.80	316.0
73.00	2685.0
74.00	9953.0
75.00	28360.0
76.00	2939.0
76.80	298.0
78.00	111.0
78.90	2808.0
79.90	942.0
80.90	2963.0
81.90	736.0
86.80	1990.0
88.00	1923.0
90.90	344.0
92.00	1892.0
93.00	2692.0
94.00	6899.0
95.00	54120.0
96.00	3525.0
96.90	124.0
103.90	325.0
105.80	323.0
106.90	102.0
110.80	135.0
114.80	58.0
115.80	162.0
116.80	624.0
118.00	190.0
119.00	471.0
122.70	64.0
127.90	261.0
129.90	334.0
134.80	120.0
136.90	167.0
140.20	64.0
141.00	625.0
143.00	670.0
143.90	79.0
148.00	103.0
154.80	135.0
161.00	97.0
171.70	254.0
172.80	439.0
174.00	43464.0
175.00	3399.0
175.90	41648.0
176.90	2975.0
178.00	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB710

m/z	Abundance
36.10	309.0
37.00	1873.0
38.00	1990.0
39.00	1255.0
40.10	496.0
40.90	99.0
44.00	593.0
45.10	301.0
46.00	114.0
47.10	403.0
48.00	202.0
49.00	1843.0
50.00	6748.0
51.00	2500.0
51.90	75.0
55.10	127.0
55.90	558.0
57.00	1086.0
57.90	82.0
59.90	428.0
61.00	2100.0
62.00	1635.0
63.10	1477.0
64.20	175.0
65.10	236.0
67.00	117.0
68.00	4182.0
69.00	4270.0
70.10	344.0
72.00	239.0
73.00	1677.0
74.00	6126.0
75.00	19192.0
76.00	1330.0
76.90	181.0
77.80	164.0
78.90	1901.0
80.00	587.0
80.90	2179.0
81.80	412.0
86.90	1255.0
88.00	1079.0
90.90	208.0
92.00	1575.0
92.90	1867.0
94.00	5316.0
95.00	39912.0
96.00	2831.0
103.70	156.0
104.10	140.0
104.60	70.0
105.90	236.0
107.10	62.0
113.10	100.0
116.10	111.0
116.90	236.0
117.80	259.0
118.90	402.0
127.90	196.0
130.00	227.0
130.90	101.0
134.80	153.0
136.90	144.0
141.00	589.0
143.00	689.0
145.00	70.0
147.90	200.0
149.00	55.0
155.00	73.0
169.10	65.0
170.10	95.0
171.90	130.0
172.90	425.0
173.90	35600.0
174.90	2531.0
176.00	35104.0
177.00	2055.0

Instrument :
MSVOA_X
ClientSampleId :
BFB710