

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123120\
 Data File : VX020492.D
 Acq On : 31 Dec 2020 18:43
 Operator : JC/MD
 Sample : L5253-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SLUICEWAY-123020

Integration Parameters: RTEINT.P

Integrator: RTE

Soothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M

Title : Sw846 8260

Signal : TIC: VX020492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.416	212	218	236	rVB	53952	95701	7.64%	1.360%
2	2.581	236	245	252	rBV	16954	31014	2.48%	0.441%
3	2.684	256	262	270	rBV	26744	50285	4.01%	0.715%
4	5.178	663	671	681	rVB3	5879	17401	1.39%	0.247%
5	5.464	706	718	731	rBV	146203	420072	33.53%	5.971%
6	5.629	733	745	765	rVB	247230	690950	55.16%	9.822%
7	6.031	799	811	829	rBV	161986	430471	34.36%	6.119%
8	6.830	931	942	957	rBV	382949	911006	72.72%	12.950%
9	8.695	1240	1248	1256	rBV	833110	1252726	100.00%	17.807%
10	10.097	1471	1478	1487	rBV	779590	1069945	85.41%	15.209%
11	10.719	1574	1580	1587	rBV	57265	70611	5.64%	1.004%
12	11.122	1640	1646	1658	rBV	633268	783528	62.55%	11.138%
13	12.061	1795	1800	1808	rVB	756619	942039	75.20%	13.391%
14	12.615	1885	1891	1902	rBV2	55173	71692	5.72%	1.019%
15	12.853	1925	1930	1934	rBV	21216	27173	2.17%	0.386%
16	13.627	2051	2057	2069	rVB3	16476	28227	2.25%	0.401%
17	13.786	2076	2083	2088	rBV5	7027	16447	1.31%	0.234%
18	14.773	2234	2245	2251	rBV2	24907	62612	5.00%	0.890%
19	14.834	2251	2255	2261	rVB	26188	33193	2.65%	0.472%
20	14.944	2269	2273	2283	rVB2	13507	16502	1.32%	0.235%
21	16.407	2508	2513	2523	rVB2	5300	13283	1.06%	0.189%




Sum of corrected areas: 7034878

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123120\
Data File : VX020492.D
Acq On : 31 Dec 2020 18:43
Operator : JC/MD
Sample : L5253-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SLUICEWAY-123020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

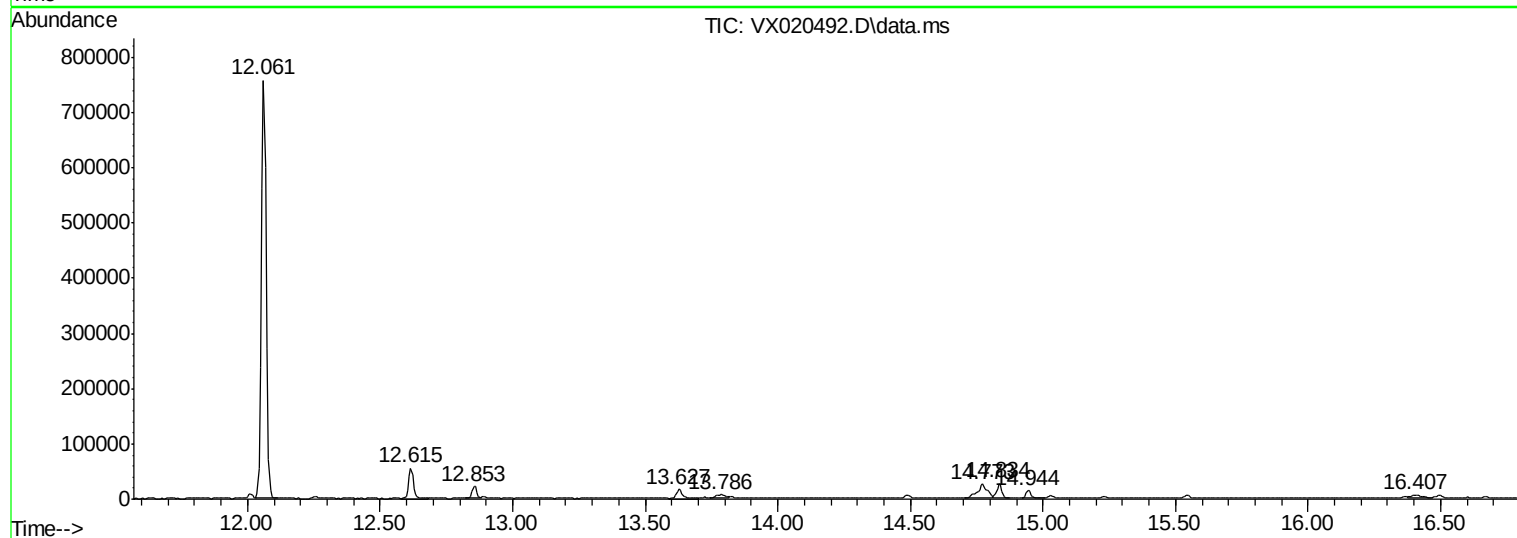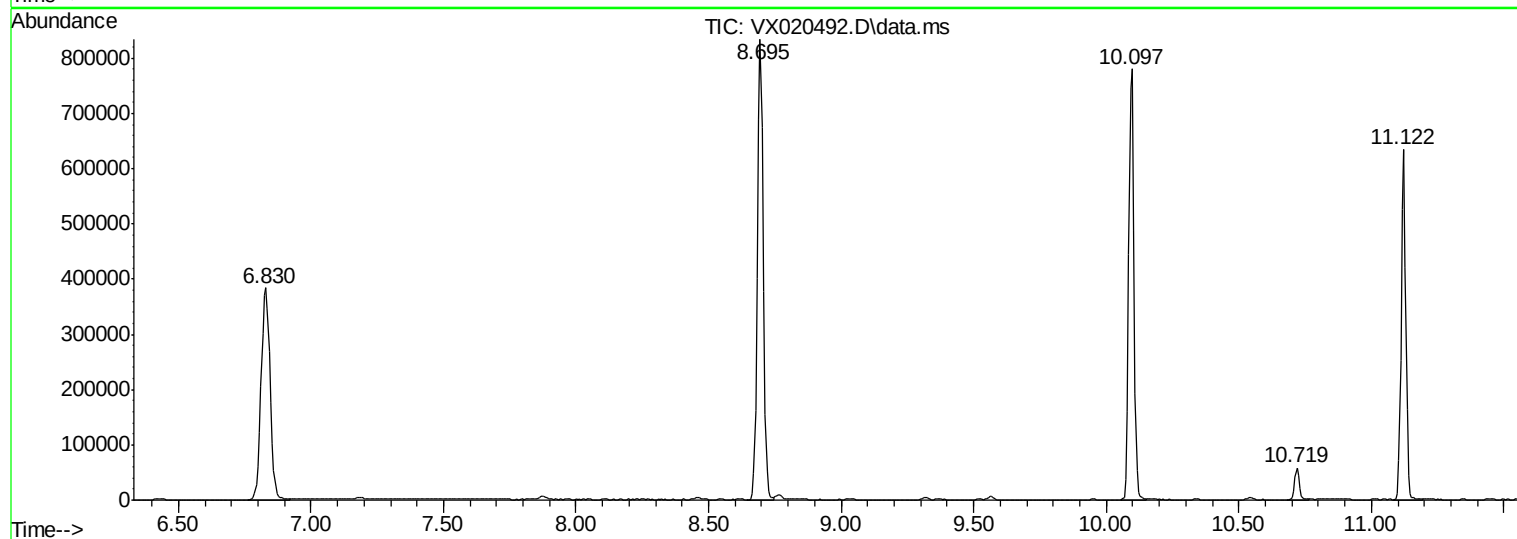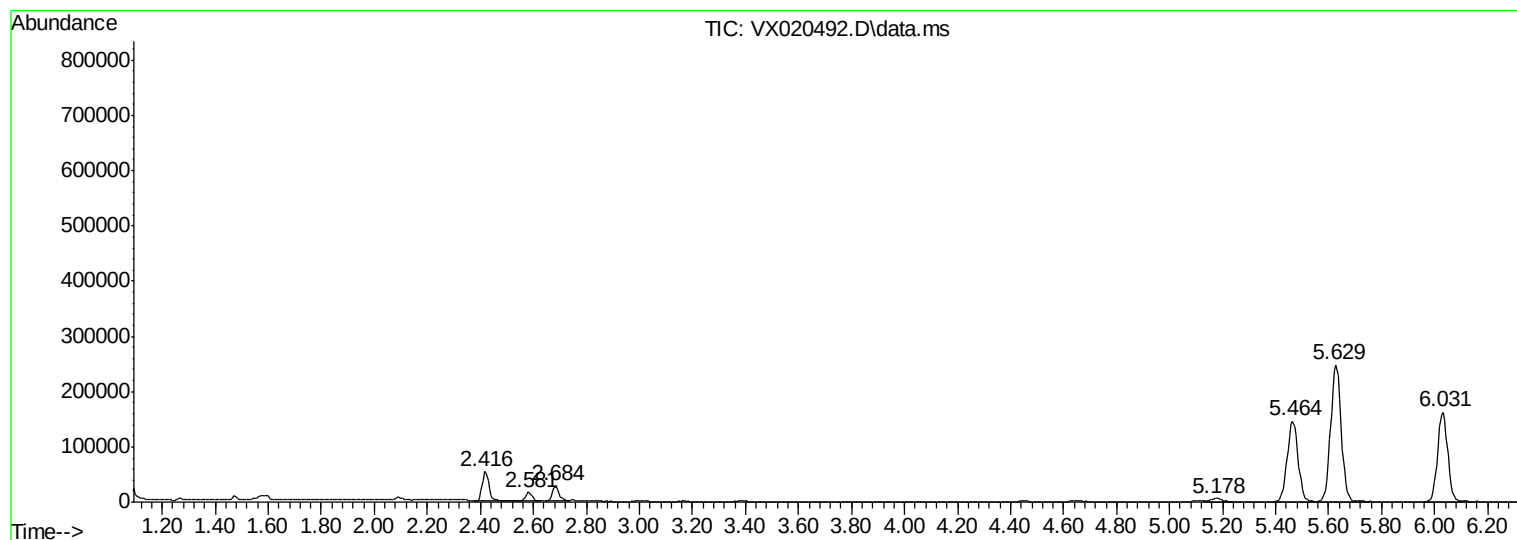

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123120\
Data File : VX020492.D
Acq On : 31 Dec 2020 18:43
Operator : JC/MD
Sample : L5253-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SLUICEWAY-123020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123120\
Data File : VX020492.D
Acq On : 31 Dec 2020 18:43
Operator : JC/MD
Sample : L5253-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SLUICEWAY-123020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

						--Internal Standard--			
TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc	
