

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
 Data File : VX026168.D
 Acq On : 30 Dec 2021 15:13
 Operator : JC/MD
 Sample : M5207-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3D-122021

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M

Title : SW846 8260

Signal : TIC: VX026168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	550	559	571	rBV	35846	100644	13.06%	2.309%
2	5.391	695	706	719	rBV	94903	276587	35.89%	6.345%
3	5.556	722	733	746	rBV	155257	440293	57.13%	10.101%
4	5.964	787	800	812	rBV	109661	291652	37.85%	6.691%
5	6.769	921	932	945	rBV	244866	586165	76.06%	13.448%
6	7.129	984	991	1001	rBV	27529	57723	7.49%	1.324%
7	8.653	1234	1241	1251	rBV	504226	770638	100.00%	17.680%
8	9.275	1338	1343	1349	rVB	58117	85011	11.03%	1.950%
9	10.055	1465	1471	1480	rBV	502237	672010	87.20%	15.417%
10	11.085	1634	1640	1646	rBV	395955	494972	64.23%	11.355%
11	12.024	1789	1794	1805	rVB	491282	583218	75.68%	13.380%




Sum of corrected areas: 4358913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
Data File : VX026168.D
Acq On : 30 Dec 2021 15:13
Operator : JC/MD
Sample : M5207-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3D-122021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

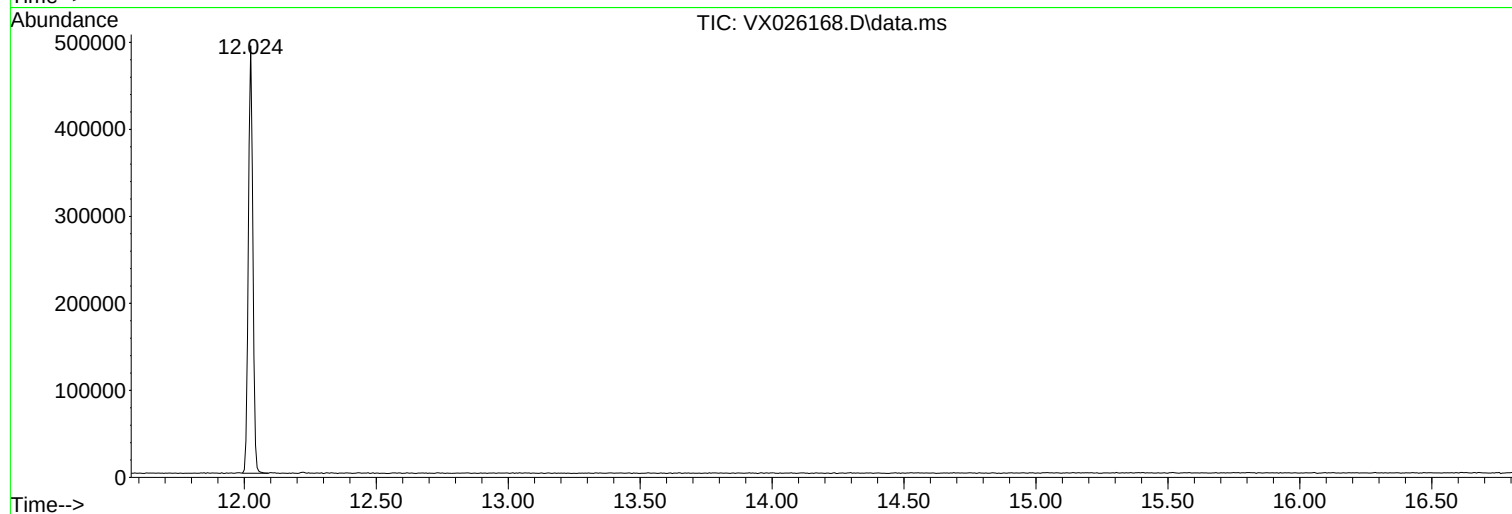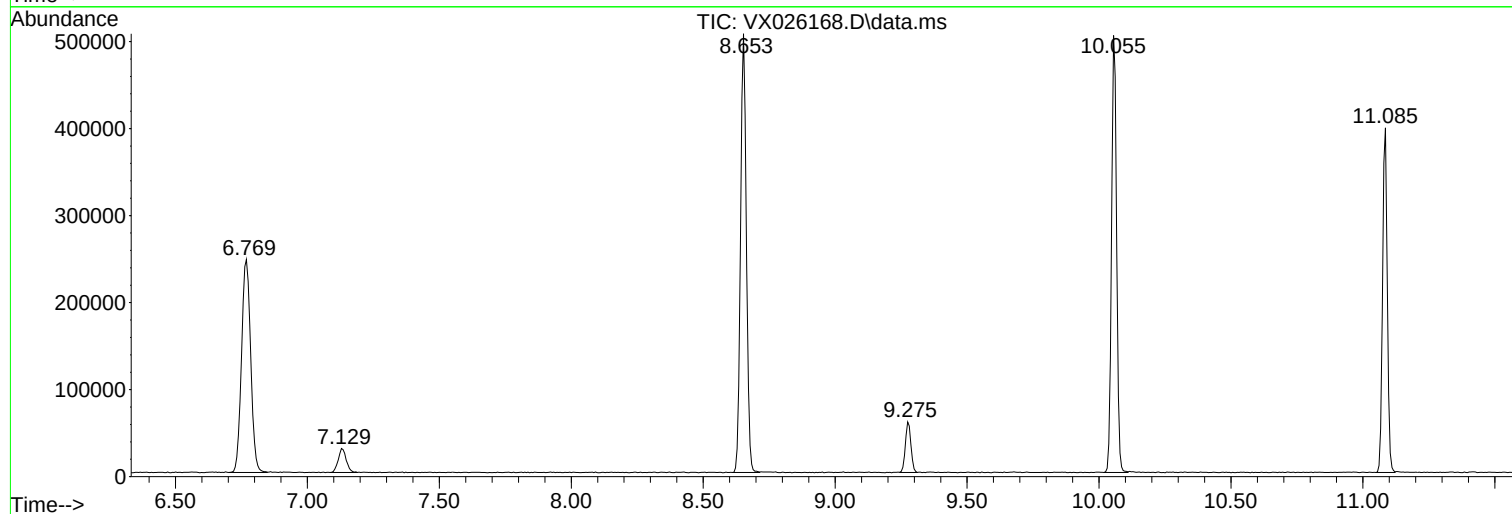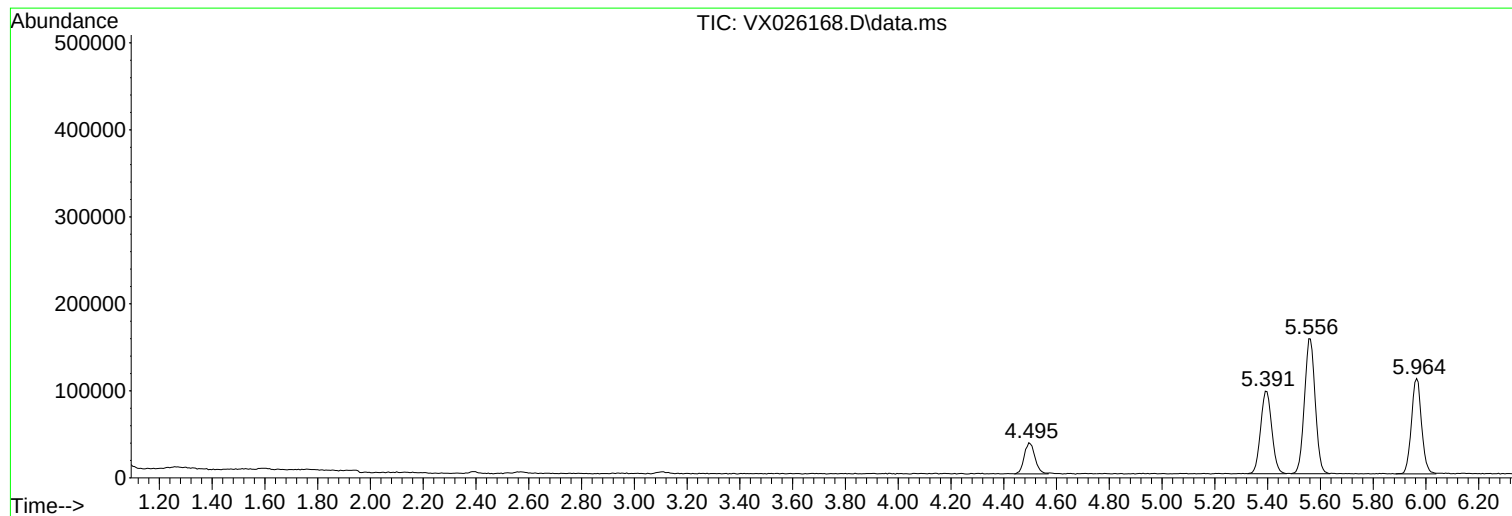

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
Data File : VX026168.D
Acq On : 30 Dec 2021 15:13
Operator : JC/MD
Sample : M5207-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3D-122021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
Data File : VX026168.D
Acq On : 30 Dec 2021 15:13
Operator : JC/MD
Sample : M5207-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3D-122021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------