

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
 Data File : VX026170.D
 Acq On : 30 Dec 2021 16:00
 Operator : JC/MD
 Sample : M5207-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SLUCE-WAY-122021

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Title : SW846 8260

Signal : TIC: VX026170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.093	157	165	179	rBV	20195	68193	8.96%	1.568%
2	2.386	207	213	218	rBV	18882	32788	4.31%	0.754%
3	2.557	237	241	251	rVB2	4313	11787	1.55%	0.271%
4	5.105	650	659	668	rBV5	3673	10510	1.38%	0.242%
5	5.391	692	706	719	rBV	96036	278092	36.52%	6.395%
6	5.562	722	734	748	rVV	153099	432696	56.83%	9.951%
7	5.964	790	800	813	rBV	107568	287228	37.72%	6.605%
8	6.769	923	932	945	rVB	246589	578786	76.02%	13.310%
9	7.824	1100	1105	1113	rBV4	3732	7680	1.01%	0.177%
10	8.653	1234	1241	1249	rBV	493694	761399	100.00%	17.510%
11	9.525	1379	1384	1392	rVB4	5699	9093	1.19%	0.209%
12	10.055	1465	1471	1481	rBV	502610	666749	87.57%	15.333%
13	10.683	1569	1574	1581	rBV	47906	58739	7.71%	1.351%
14	11.085	1634	1640	1649	rBV	384484	497044	65.28%	11.430%
15	12.024	1788	1794	1804	rBV	503121	601911	79.05%	13.842%
16	12.579	1880	1885	1894	rBV2	16128	23459	3.08%	0.539%
17	12.768	1912	1916	1921	rBV4	5490	7950	1.04%	0.183%
18	13.597	2043	2052	2057	rBV4	8434	14358	1.89%	0.330%




Sum of corrected areas: 4348462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
Data File : VX026170.D
Acq On : 30 Dec 2021 16:00
Operator : JC/MD
Sample : M5207-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SLUCE-WAY-122021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

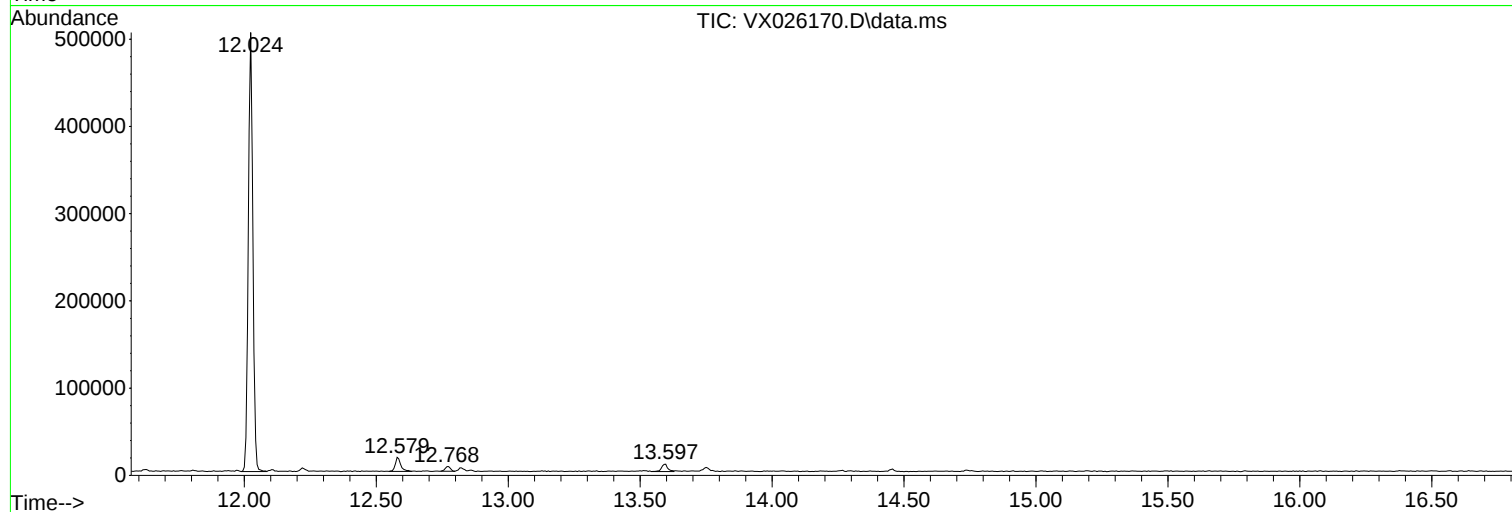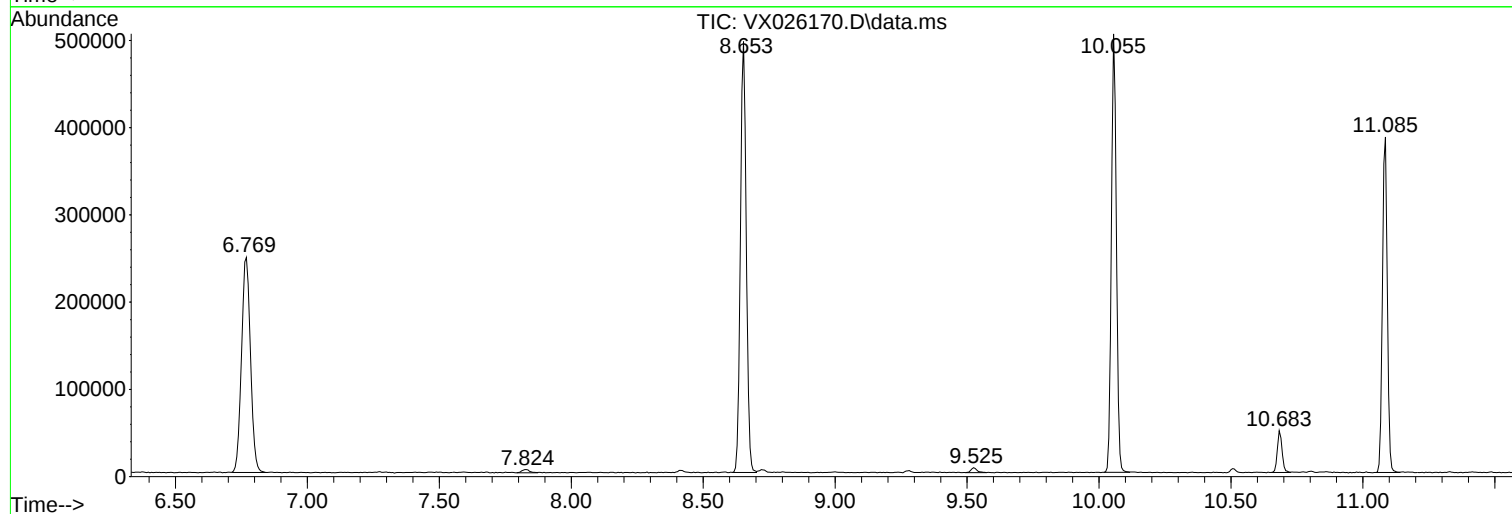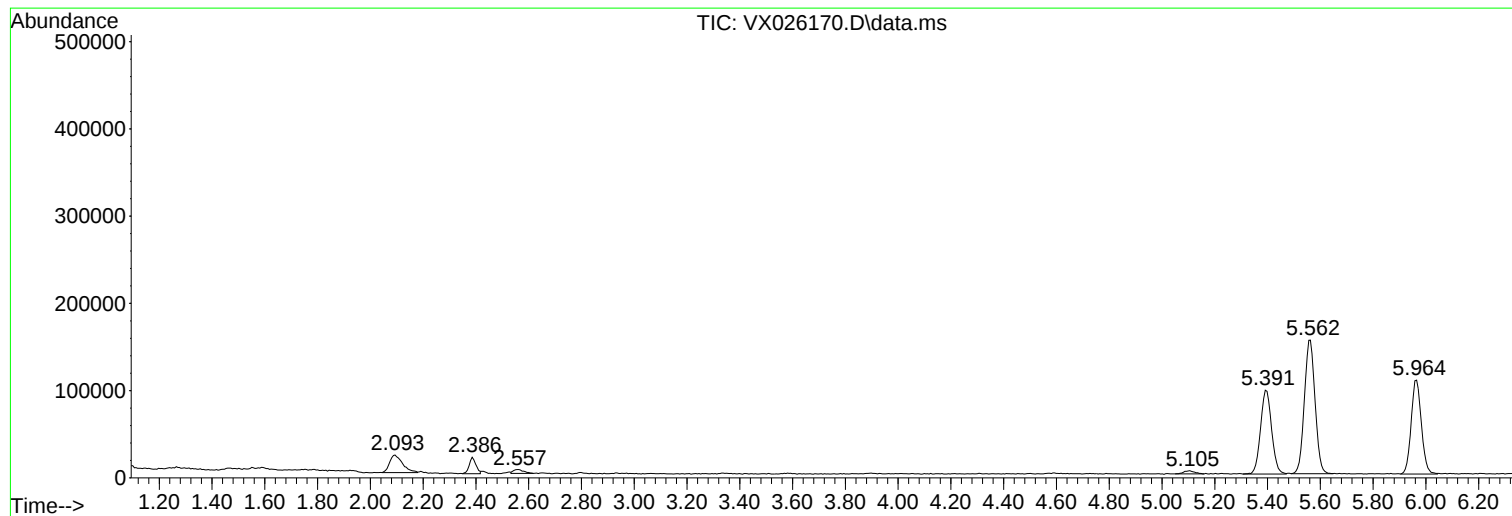

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
Data File : VX026170.D
Acq On : 30 Dec 2021 16:00
Operator : JC/MD
Sample : M5207-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SLUCE-WAY-122021










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.093	7.88 ug/l	68193	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol	46	C2H6O	000064-17-5	64
2			Dimethyl ether	46	C2H6O	000115-10-6	9
3			Methane, nitroso-	45	CH3NO	000865-40-7	4
4			Formic acid	46	CH2O2	000064-18-6	4
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	2

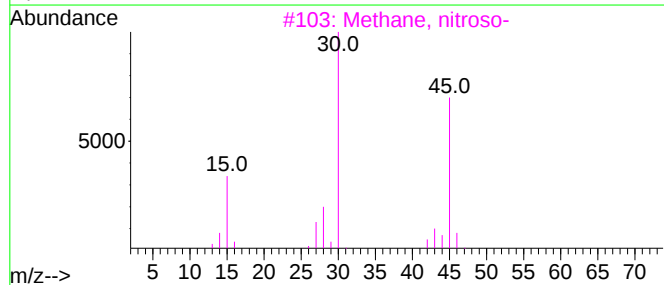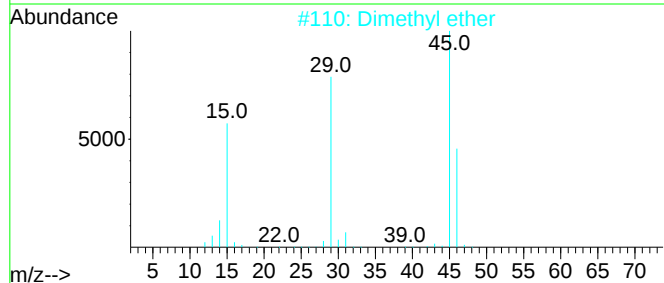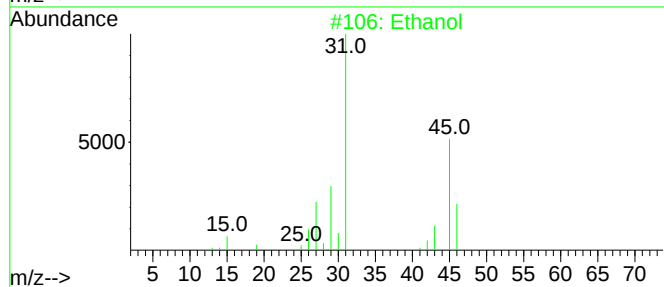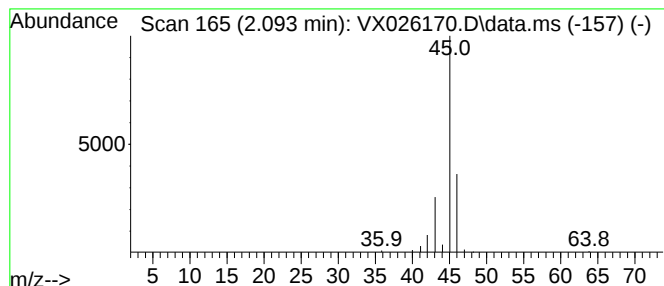

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
Data File : VX026170.D
Acq On : 30 Dec 2021 16:00
Operator : JC/MD
Sample : M5207-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SLUCE-WAY-122021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	2.093	7.9	ug/l	68193	1	5.562	432696	50.0