
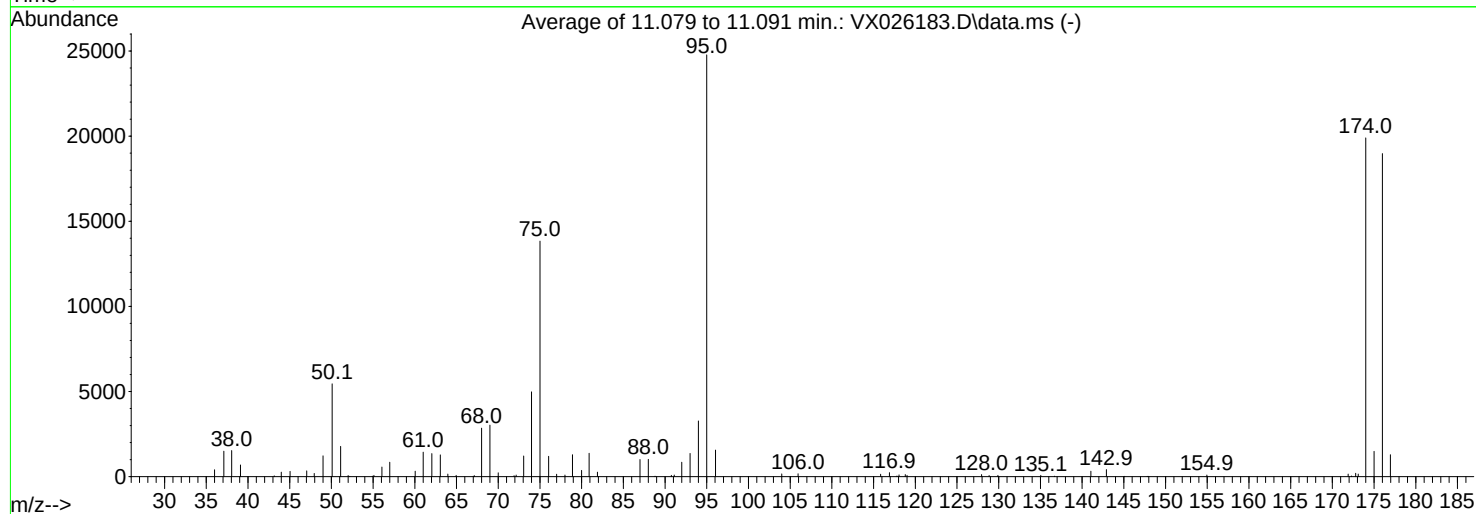


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123121\
 Data File : VX026183.D
 Acq On : 30 Dec 2021 21:03
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X123021W.M
 Title : SW846 8260
 Last Update : Thu Dec 30 08:02:21 2021

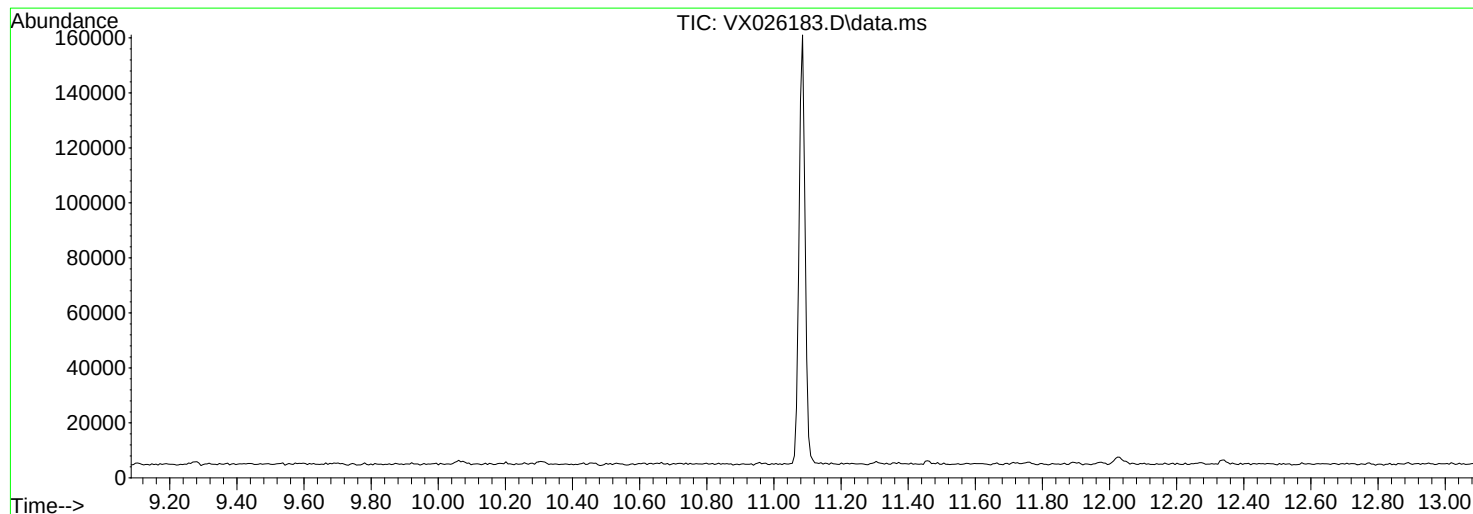

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	5451	PASS
75	95	30	60	55.9	13838	PASS
95	95	100	100	100.0	24776	PASS
96	95	5	9	6.3	1564	PASS
173	174	0.00	2	1.0	202	PASS
174	95	50	100	80.3	19901	PASS
175	174	5	9	7.4	1482	PASS
176	174	95	101	95.3	18973	PASS
177	176	5	9	6.8	1287	PASS