

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
 Data File : VX044546.D
 Acq On : 30 Dec 2024 16:08
 Operator : JC/MD
 Sample : P5376-03 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE115D2-20241218

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
 Title : SW846 8260

Signal : TIC: VX044546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.538	69	74	75	rBV2	6416	7601	1.13%	0.204%
2	2.313	196	201	209	rVB5	9061	18714	2.77%	0.501%
3	2.940	296	304	311	rBV	7634	17545	2.60%	0.470%
4	5.385	694	705	718	rBV2	81141	244203	36.21%	6.539%
5	5.544	721	731	746	rVV2	124069	361182	53.56%	9.672%
6	5.952	787	798	815	rBV	90857	250737	37.18%	6.714%
7	6.757	920	930	945	rBV	197253	483501	71.69%	12.948%
8	7.123	982	990	1004	rBV2	127407	291061	43.16%	7.794%
9	8.647	1233	1240	1253	rBV	424316	674401	100.00%	18.060%
10	10.055	1465	1471	1484	rBV	378260	548792	81.37%	14.696%
11	11.079	1634	1639	1650	rBV	306211	402397	59.67%	10.776%
12	12.018	1788	1793	1804	rBV	333606	434165	64.38%	11.626%




Sum of corrected areas: 3734299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044546.D
Acq On : 30 Dec 2024 16:08
Operator : JC/MD
Sample : P5376-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE115D2-20241218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

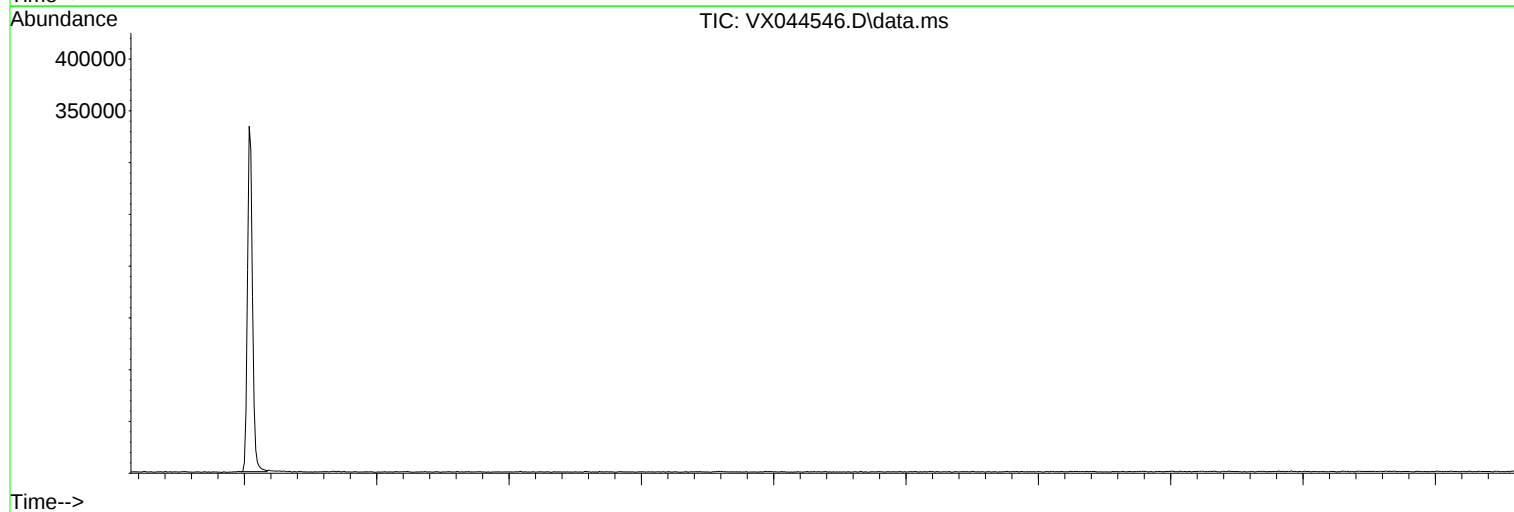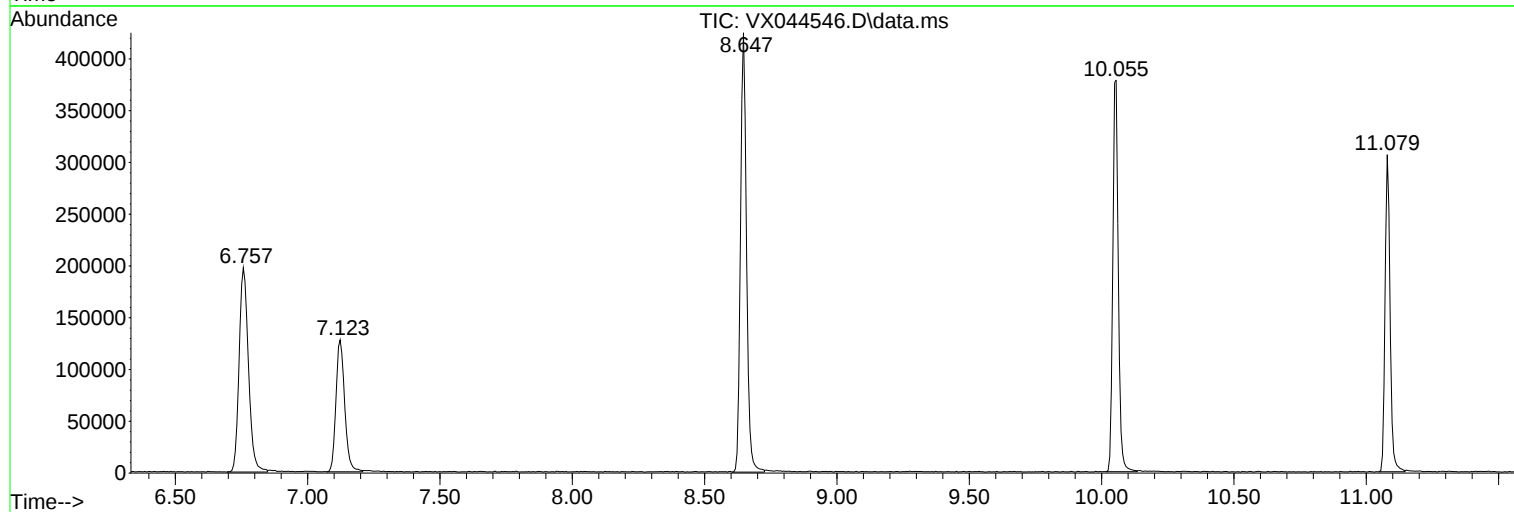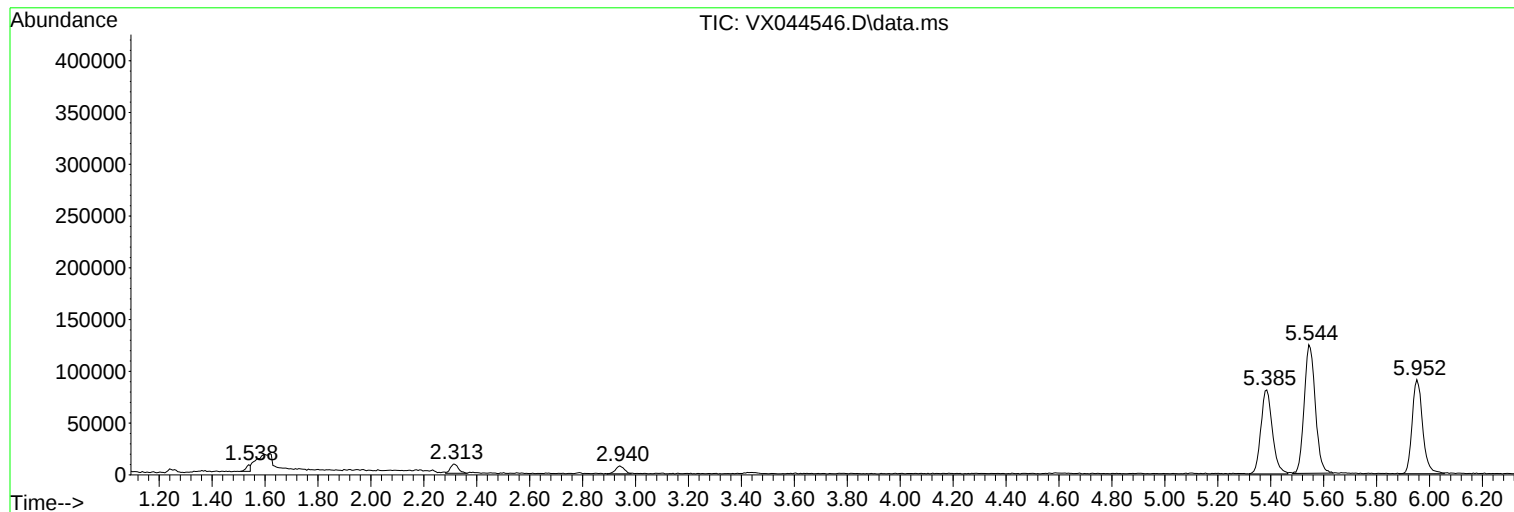

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044546.D
Acq On : 30 Dec 2024 16:08
Operator : JC/MD
Sample : P5376-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE115D2-20241218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044546.D
Acq On : 30 Dec 2024 16:08
Operator : JC/MD
Sample : P5376-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE115D2-20241218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------