

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044553.D
Acq On : 30 Dec 2024 18:51
Operator : JC/MD
Sample : P5376-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT17411-20241218

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Title : SW846 8260

Signal : TIC: VX044553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	66	80	81	rBV3	12341	34449	4.89%	0.910%
2	1.630	81	89	93	rVB4	15277	47278	6.71%	1.249%
3	3.611	406	414	420	rBV2	7306	17414	2.47%	0.460%
4	5.385	695	705	719	rBV	86776	252848	35.89%	6.677%
5	5.544	721	731	745	rVV	129940	378445	53.72%	9.994%
6	5.952	789	798	813	rBV	93852	257067	36.49%	6.789%
7	6.757	922	930	948	rBV	208921	508487	72.18%	13.428%
8	7.135	984	992	1000	rBV2	6210	14471	2.05%	0.382%
9	8.647	1233	1240	1253	rBV	440583	704493	100.00%	18.604%
10	10.049	1465	1470	1484	rBV	432461	610228	86.62%	16.115%
11	11.079	1634	1639	1655	rBV	330112	439847	62.43%	11.615%
12	12.018	1788	1793	1806	rBV	410508	521750	74.06%	13.778%




Sum of corrected areas: 3786777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044553.D
Acq On : 30 Dec 2024 18:51
Operator : JC/MD
Sample : P5376-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT17411-20241218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

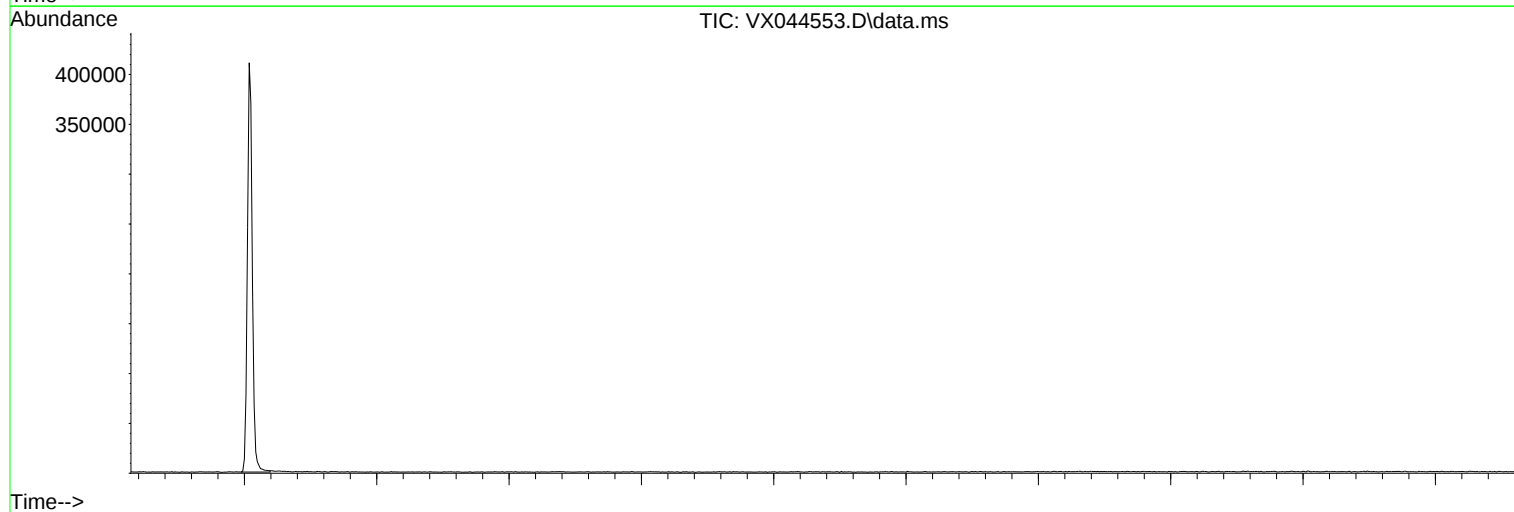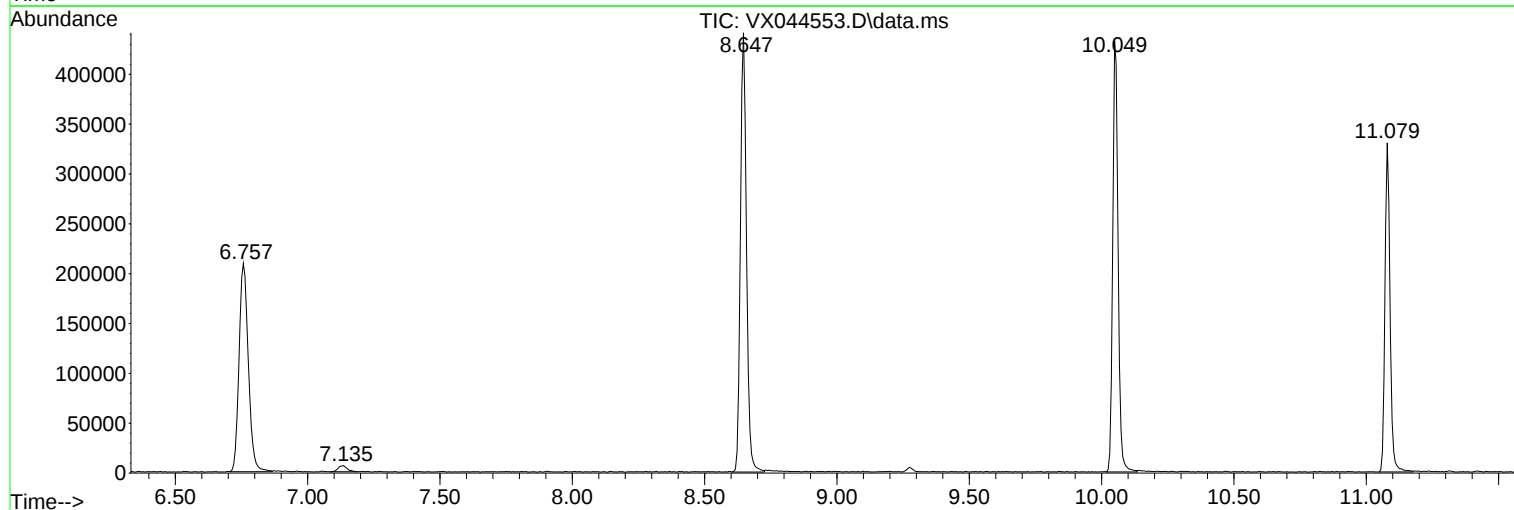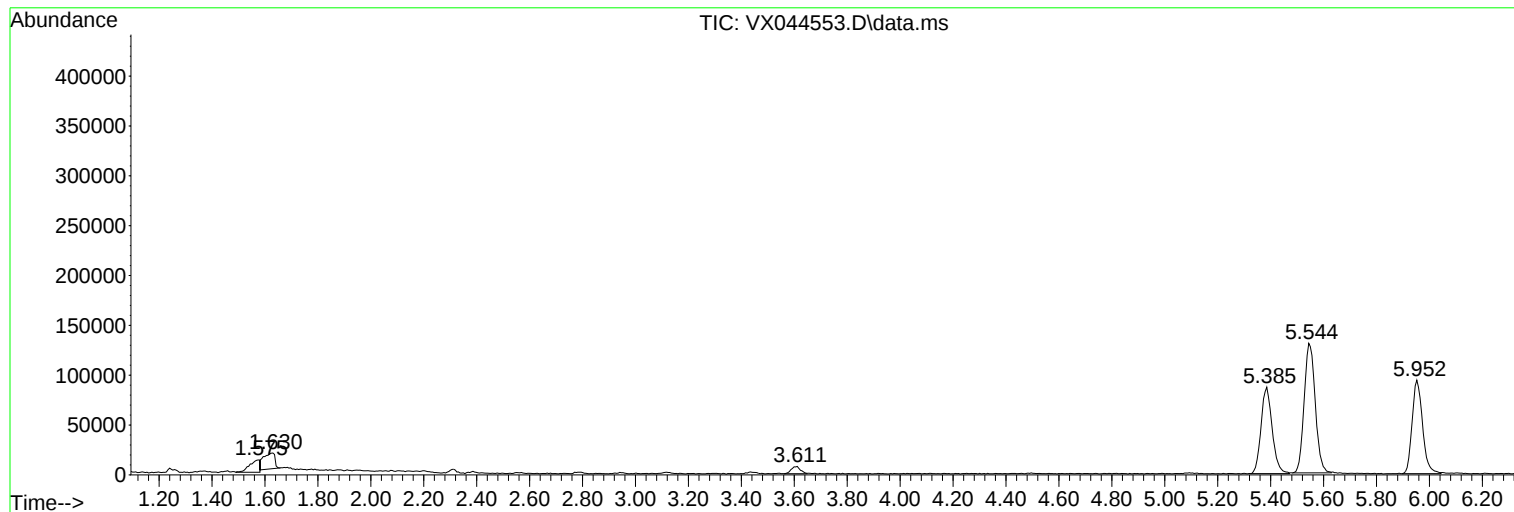

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044553.D
Acq On : 30 Dec 2024 18:51
Operator : JC/MD
Sample : P5376-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT174I1-20241218










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.630 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.630	6.25 ug/l	47278	Pentafluorobenzene	5.550

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Chloroethyl methyl sulfone	142	C3H7ClO2S	050890-51-2	45
2	Propane, 1,2-dichloro-	112	C3H6Cl2	000078-87-5	27
3	Ethane, 1,1-dichloro-	98	C2H4Cl2	000075-34-3	9
4	Ethanol, 2-chloro-, phosphite (3:1)	268	C6H12Cl3O3P	000140-08-9	9
5	Propane, 1,1,2-trichloro-	146	C3H5Cl3	000598-77-6	9

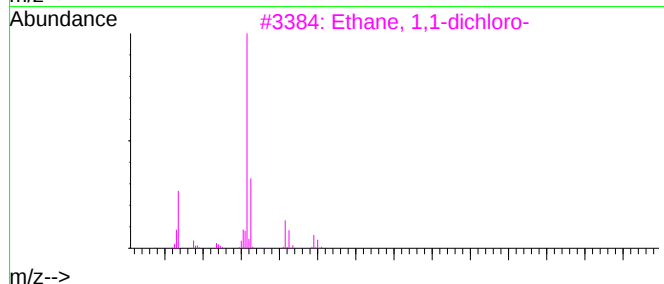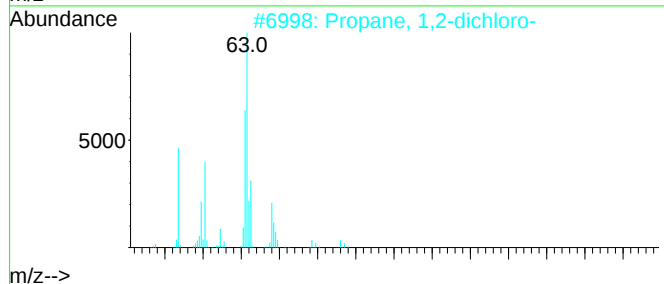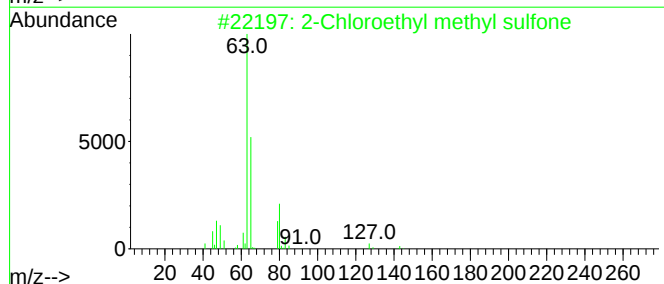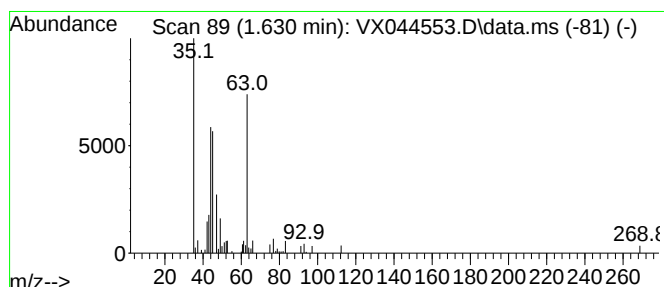

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044553.D
Acq On : 30 Dec 2024 18:51
Operator : JC/MD
Sample : P5376-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT17411-20241218

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.630	1.630	6.3	ug/l	47278	1	5.550	378445	50.0