

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
 Data File : VX029543.D
 Acq On : 17 Jun 2022 10:04
 Operator : JC/MD
 Sample : VX0617WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0617WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M

Title : SW846 8260

Signal : TIC: VX029543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.295	26	34	40	rBV4	5229	14011	1.13%	0.241%
2	2.947	297	305	315	rVB2	13412	32508	2.62%	0.559%
3	5.391	694	706	721	rBV	149884	434209	35.04%	7.471%
4	5.556	722	733	746	rVB	173847	486611	39.26%	8.372%
5	5.958	789	799	815	rBV	162170	431968	34.86%	7.432%
6	6.763	921	931	946	rBV	254175	607609	49.03%	10.454%
7	7.129	982	991	1001	rVB3	12897	27765	2.24%	0.478%
8	8.653	1233	1241	1251	rBV	759418	1239321	100.00%	21.323%
9	10.055	1465	1471	1485	rBV	584151	793648	64.04%	13.655%
10	11.085	1634	1640	1653	rBV	611287	805968	65.03%	13.867%
11	12.024	1788	1794	1804	rBV	763405	938619	75.74%	16.149%




Sum of corrected areas: 5812237

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029543.D
Acq On : 17 Jun 2022 10:04
Operator : JC/MD
Sample : VX0617WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0617WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

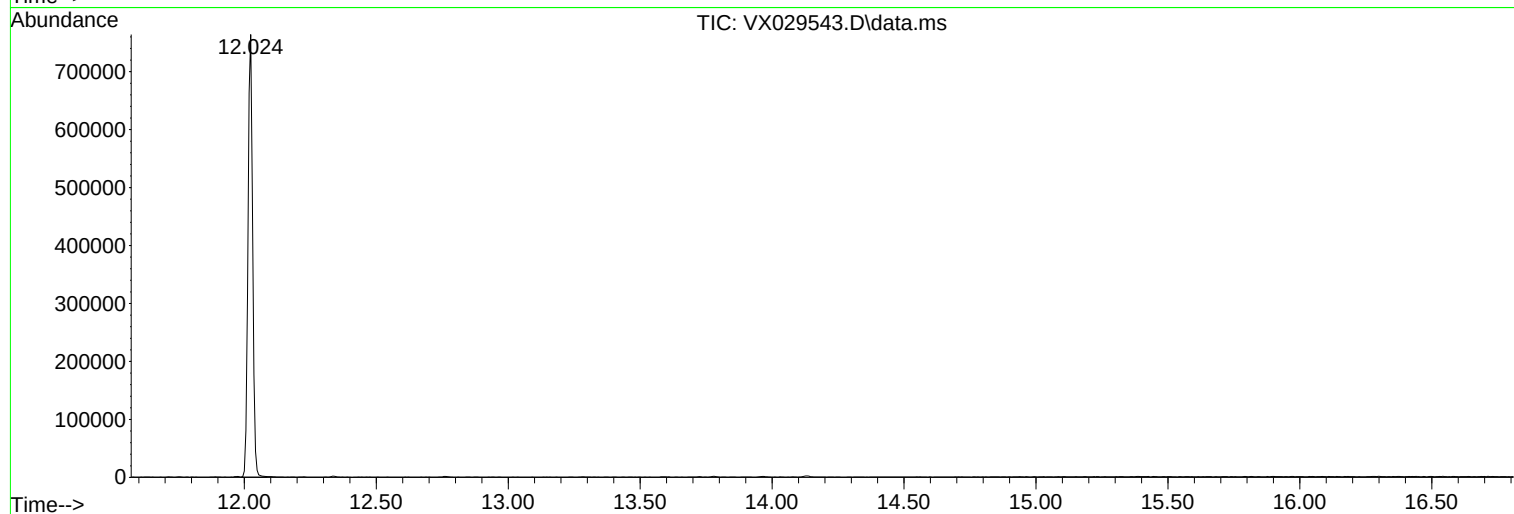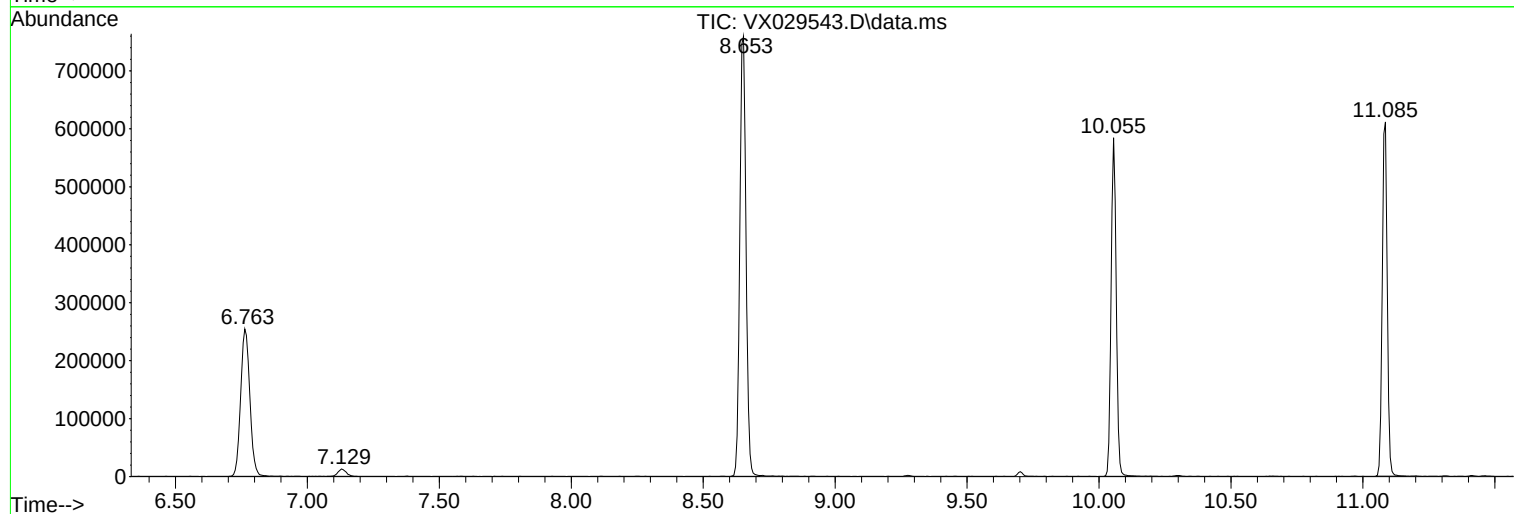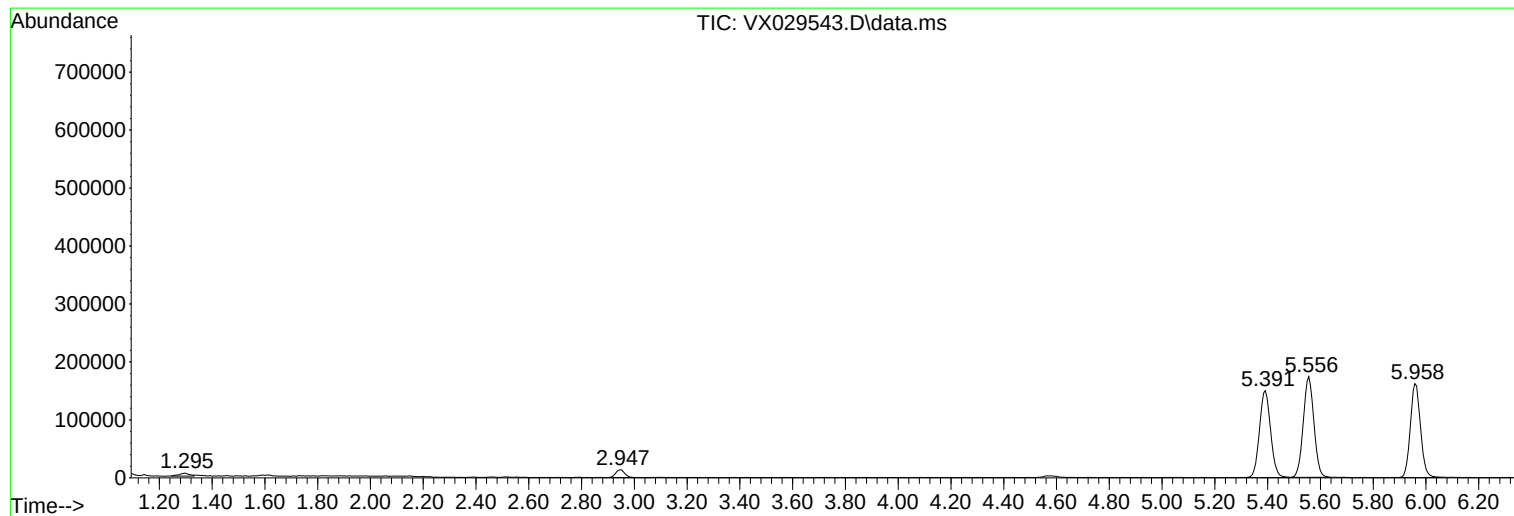

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029543.D
Acq On : 17 Jun 2022 10:04
Operator : JC/MD
Sample : VX0617WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0617WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029543.D
Acq On : 17 Jun 2022 10:04
Operator : JC/MD
Sample : VX0617WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0617WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc