

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
 Data File : VX029548.D
 Acq On : 17 Jun 2022 18:07
 Operator : JC/MD
 Sample : N3334-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14A-1A-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Title : SW846 8260

Signal : TIC: VX029551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	206	212	221	rBV	43246	71185	3.06%	0.454%
2	2.788	272	279	294	rVB	147858	269136	11.55%	1.715%
3	2.953	296	306	316	rVB	11234	28070	1.20%	0.179%
4	3.855	446	454	466	rBV4	9229	26002	1.12%	0.166%
5	4.568	561	571	589	rBV2	12533	38959	1.67%	0.248%
6	5.391	694	706	723	rBV2	123623	362732	15.57%	2.311%
7	5.556	723	733	750	rVB2	172828	495445	21.26%	3.157%
8	5.964	789	800	811	rBV	130956	358255	15.38%	2.283%
9	6.348	855	863	877	rBV2	19169	51030	2.19%	0.325%
10	6.763	922	931	950	rBV	253157	619207	26.58%	3.945%
11	7.135	984	992	1001	rBV3	10705	23771	1.02%	0.151%
12	7.379	1024	1032	1039	rVB2	13192	30155	1.29%	0.192%
13	7.464	1041	1046	1054	rBV2	14133	29002	1.24%	0.185%
14	7.647	1071	1076	1081	rBV	15924	26659	1.14%	0.170%
15	7.799	1093	1101	1115	rBV	1321662	2329908	100.00%	14.846%
16	8.549	1219	1224	1235	rBV	226094	372823	16.00%	2.376%
17	8.653	1235	1241	1249	rVV	649763	1037704	44.54%	6.612%
18	9.250	1331	1339	1345	rBV	51697	78991	3.39%	0.503%
19	9.311	1345	1349	1352	rVV	17273	25080	1.08%	0.160%
20	9.348	1352	1355	1358	rVV	22260	32789	1.41%	0.209%
21	9.378	1358	1360	1365	rVV	18009	24925	1.07%	0.159%
22	9.488	1372	1378	1385	rVV	697308	952015	40.86%	6.066%
23	9.580	1388	1393	1405	rVB	82218	129682	5.57%	0.826%
24	9.915	1442	1448	1461	rBV	552537	686679	29.47%	4.375%
25	10.055	1464	1471	1480	rBV	614642	836645	35.91%	5.331%
26	10.305	1505	1512	1518	rVB	46289	69771	2.99%	0.445%
27	10.646	1563	1568	1572	rVV	75029	100321	4.31%	0.639%
28	10.774	1582	1589	1598	rBV4	13101	24416	1.05%	0.156%
29	10.963	1615	1620	1627	rBV	57667	71219	3.06%	0.454%
30	11.085	1634	1640	1646	rBV	560213	706854	30.34%	4.504%
31	11.305	1672	1676	1681	rBV	48778	67851	2.91%	0.432%
32	11.378	1681	1688	1696	rVV	56603	121298	5.21%	0.773%
33	11.451	1696	1700	1711	rVB	95988	132820	5.70%	0.846%
34	11.616	1722	1727	1737	rBV	90433	126623	5.43%	0.807%
35	11.701	1737	1741	1745	rVV3	14789	27048	1.16%	0.172%
36	11.756	1745	1750	1755	rVB	260079	321389	13.79%	2.048%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
 Data File : VX029548.D
 Acq On : 17 Jun 2022 18:07
 Operator : JC/MD
 Sample : N3334-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-14A-1A-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Title : SW846 8260

37	11.890	1769	1772	1779	rVB	25756	36230	1.55%	0.231%
38	11.969	1779	1785	1789	rBV	19016	25118	1.08%	0.160%
39	12.024	1789	1794	1800	rVV	842523	1022775	43.90%	6.517%
40	12.091	1800	1805	1814	rVB	190351	244704	10.50%	1.559%
41	12.244	1823	1830	1838	rBV2	108452	171415	7.36%	1.092%
42	12.317	1838	1842	1852	rVB3	55072	100312	4.31%	0.639%
43	12.408	1852	1857	1862	rBV	22082	30308	1.30%	0.193%
44	12.463	1862	1866	1870	rBV	23765	29618	1.27%	0.189%
45	12.530	1873	1877	1879	rVV	28082	33300	1.43%	0.212%
46	12.555	1879	1881	1886	rVB	26684	29104	1.25%	0.185%
47	12.616	1886	1891	1894	rBV	97533	115764	4.97%	0.738%
48	12.646	1894	1896	1901	rVV	32335	34535	1.48%	0.220%
49	12.701	1901	1905	1913	rVB2	101427	169093	7.26%	1.077%
50	12.847	1924	1929	1934	rVB3	35162	53603	2.30%	0.342%
51	12.920	1934	1941	1945	rBV	80062	122704	5.27%	0.782%
52	12.963	1945	1948	1954	rVB2	68470	89997	3.86%	0.573%
53	13.030	1954	1959	1964	rBV6	17988	34891	1.50%	0.222%
54	13.140	1973	1977	1979	rBV	19267	24402	1.05%	0.155%
55	13.170	1979	1982	1985	rVB	43030	47401	2.03%	0.302%
56	13.292	1997	2002	2008	rVB2	244952	344516	14.79%	2.195%
57	13.426	2019	2024	2029	rVB2	34895	50686	2.18%	0.323%
58	13.506	2029	2037	2040	rBV3	20547	33355	1.43%	0.213%
59	13.542	2040	2043	2046	rVV	25361	30363	1.30%	0.193%
60	13.585	2046	2050	2055	rBV3	40379	62802	2.70%	0.400%
61	13.664	2060	2063	2071	rVV2	59587	103333	4.44%	0.658%
62	13.780	2074	2082	2091	rVB	136217	213836	9.18%	1.363%
63	13.926	2099	2106	2110	rBV3	31552	55039	2.36%	0.351%
64	14.079	2126	2131	2134	rBV2	26315	37110	1.59%	0.236%
65	14.219	2148	2154	2163	rBV3	46192	96156	4.13%	0.613%
66	14.323	2167	2171	2175	rVV2	25847	33828	1.45%	0.216%
67	14.377	2175	2180	2185	rVB3	43119	61656	2.65%	0.393%
68	14.481	2193	2197	2207	rBV2	42946	66107	2.84%	0.421%
69	14.603	2210	2217	2219	rBV2	22725	40550	1.74%	0.258%
70	14.640	2219	2223	2227	rVV	179372	218264	9.37%	1.391%
71	14.780	2241	2246	2256	rBV	257363	350662	15.05%	2.234%
72	15.188	2306	2313	2321	rBV3	16010	31754	1.36%	0.202%
73	15.377	2336	2344	2347	rBV2	33929	61484	2.64%	0.392%
74	15.408	2347	2349	2354	rVB	22593	27470	1.18%	0.175%
75	15.481	2355	2361	2365	rBV	81141	128496	5.52%	0.819%
76	15.615	2374	2383	2387	rBV	138763	234673	10.07%	1.495%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029548.D
Acq On : 17 Jun 2022 18:07
Operator : JC/MD
Sample : N3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Title : SW846 8260

77	15.652	2387	2389	2396	rVB	75816	101688	4.36%	0.648%
78	15.737	2396	2403	2409	rBV	14453	27719	1.19%	0.177%
79	15.841	2409	2420	2430	rVB2	42737	118604	5.09%	0.756%
80	15.993	2439	2445	2450	rBV	24705	42128	1.81%	0.268%




Sum of corrected areas: 15694012

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029548.D
Acq On : 17 Jun 2022 18:07
Operator : JC/MD
Sample : N3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

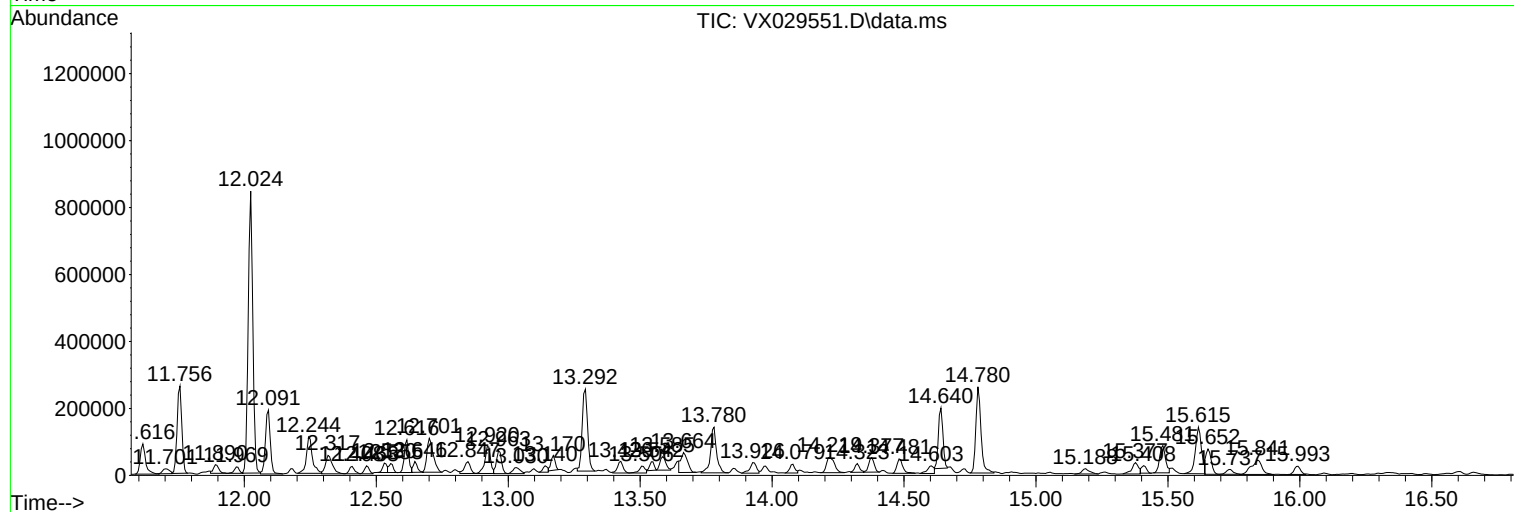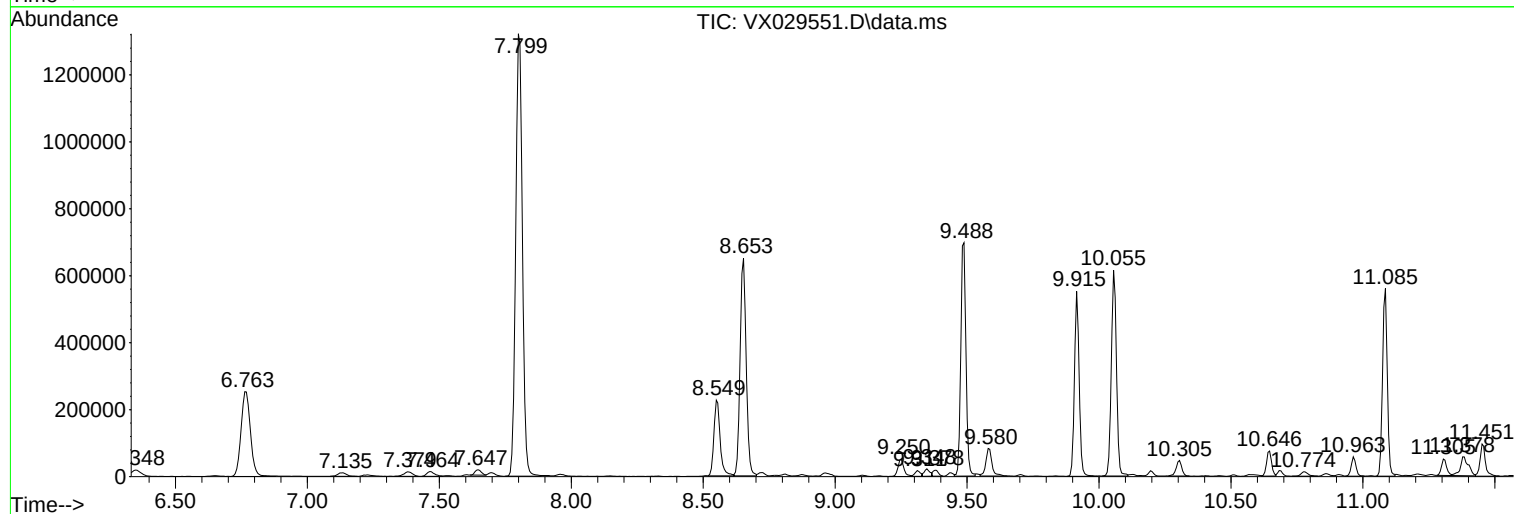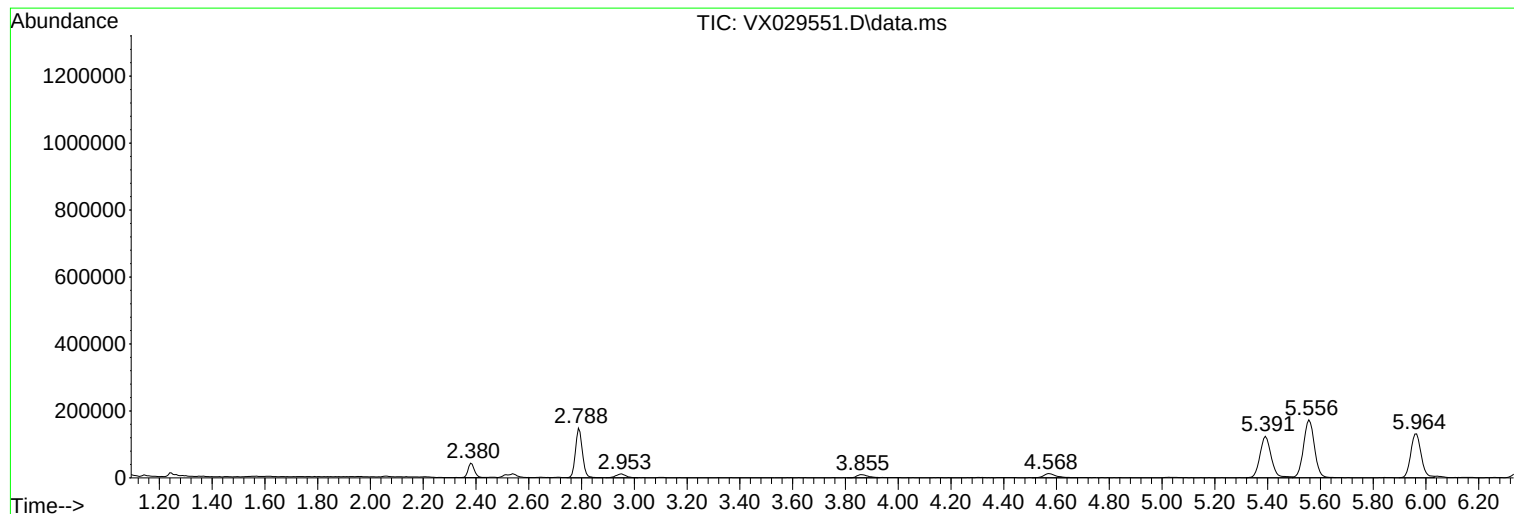

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029548.D
Acq On : 17 Jun 2022 18:07
Operator : JC/MD
Sample : N3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
Data File : VX029548.D
Acq On : 17 Jun 2022 18:07
Operator : JC/MD
Sample : N3334-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-14A-1A-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------