
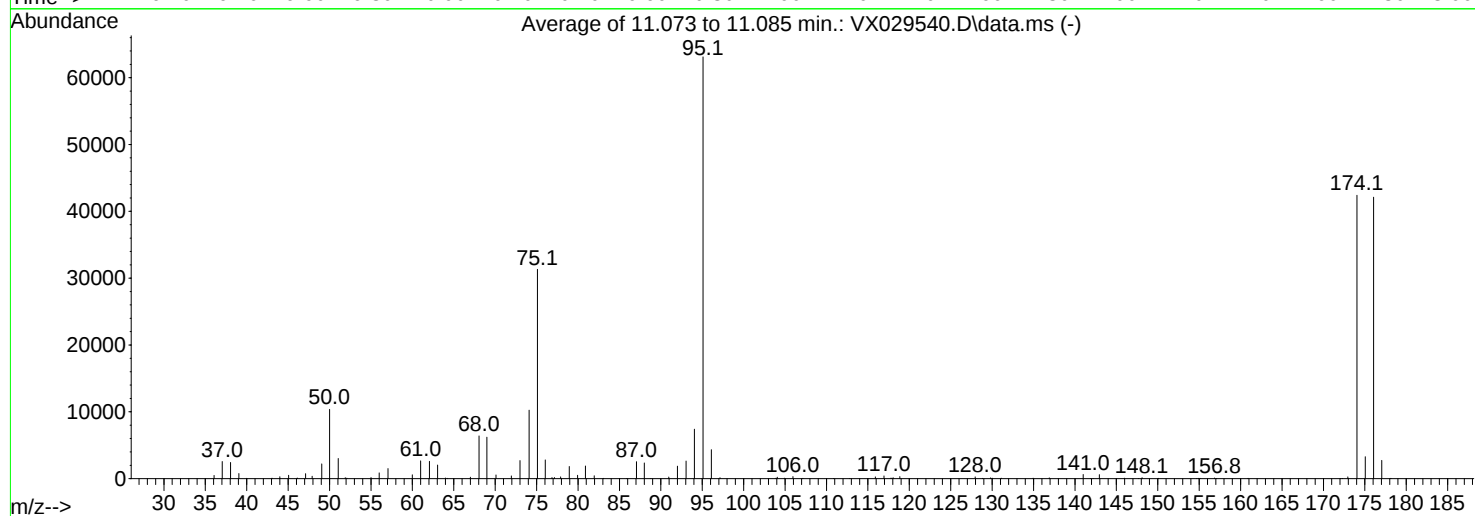


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061722\
 Data File : VX029540.D
 Acq On : 17 Jun 2022 07:58
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X060722W.M
 Title : SW846 8260
 Last Update : Wed Jun 08 03:00:38 2022

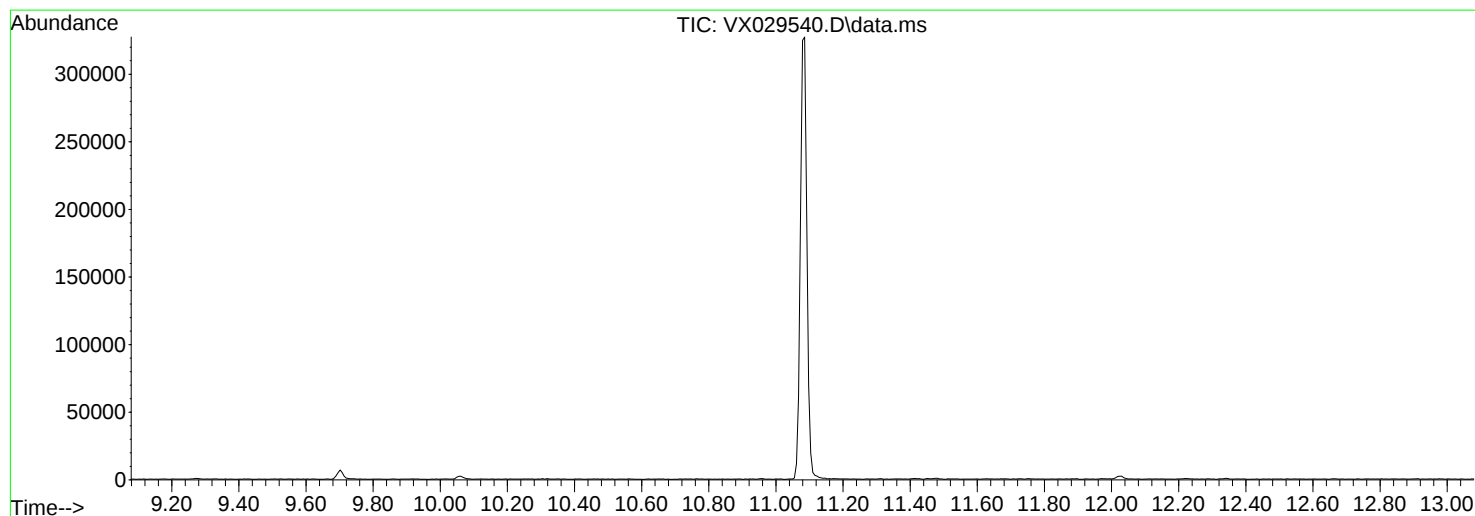

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	10377	PASS
75	95	30	60	49.6	31312	PASS
95	95	100	100	100.0	63123	PASS
96	95	5	9	6.9	4332	PASS
173	174	0.00	2	0.6	265	PASS
174	95	50	100	67.2	42416	PASS
175	174	5	9	7.7	3282	PASS
176	174	95	101	99.3	42131	PASS
177	176	5	9	6.5	2738	PASS