

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030821.D
 Acq On : 26 Aug 2022 13:53
 Operator : JC/MD
 Sample : N4245-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE109D3-20220817

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Title : SW846 8260

Signal : TIC: VX030821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.324	199	203	209	rVB5	6788	11729	1.04%	0.180%
2	5.391	694	706	720	rBV2	131662	383907	33.93%	5.899%
3	5.556	720	733	748	rVV	235931	659951	58.33%	10.140%
4	5.964	790	800	813	rBV	148702	389154	34.39%	5.979%
5	6.769	920	932	947	rBV	359780	856679	75.71%	13.163%
6	7.135	981	992	1007	rBV	241310	531976	47.02%	8.174%
7	8.653	1231	1241	1252	rBV	742886	1131477	100.00%	17.385%
8	9.281	1338	1344	1350	rVB3	11665	18400	1.63%	0.283%
9	10.055	1465	1471	1482	rBV	714193	969163	85.65%	14.891%
10	11.085	1634	1640	1649	rBV	548075	695248	61.45%	10.682%
11	12.024	1789	1794	1805	rBV	722088	860612	76.06%	13.223%




Sum of corrected areas: 6508296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030821.D
Acq On : 26 Aug 2022 13:53
Operator : JC/MD
Sample : N4245-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE109D3-20220817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

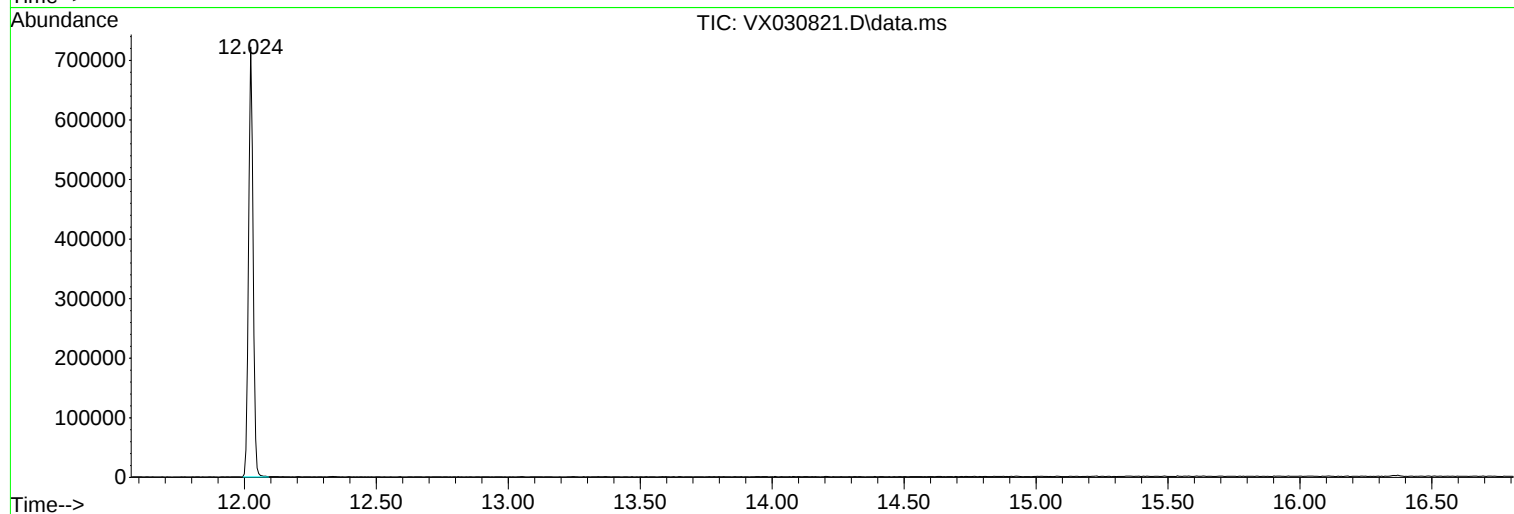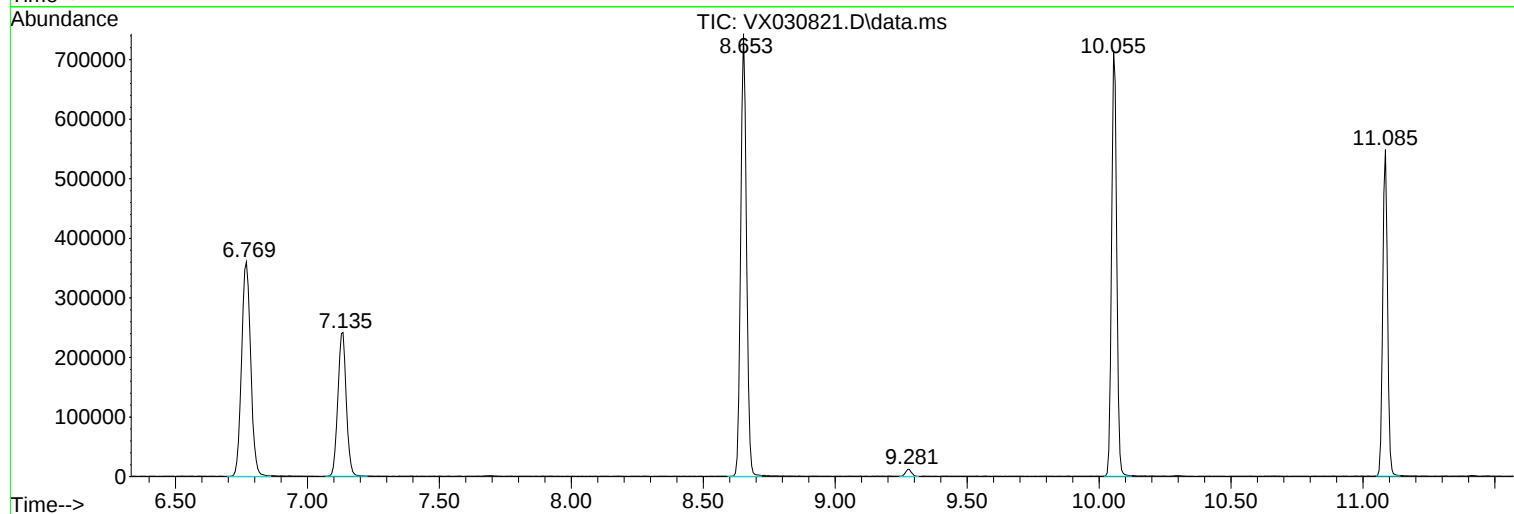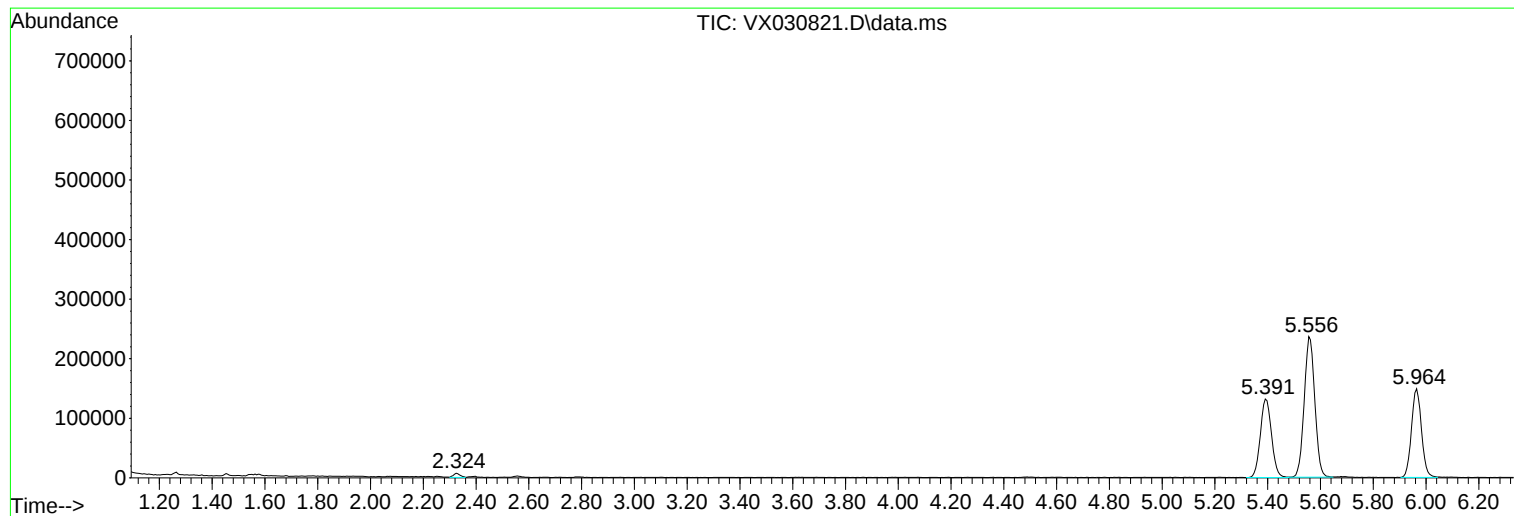

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030821.D
Acq On : 26 Aug 2022 13:53
Operator : JC/MD
Sample : N4245-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE109D3-20220817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030821.D
Acq On : 26 Aug 2022 13:53
Operator : JC/MD
Sample : N4245-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE109D3-20220817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------