

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030830.D
 Acq On : 26 Aug 2022 17:25
 Operator : JC/MD
 Sample : N4262-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-102I

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.550	70	76	81	rBV5	4898	10877	1.02%	0.164%
2	4.501	549	560	570	rBV2	11675	32291	3.03%	0.488%
3	5.391	695	706	723	rBV2	127293	362620	34.02%	5.481%
4	5.555	723	733	750	rVB	215765	616399	57.82%	9.317%
5	5.964	789	800	816	rBV	136420	363911	34.14%	5.500%
6	6.769	922	932	948	rBV	333871	803616	75.39%	12.147%
7	7.128	983	991	1002	rBV	128576	284138	26.65%	4.295%
8	8.652	1233	1241	1252	rBV	684814	1066014	100.00%	16.113%
9	9.274	1333	1343	1355	rBV	461405	683081	64.08%	10.325%
10	10.055	1465	1471	1487	rBV	674670	932192	87.45%	14.090%
11	11.085	1634	1640	1651	rBV	522221	663755	62.27%	10.033%
12	12.024	1789	1794	1807	rVB	658603	797108	74.77%	12.048%




Sum of corrected areas: 6616002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030830.D
Acq On : 26 Aug 2022 17:25
Operator : JC/MD
Sample : N4262-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-102I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

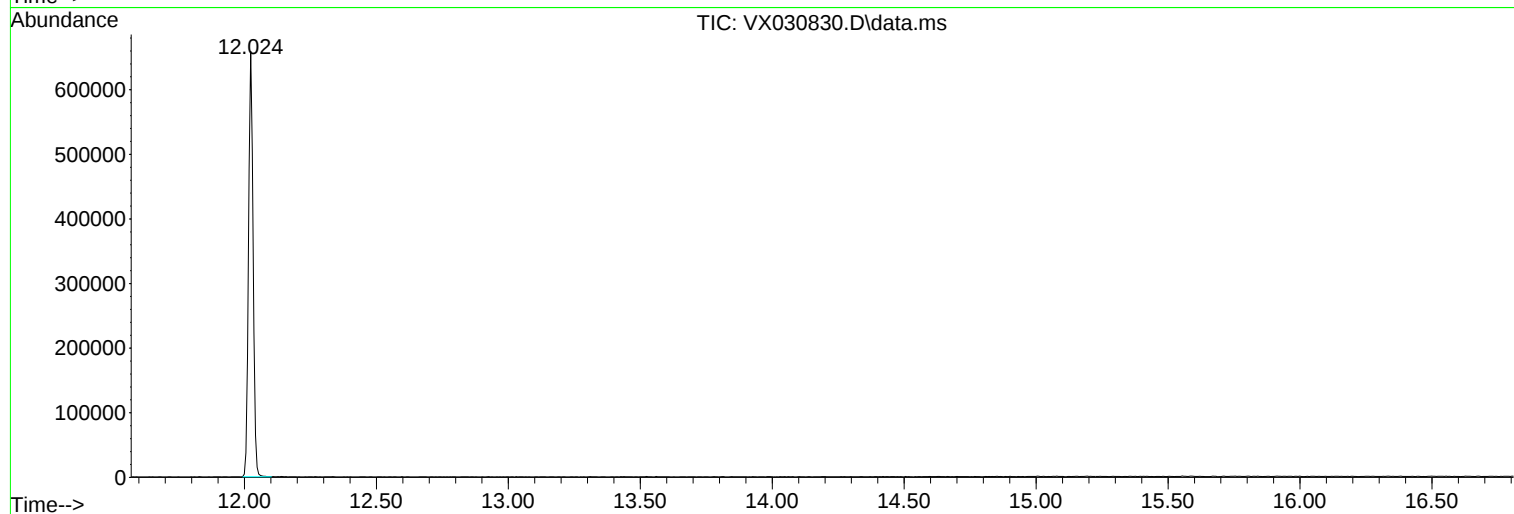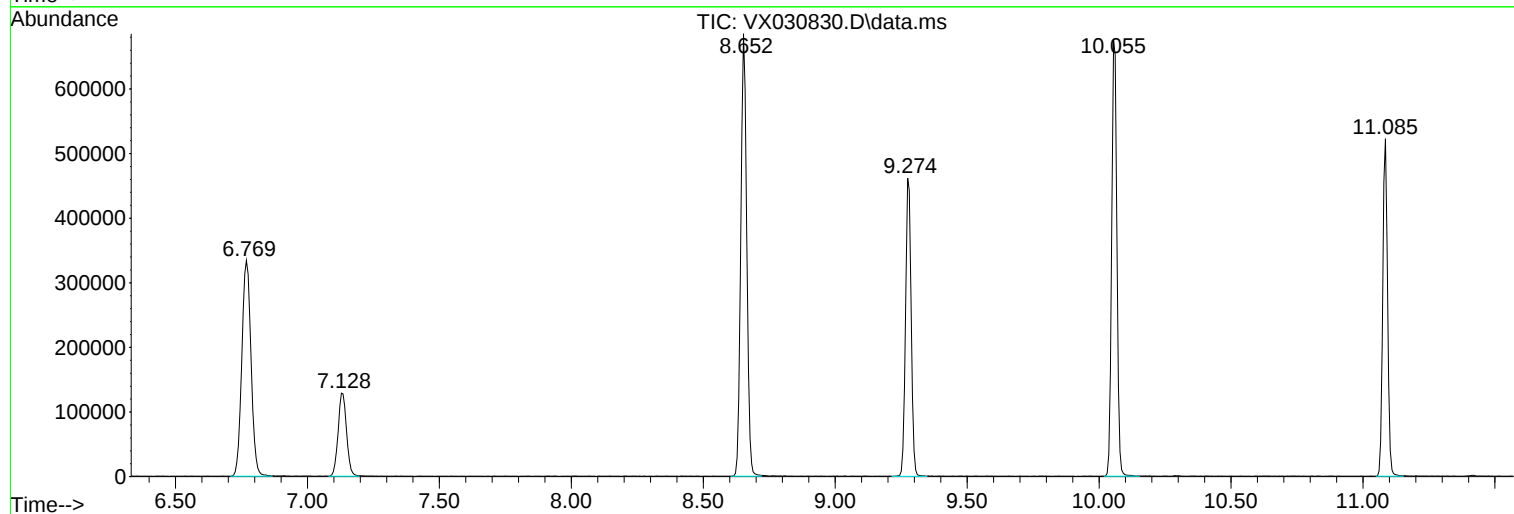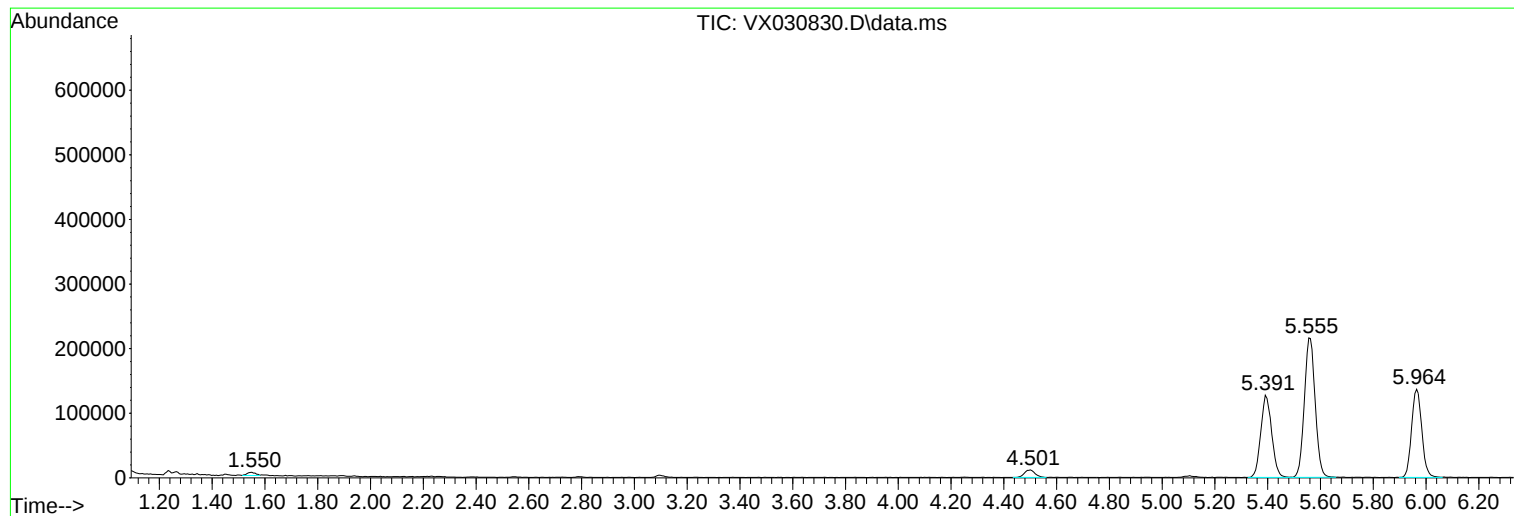

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030830.D
Acq On : 26 Aug 2022 17:25
Operator : JC/MD
Sample : N4262-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030830.D
Acq On : 26 Aug 2022 17:25
Operator : JC/MD
Sample : N4262-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-102I

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------