

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030835.D
 Acq On : 26 Aug 2022 19:24
 Operator : JC/MD
 Sample : N4278-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20220818

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.544	229	239	249	rBV	24196	46288	4.35%	0.828%
2	2.953	299	306	315	rVB2	4318	11116	1.04%	0.199%
3	4.586	563	574	576	rBV	5735	12810	1.20%	0.229%
4	5.391	694	706	721	rBV2	124737	358428	33.68%	6.413%
5	5.562	721	734	749	rVV	215387	612442	57.54%	10.958%
6	5.964	788	800	814	rBV	137822	364694	34.27%	6.525%
7	6.769	922	932	948	rBV	342508	795231	74.72%	14.229%
8	8.653	1234	1241	1254	rBV	691534	1064304	100.00%	19.043%
9	10.055	1464	1471	1486	rBV	668422	916430	86.11%	16.397%
10	11.085	1634	1640	1649	rBV	517577	641775	60.30%	11.483%
11	12.024	1789	1794	1803	rBV	642667	765456	71.92%	13.696%




Sum of corrected areas: 5588974

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030835.D
Acq On : 26 Aug 2022 19:24
Operator : JC/MD
Sample : N4278-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

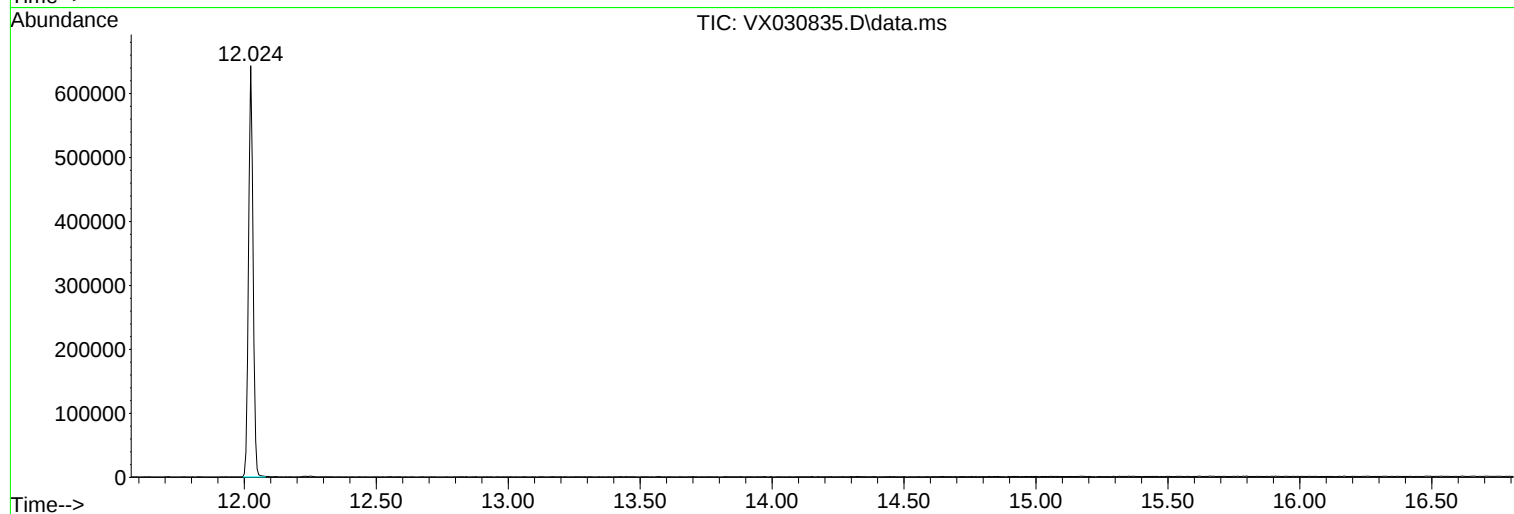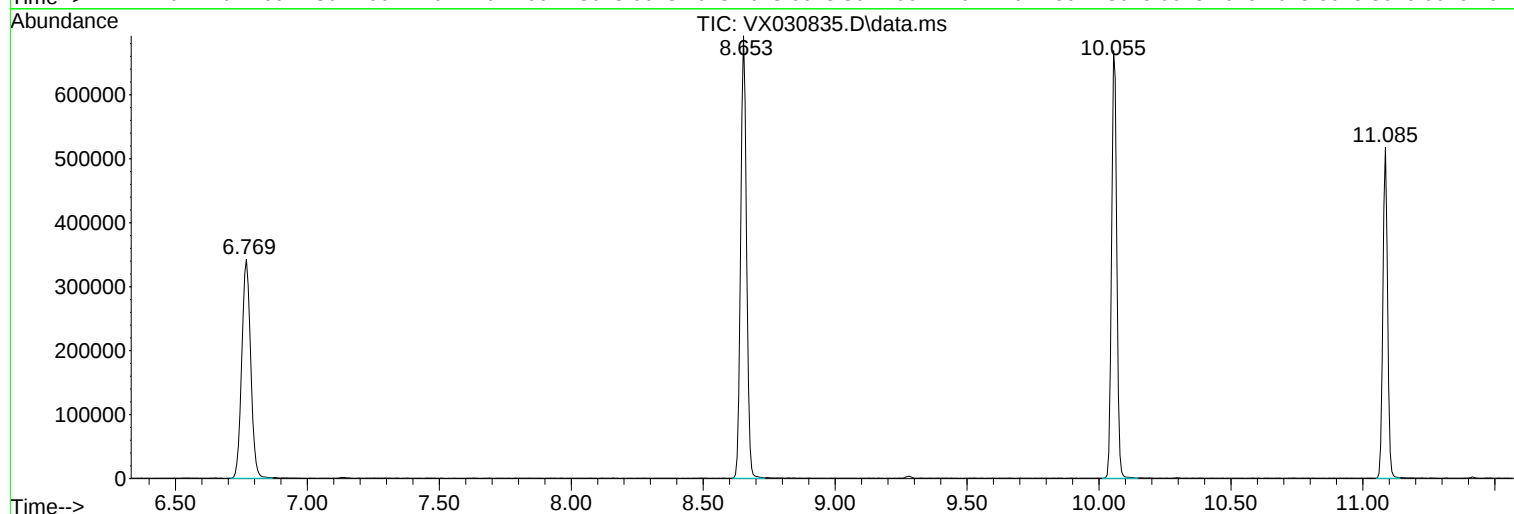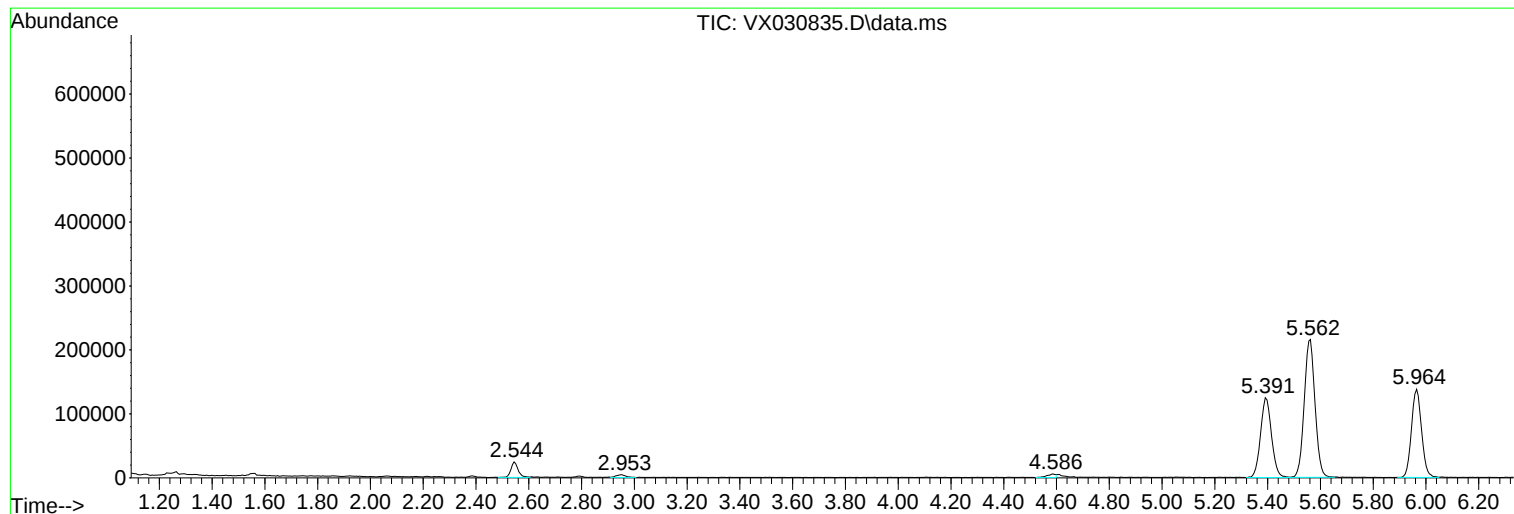

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030835.D
Acq On : 26 Aug 2022 19:24
Operator : JC/MD
Sample : N4278-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030835.D
Acq On : 26 Aug 2022 19:24
Operator : JC/MD
Sample : N4278-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------