

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030844.D
 Acq On : 27 Aug 2022 03:49
 Operator : JC/MD
 Sample : N4281-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20220818

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Title : SW846 8260

Signal : TIC: VX030844.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	293	305	316	rBB	10233	25412	2.08%	0.343%
2	4.574	561	572	587	rBV2	11084	41953	3.44%	0.566%
3	5.385	694	705	719	rBV2	131976	380602	31.18%	5.137%
4	5.550	719	732	744	rBV	232400	655207	53.67%	8.844%
5	5.952	787	798	816	rBV2	148052	396688	32.49%	5.354%
6	6.763	920	931	944	rBV	360090	861710	70.59%	11.631%
7	7.123	981	990	1004	rBV	558407	1220805	100.00%	16.478%
8	8.647	1233	1240	1254	rBV	737760	1161105	95.11%	15.672%
9	10.055	1465	1471	1481	rBV	784701	1018556	83.43%	13.748%
10	11.079	1634	1639	1649	rBV	563896	728682	59.69%	9.836%
11	12.024	1789	1794	1804	rVB	747664	917915	75.19%	12.390%




Sum of corrected areas: 7408635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030844.D
 Acq On : 27 Aug 2022 03:49
 Operator : JC/MD
 Sample : N4281-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
 TIC Integration Parameters: LSCINT.P

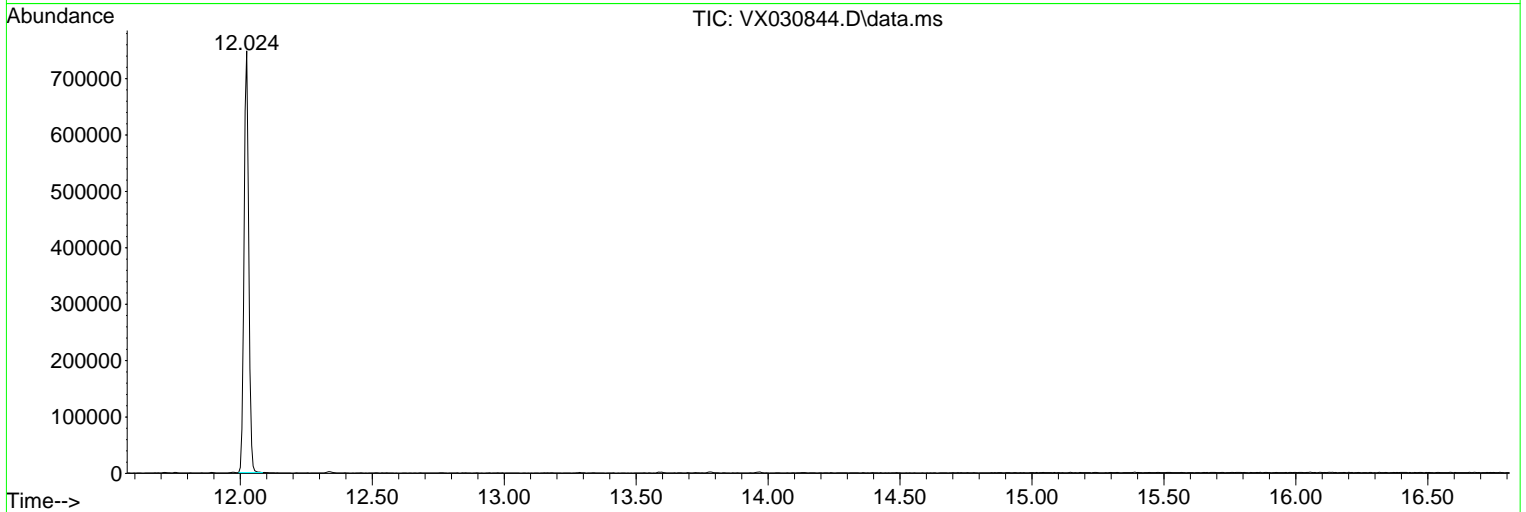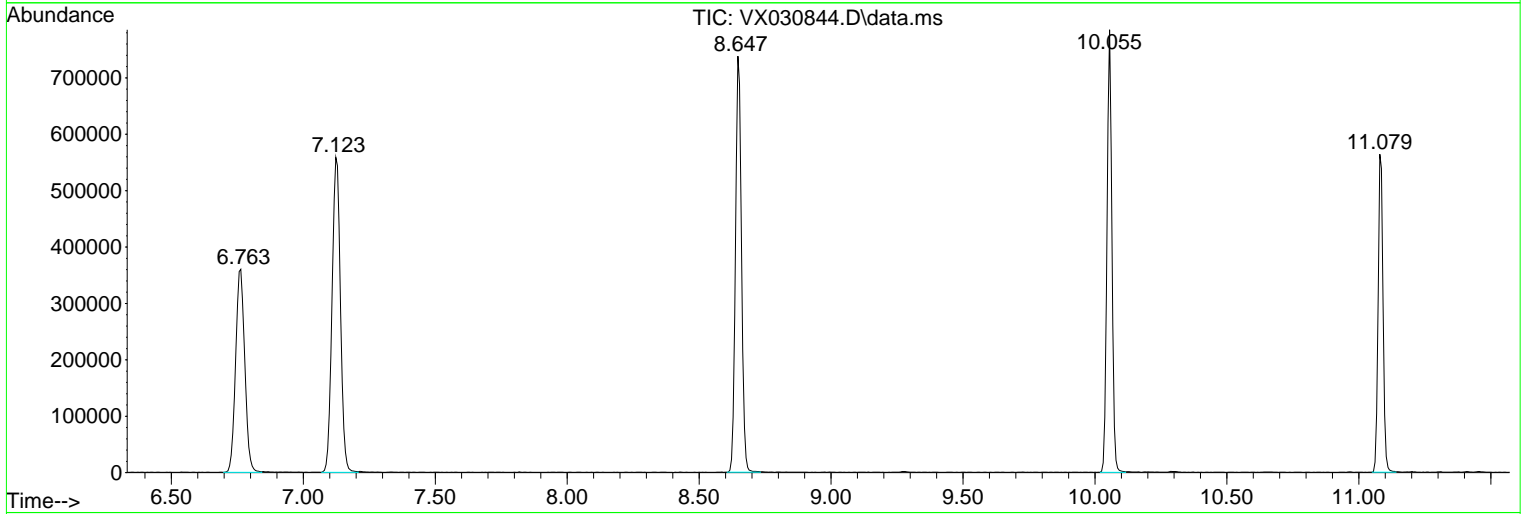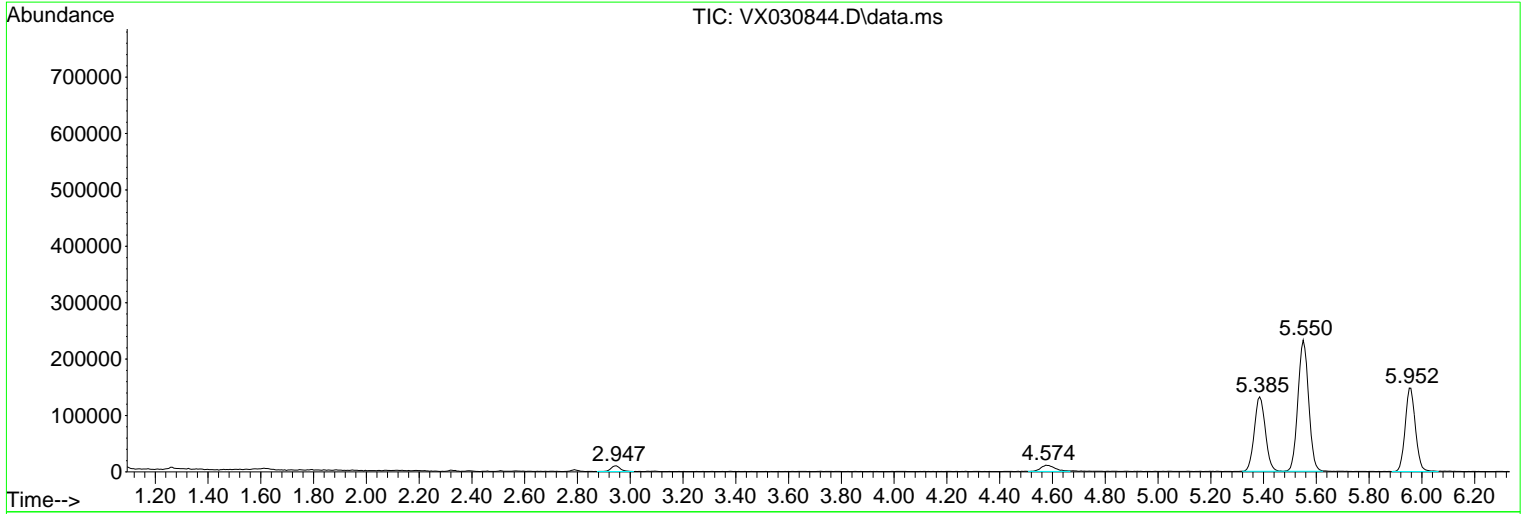

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030844.D
Acq On : 27 Aug 2022 03:49
Operator : JC/MD
Sample : N4281-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030844.D
Acq On : 27 Aug 2022 03:49
Operator : JC/MD
Sample : N4281-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
