

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030845.D
 Acq On : 27 Aug 2022 04:19
 Operator : JC/MD
 Sample : N4281-03 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE108D2-20220818

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	297	305	314	rBV	9692	23010	1.94%	0.322%
2	4.587	562	574	584	rBV2	12494	45235	3.81%	0.633%
3	5.385	693	705	719	rBV	135173	399337	33.62%	5.588%
4	5.556	721	733	747	rVV	237612	680294	57.27%	9.519%
5	5.958	789	799	815	rBV2	148201	403013	33.93%	5.639%
6	6.763	920	931	943	rBV	370919	887921	74.75%	12.424%
7	7.123	981	990	1003	rBV	402546	879384	74.03%	12.305%
8	8.653	1234	1241	1250	rBV	750910	1187800	100.00%	16.620%
9	10.055	1465	1471	1482	rBV	772807	1017971	85.70%	14.244%
10	11.085	1634	1640	1650	rBV	553207	724937	61.03%	10.144%
11	12.024	1788	1794	1806	rBV	734685	897847	75.59%	12.563%




Sum of corrected areas: 7146749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030845.D
Acq On : 27 Aug 2022 04:19
Operator : JC/MD
Sample : N4281-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D2-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

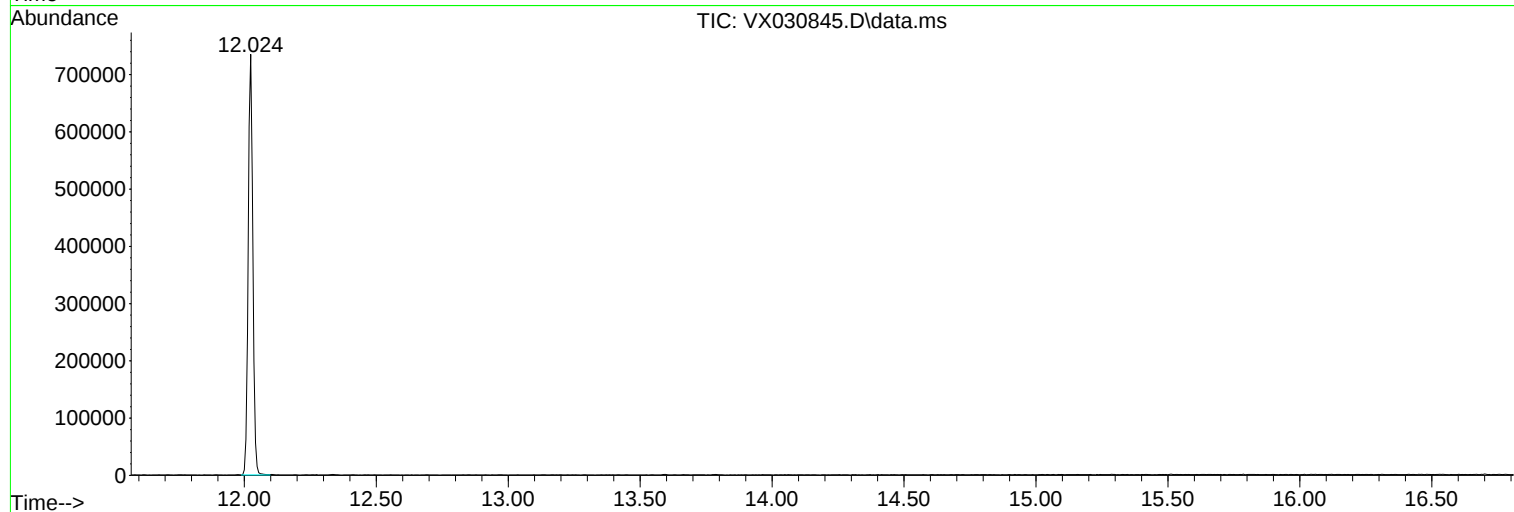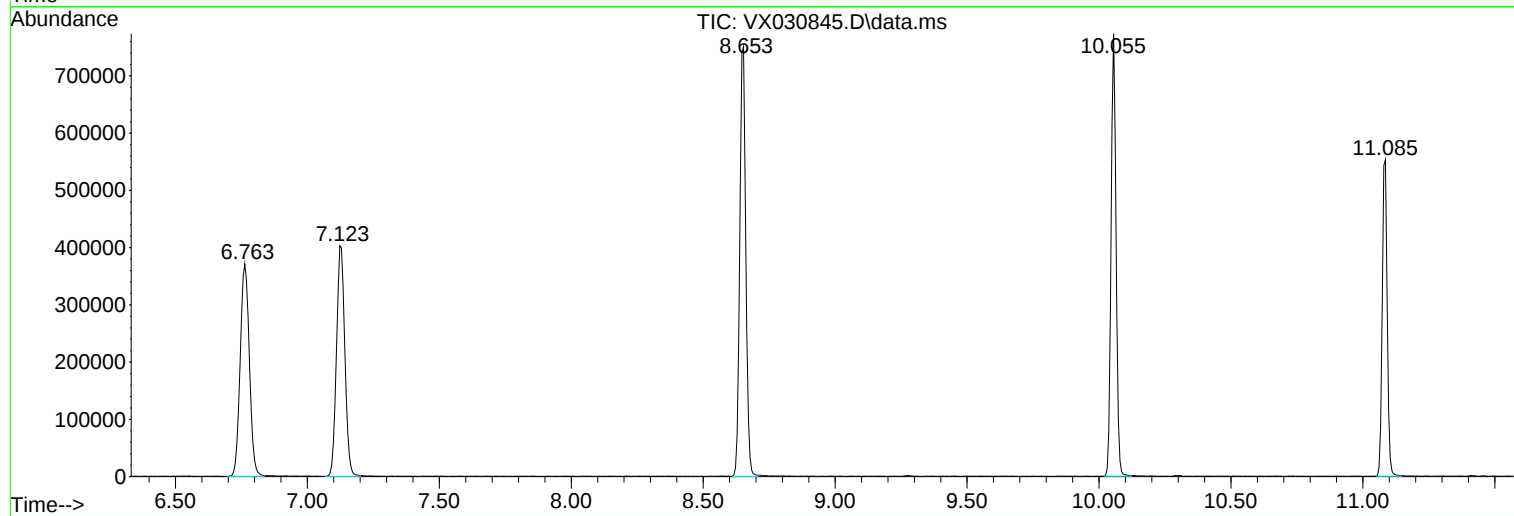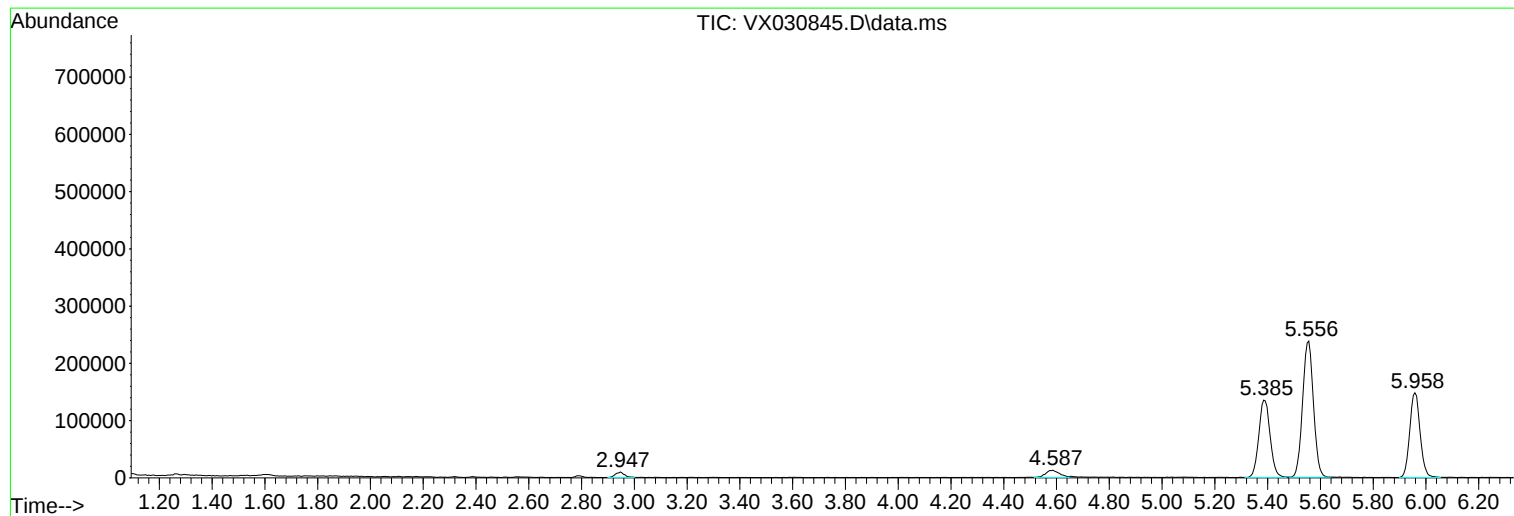

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030845.D
Acq On : 27 Aug 2022 04:19
Operator : JC/MD
Sample : N4281-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D2-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030845.D
Acq On : 27 Aug 2022 04:19
Operator : JC/MD
Sample : N4281-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D2-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------