

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030846.D
 Acq On : 27 Aug 2022 04:42
 Operator : JC/MD
 Sample : N4281-10 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP06-20220818

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Title : SW846 8260

Signal : TIC: VX030846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	295	305	314	rBV	19403	42887	3.54%	0.655%
2	4.580	564	573	587	rBV	12375	42960	3.54%	0.656%
3	5.391	694	706	721	rBV	142190	405740	33.47%	6.195%
4	5.556	721	733	750	rVB2	243780	693126	57.18%	10.583%
5	5.958	789	799	816	rBV	154675	414788	34.22%	6.333%
6	6.763	922	931	944	rBV	394778	922103	76.07%	14.079%
7	7.129	981	991	1002	rVB2	30496	64029	5.28%	0.978%
8	8.653	1234	1241	1251	rBV	786257	1212126	100.00%	18.507%
9	10.055	1465	1471	1478	rBV	797146	1055929	87.11%	16.122%
10	11.085	1634	1640	1651	rBV	571160	757867	62.52%	11.571%
11	12.024	1789	1794	1806	rVB	777651	938001	77.38%	14.322%




Sum of corrected areas: 6549556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030846.D
Acq On : 27 Aug 2022 04:42
Operator : JC/MD
Sample : N4281-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

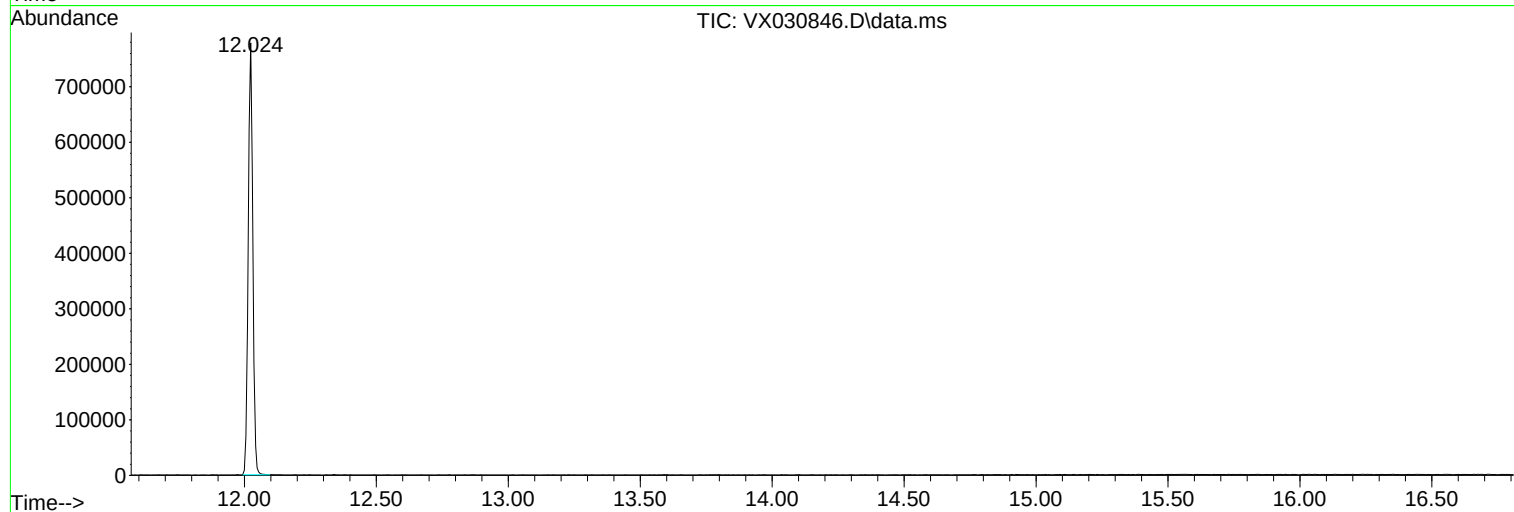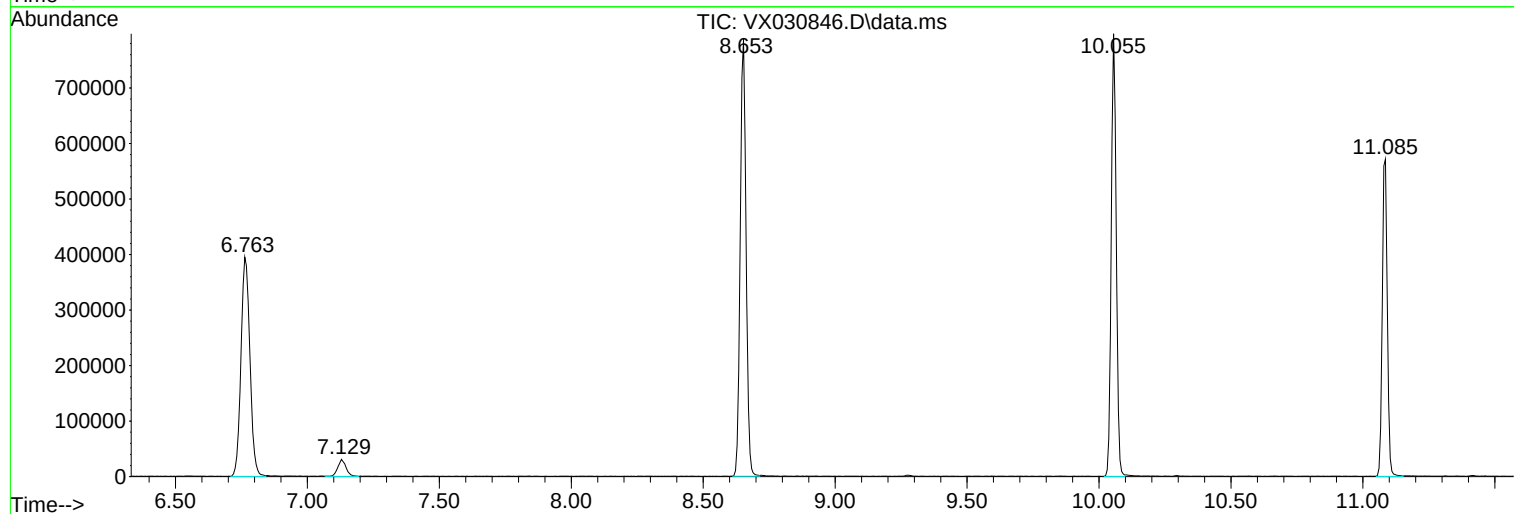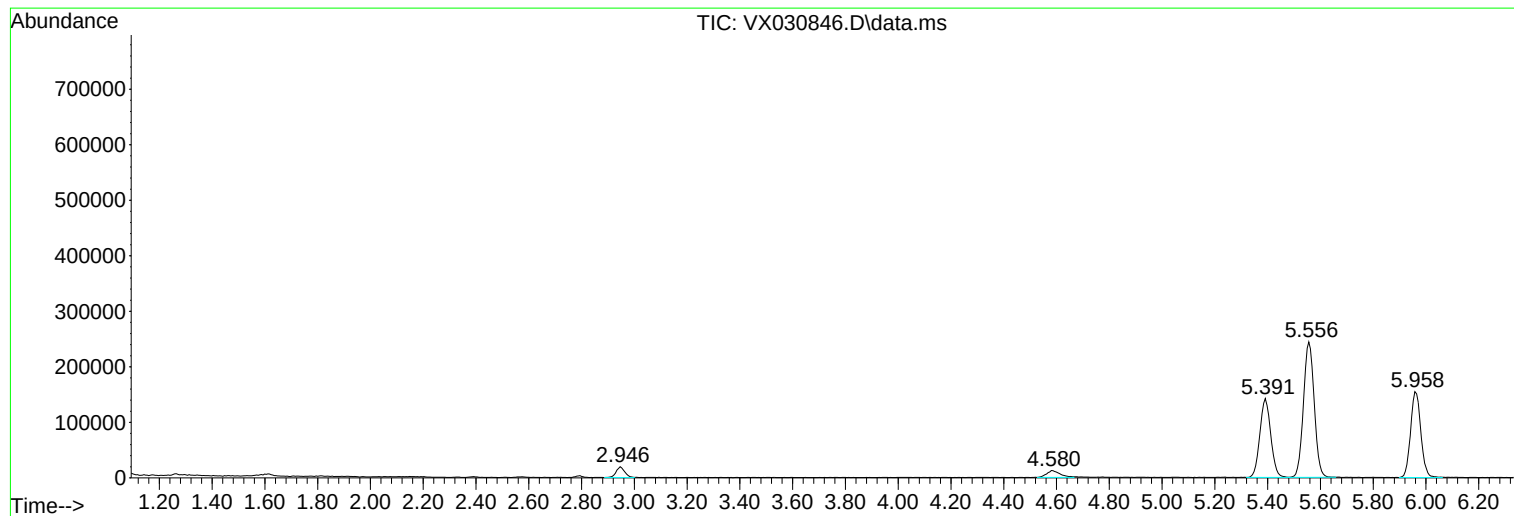

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030846.D
Acq On : 27 Aug 2022 04:42
Operator : JC/MD
Sample : N4281-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030846.D
Acq On : 27 Aug 2022 04:42
Operator : JC/MD
Sample : N4281-10 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------