

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030851.D
Acq On : 27 Aug 2022 06:39
Operator : JC/MD
Sample : N4281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D2-20220818

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.136	167	172	180	rVB	21409	36401	3.11%	0.574%
2	2.331	197	204	209	rBV2	23783	43923	3.76%	0.693%
3	5.391	695	706	720	rBV	135423	392667	33.57%	6.196%
4	5.556	723	733	748	rVB2	236752	667500	57.07%	10.533%
5	5.964	789	800	817	rBV	149455	405177	34.64%	6.393%
6	6.763	922	931	948	rBV	385974	899005	76.87%	14.186%
7	7.129	982	991	1004	rBV2	35966	79859	6.83%	1.260%
8	8.653	1233	1241	1251	rBV	764897	1169550	100.00%	18.455%
9	10.055	1465	1471	1484	rBV	772512	1017881	87.03%	16.061%
10	11.085	1634	1640	1652	rBV	560807	720463	61.60%	11.368%
11	12.024	1788	1794	1803	rBV	726160	905040	77.38%	14.281%




Sum of corrected areas: 6337466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030851.D
Acq On : 27 Aug 2022 06:39
Operator : JC/MD
Sample : N4281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D2-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

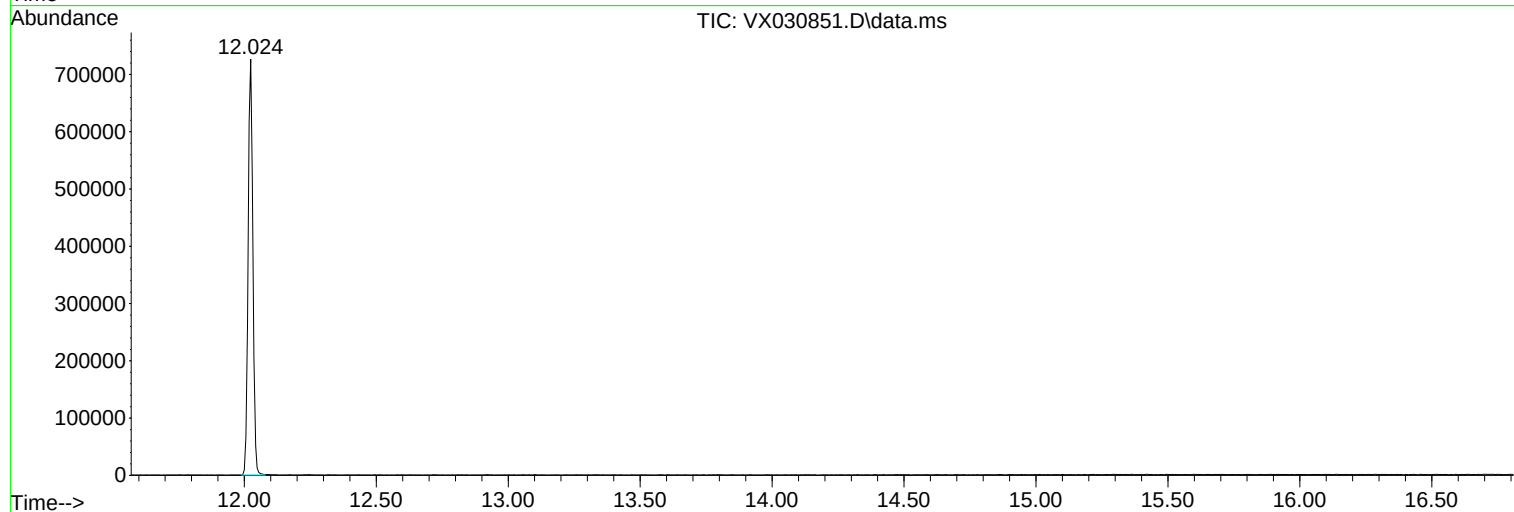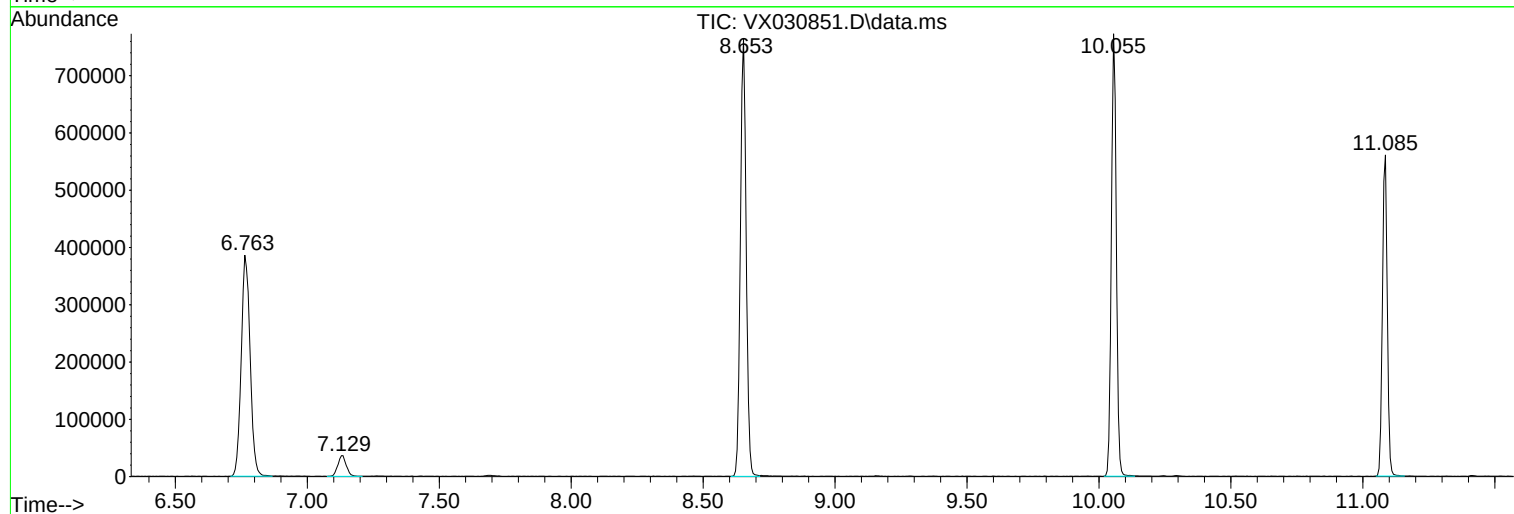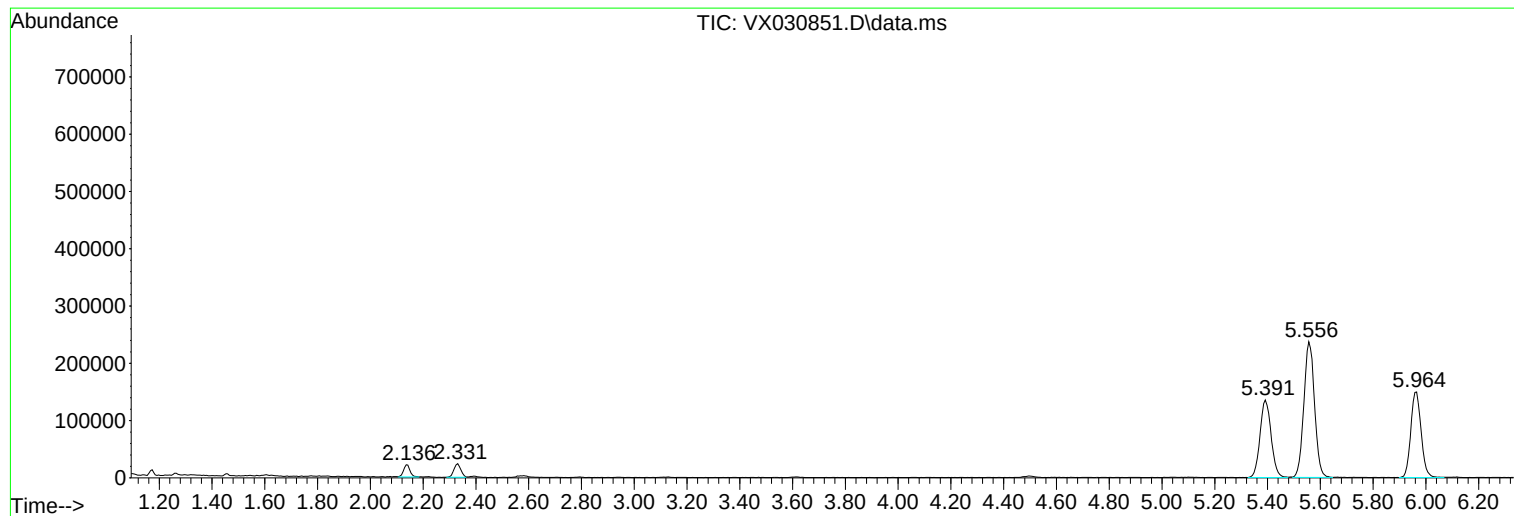

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030851.D
Acq On : 27 Aug 2022 06:39
Operator : JC/MD
Sample : N4281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D2-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030851.D
Acq On : 27 Aug 2022 06:39
Operator : JC/MD
Sample : N4281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D2-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------