

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030852.D
Acq On : 27 Aug 2022 07:03
Operator : JC/MD
Sample : N4281-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D3-20220818

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	197	204	211	rBV3	24995	47131	4.05%	0.657%
2	5.391	694	706	720	rBV2	135955	391448	33.61%	5.457%
3	5.556	720	733	747	rVV	235046	665594	57.15%	9.278%
4	5.958	788	799	815	rBV	152560	400403	34.38%	5.581%
5	6.763	922	931	947	rBV	366401	880052	75.56%	12.267%
6	7.129	982	991	1004	rBV	467725	997340	85.64%	13.902%
7	8.653	1234	1241	1257	rBV	767361	1164640	100.00%	16.234%
8	9.275	1338	1343	1349	rBV	24148	34189	2.94%	0.477%
9	10.055	1465	1471	1482	rBV	755582	1006592	86.43%	14.031%
10	11.085	1634	1640	1653	rBV	547807	708358	60.82%	9.874%
11	12.024	1788	1794	1803	rBV	716727	878165	75.40%	12.241%




Sum of corrected areas: 7173912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030852.D
Acq On : 27 Aug 2022 07:03
Operator : JC/MD
Sample : N4281-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D3-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

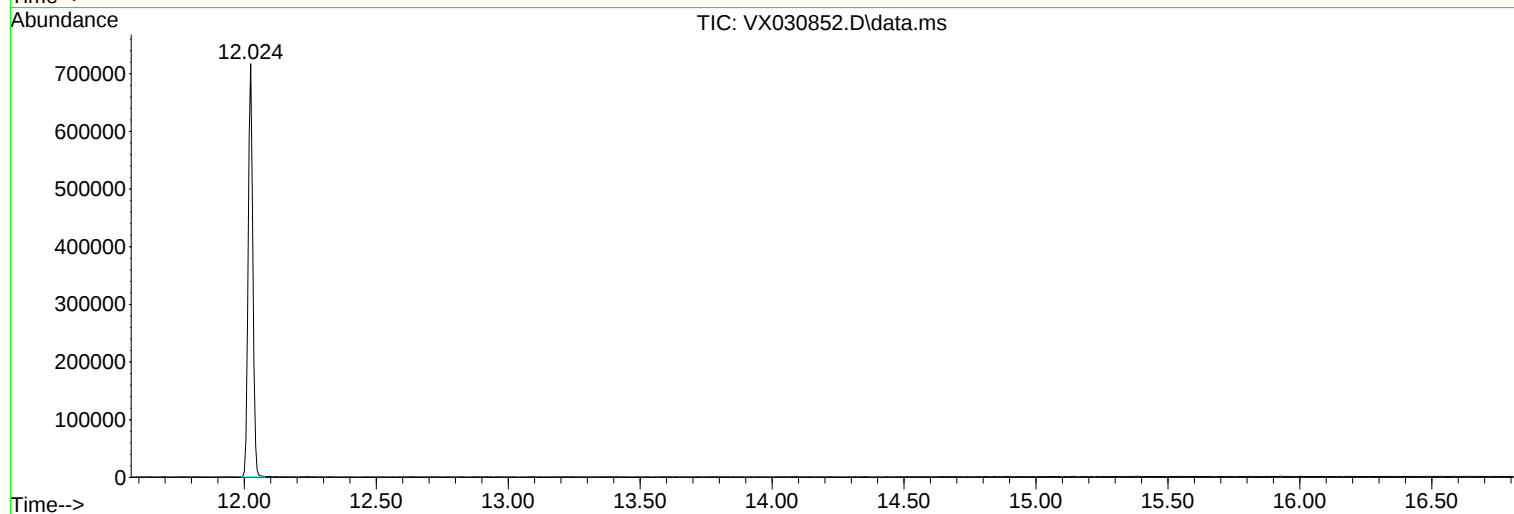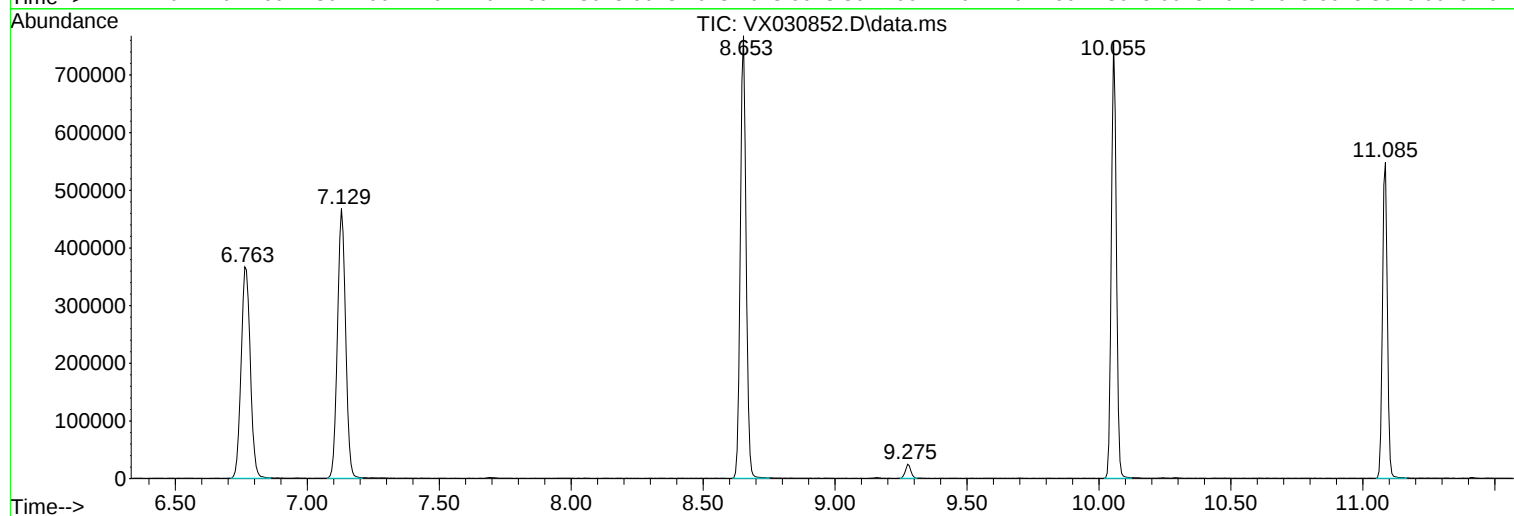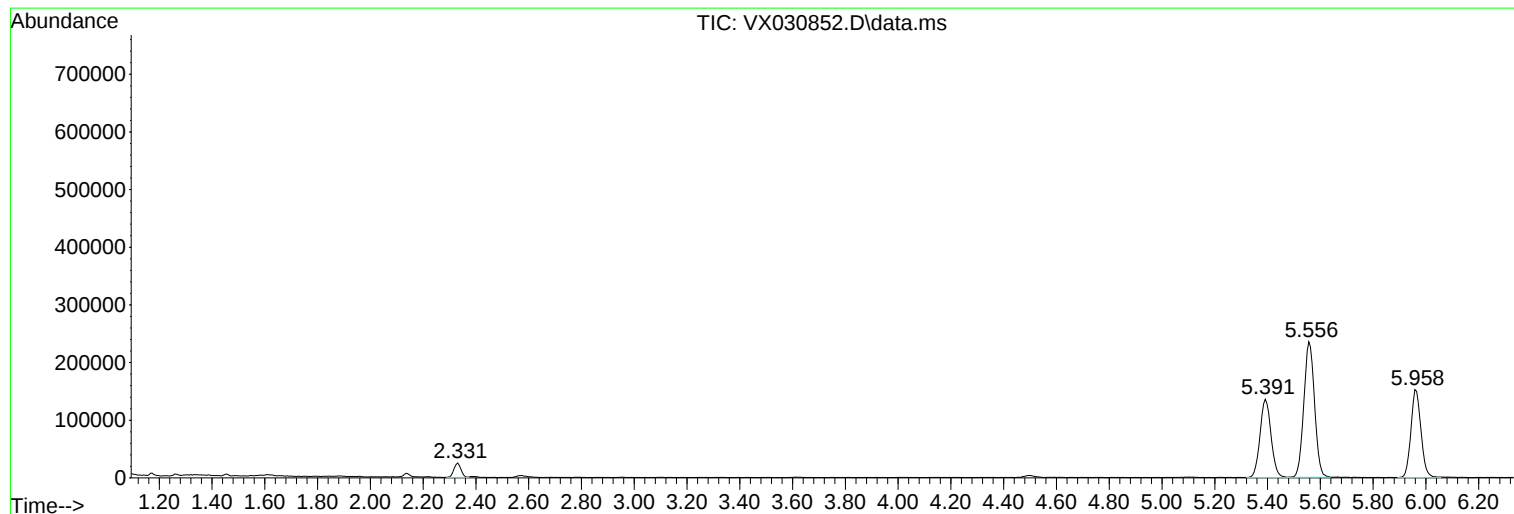

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030852.D
Acq On : 27 Aug 2022 07:03
Operator : JC/MD
Sample : N4281-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D3-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030852.D
Acq On : 27 Aug 2022 07:03
Operator : JC/MD
Sample : N4281-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D3-20220818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------