

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
 Data File : VX030855.D
 Acq On : 27 Aug 2022 08:13
 Operator : JC/MD
 Sample : N4281-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D1-20220819

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	198	204	210	rBV2	11346	20173	1.72%	0.288%
2	5.391	694	706	722	rBV	133016	392693	33.48%	5.600%
3	5.556	722	733	748	rVV	232914	660395	56.31%	9.417%
4	5.958	789	799	817	rBV	148857	403168	34.38%	5.749%
5	6.769	922	932	947	rBV	367889	872053	74.35%	12.436%
6	7.129	981	991	1005	rBV	383975	821624	70.05%	11.717%
7	8.653	1232	1241	1249	rBV	759343	1172844	100.00%	16.725%
8	9.275	1338	1343	1350	rVB	31535	47828	4.08%	0.682%
9	10.055	1465	1471	1483	rBV	753324	1009904	86.11%	14.401%
10	11.085	1634	1640	1653	rBV	579070	727389	62.02%	10.373%
11	12.024	1789	1794	1803	rVB	743641	884442	75.41%	12.612%




Sum of corrected areas: 7012513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030855.D
Acq On : 27 Aug 2022 08:13
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

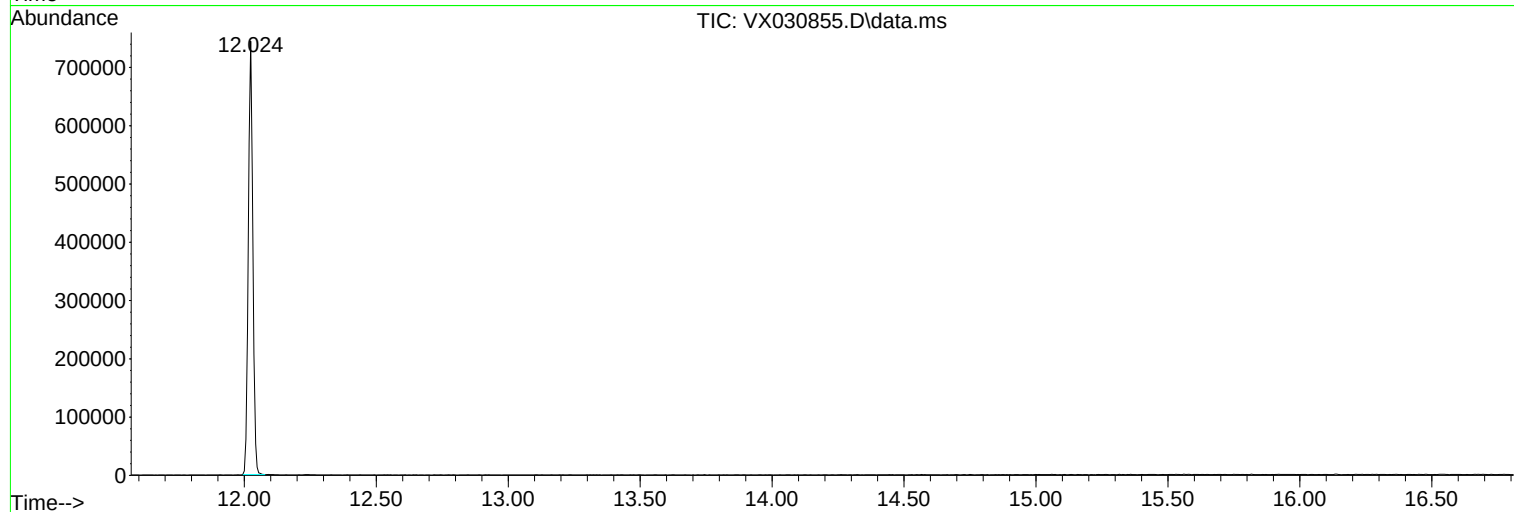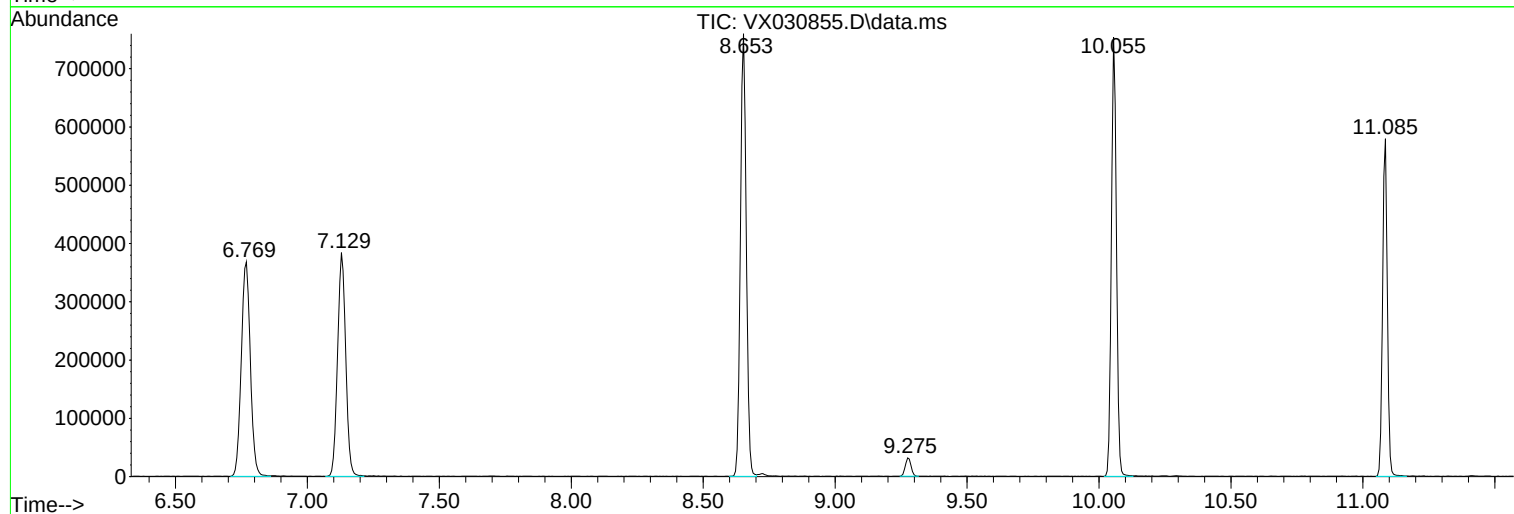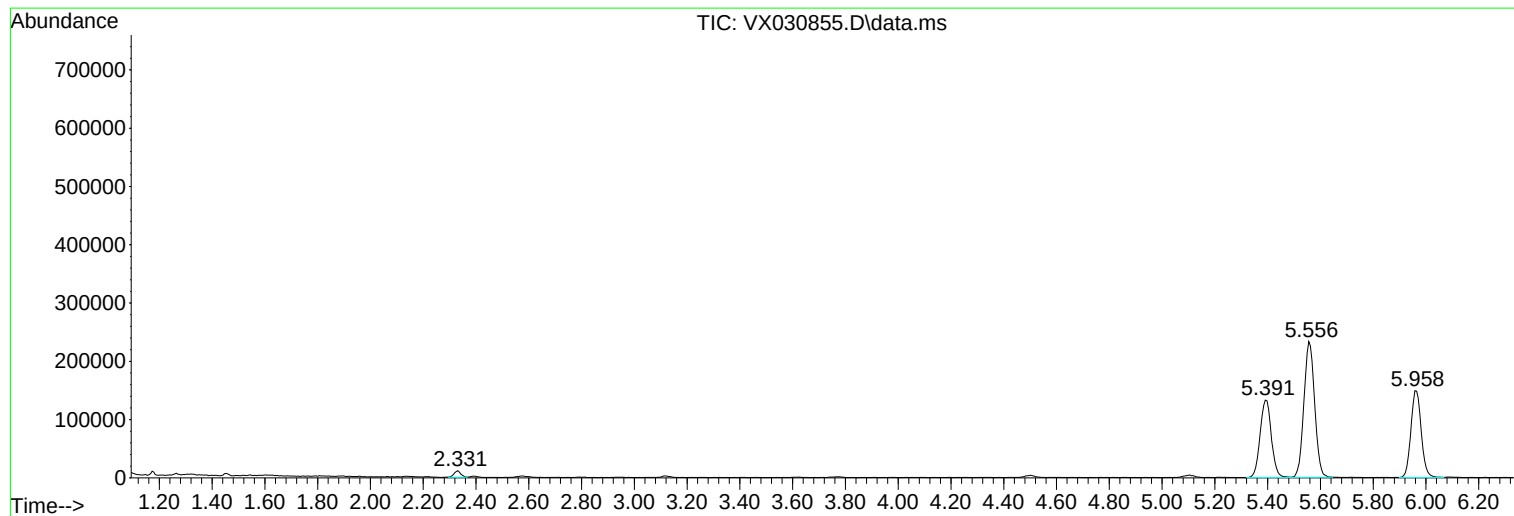

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030855.D
Acq On : 27 Aug 2022 08:13
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030855.D
Acq On : 27 Aug 2022 08:13
Operator : JC/MD
Sample : N4281-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D1-20220819

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------