



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082622\
Data File : VX030811.D
Acq On : 26 Aug 2022 09:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Title : SW846 8260
Last Update : Fri Aug 26 02:03:28 2022

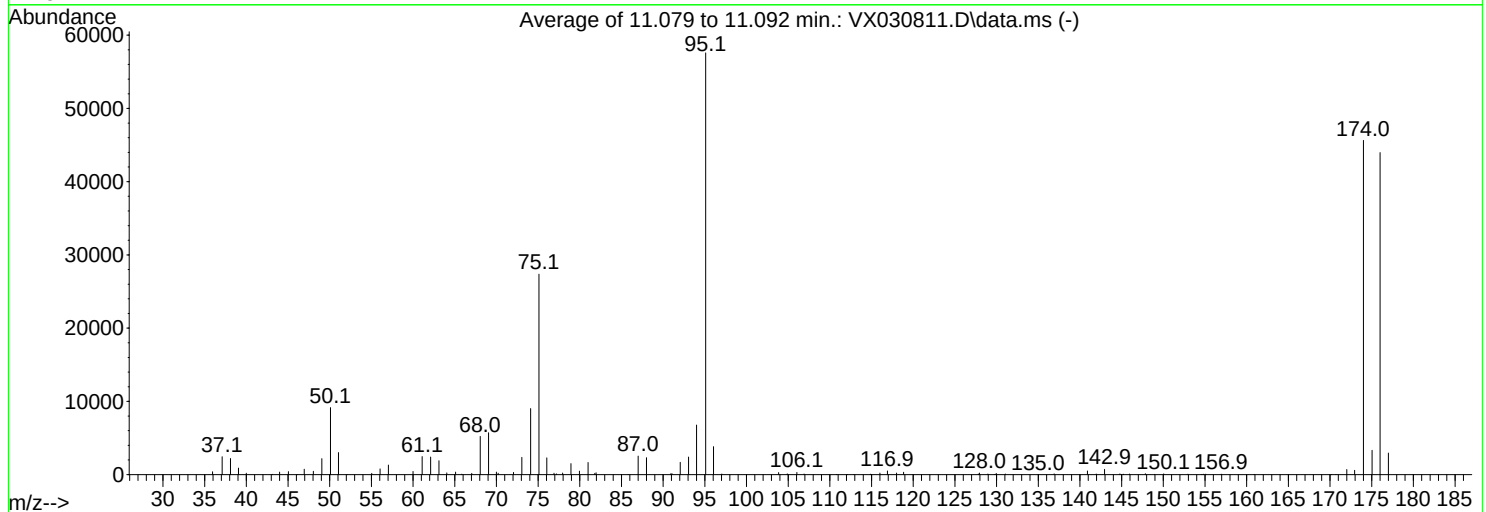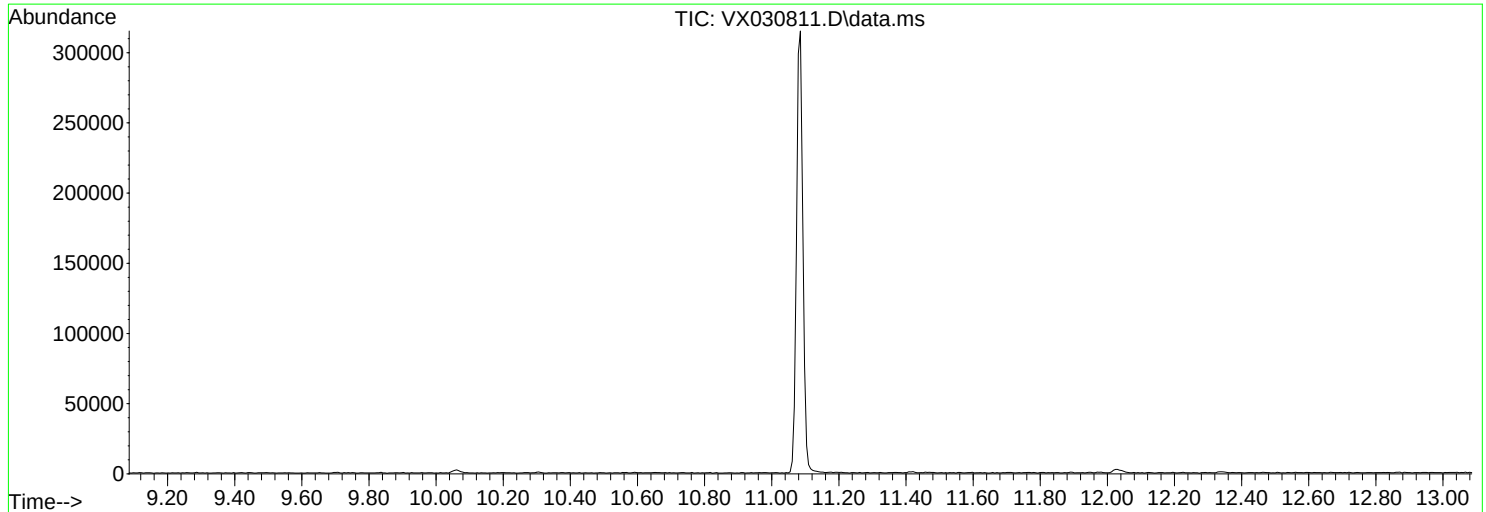

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	9148	PASS
75	95	30	60	47.5	27363	PASS
95	95	100	100	100.0	57587	PASS
96	95	5	9	6.6	3820	PASS
173	174	0.00	2	1.3	585	PASS
174	95	50	100	79.2	45632	PASS
175	174	5	9	7.3	3315	PASS
176	174	95	101	96.4	43976	PASS
177	176	5	9	6.7	2948	PASS