

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033283.D
Acq On : 07 Dec 2022 15:53
Operator : JC/MD
Sample : VX1207MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1207MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	719	rBV	91467	264596	36.04%	6.616%
2	5.550	721	732	748	rVB	163291	456109	62.13%	11.405%
3	5.958	787	799	814	rBV	97564	260244	35.45%	6.508%
4	6.763	921	931	950	rBV	234697	559890	76.26%	14.000%
5	8.647	1234	1240	1250	rBV	472205	734171	100.00%	18.358%
6	10.055	1465	1471	1487	rBV	477916	643503	87.65%	16.091%
7	11.079	1634	1639	1656	rBV	382166	486780	66.30%	12.172%
8	12.024	1788	1794	1807	rBV	469436	593832	80.88%	14.849%




Sum of corrected areas: 3999125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033283.D
Acq On : 07 Dec 2022 15:53
Operator : JC/MD
Sample : VX1207MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1207MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

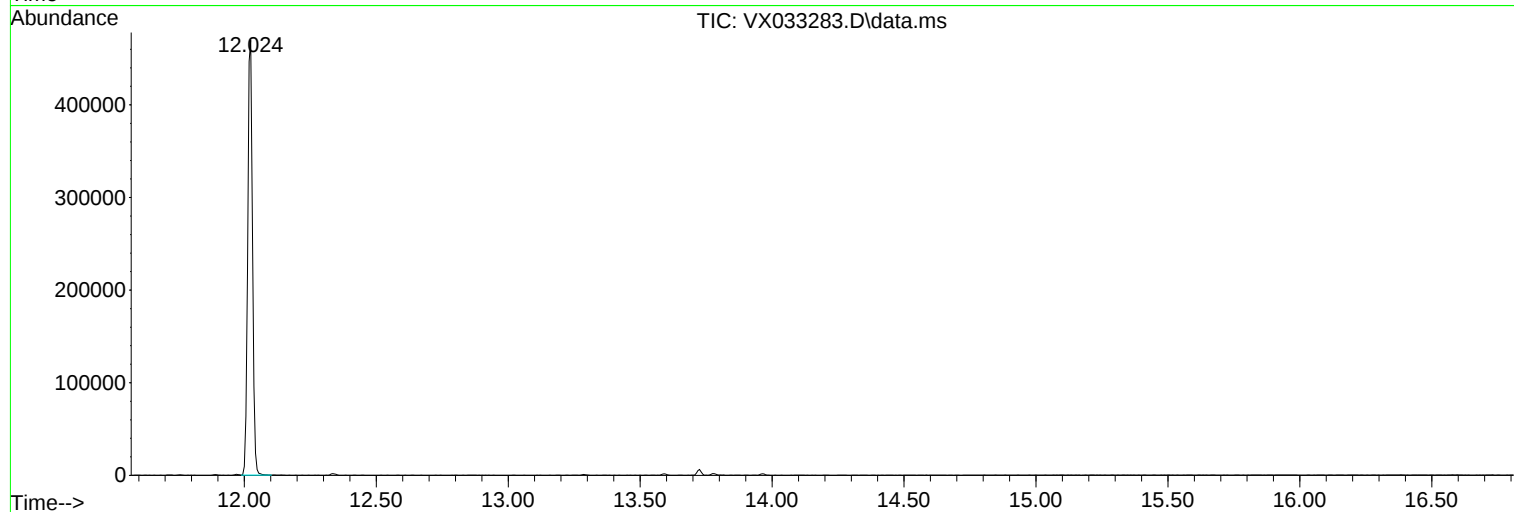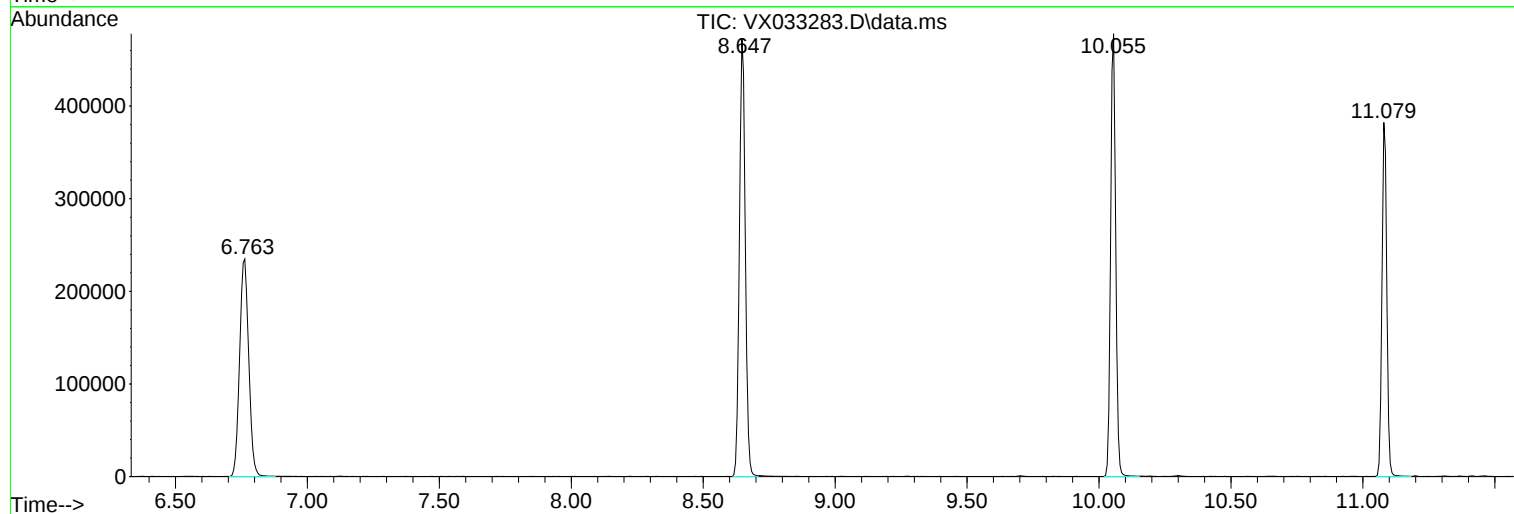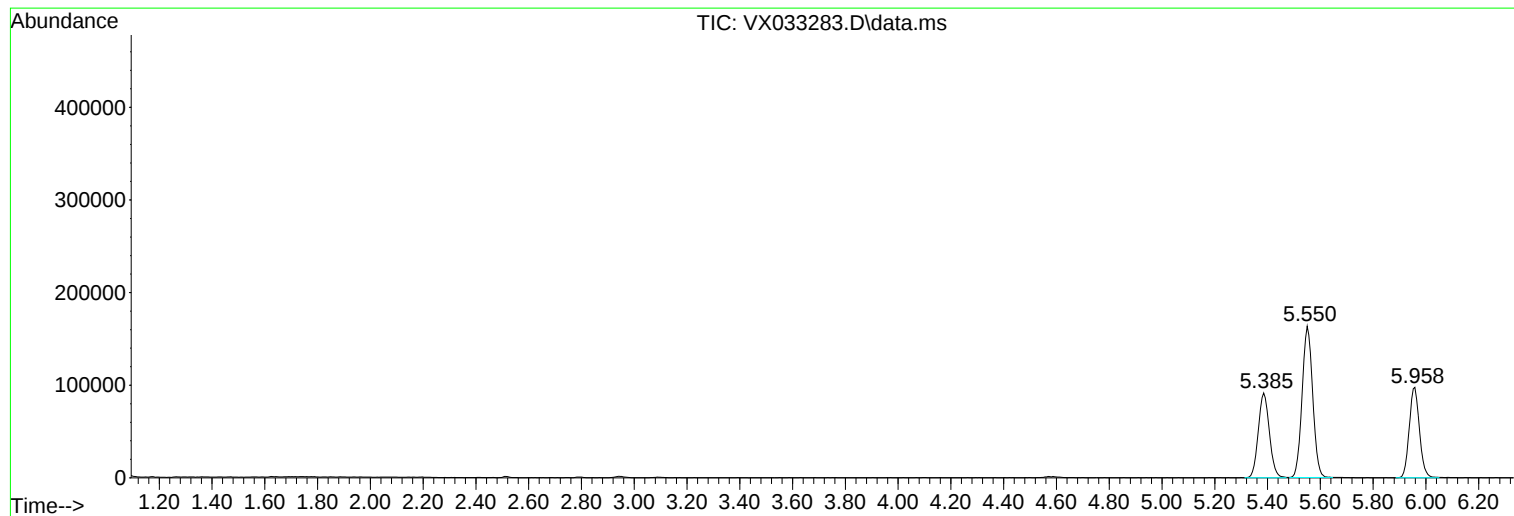

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033283.D
Acq On : 07 Dec 2022 15:53
Operator : JC/MD
Sample : VX1207MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1207MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033283.D
Acq On : 07 Dec 2022 15:53
Operator : JC/MD
Sample : VX1207MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1207MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc