

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
 Data File : VX033290.D
 Acq On : 07 Dec 2022 18:46
 Operator : JC/MD
 Sample : N5875-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-38

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	36	47	49	rBV2	12416	29877	5.06%	0.875%
2	1.752	105	109	114	rVB2	10042	13649	2.31%	0.400%
3	2.989	300	312	324	rVB4	2218	8269	1.40%	0.242%
4	3.117	324	333	342	rBV2	10273	24539	4.16%	0.718%
5	4.306	519	528	538	rVB3	2219	6119	1.04%	0.179%
6	5.019	636	645	662	rBV2	7982	25231	4.27%	0.739%
7	5.391	693	706	716	rBV2	53775	158767	26.88%	4.648%
8	5.556	723	733	750	rVB	145680	415183	70.30%	12.154%
9	5.958	787	799	808	rBV	42641	114939	19.46%	3.365%
10	6.038	808	812	823	rVB3	4669	11635	1.97%	0.341%
11	6.763	920	931	944	rBV	218817	519259	87.92%	15.201%
12	8.653	1233	1241	1248	rBV	158204	257247	43.56%	7.531%
13	10.055	1465	1471	1482	rBV	450157	590579	100.00%	17.289%
14	10.195	1489	1494	1499	rBV	7465	9655	1.63%	0.283%
15	10.305	1507	1512	1518	rVB2	4588	6668	1.13%	0.195%
16	10.964	1615	1620	1625	rBV2	7189	8826	1.49%	0.258%
17	11.079	1634	1639	1652	rBV	284670	369680	62.60%	10.822%
18	11.305	1672	1676	1683	rBV	5628	7137	1.21%	0.209%
19	11.616	1723	1727	1733	rVB	5445	6683	1.13%	0.196%
20	12.024	1788	1794	1801	rBV	447490	555908	94.13%	16.274%
21	12.244	1824	1830	1838	rBV2	34992	45302	7.67%	1.326%
22	12.616	1886	1891	1894	rBV	7388	8943	1.51%	0.262%
23	12.701	1899	1905	1912	rVB2	17616	26091	4.42%	0.764%
24	12.921	1935	1941	1945	rBV	10775	13949	2.36%	0.408%
25	13.170	1979	1982	1990	rVB	4918	6990	1.18%	0.205%
26	13.292	1997	2002	2008	rVB2	20079	26636	4.51%	0.780%
27	13.420	2019	2023	2029	rVB2	6807	9187	1.56%	0.269%
28	13.774	2076	2081	2089	rVB	20336	29074	4.92%	0.851%
29	13.926	2100	2106	2110	rBV2	5191	6408	1.09%	0.188%
30	14.219	2148	2154	2159	rBV4	3752	7628	1.29%	0.223%
31	14.378	2176	2180	2184	rBV4	4461	6277	1.06%	0.184%
32	14.640	2219	2223	2227	rVB	9220	11704	1.98%	0.343%
33	14.780	2239	2246	2255	rBV	43224	57305	9.70%	1.678%
34	15.615	2375	2383	2386	rBV2	8038	11519	1.95%	0.337%
35	16.328	2491	2500	2510	rVB	5066	9129	1.55%	0.267%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033290.D
Acq On : 07 Dec 2022 18:46
Operator : JC/MD
Sample : N5875-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Title : SW846 8260




Sum of corrected areas: 3415992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033290.D
Acq On : 07 Dec 2022 18:46
Operator : JC/MD
Sample : N5875-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

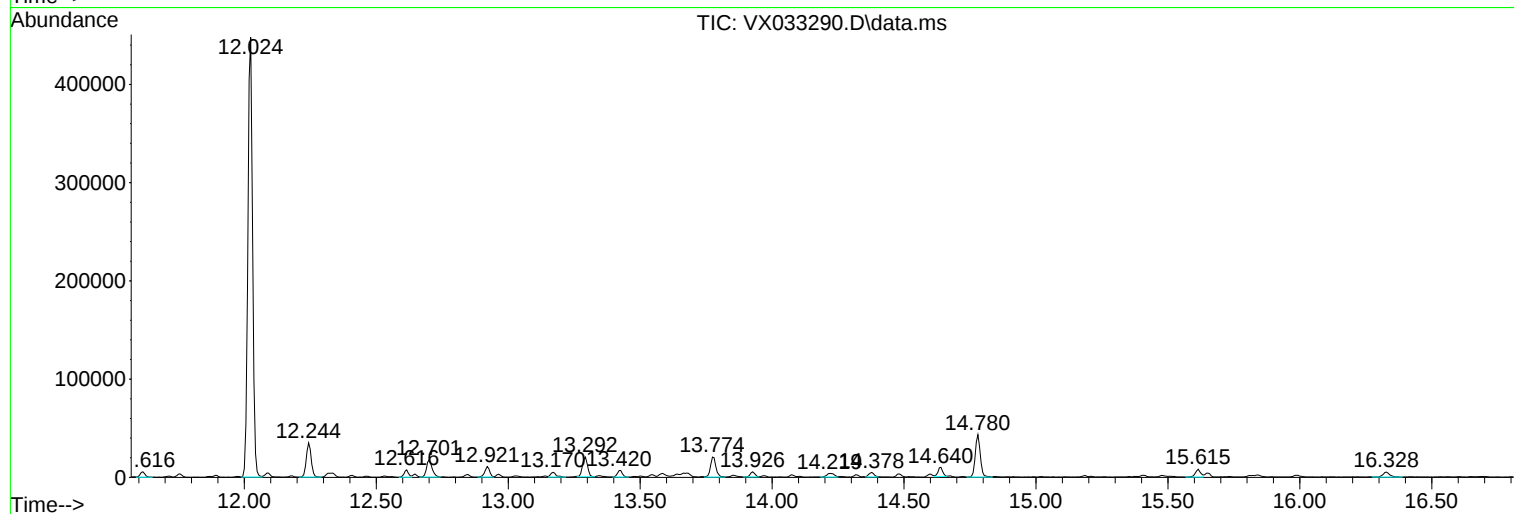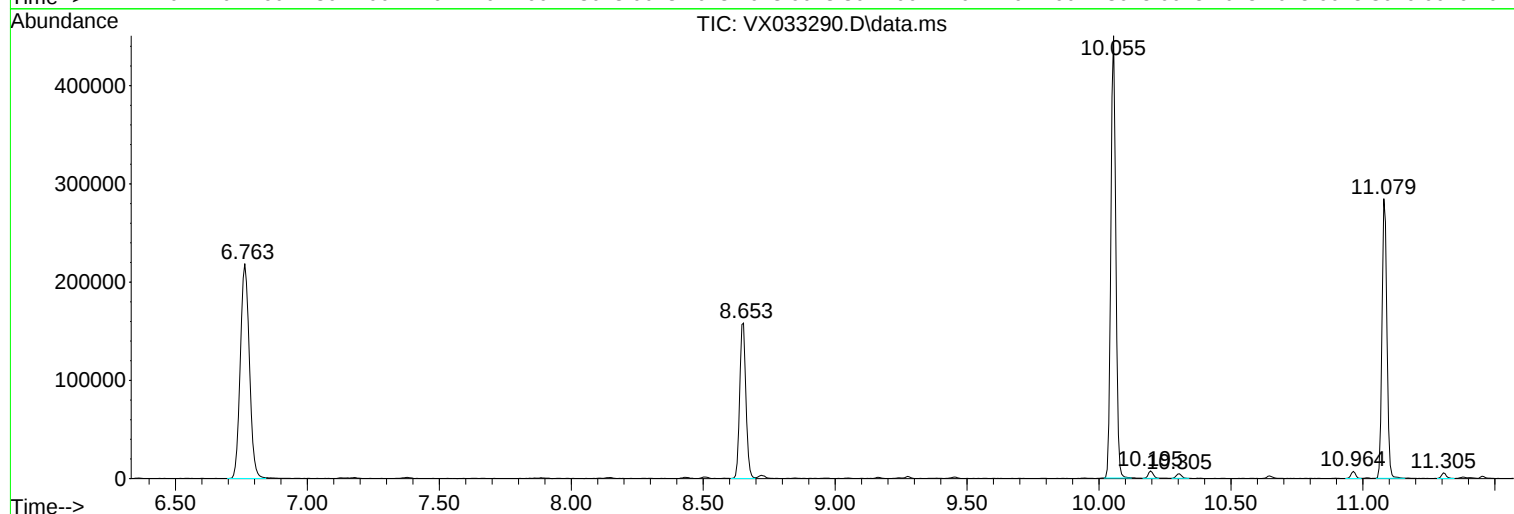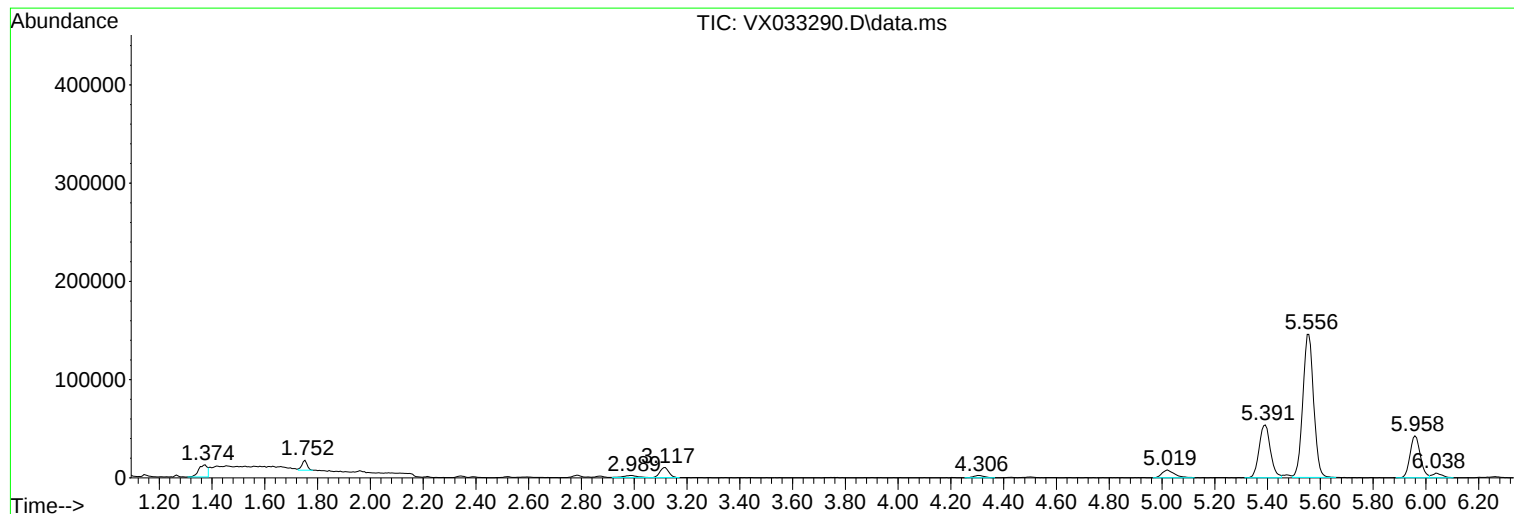

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033290.D
Acq On : 07 Dec 2022 18:46
Operator : JC/MD
Sample : N5875-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Naphthalene, 1-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.780	5.15 ug/l	57305	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 1-methyl-	142	C11H10	000090-12-0	96
2			Naphthalene, 2-methyl-	142	C11H10	000091-57-6	96
3			Benzocycloheptatriene	142	C11H10	000264-09-5	91
4			1,4-Methanonaphthalene, 1,4-dihy...	142	C11H10	004453-90-1	90
5			1H-Indene, 1-ethylidene-	142	C11H10	002471-83-2	59

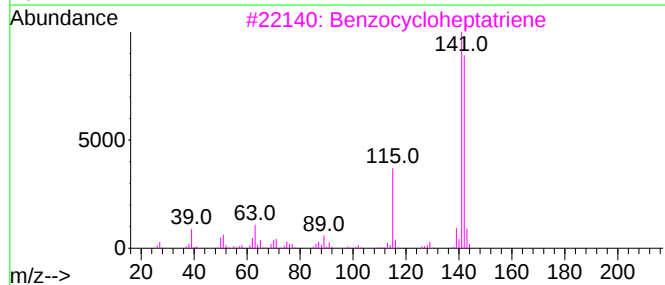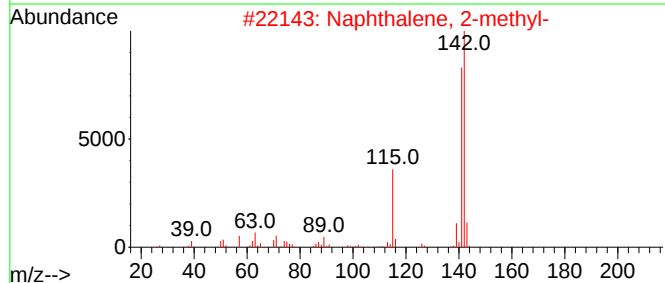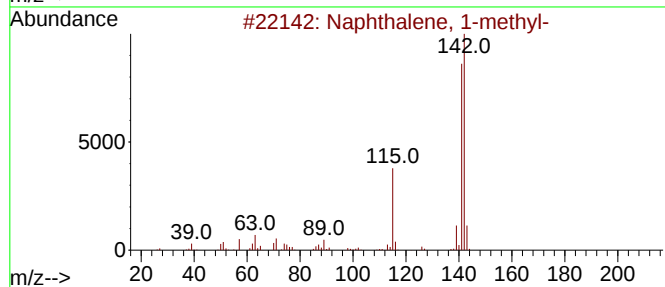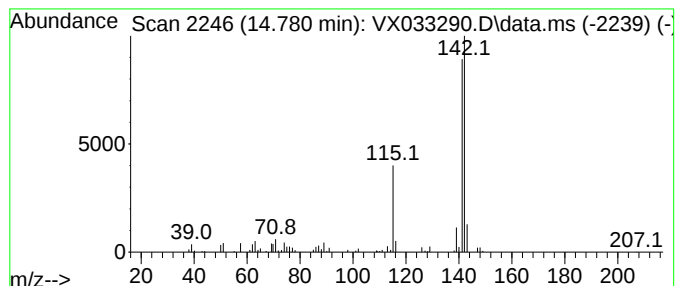

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033290.D
Acq On : 07 Dec 2022 18:46
Operator : JC/MD
Sample : N5875-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 1-...	14.780	5.2	ug/l	57305	4	12.024	555908	50.0