

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
 Data File : VX033292.D
 Acq On : 07 Dec 2022 19:32
 Operator : JC/MD
 Sample : N5865-09DL 2000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LEA-5IDL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	24	29	44	rBV	19859	56028	9.51%	1.594%
2	2.941	297	304	318	rVB	7604	17564	2.98%	0.500%
3	4.489	548	558	584	rBV	124712	346903	58.86%	9.868%
4	5.391	695	706	720	rBV	53445	157516	26.73%	4.481%
5	5.556	722	733	752	rVB	144712	408932	69.38%	11.632%
6	5.958	790	799	823	rVB	42070	113301	19.22%	3.223%
7	6.763	922	931	948	rBV	220249	515841	87.52%	14.673%
8	7.129	983	991	1005	rBV	66242	145611	24.71%	4.142%
9	8.653	1234	1241	1250	rBV	161368	257141	43.63%	7.314%
10	10.055	1465	1471	1482	rBV	445691	589385	100.00%	16.765%
11	11.079	1634	1639	1651	rBV	282995	364006	61.76%	10.354%
12	12.024	1788	1794	1804	rBV	438264	543347	92.19%	15.455%




Sum of corrected areas: 3515575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033292.D
Acq On : 07 Dec 2022 19:32
Operator : JC/MD
Sample : N5865-09DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-5IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

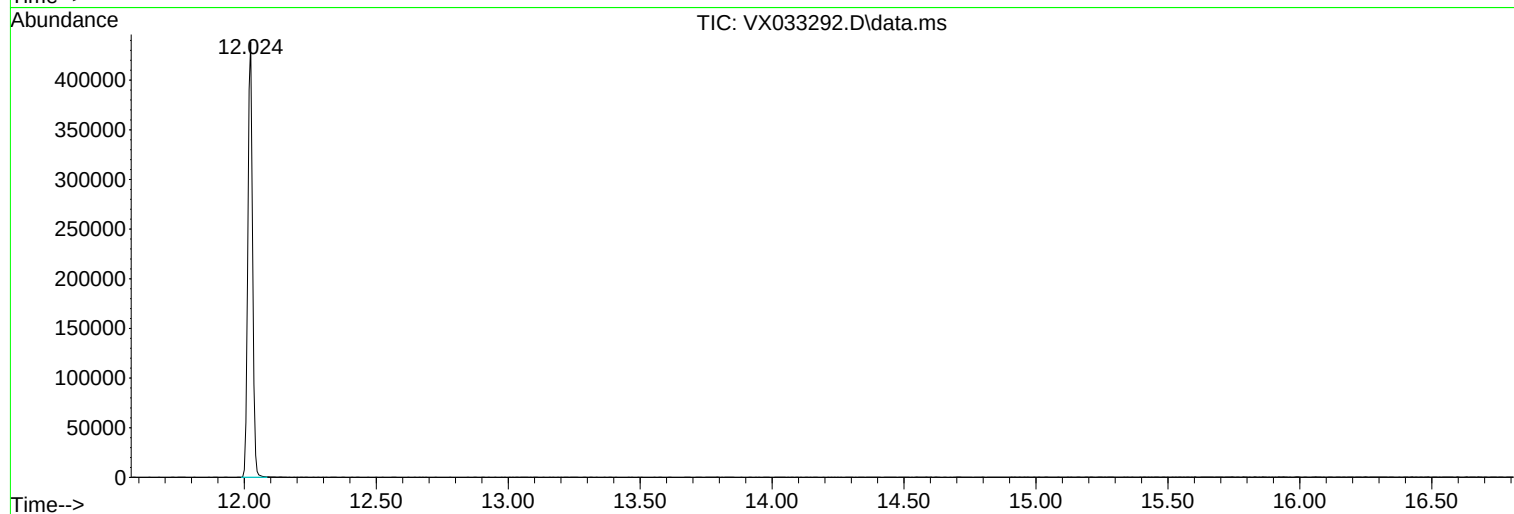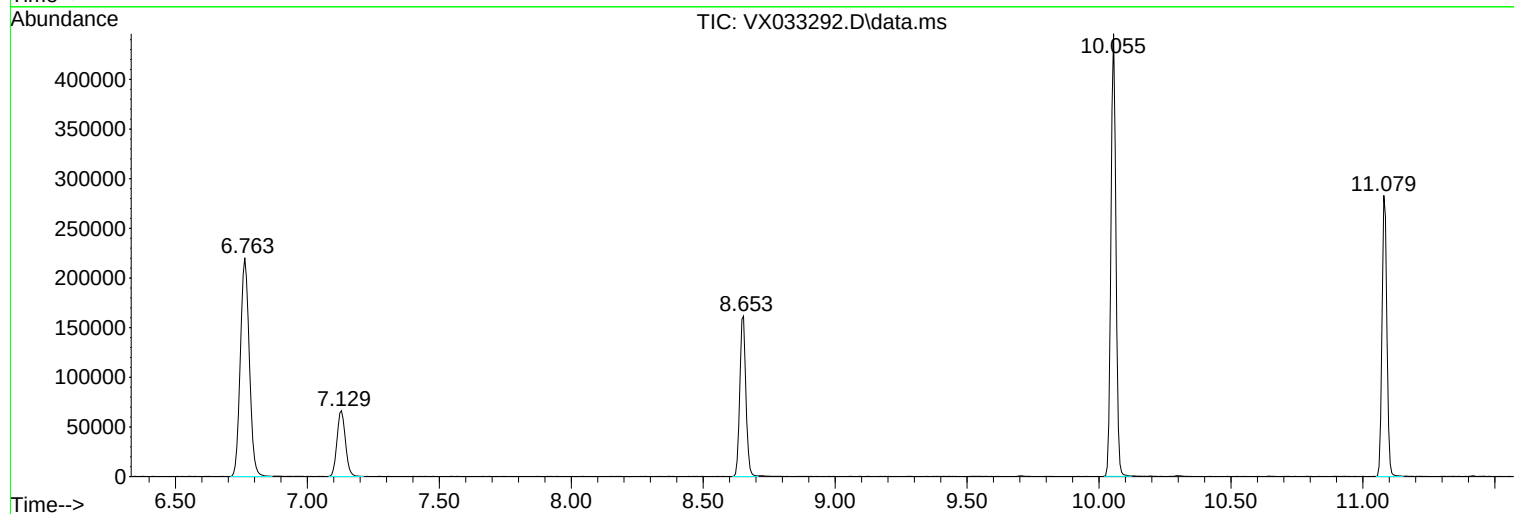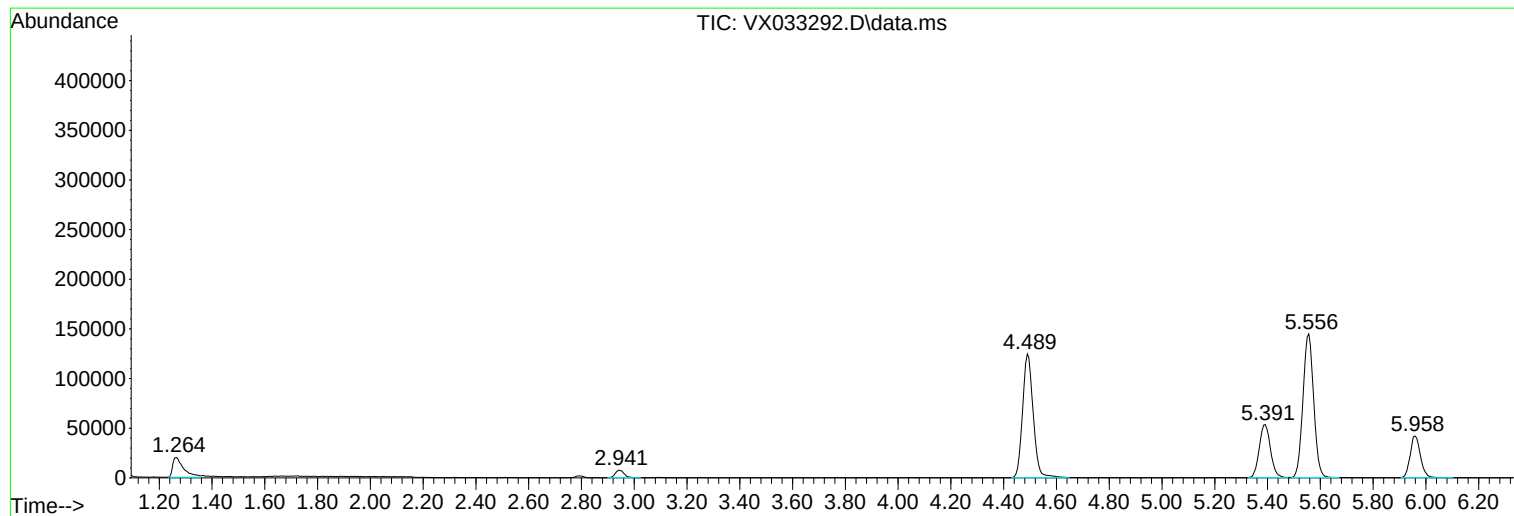

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033292.D
Acq On : 07 Dec 2022 19:32
Operator : JC/MD
Sample : N5865-09DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-5IDL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.264	6.85 ug/l	56028	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
3			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
4			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	4
5			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4

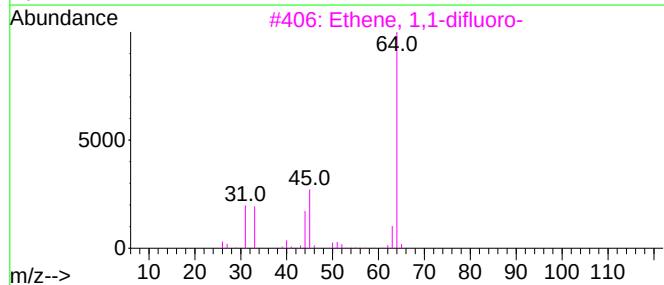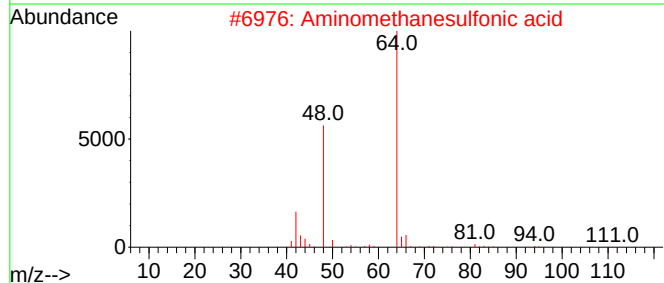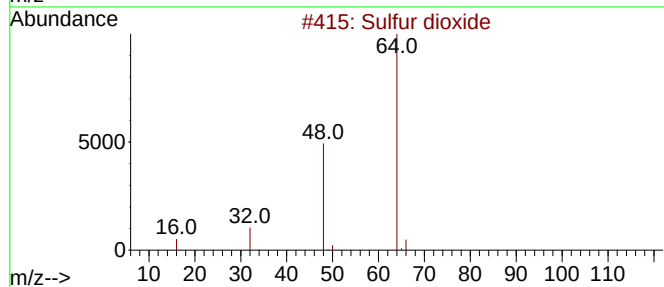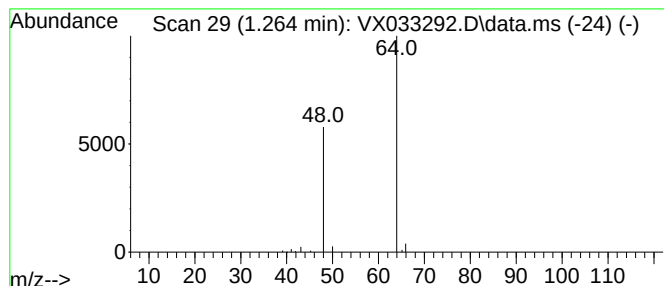

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033292.D
Acq On : 07 Dec 2022 19:32
Operator : JC/MD
Sample : N5865-09DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-5IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.264	6.8	ug/l	56028	1	5.556	408932	50.0