

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
 Data File : VX033293.D
 Acq On : 07 Dec 2022 19:55
 Operator : JC/MD
 Sample : N5865-11DL 2000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-01DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	25	31	50	rBV	11583	37663	6.63%	1.273%
2	2.947	297	305	315	rBV	3271	7532	1.33%	0.255%
3	5.391	694	706	719	rBV	55546	161304	28.40%	5.453%
4	5.556	721	733	749	rVB	138441	391116	68.85%	13.222%
5	5.958	788	799	813	rBV2	44702	119243	20.99%	4.031%
6	6.763	920	931	953	rBV	212077	497747	87.62%	16.826%
7	7.129	984	991	1007	rBV3	26300	57550	10.13%	1.945%
8	8.653	1234	1241	1250	rBV	159766	252197	44.40%	8.525%
9	10.055	1465	1471	1487	rVB	433424	568066	100.00%	19.203%
10	11.079	1634	1639	1650	rBV	276742	356456	62.75%	12.050%
11	12.024	1788	1794	1806	rBV	406691	509297	89.65%	17.217%




Sum of corrected areas: 2958171

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033293.D
Acq On : 07 Dec 2022 19:55
Operator : JC/MD
Sample : N5865-11DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

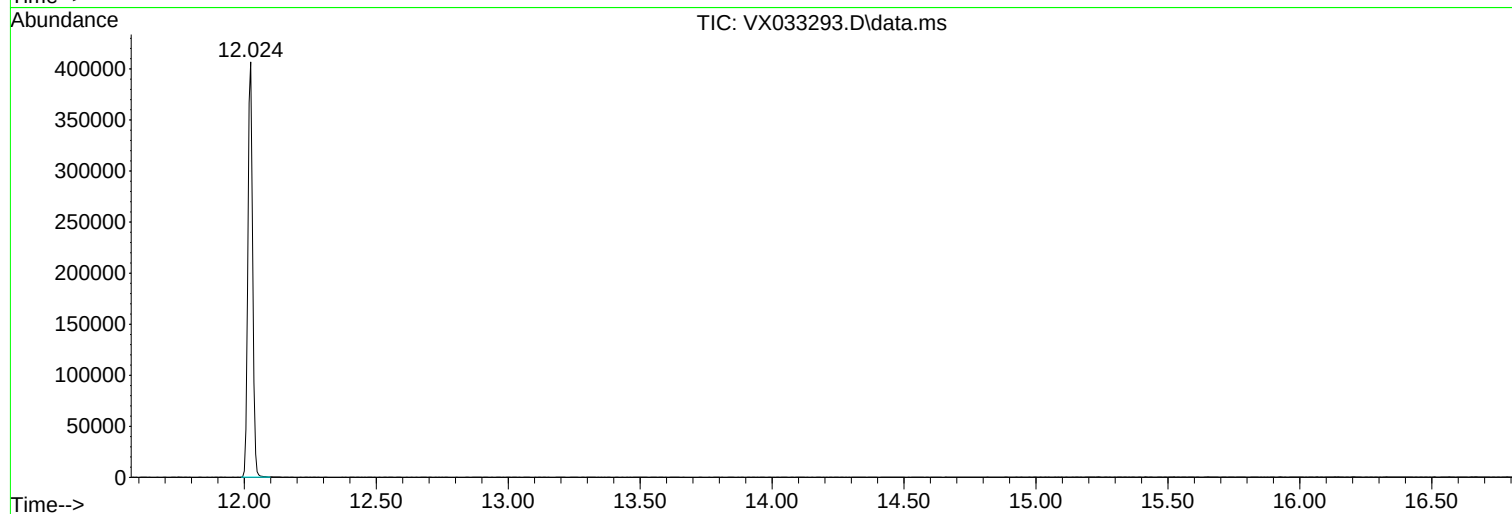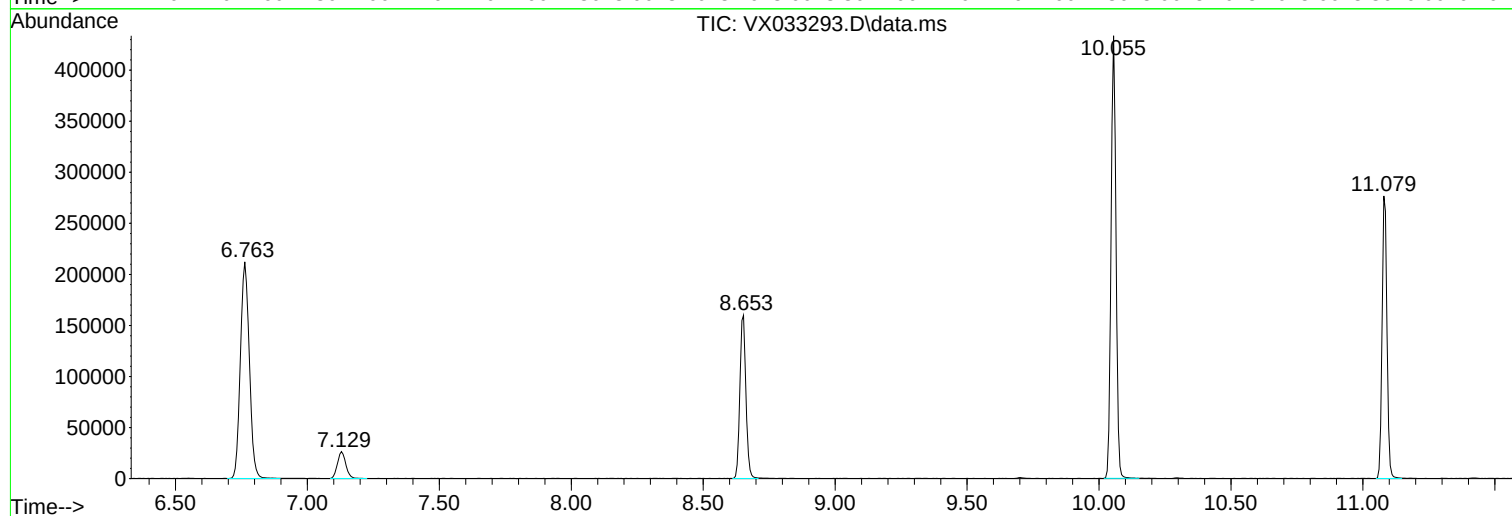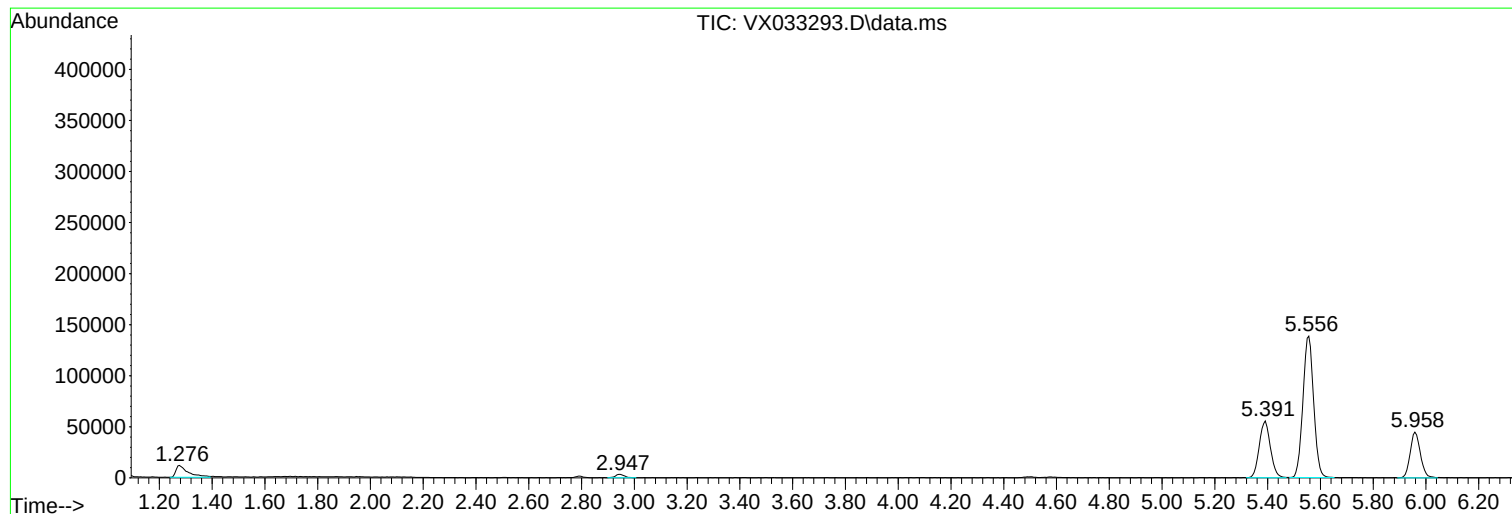

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033293.D
Acq On : 07 Dec 2022 19:55
Operator : JC/MD
Sample : N5865-11DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033293.D
Acq On : 07 Dec 2022 19:55
Operator : JC/MD
Sample : N5865-11DL 2000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------