

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
 Data File : VX033294.D
 Acq On : 07 Dec 2022 20:18
 Operator : JC/MD
 Sample : N5865-01DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LEA-7IDL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.489	547	558	580	rBV	675789	1814074	100.00%	32.204%
2	5.391	694	706	721	rBV	55692	165784	9.14%	2.943%
3	5.556	721	733	750	rVV	149210	421555	23.24%	7.484%
4	5.958	790	799	815	rBV	44131	117545	6.48%	2.087%
5	6.763	921	931	946	rBV	221645	523933	28.88%	9.301%
6	7.129	982	991	1008	rBV	364162	791156	43.61%	14.045%
7	8.647	1234	1240	1249	rBV	169153	268500	14.80%	4.767%
8	10.055	1465	1471	1486	rBV	457017	602990	33.24%	10.705%
9	11.079	1634	1639	1653	rBV	288323	377305	20.80%	6.698%
10	12.024	1788	1794	1812	rBV	445633	550180	30.33%	9.767%




Sum of corrected areas: 5633022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033294.D
Acq On : 07 Dec 2022 20:18
Operator : JC/MD
Sample : N5865-01DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-7IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

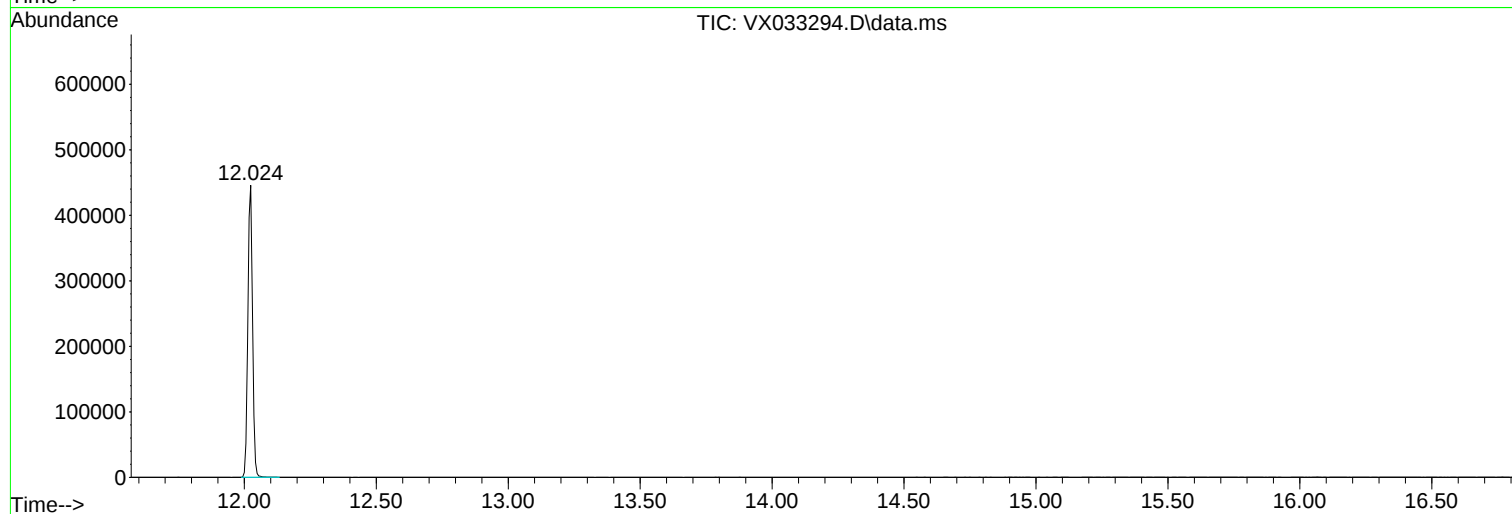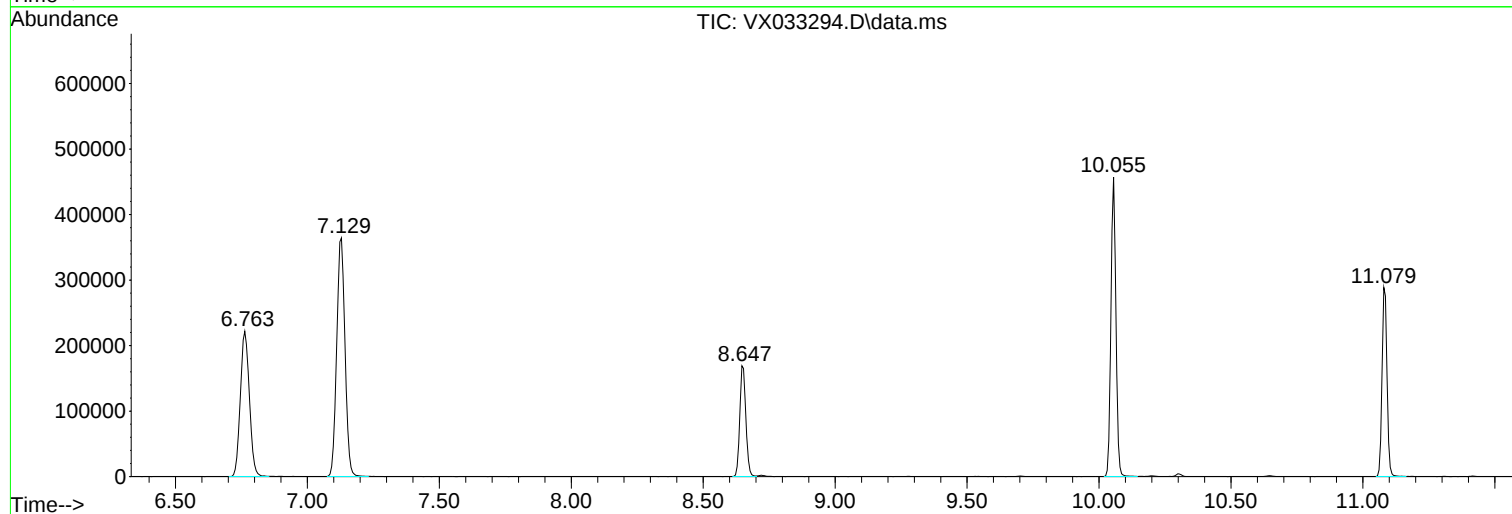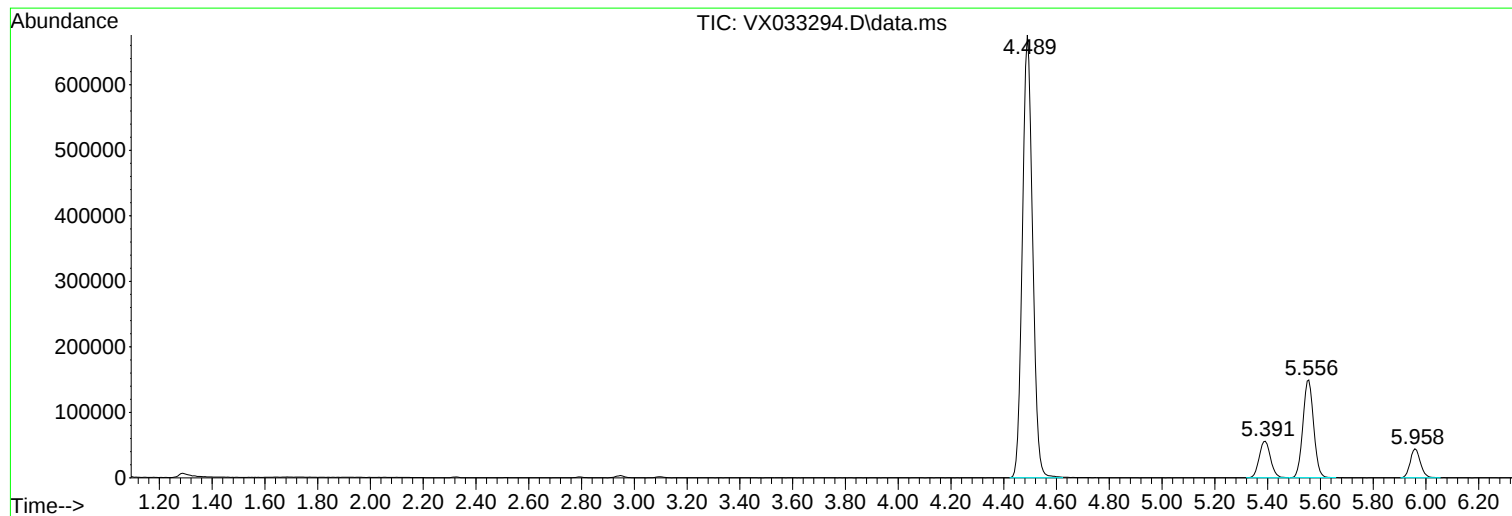

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033294.D
Acq On : 07 Dec 2022 20:18
Operator : JC/MD
Sample : N5865-01DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-7IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033294.D
Acq On : 07 Dec 2022 20:18
Operator : JC/MD
Sample : N5865-01DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-7IDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc