

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
 Data File : VX033303.D
 Acq On : 07 Dec 2022 23:47
 Operator : JC/MD
 Sample : N5906-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3RR

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.489	547	558	575	rBV	235847	642076	19.06%	8.600%
2	5.391	694	706	719	rBV	57293	167441	4.97%	2.243%
3	5.556	721	733	747	rVB	144728	415596	12.34%	5.567%
4	5.958	790	799	811	rBV	44830	119596	3.55%	1.602%
5	6.763	920	931	947	rBV	219169	520233	15.45%	6.968%
6	7.129	982	991	1006	rBV	193407	415859	12.35%	5.570%
7	8.647	1234	1240	1252	rBV	171561	274528	8.15%	3.677%
8	9.275	1336	1343	1358	rBV	2433745	3368261	100.00%	45.115%
9	10.055	1465	1471	1484	rBV	447729	596010	17.69%	7.983%
10	11.079	1634	1639	1654	rBV	304262	393614	11.69%	5.272%
11	12.024	1788	1794	1802	rBV	447075	552692	16.41%	7.403%




Sum of corrected areas: 7465906

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033303.D
Acq On : 07 Dec 2022 23:47
Operator : JC/MD
Sample : N5906-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3RR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

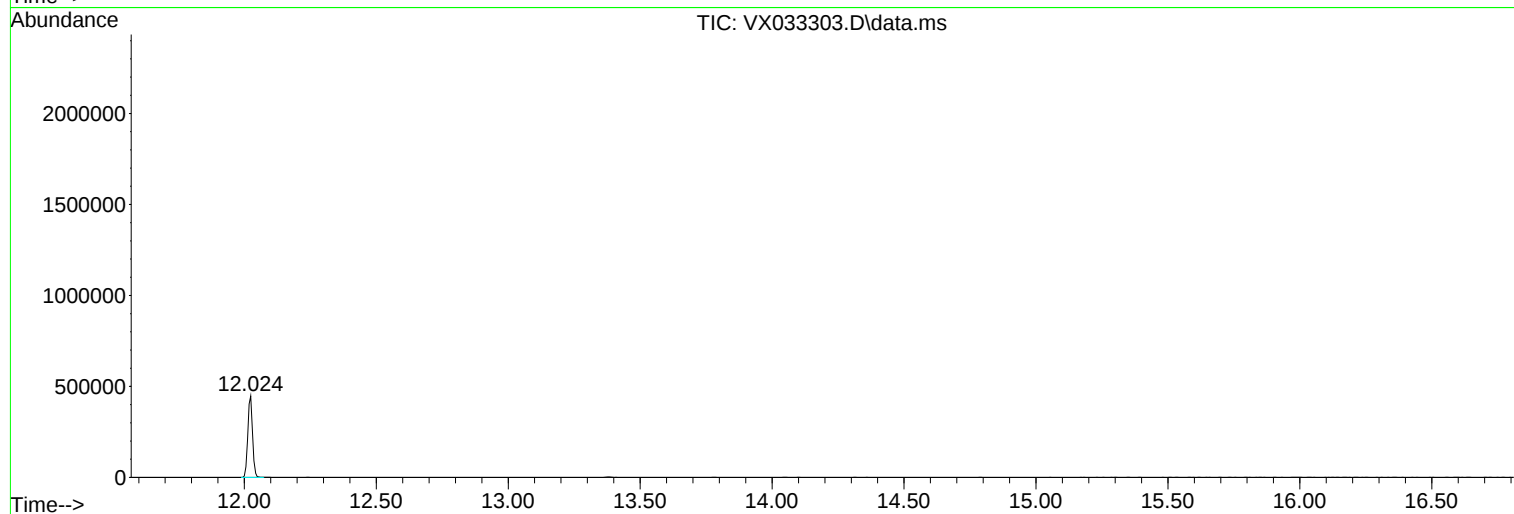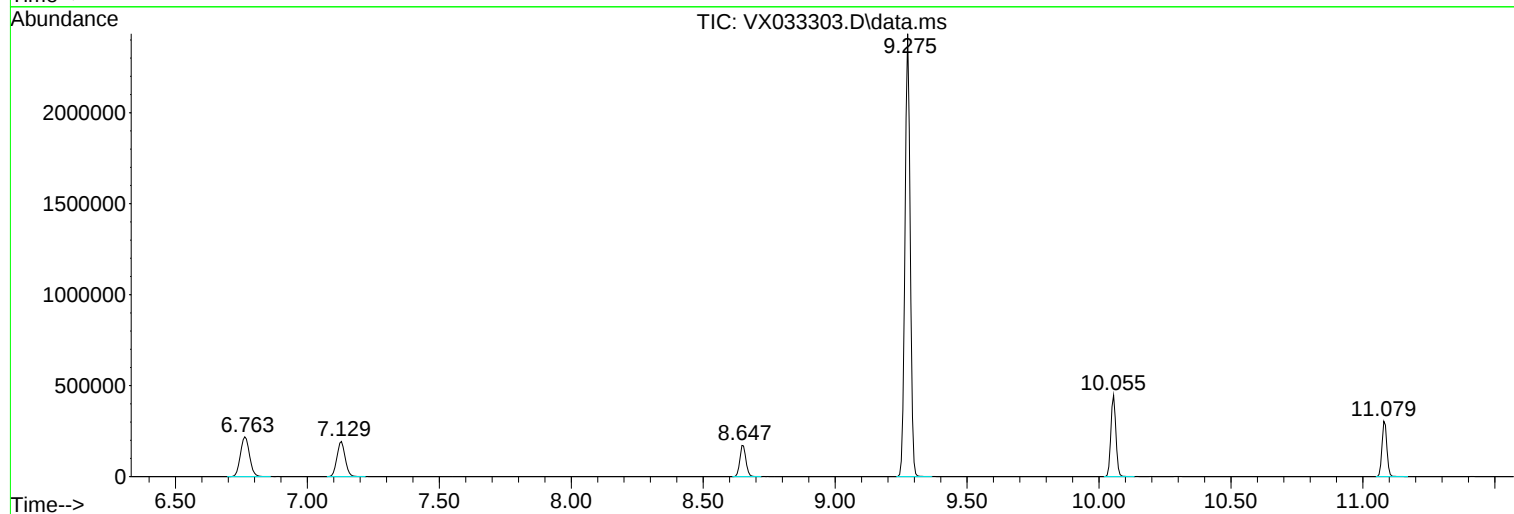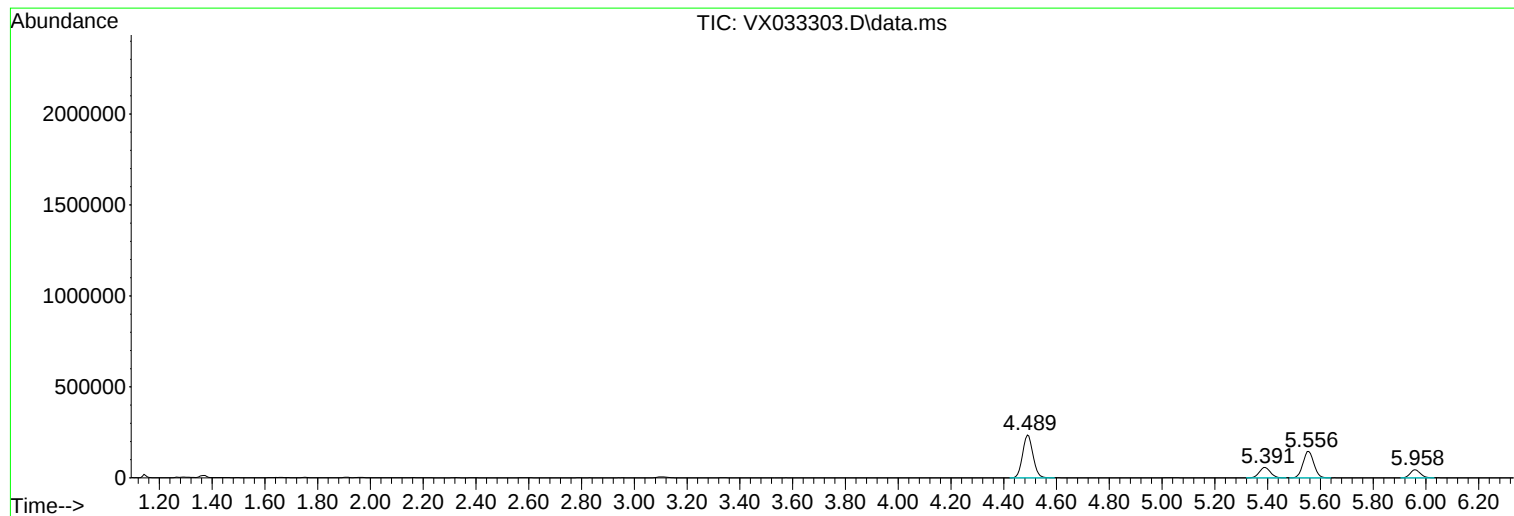

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033303.D
Acq On : 07 Dec 2022 23:47
Operator : JC/MD
Sample : N5906-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3RR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX120722\
Data File : VX033303.D
Acq On : 07 Dec 2022 23:47
Operator : JC/MD
Sample : N5906-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3RR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------