

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030623\
 Data File : VX034352.D
 Acq On : 06 Mar 2023 16:11
 Operator : JC/MD
 Sample : 01803-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-VOC

Quant Time: Mar 07 00:40:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 17 12:33:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	280975	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	474019	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	426056	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	211537	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	190309	50.292	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 100.580%			
35) Dibromofluoromethane	5.391	113	152970	49.564	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.120%			
50) Toluene-d8	8.647	98	575607	51.946	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 103.900%			
62) 4-Bromofluorobenzene	11.079	95	215007	50.727	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 101.460%			
Target Compounds						
					Qvalue	
5) Bromomethane	1.624	94	215	Below Cal	#	3
11) Tert butyl alcohol	2.953	59	7771	9.182	ug/l #	74
13) Acrolein	2.276	56	123	0.318	ug/l #	66
16) Acetone	2.380	43	40035	20.510	ug/l	100
18) Methyl Acetate	2.709	43	5033	0.833	ug/l	94
20) Methylene Chloride	2.788	84	764	0.217	ug/l	88
25) 2-Butanone	4.568	43	24046	8.514	ug/l	99
31) Cyclohexane	5.544	56	6314	1.118	ug/l #	10
36) 1,1-Dichloropropene	5.550	75	22900	5.017	ug/l #	48
37) Ethyl Acetate	4.568	43	24046	4.714	ug/l #	68
38) Carbon Tetrachloride	5.556	117	29490	6.279	ug/l #	15
43) Isopropyl Acetate	6.123	43	8883	0.987	ug/l #	61
49) 1,4-Dioxane	7.677	88	406	4.764	ug/l #	54
52) Toluene	8.720	92	4124	0.503	ug/l	92
67) Ethyl Benzene	10.195	91	5890	0.369	ug/l	99
68) m/p-Xylenes	10.299	106	7888	1.292	ug/l	96
69) o-Xylene	10.640	106	4148	0.682	ug/l	97
74) N-amyl acetate	10.860	43	5682	0.702	ug/l #	25
75) 1,1,2,2-Tetrachloroethane	11.195	83	3583	0.650	ug/l	84
76) 1,2,3-Trichloropropane	11.079	75	110722	20.801	ug/l #	34
78) n-propylbenzene	11.305	91	9905	0.528	ug/l	96
80) 1,3,5-Trimethylbenzene	11.451	105	10195	0.752	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.079	75	110722	53.436	ug/l #	9
83) tert-Butylbenzene	11.969	119	4708	0.339	ug/l	82
84) 1,2,4-Trimethylbenzene	11.750	105	43574	3.179	ug/l	97
85) sec-Butylbenzene	11.890	105	3996	0.237	ug/l #	70
86) p-Isopropyltoluene	12.012	119	2855	0.205	ug/l #	70
89) n-Butylbenzene	12.329	91	12087	0.973	ug/l #	57
90) Hexachloroethane	12.530	117	1163	0.399	ug/l #	17
95) Naphthalene	13.780	128	16718	1.086	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030623\
Data File : VX034352.D
Acq On : 06 Mar 2023 16:11
Operator : JC/MD
Sample : 01803-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Quant Time: Mar 07 00:40:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 17 12:33:35 2023
Response via : Initial Calibration

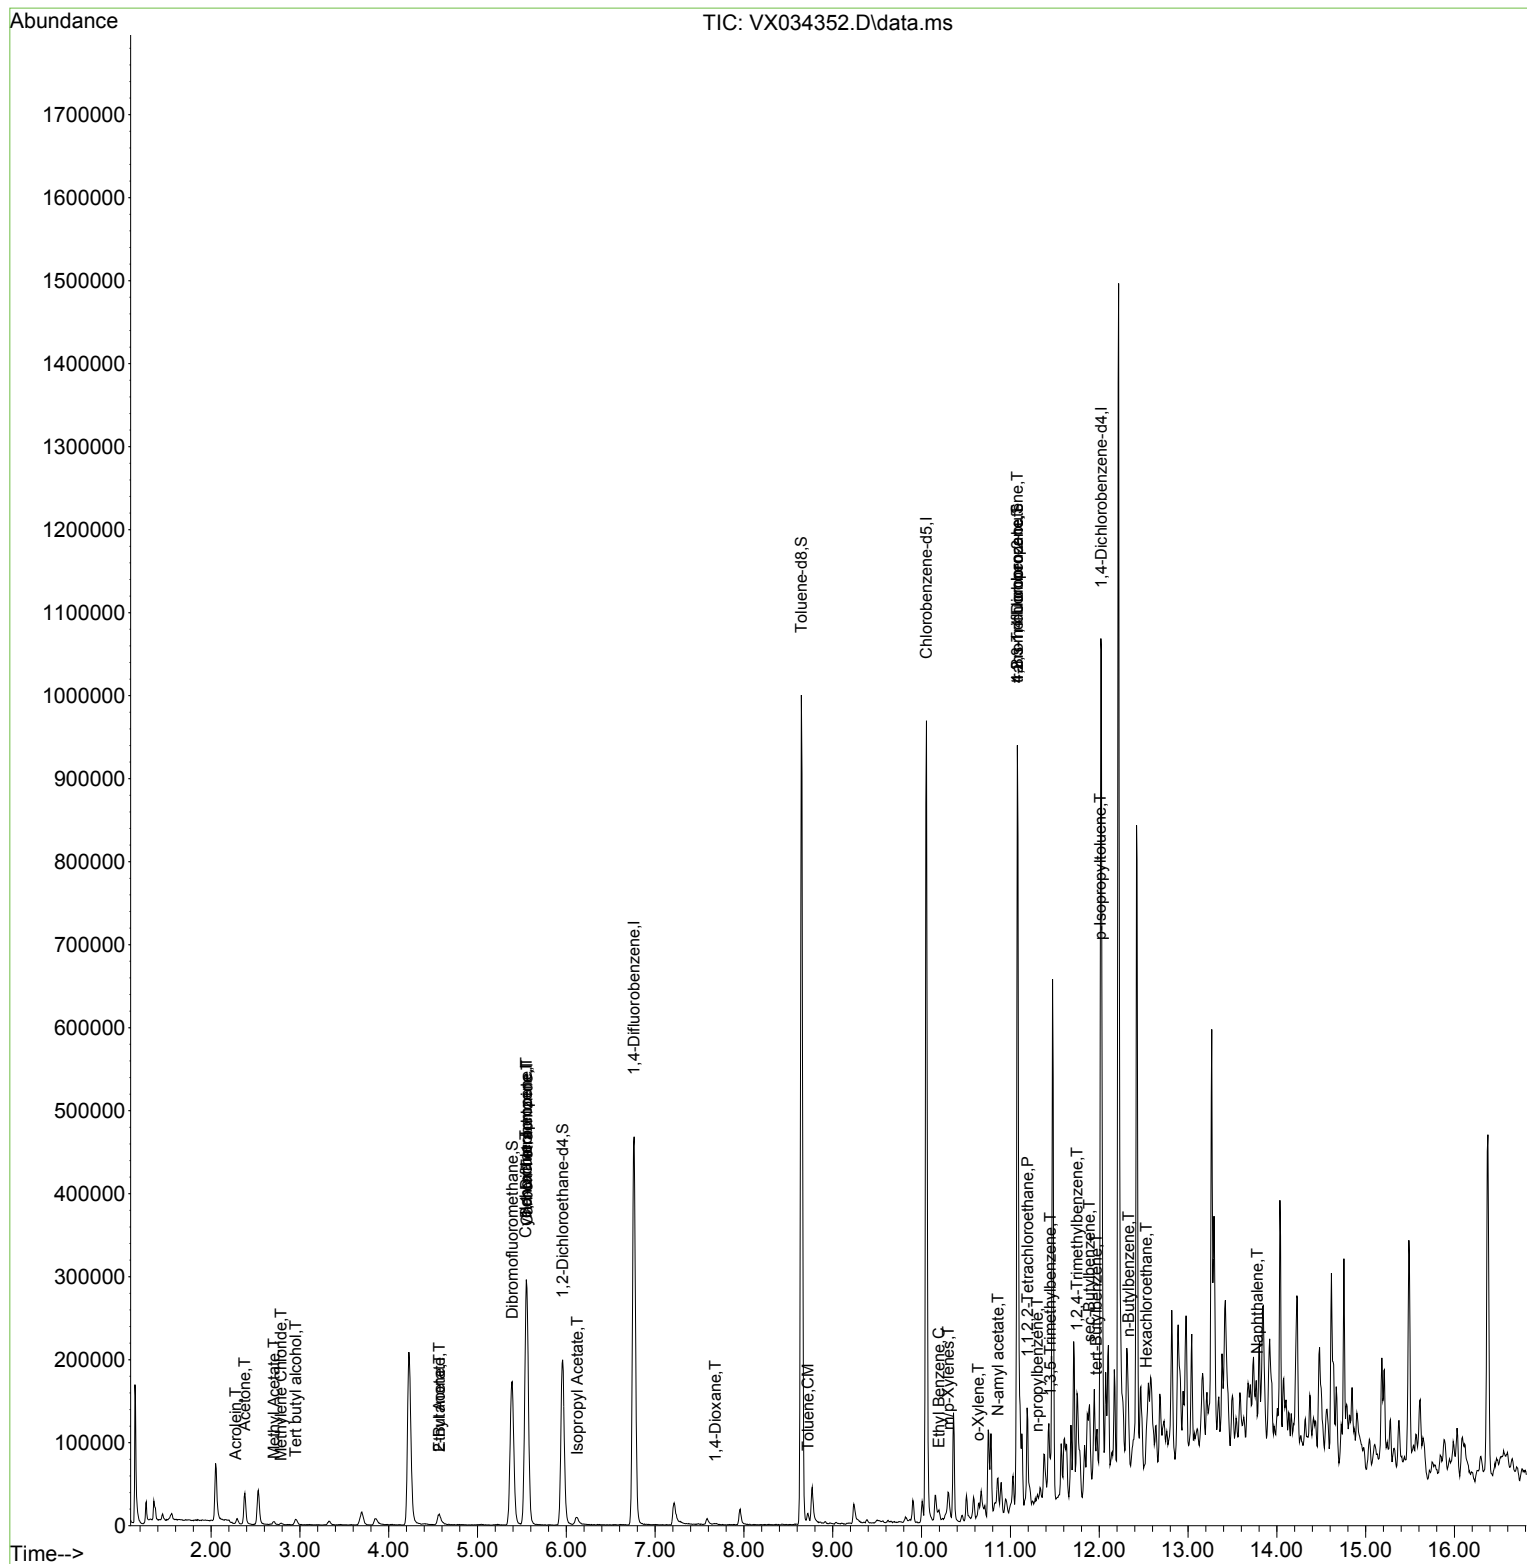






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC







Tgt Ion:168 Resp: 280975
Ion Ratio Lower Upper
168 100
99 59.6 39.6 59.4#

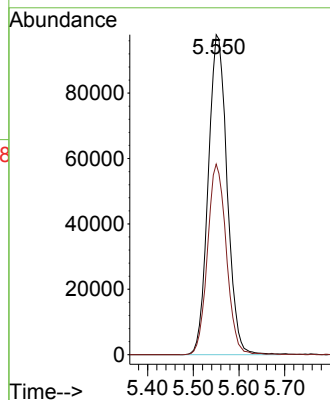

#5
Bromomethane
Concen: Below Cal
RT: 1.624 min Scan# 88
Delta R.T. 0.025 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 94 Resp: 215
Ion Ratio Lower Upper
94 100
96 0.0 74.3 111.5#

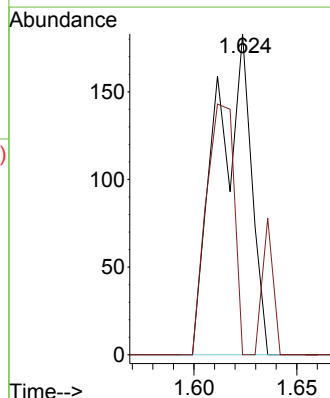

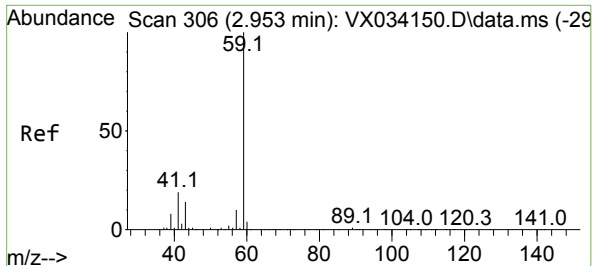

#11

Tert butyl alcohol

Concen: 9.182 ug/l

RT: 2.953 min Scan# 306

Delta R.T. 0.000 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





COMP-VOC

Tgt Ion: 59 Resp: 7771

Ion Ratio Lower Upper

59 100

57 13.1 3.7 5.5#

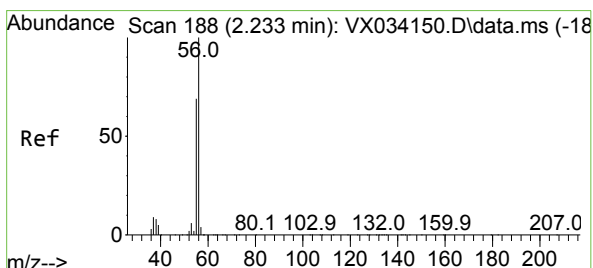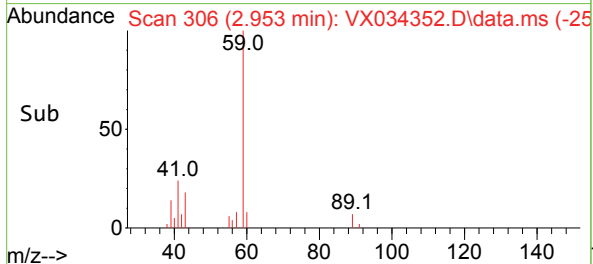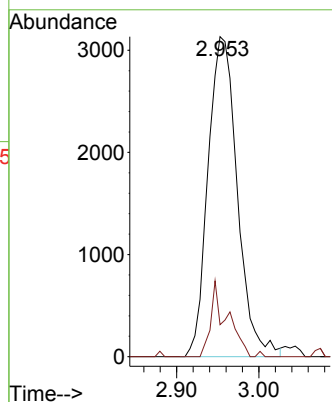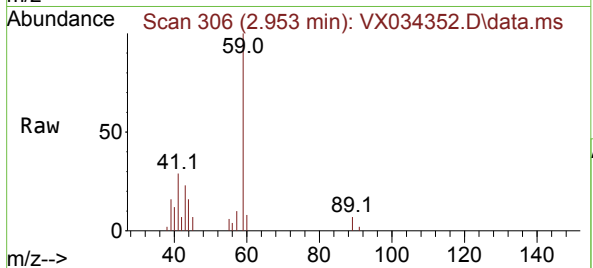

#13

Acrolein

Concen: 0.318 ug/l

RT: 2.276 min Scan# 195

Delta R.T. 0.043 min

Lab File: VX034352.D




Acq: 06 Mar 2023 16:11


Tgt Ion: 56 Resp: 123

Ion Ratio Lower Upper

56 100

55 98.4 56.3 84.5#


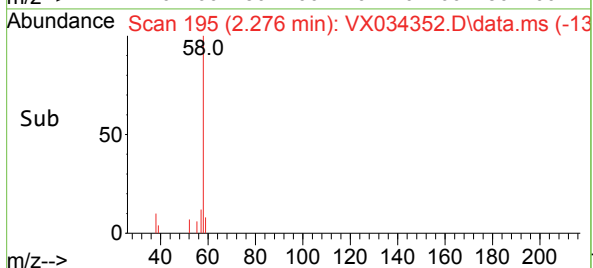

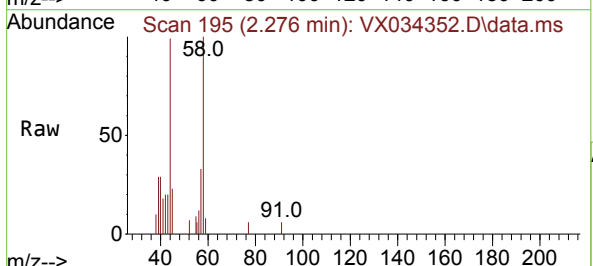




#16
Acetone
Concen: 20.510 ug/l
RT: 2.380 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion: 43 Resp: 40035
Ion Ratio Lower Upper
43 100
58 28.0 22.6 33.8



#18
Methyl Acetate
Concen: 0.833 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.012 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11


Tgt Ion: 43 Resp: 5033
Ion Ratio Lower Upper
43 100
74 19.8 18.2 27.4








#20
Methylene Chloride
Concen: 0.217 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC







Tgt Ion:	84	Resp:	764
Ion	Ratio	Lower	Upper
84	100		
49	146.8	101.1	151.7
51	39.0	31.0	46.6
86	58.4	52.6	79.0

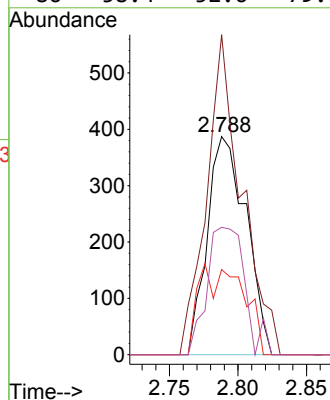

#25
2-Butanone
Concen: 8.514 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.025 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion:	43	Resp:	24046
Ion	Ratio	Lower	Upper
43	100		
72	23.6	19.4	29.2



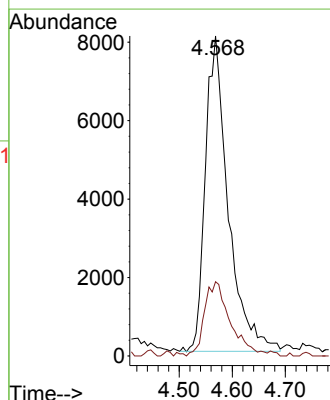





#31
Cyclohexane
Concen: 1.118 ug/l
RT: 5.544 min Scan# 719
Delta R.T. 0.073 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion: 56 Resp: 6314
Ion Ratio Lower Upper
56 100
69 179.4 24.6 37.0#
84 114.8 71.0 106.6#



#33
1,2-Dichloroethane-d4
Concen: 50.292 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 65 Resp: 190309
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.8

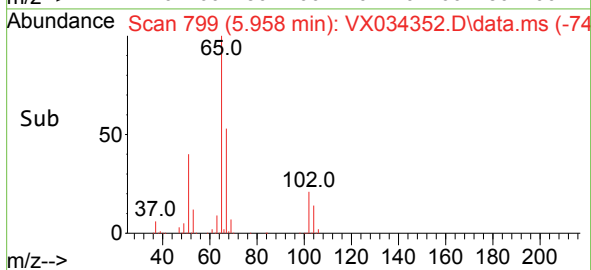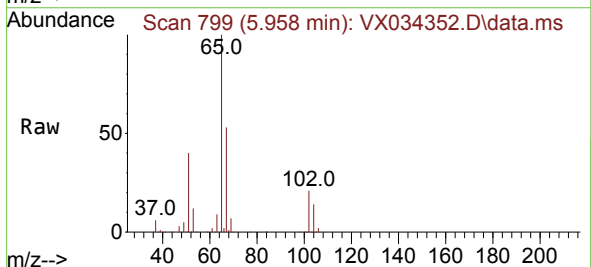



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. 0.006 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :

COMP-VOC





Tgt Ion:114 Resp: 474019

Ion Ratio Lower Upper

114 100

63 20.9 0.0 37.4

88 16.5 0.0 30.6

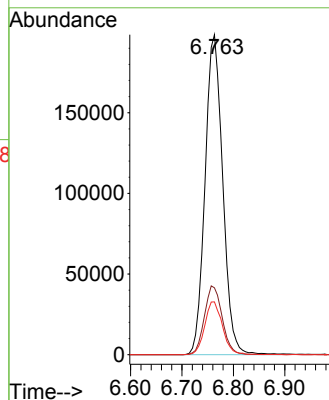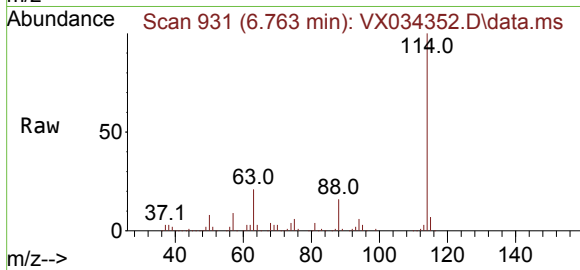

#35

Dibromofluoromethane

Concen: 49.564 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.006 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11




Tgt Ion:113 Resp: 152970


Ion Ratio Lower Upper

113 100

111 101.9 83.0 124.6

192 19.5 19.0 28.4


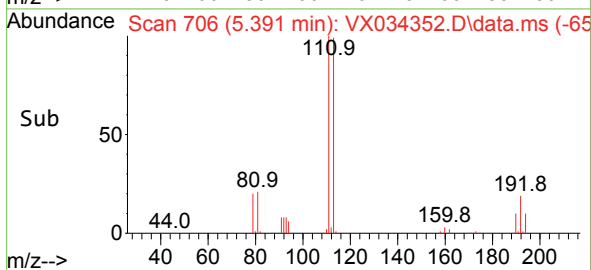
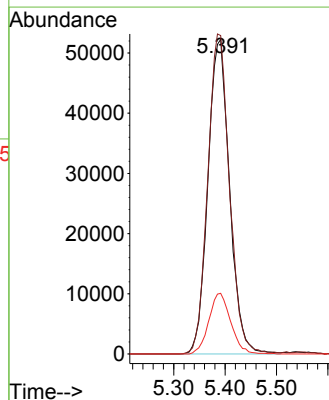
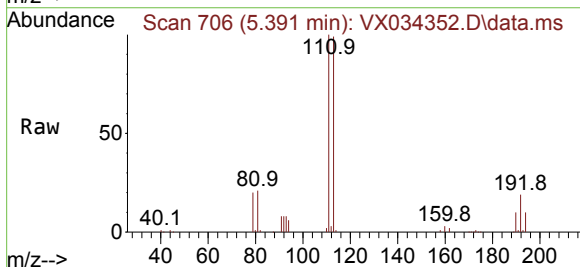




#36
1,1-Dichloropropene
Concen: 5.017 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion: 75 Resp: 22900
Ion Ratio Lower Upper
75 100
110 9.2 18.8 56.4#
77 0.1 25.1 37.7#



#37
Ethyl Acetate
Concen: 4.714 ug/l
RT: 4.568 min Scan# 571
Delta R.T. -0.140 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 43 Resp: 24046
Ion Ratio Lower Upper
43 100
61 0.0 11.1 16.7#
70 0.0 8.5 12.7#


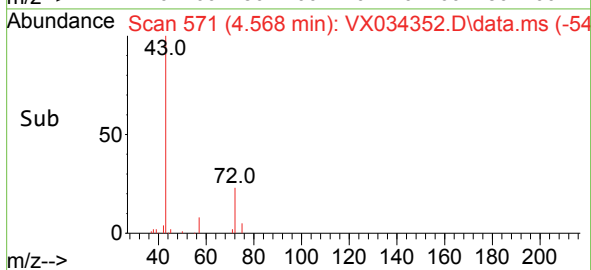






#38
Carbon Tetrachloride
Concen: 6.279 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.116 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion:117 Resp: 29490
Ion Ratio Lower Upper
117 100
119 5.2 78.0 117.0#
121 0.0 24.4 36.6#



#43
Isopropyl Acetate
Concen: 0.987 ug/l
RT: 6.123 min Scan# 826
Delta R.T. -0.213 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 43 Resp: 8883
Ion Ratio Lower Upper
43 100
61 0.0 15.7 23.5#
87 0.0 10.6 15.8#


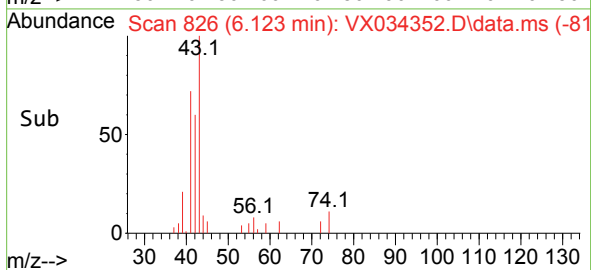

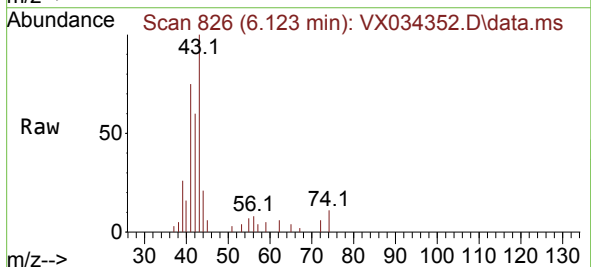




#49
1,4-Dioxane
Concen: 4.764 ug/l
RT: 7.677 min Scan# 1081
Delta R.T. 0.025 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion: 88 Resp: 406
Ion Ratio Lower Upper
88 100
43 0.0 0.0 0.0
58 108.6 56.5 84.7#

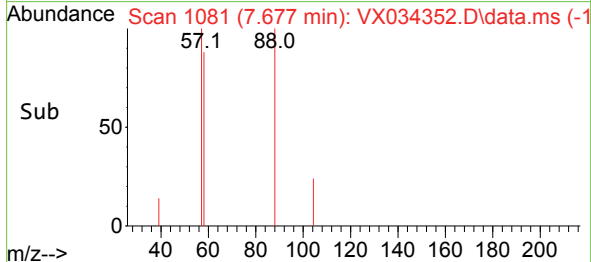

#50
Toluene-d8
Concen: 51.946 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 98 Resp: 575607
Ion Ratio Lower Upper
98 100
100 65.8 53.6 80.4

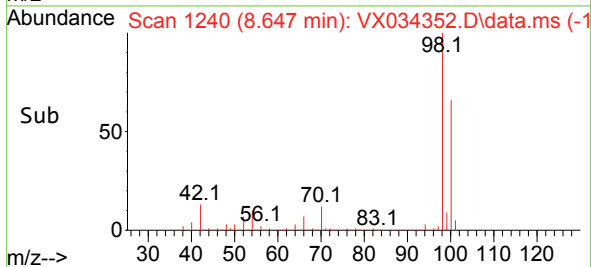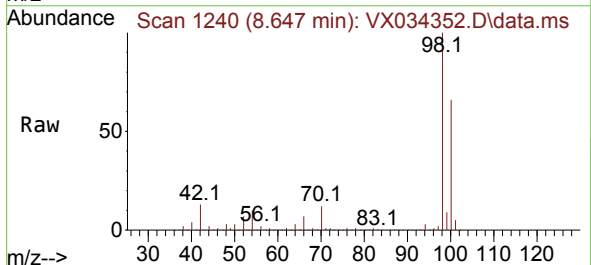



#52

Toluene

Concen: 0.503 ug/l

RT: 8.720 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





COMP-VOC

Tgt Ion: 92 Resp: 4124

Ion Ratio Lower Upper

92 100

91 181.0 135.5 203.3

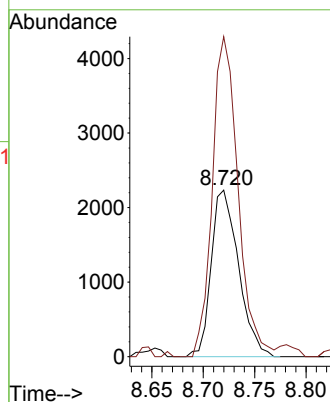

#62

4-Bromofluorobenzene

Concen: 50.727 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11




Tgt Ion: 95 Resp: 215007


Ion Ratio Lower Upper

95 100

174 76.0 0.0 184.4

176 72.4 0.0 178.8

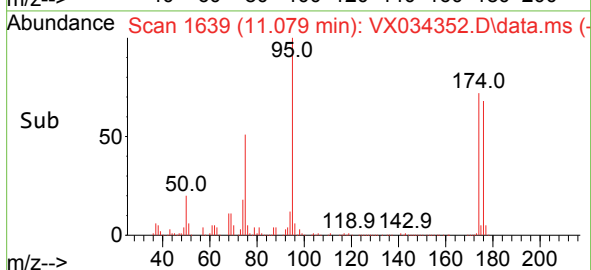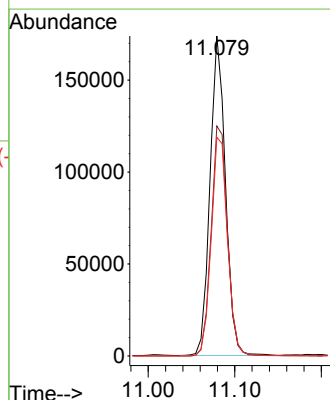



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :

COMP-VOC





Tgt Ion:117 Resp: 426056

Ion Ratio Lower Upper

117 100

82 55.9 40.6 60.8

119 32.2 25.6 38.4

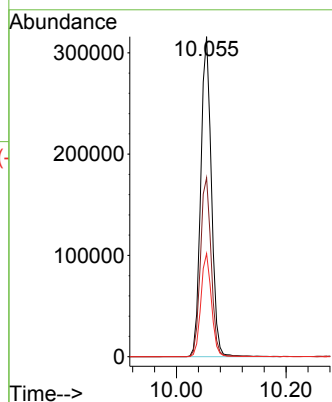

#67

Ethyl Benzene

Concen: 0.369 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX034352.D




Acq: 06 Mar 2023 16:11


Tgt Ion: 91 Resp: 5890

Ion Ratio Lower Upper

91 100

106 33.0 25.8 38.8


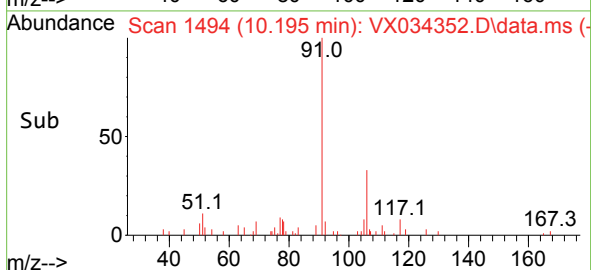




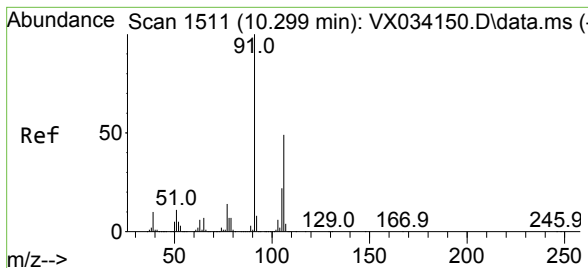

#68
m/p-Xylenes
Concen: 1.292 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion:106 Resp: 7888
Ion Ratio Lower Upper
106 100
91 202.0 156.4 234.6

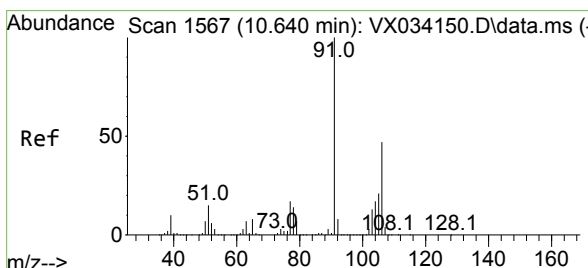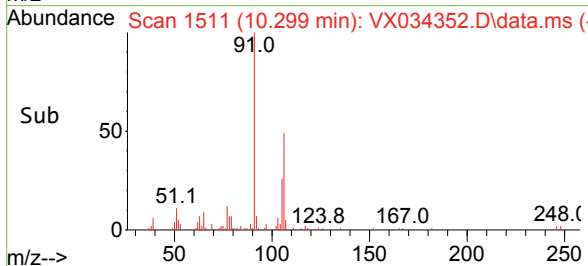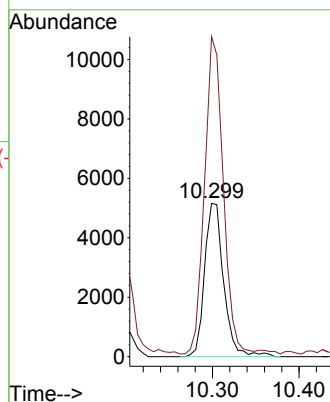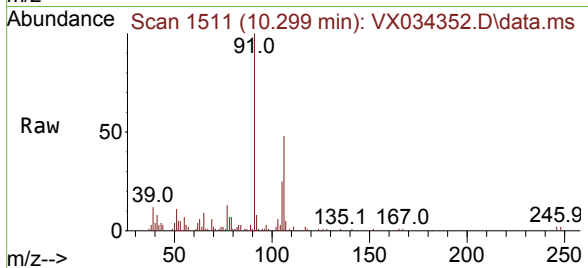

#69
o-Xylene
Concen: 0.682 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion:106 Resp: 4148
Ion Ratio Lower Upper
106 100
91 210.5 103.1 309.3


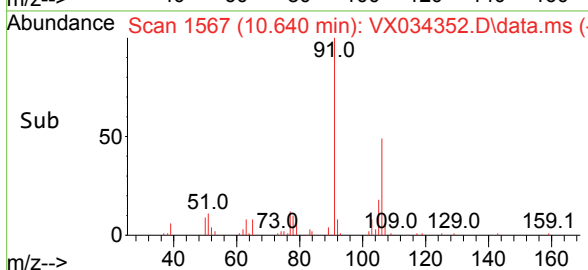
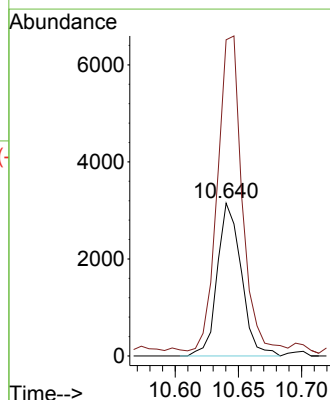
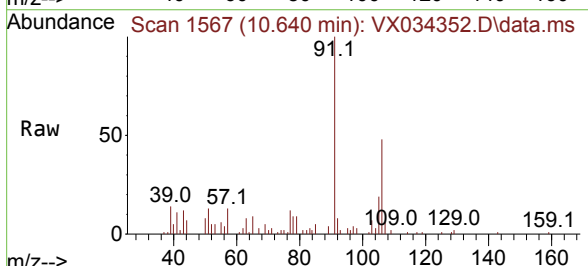




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion:152 Resp: 211537
Ion Ratio Lower Upper
152 100
115 60.4 38.7 116.1
150 157.1 0.0 348.2

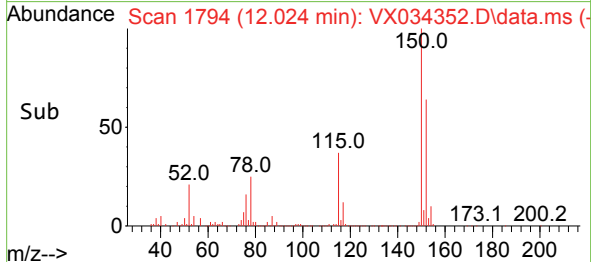

#74
N-ethyl acetate
Concen: 0.702 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.018 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 43 Resp: 5682
Ion Ratio Lower Upper
43 100
70 17.8 34.8 52.2#
55 106.0 19.4 29.0#
61 0.0 19.4 29.2#


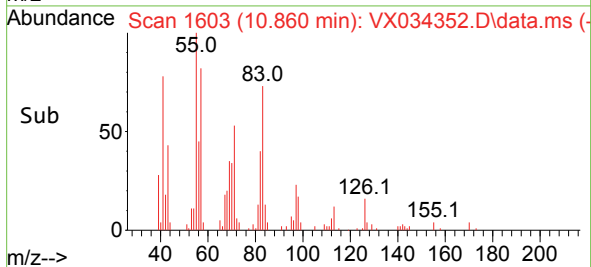

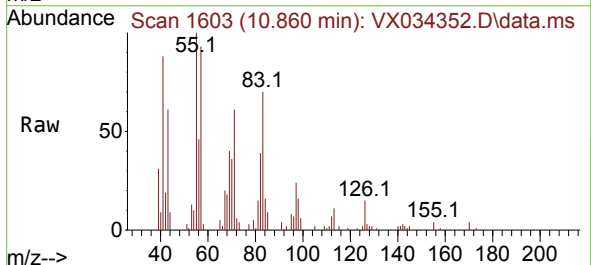


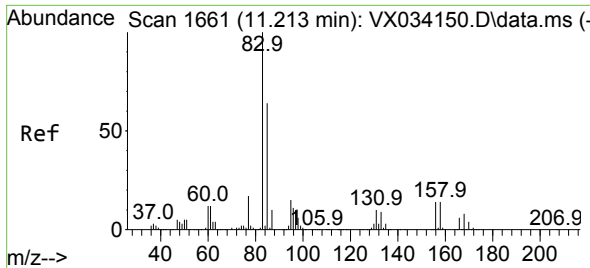

#75
1,1,2,2-Tetrachloroethane
Concen: 0.650 ug/l
RT: 11.195 min Scan# 1658
Delta R.T. -0.018 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion: 83 Resp: 3583
Ion Ratio Lower Upper
83 100
131 11.5 5.5 16.7
85 49.9 32.3 96.9

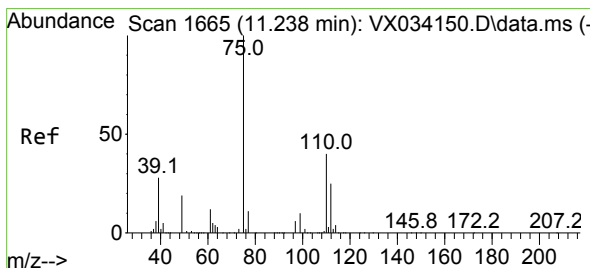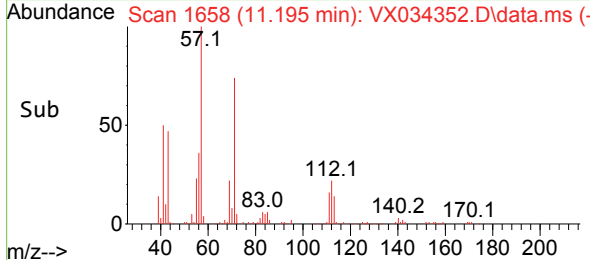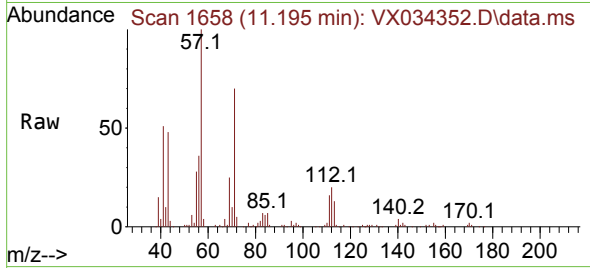

#76
1,2,3-Trichloropropane
Concen: 20.801 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 75 Resp: 110722
Ion Ratio Lower Upper
75 100
77 1.4 21.8 65.4#

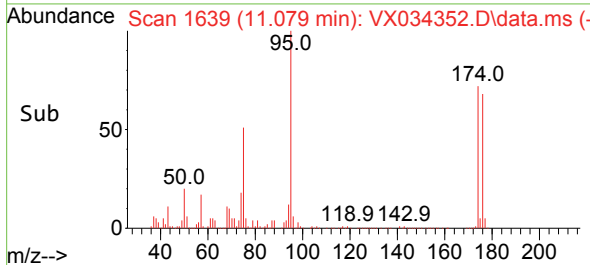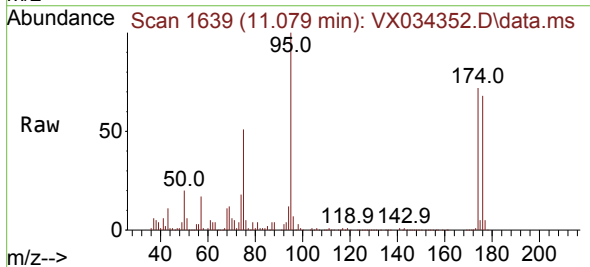

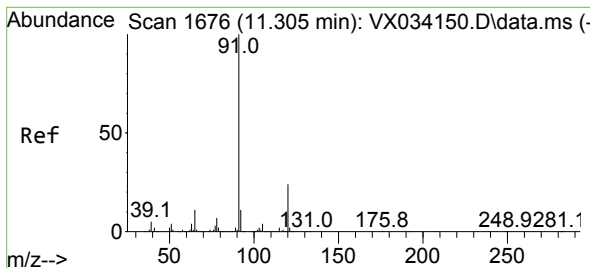

#78

n-propylbenzene

Concen: 0.528 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





COMP-VOC

Tgt Ion: 91 Resp: 9905

Ion Ratio Lower Upper

91 100

120 22.3 12.3 36.8

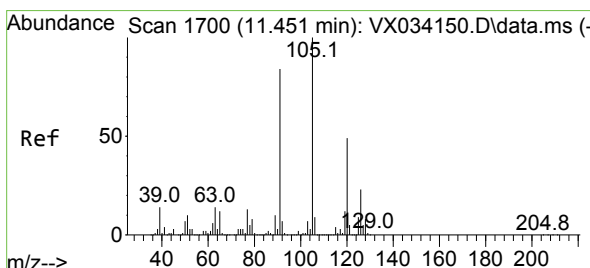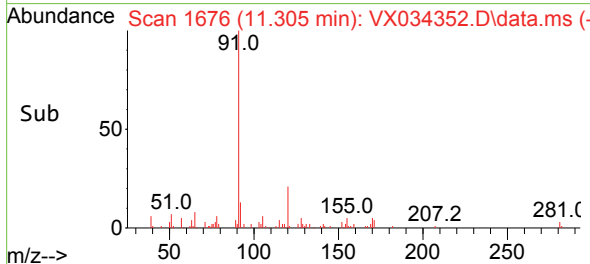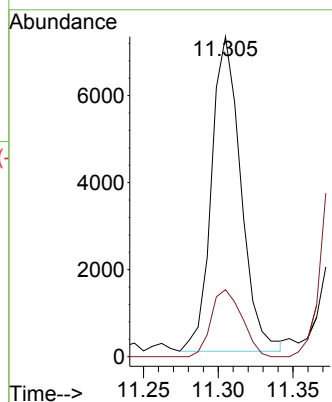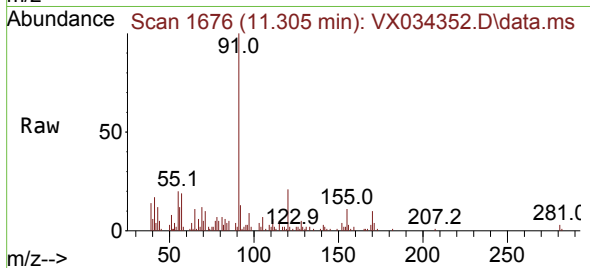

#80

1,3,5-Trimethylbenzene

Concen: 0.752 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX034352.D




Acq: 06 Mar 2023 16:11


Tgt Ion: 105 Resp: 10195

Ion Ratio Lower Upper

105 100

120 47.8 25.6 76.8


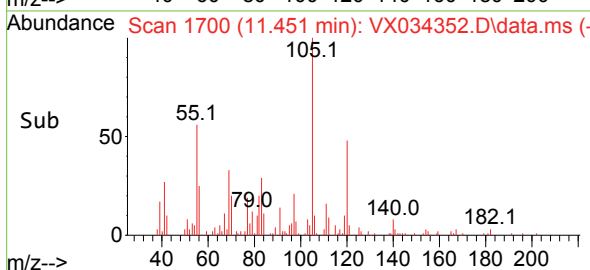

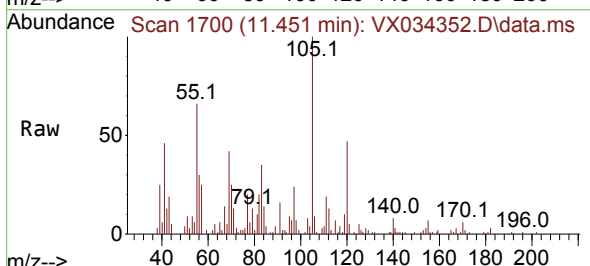


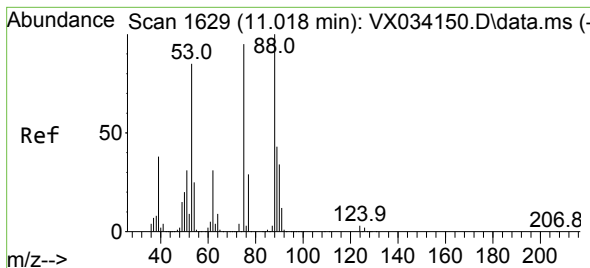

#81
 trans-1,4-Dichloro-2-butene
 Concen: 53.436 ug/l
 RT: 11.079 min Scan# 110722
 Delta R.T. 0.061 min
 Lab File: VX034352.D
 Acq: 06 Mar 2023 16:11




Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-VOC


Tgt Ion: 75 Resp: 110722
 Ion Ratio Lower Upper
 75 100
 53 1.2 83.0 124.6#
 89 0.0 37.7 56.5#

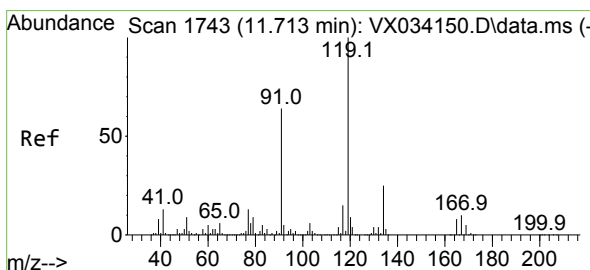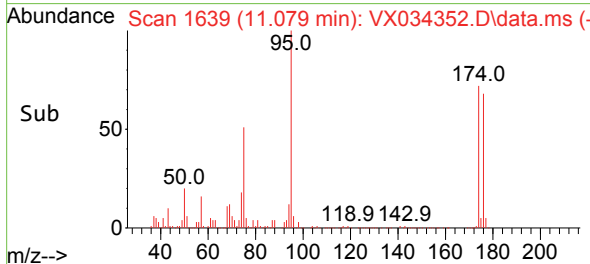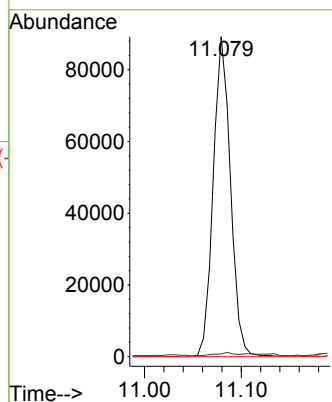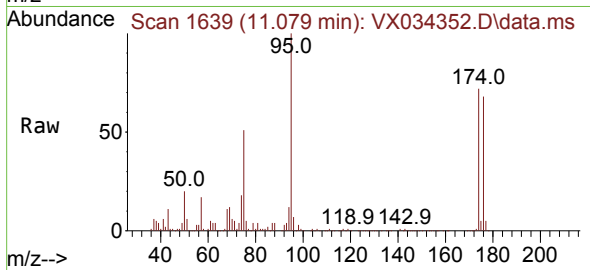

#83
 tert-Butylbenzene
 Concen: 0.339 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. 0.256 min
 Lab File: VX034352.D
 Acq: 06 Mar 2023 16:11

Tgt Ion: 119 Resp: 4708
 Ion Ratio Lower Upper
 119 100
 91 41.3 26.9 80.7
 134 34.0 12.3 36.8

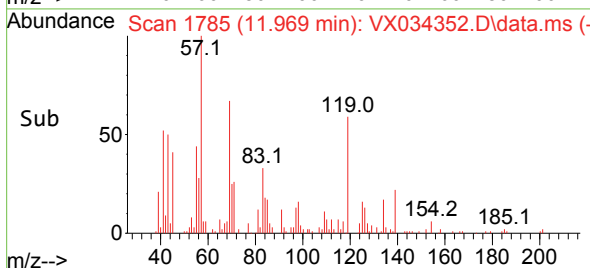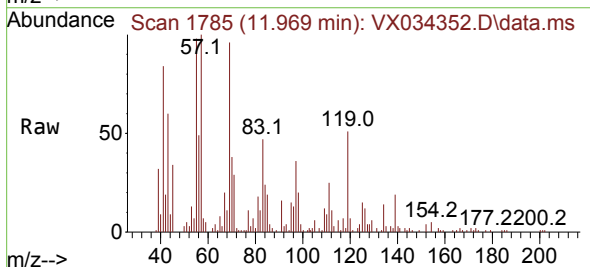



#84

1,2,4-Trimethylbenzene

Concen: 3.179 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX034352.D

Acq: 06 Mar 2023 16:11

Instrument :

MSVOA_X

ClientSampleId :





COMP-VOC

Tgt Ion:105 Resp: 43574

Ion Ratio Lower Upper

105 100

120 44.5 23.4 70.2

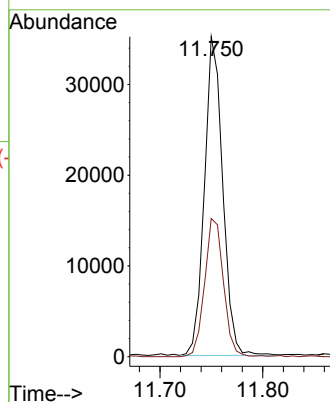

#85

sec-Butylbenzene

Concen: 0.237 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX034352.D




Acq: 06 Mar 2023 16:11


Tgt Ion:105 Resp: 3996

Ion Ratio Lower Upper

105 100

134 35.6 10.8 32.3#


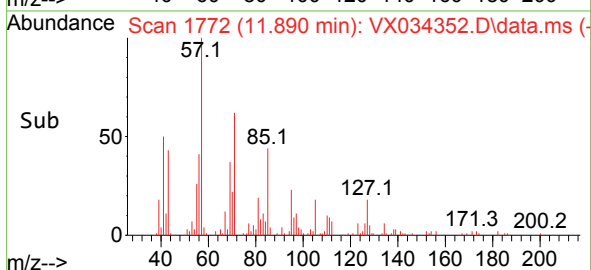
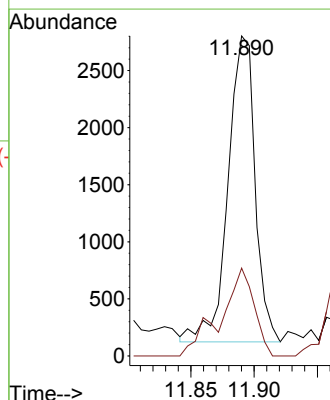





#86
p-Isopropyltoluene
Concen: 0.205 ug/l
RT: 12.012 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11




Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC


Tgt Ion:119 Resp: 2855
Ion Ratio Lower Upper
119 100
134 38.4 13.6 40.8
91 40.8 11.0 33.0#

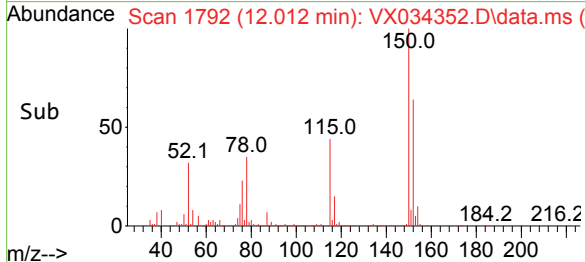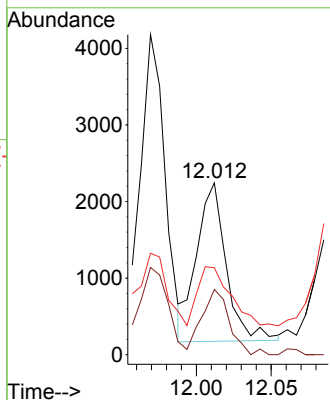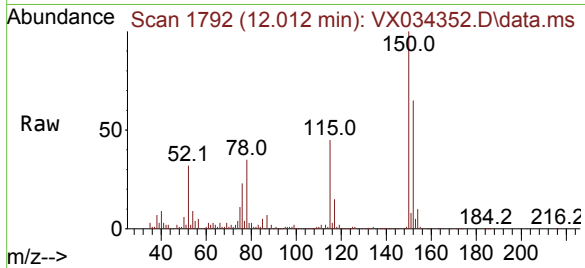

#89
n-Butylbenzene
Concen: 0.973 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion: 91 Resp: 12087
Ion Ratio Lower Upper
91 100
92 40.0 27.5 82.5
134 73.5 14.3 42.9#


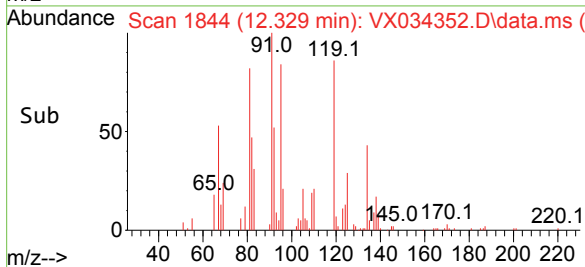
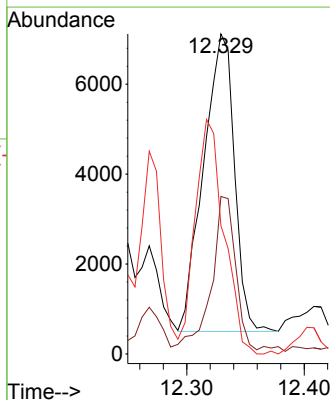
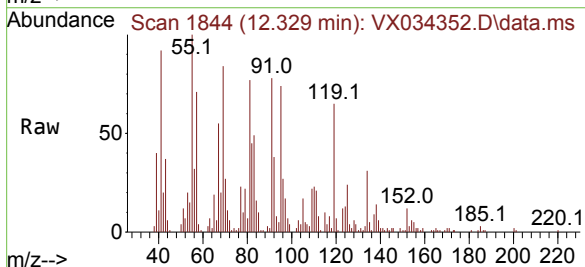




#90
Hexachloroethane
Concen: 0.399 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.006 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Instrument :
MSVOA_X
ClientSampleId :
COMP-VOC

Tgt Ion:117 Resp: 1163
Ion Ratio Lower Upper
117 100
201 11.4 45.1 135.3#

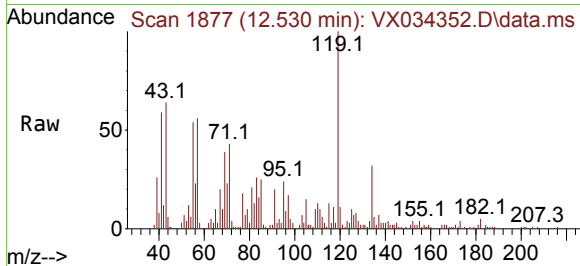

#95
Naphthalene
Concen: 1.086 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX034352.D
Acq: 06 Mar 2023 16:11

Tgt Ion:128 Resp: 16718
Ion Ratio Lower Upper
128 100
127 16.6 10.3 15.5#
129 16.3 8.7 13.1#

