

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030623\
 Data File : VX034355.D
 Acq On : 06 Mar 2023 17:22
 Operator : JC/MD
 Sample : 01816-05RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31957

Quant Time: Mar 07 00:41:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 17 12:33:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	268630	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	447415	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	395707	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	175093	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	168113	46.468	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.940%
35) Dibromofluoromethane	5.385	113	142245	48.829	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.660%
50) Toluene-d8	8.647	98	540972	51.723	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	103.440%
62) 4-Bromofluorobenzene	11.079	95	186348	46.580	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.160%


Target Compounds				Qvalue		
5) Bromomethane	1.618	94	162	Below Cal	#	3
11) Tert butyl alcohol	2.953	59	34729	42.919	ug/l #	85
13) Acrolein	2.185	56	219	0.593	ug/l #	14
16) Acetone	2.380	43	128767	68.998	ug/l	92
18) Methyl Acetate	2.703	43	8774	1.519	ug/l	100
20) Methylene Chloride	2.788	84	961	0.286	ug/l #	73
22) Diisopropyl ether	3.703	45	3303	0.306	ug/l #	3
25) 2-Butanone	4.556	43	147859	54.757	ug/l	100
29) Tetrahydrofuran	5.007	42	2038	1.237	ug/l #	73
31) Cyclohexane	5.464	56	1284	0.238	ug/l #	78
36) 1,1-Dichloropropene	5.550	75	20716	4.808	ug/l #	48
37) Ethyl Acetate	4.556	43	147859	30.709	ug/l #	68
38) Carbon Tetrachloride	5.550	117	25714	5.800	ug/l #	15
39) Methylcyclohexane	7.379	83	1183	0.213	ug/l #	76
40) Benzene	6.038	78	99407	7.786	ug/l	98
41) Methacrylonitrile	4.995	41	5500	2.050	ug/l #	37
48) Methyl methacrylate	7.690	41	902	0.224	ug/l #	30
49) 1,4-Dioxane	7.665	88	2488	30.931	ug/l #	96
51) 4-Methyl-2-Pentanone	8.580	43	3396	0.726	ug/l	99
52) Toluene	8.720	92	62185	8.038	ug/l	100
59) 2-Hexanone	9.439	43	2061	0.579	ug/l	98
67) Ethyl Benzene	10.195	91	12855	0.867	ug/l	96
68) m/p-Xylenes	10.299	106	24550	4.329	ug/l	98
69) o-Xylene	10.640	106	11013	1.951	ug/l	94
70) Styrene	10.659	104	31577	3.439	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	93606	21.246	ug/l #	35
78) n-propylbenzene	11.305	91	4229	0.272	ug/l	90
79) 2-Chlorotoluene	11.378	91	2399	0.252	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.451	105	8252	0.736	ug/l	93
81) trans-1,4-Dichloro-2-b...	11.079	75	93606	54.579	ug/l #	8
84) 1,2,4-Trimethylbenzene	11.750	105	25284	2.229	ug/l	97
95) Naphthalene	13.774	128	27350	2.146	ug/l #	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030623\
Data File : VX034355.D
Acq On : 06 Mar 2023 17:22
Operator : JC/MD
Sample : 01816-05RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31957

Quant Time: Mar 07 00:41:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 17 12:33:35 2023
Response via : Initial Calibration




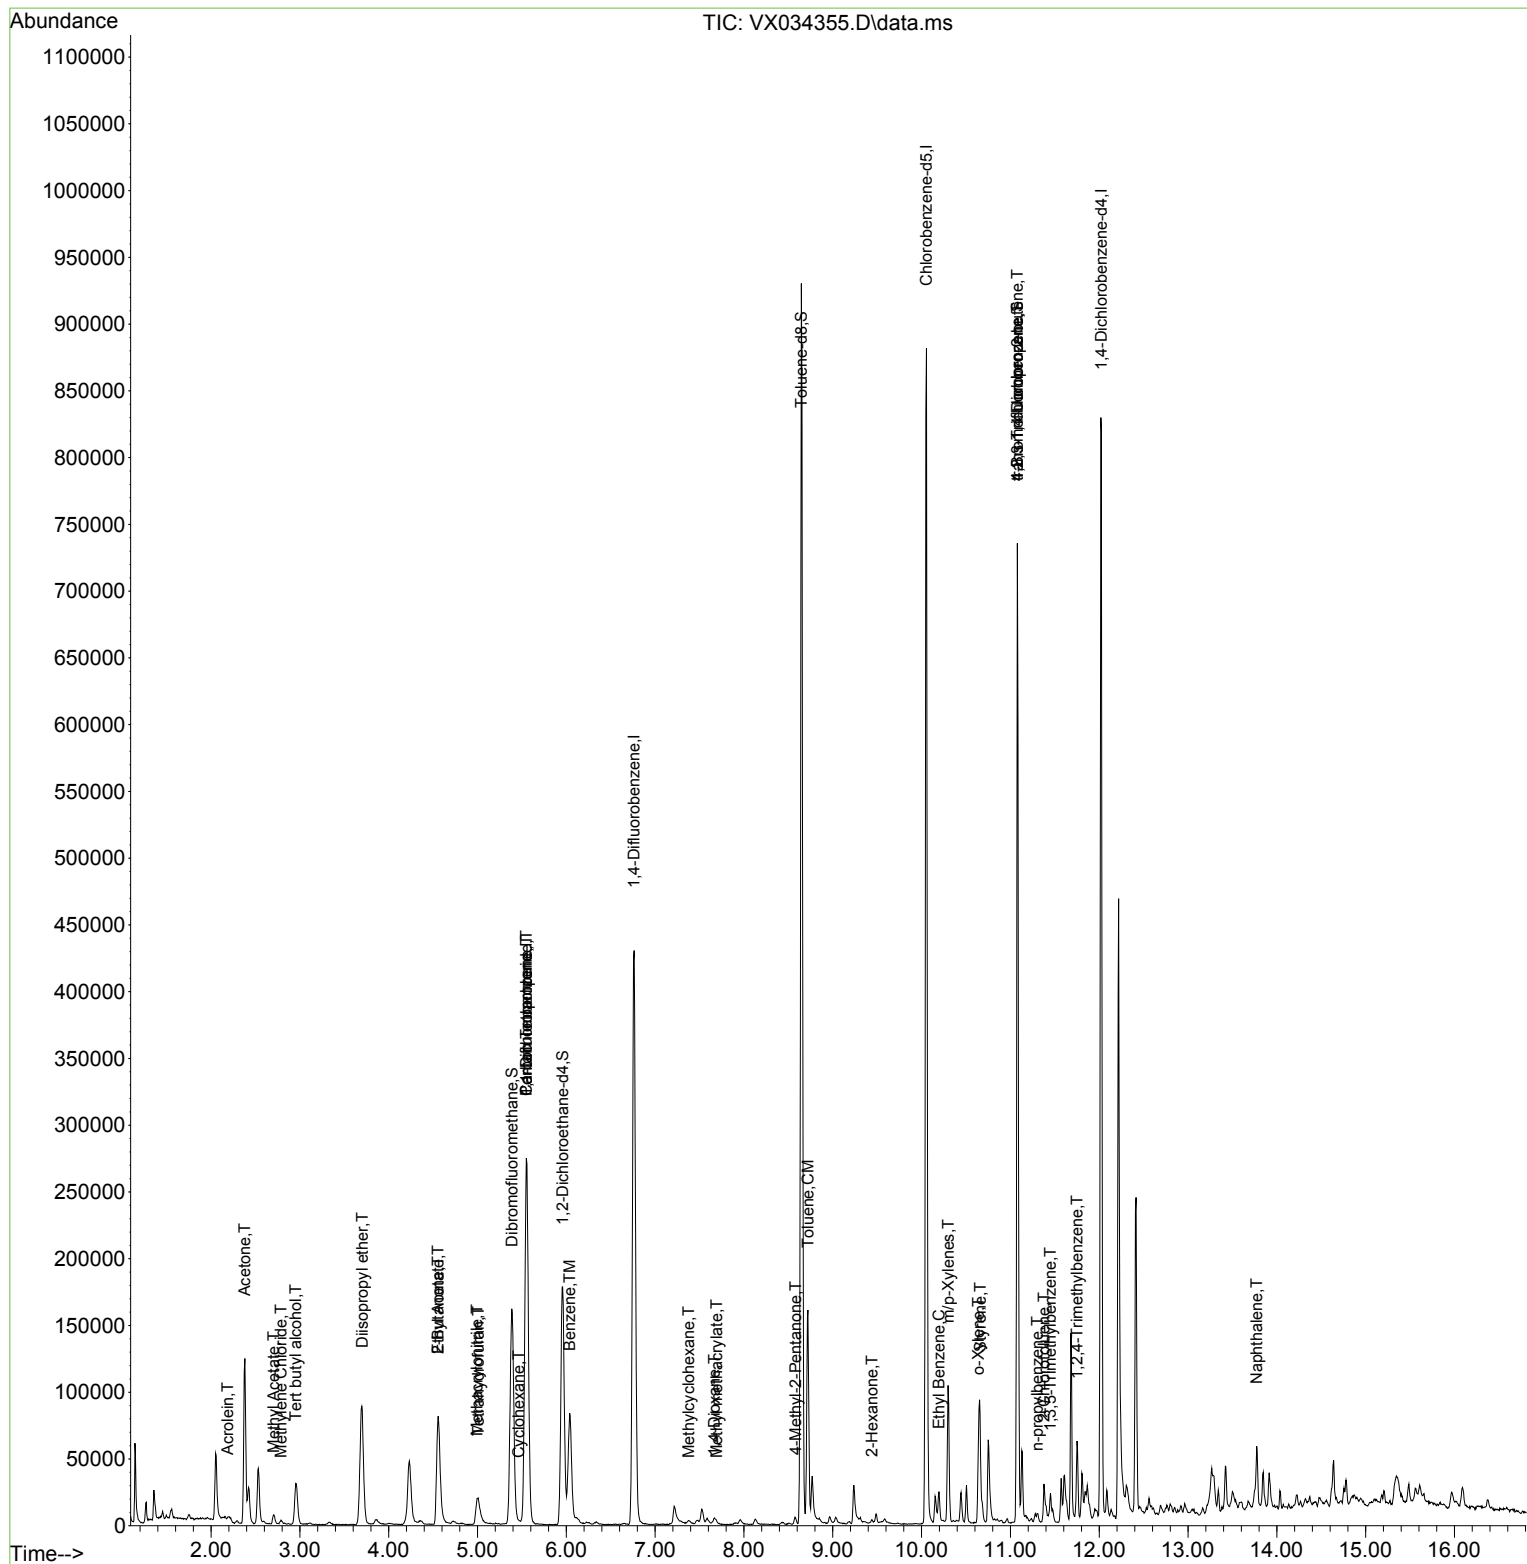




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion:168 Resp: 268630
Ion Ratio Lower Upper
168 100
99 58.2 39.6 59.4

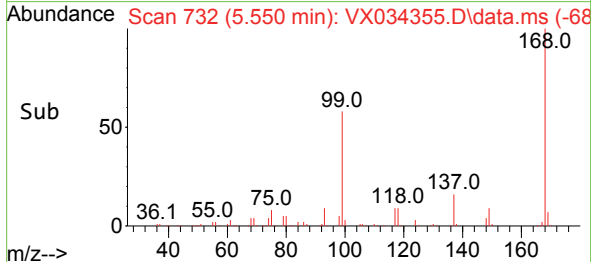

#5
Bromomethane
Concen: Below Cal
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 94 Resp: 162
Ion Ratio Lower Upper
94 100
96 0.0 74.3 111.5#

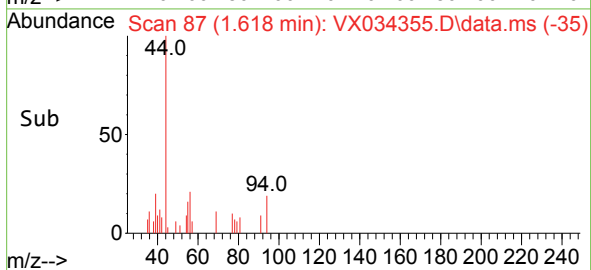

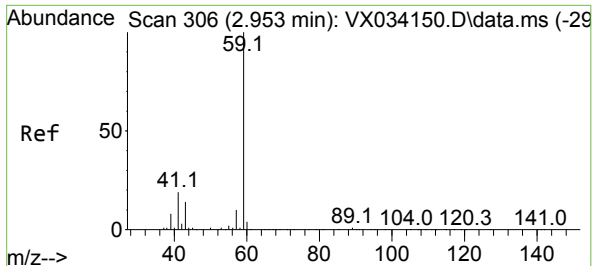

#11

Tert butyl alcohol

Concen: 42.919 ug/l

RT: 2.953 min Scan# 306

Delta R.T. 0.000 min

Lab File: VX034355.D

Acq: 06 Mar 2023 17:22

Instrument :

MSVOA_X

ClientSampleId :





31957

Tgt Ion: 59 Resp: 34729

Ion Ratio Lower Upper

59 100

57 9.5 3.7 5.5#

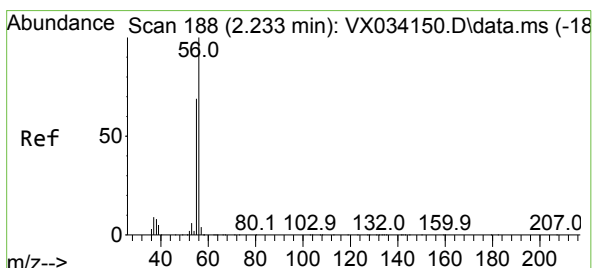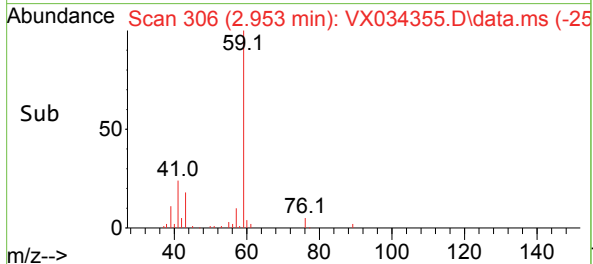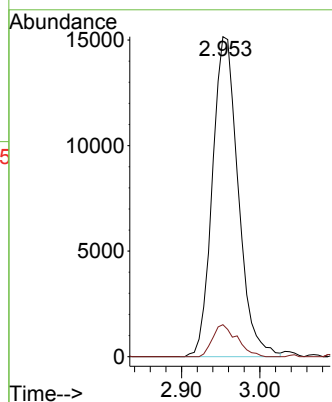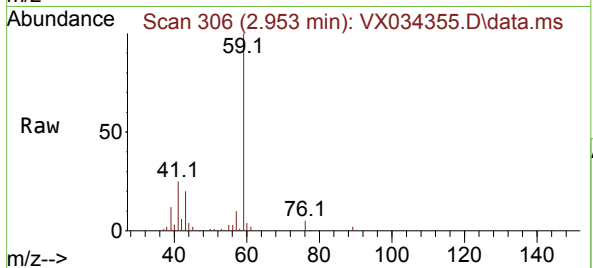

#13

Acrolein

Concen: 0.593 ug/l

RT: 2.185 min Scan# 180

Delta R.T. -0.049 min

Lab File: VX034355.D




Acq: 06 Mar 2023 17:22


Tgt Ion: 56 Resp: 219

Ion Ratio Lower Upper

56 100

55 0.0 56.3 84.5#


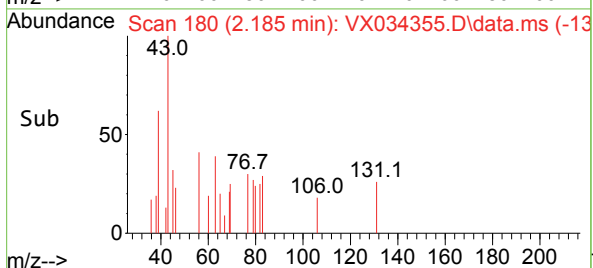

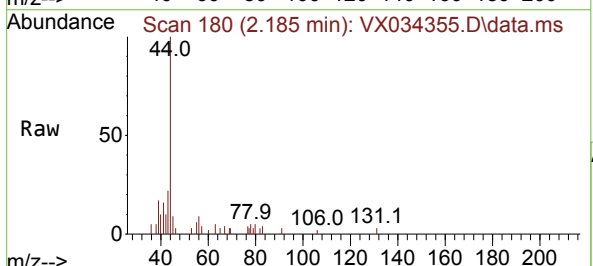




#16
Acetone
Concen: 68.998 ug/l
RT: 2.380 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 43 Resp: 128767
Ion Ratio Lower Upper
43 100
58 32.5 22.6 33.8

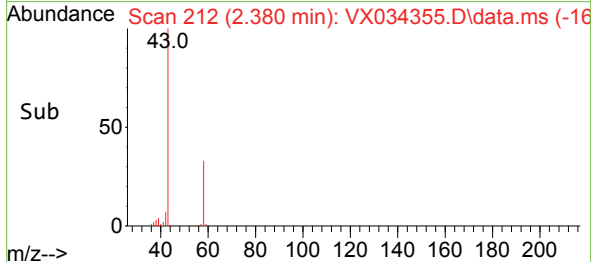

#18
Methyl Acetate
Concen: 1.519 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22


Tgt Ion: 43 Resp: 8774
Ion Ratio Lower Upper
43 100
74 22.6 18.2 27.4

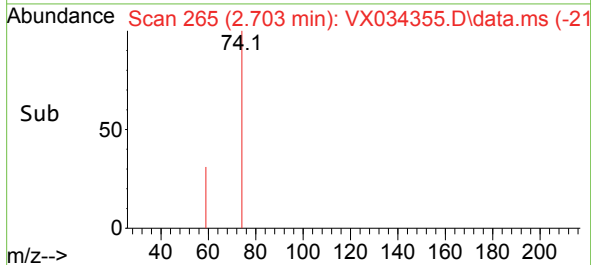






#20
Methylene Chloride
Concen: 0.286 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Instrument :
MSVOA_X
ClientSampleId :
31957



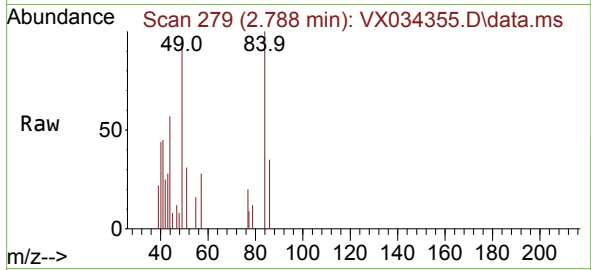



Tgt Ion: 84 Resp: 961
Ion Ratio Lower Upper
84 100
49 96.9 101.1 151.7#
51 31.4 31.0 46.6
86 35.5 52.6 79.0#

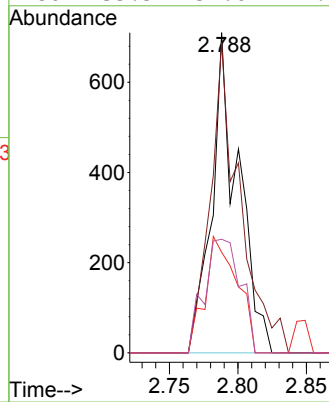

#22
Diisopropyl ether
Concen: 0.306 ug/l
RT: 3.703 min Scan# 429
Delta R.T. -0.055 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 45 Resp: 3303
Ion Ratio Lower Upper
45 100
43 17.5 64.6 97.0#
87 0.0 21.9 32.9#
59 157.5 9.2 13.8#



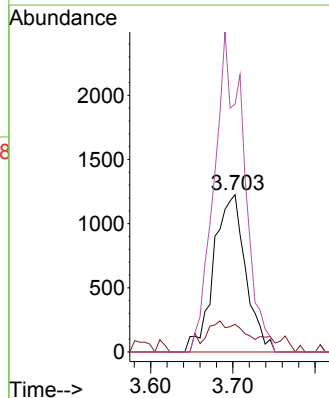





#25
2-Butanone
Concen: 54.757 ug/l
RT: 4.556 min Scan# 50
Delta R.T. 0.012 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 43 Resp: 147859
Ion Ratio Lower Upper
43 100
72 24.3 19.4 29.2

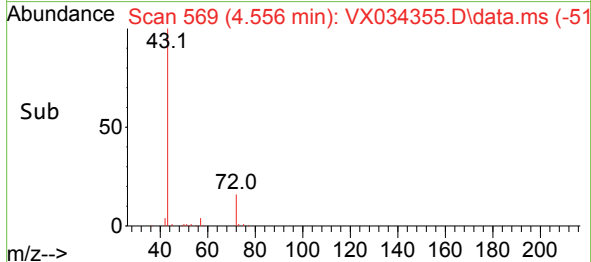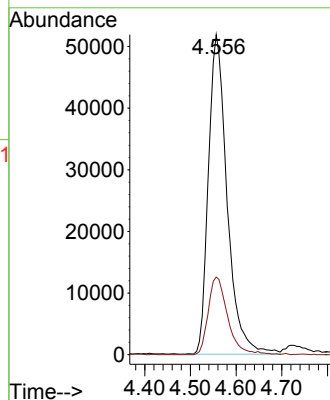

#29
Tetrahydrofuran
Concen: 1.237 ug/l
RT: 5.007 min Scan# 643
Delta R.T. 0.012 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 42 Resp: 2038
Ion Ratio Lower Upper
42 100
72 34.5 34.8 52.2#
71 14.2 32.2 48.2#


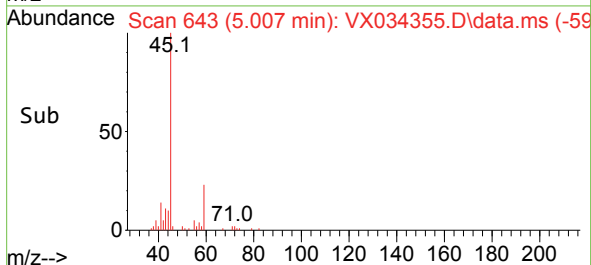
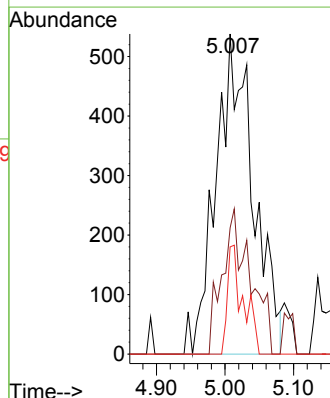
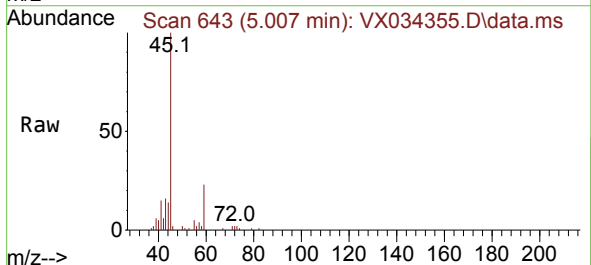




#31
Cyclohexane
Concen: 0.238 ug/l
RT: 5.464 min Scan# 719
Delta R.T. -0.006 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 56 Resp: 1284
Ion Ratio Lower Upper
56 100
69 29.2 24.6 37.0
84 62.3 71.0 106.6#

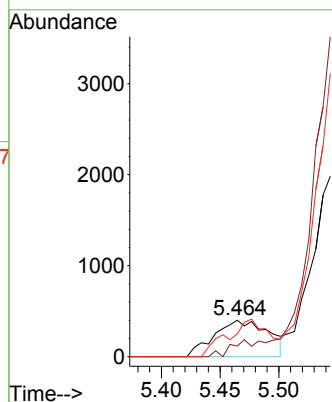

#33
1,2-Dichloroethane-d4
Concen: 46.468 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 65 Resp: 168113
Ion Ratio Lower Upper
65 100
67 53.2 0.0 104.8



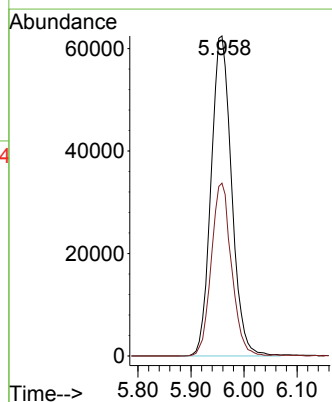





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion:114 Resp: 447415
Ion Ratio Lower Upper
114 100
63 20.4 0.0 37.4
88 15.9 0.0 30.6

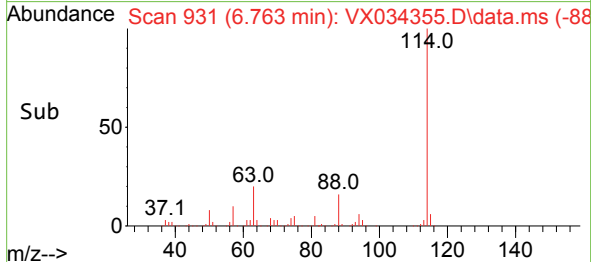

#35
Dibromofluoromethane
Concen: 48.829 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion:113 Resp: 142245
Ion Ratio Lower Upper
113 100
111 103.7 83.0 124.6
192 19.6 19.0 28.4


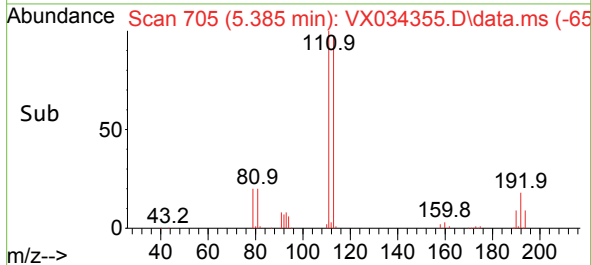






#36
1,1-Dichloropropene
Concen: 4.808 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 75 Resp: 20716
Ion Ratio Lower Upper
75 100
110 8.5 18.8 56.4#
77 0.0 25.1 37.7#



#37
Ethyl Acetate
Concen: 30.709 ug/l
RT: 4.556 min Scan# 569
Delta R.T. -0.152 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22


Tgt Ion: 43 Resp: 147859
Ion Ratio Lower Upper
43 100
61 0.0 11.1 16.7#
70 0.0 8.5 12.7#








#38
Carbon Tetrachloride
Concen: 5.800 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Instrument :
MSVOA_X
ClientSampleId :
31957



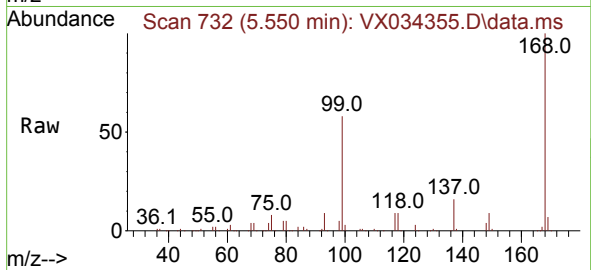



Tgt Ion:117 Resp: 25714
Ion Ratio Lower Upper
117 100
119 4.7 78.0 117.0#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 0.213 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 83 Resp: 1183
Ion Ratio Lower Upper
83 100
55 50.3 61.8 92.6#
98 41.0 39.3 58.9









#40
Benzene
Concen: 7.786 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 78 Resp: 99407
Ion Ratio Lower Upper
78 100
77 24.6 19.0 28.4

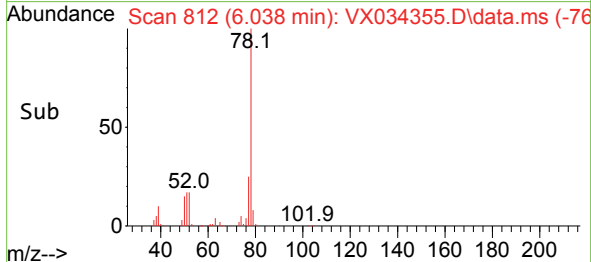

#41
Methacrylonitrile
Concen: 2.050 ug/l
RT: 4.995 min Scan# 641
Delta R.T. 0.079 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 41 Resp: 5500
Ion Ratio Lower Upper
41 100
39 24.7 43.8 65.6#
67 0.0 54.8 82.2#
52 0.0 23.0 34.6#

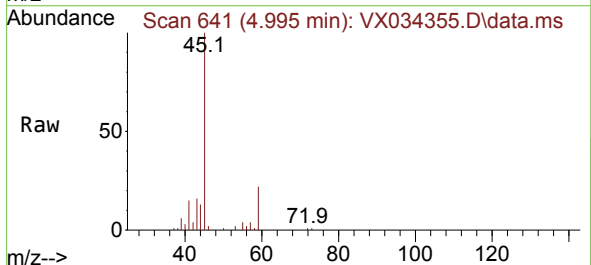



#48

Methyl methacrylate

Concen: 0.224 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX034355.D

Acq: 06 Mar 2023 17:22





Instrument :

MSVOA_X

ClientSampleId :

31957

Tgt Ion:	41	Resp:	902
Ion	Ratio	Lower	Upper
41	100		
69	0.0	63.1	94.7#
39	24.8	43.2	64.8#

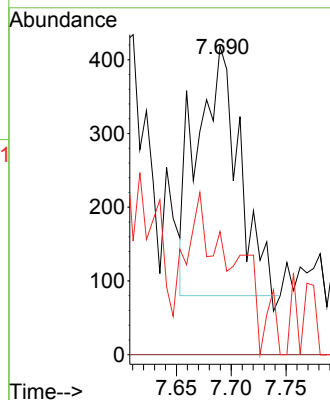

#49

1,4-Dioxane

Concen: 30.931 ug/l




RT: 7.665 min Scan# 1079


Delta R.T. 0.012 min

Lab File: VX034355.D

Acq: 06 Mar 2023 17:22

Tgt Ion:	88	Resp:	2488
Ion	Ratio	Lower	Upper
88	100		
43	33.8	0.0	0.0#
58	74.3	56.5	84.7

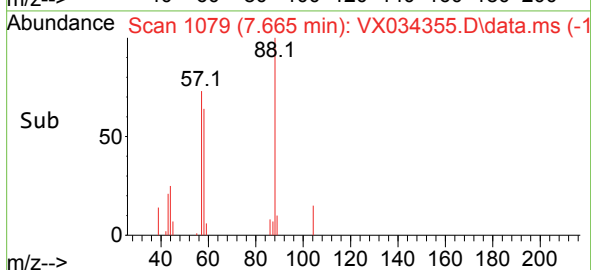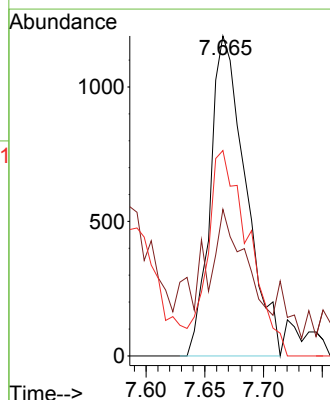



#50

Toluene-d8

Concen: 51.723 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX034355.D

Acq: 06 Mar 2023 17:22

Instrument :

MSVOA_X

ClientSampleId :





31957

Tgt Ion: 98 Resp: 540972

Ion Ratio Lower Upper

98 100

100 66.2 53.6 80.4

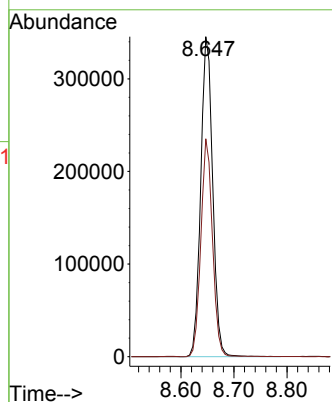

#51

4-Methyl-2-Pentanone

Concen: 0.726 ug/l

RT: 8.580 min Scan# 1229

Delta R.T. 0.012 min

Lab File: VX034355.D




Acq: 06 Mar 2023 17:22


Tgt Ion: 43 Resp: 3396

Ion Ratio Lower Upper

43 100

58 39.6 31.2 46.8


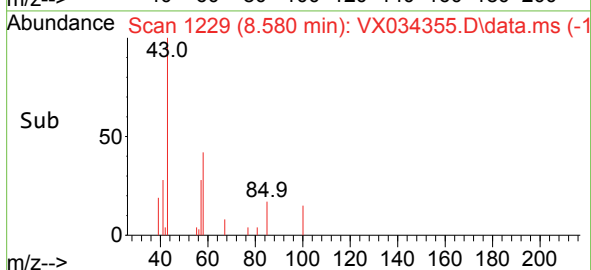






#52
Toluene
Concen: 8.038 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 92 Resp: 62185
Ion Ratio Lower Upper
92 100
91 170.0 135.5 203.3

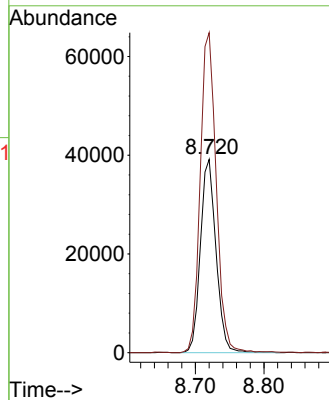

#59
2-Hexanone
Concen: 0.579 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.012 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 43 Resp: 2061
Ion Ratio Lower Upper
43 100
58 56.1 27.4 82.0


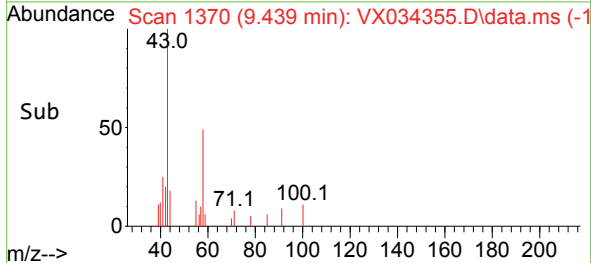
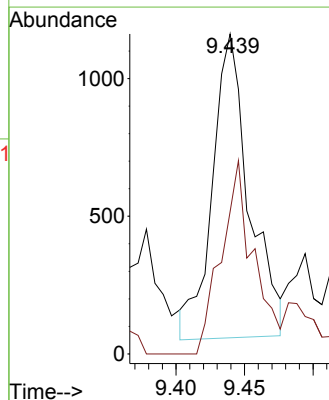





#62
4-Bromofluorobenzene
Concen: 46.580 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 95 Resp: 186348
Ion Ratio Lower Upper
95 100
174 77.2 0.0 184.4
176 76.2 0.0 178.8

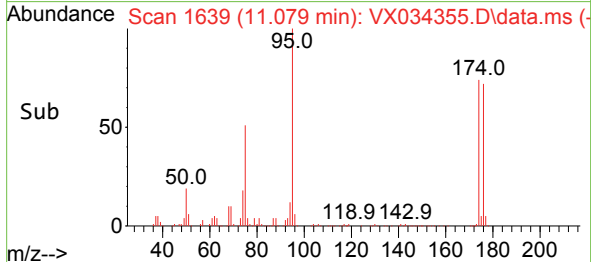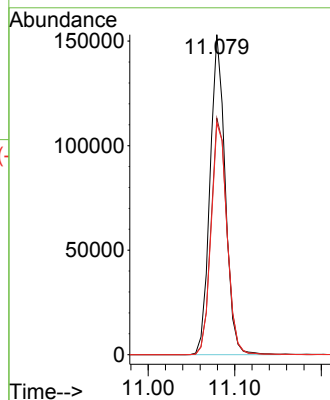

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 117 Resp: 395707
Ion Ratio Lower Upper
117 100
82 54.4 40.6 60.8
119 32.6 25.6 38.4


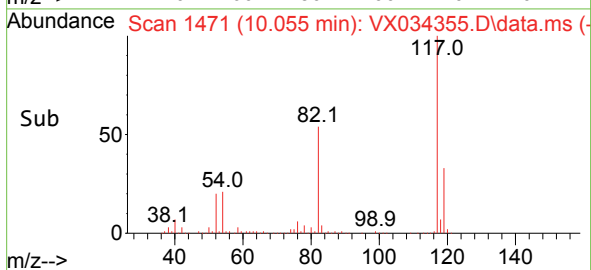
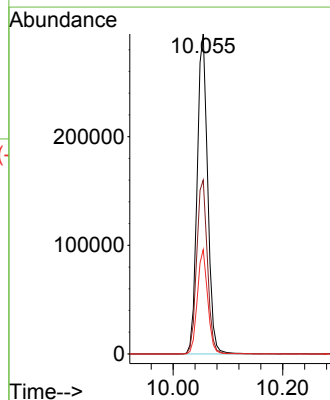



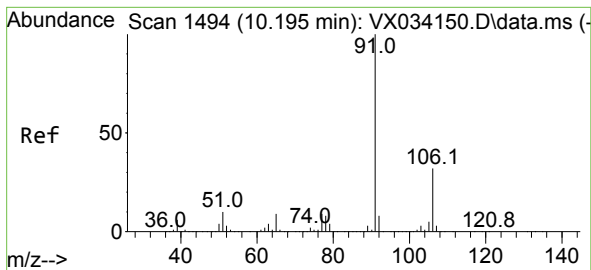

#67
Ethyl Benzene
Concen: 0.867 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 91 Resp: 12855
Ion Ratio Lower Upper
91 100
106 30.2 25.8 38.8

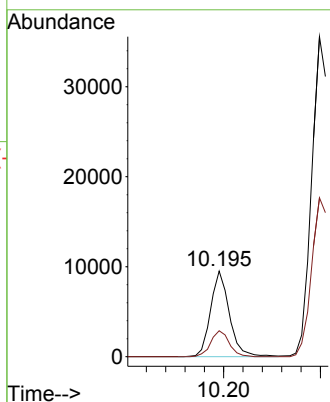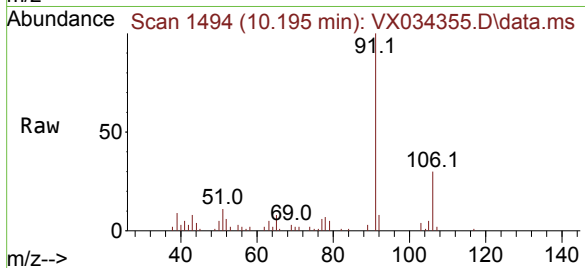

#68
m/p-Xylenes
Concen: 4.329 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 106 Resp: 24550
Ion Ratio Lower Upper
106 100
91 197.9 156.4 234.6



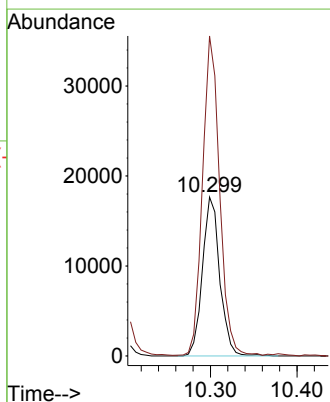
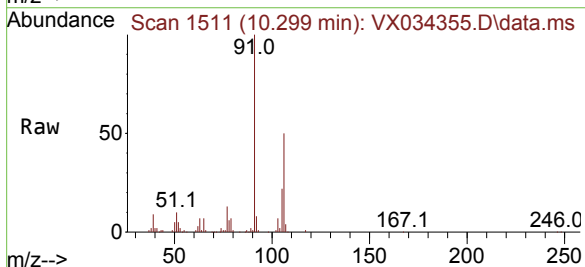




#69
o-Xylene
Concen: 1.951 ug/l
RT: 10.640 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion:106 Resp: 11013
Ion Ratio Lower Upper
106 100
91 214.8 103.1 309.3

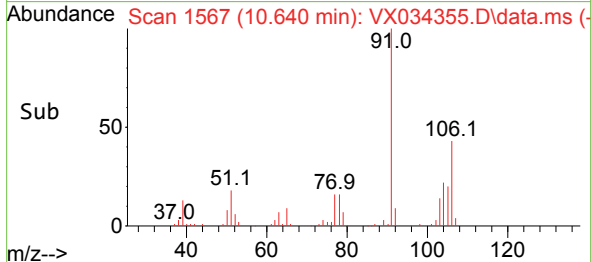

#70
Styrene
Concen: 3.439 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion:104 Resp: 31577
Ion Ratio Lower Upper
104 100
78 48.0 37.5 56.3
103 53.3 43.3 64.9









#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX034355.D
 Acq: 06 Mar 2023 17:22




Instrument :
 MSVOA_X
 ClientSampleId :
 31957


Tgt Ion:152 Resp: 175093
 Ion Ratio Lower Upper
 152 100
 115 58.7 38.7 116.1
 150 159.3 0.0 348.2

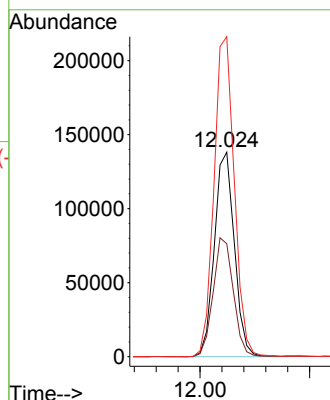

#76
 1,2,3-Trichloropropane
 Concen: 21.246 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.158 min
 Lab File: VX034355.D
 Acq: 06 Mar 2023 17:22

Tgt Ion: 75 Resp: 93606
 Ion Ratio Lower Upper
 75 100
 77 1.6 21.8 65.4#


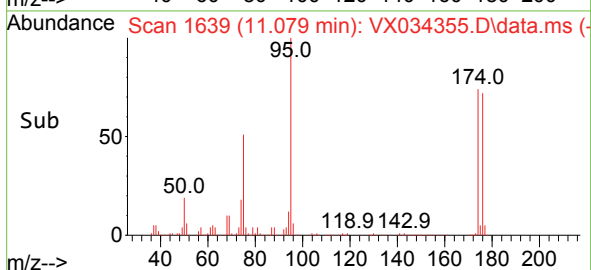
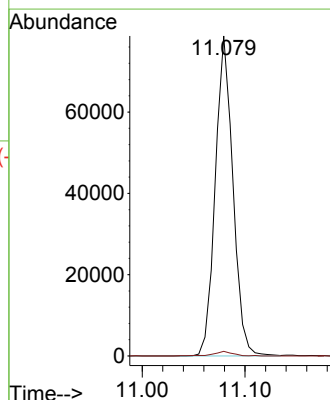
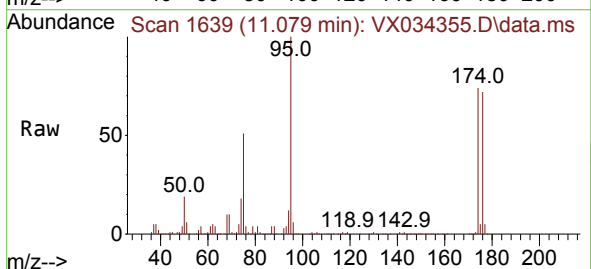


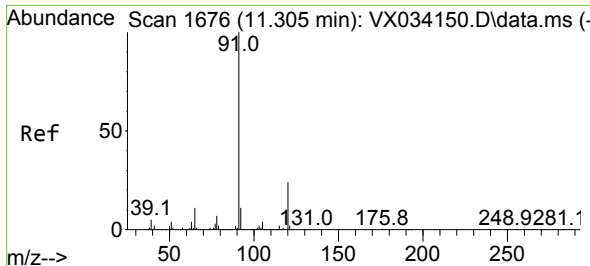

#78
n-propylbenzene
Concen: 0.272 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22




Instrument :
MSVOA_X
ClientSampleId :
31957


Tgt Ion: 91 Resp: 4229
Ion Ratio Lower Upper
91 100
120 19.6 12.3 36.8

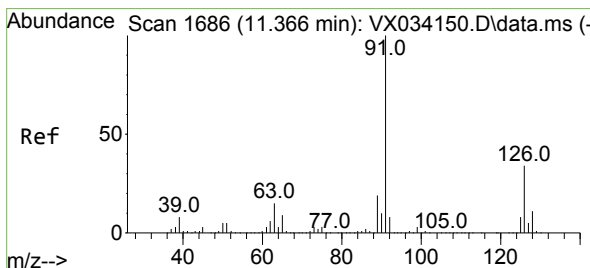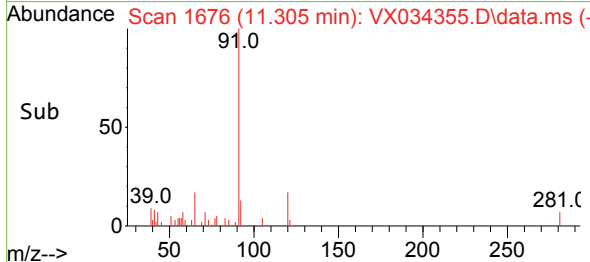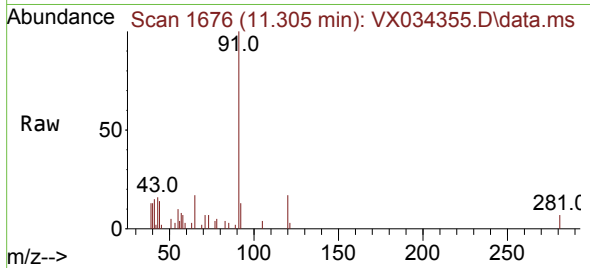

#79
2-Chlorotoluene
Concen: 0.252 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX034355.D
Acq: 06 Mar 2023 17:22

Tgt Ion: 91 Resp: 2399
Ion Ratio Lower Upper
91 100
126 0.0 18.1 54.1#

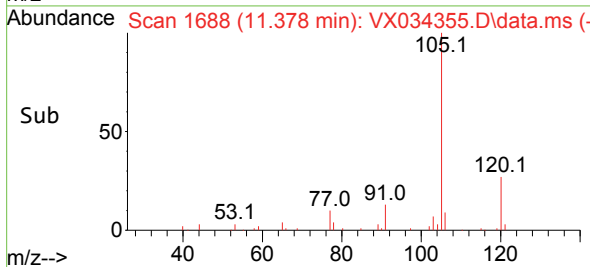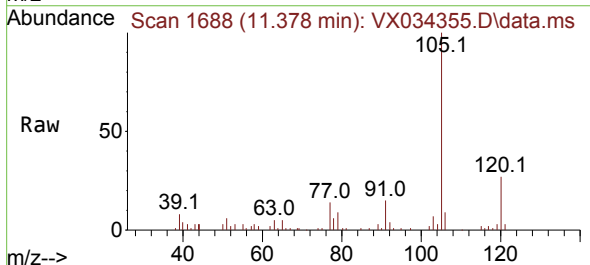



#80

1,3,5-Trimethylbenzene

Concen: 0.736 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX034355.D

Acq: 06 Mar 2023 17:22

Instrument :

MSVOA_X

ClientSampleId :





31957

Tgt Ion:105 Resp: 8252

Ion Ratio Lower Upper

105 100

120 46.2 25.6 76.8

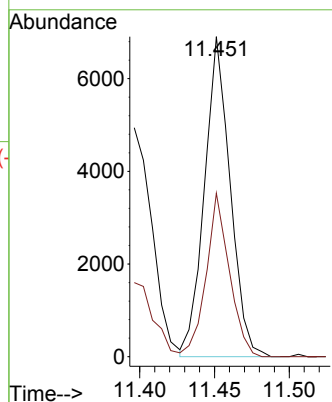

#81

trans-1,4-Dichloro-2-butene

Concen: 54.579 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX034355.D

Acq: 06 Mar 2023 17:22




Tgt Ion: 75 Resp: 93606


Ion Ratio Lower Upper

75 100

53 0.0 83.0 124.6#

89 0.1 37.7 56.5#


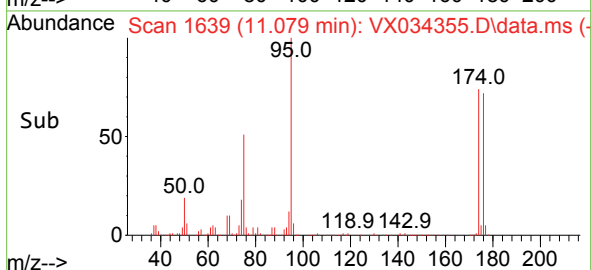




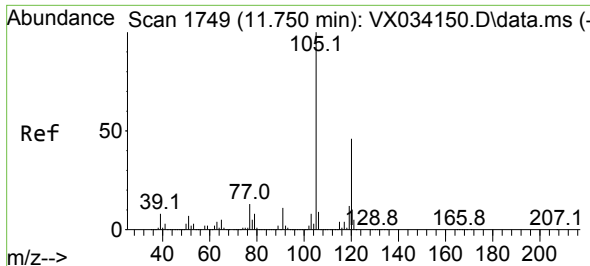

#84
 1,2,4-Trimethylbenzene
 Concen: 2.229 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX034355.D
 Acq: 06 Mar 2023 17:22

Instrument :
 MSVOA_X
 ClientSampleId :
 31957

Tgt Ion:105 Resp: 25284
 Ion Ratio Lower Upper
 105 100
 120 44.7 23.4 70.2

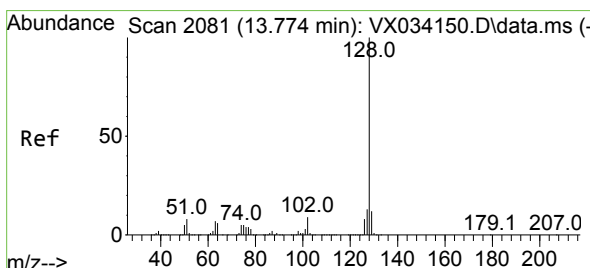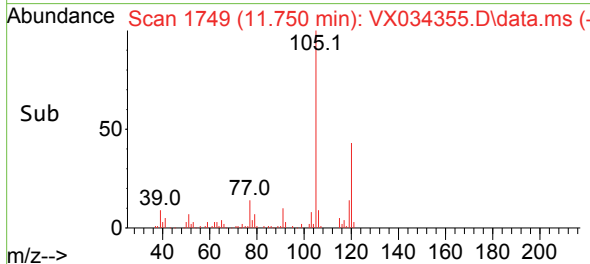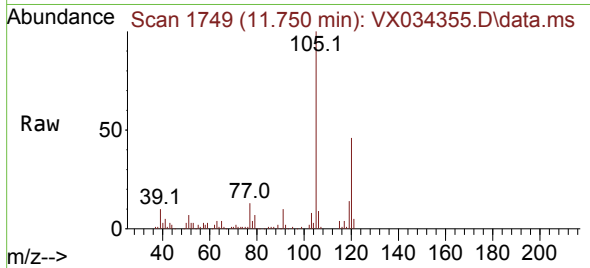

#95
 Naphthalene
 Concen: 2.146 ug/l
 RT: 13.774 min Scan# 2081
 Delta R.T. 0.000 min
 Lab File: VX034355.D
 Acq: 06 Mar 2023 17:22

Tgt Ion:128 Resp: 27350
 Ion Ratio Lower Upper
 128 100
 127 13.7 10.3 15.5
 129 13.1 8.7 13.1#

