

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
 Data File : VX029585.D
 Acq On : 18 Jun 2022 21:15
 Operator : JC/MD
 Sample : N3290-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-19

Quant Time: Jun 20 01:37:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	272600	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	456598	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	393707	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	170347	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	156712	43.429	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	86.860%		
35) Dibromofluoromethane	5.391	113	136536	45.885	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	91.780%		
50) Toluene-d8	8.653	98	523550	48.163	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	96.320%		
62) 4-Bromofluorobenzene	11.079	95	186015	45.377	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.760%		
Target Compounds						Qvalue
3) Chloromethane	1.294	50	1035	0.291	ug/l #	88
5) Bromomethane	1.617	94	803	0.481	ug/l	97
6) Chloroethane	1.587	64	3883	2.774	ug/l #	50
10) Methyl Iodide	2.453	142	351	3.119	ug/l #	76
11) Tert butyl alcohol	2.977	59	249288	319.590	ug/l	99
13) Acrolein	2.221	56	319	1.605	ug/l #	1
14) Allyl chloride	2.782	41	1090	0.244	ug/l #	59
15) Acrylonitrile	3.117	53	22328	13.229	ug/l #	30
16) Acetone	2.386	43	4702	3.269	ug/l	92
17) Carbon Disulfide	2.514	76	2563	0.358	ug/l #	91
18) Methyl Acetate	2.788	43	2596	0.683	ug/l #	46
19) Methyl tert-butyl Ether	3.117	73	2583113	269.416	ug/l	100
22) Diisopropyl ether	3.763	45	28437	3.224	ug/l #	89
23) Vinyl Acetate	3.763	43	14413	1.957	ug/l #	66
29) Tetrahydrofuran	5.025	42	399	0.263	ug/l #	73
36) 1,1-Dichloropropene	5.550	75	20909	5.192	ug/l #	50
38) Carbon Tetrachloride	5.562	117	28016	7.074	ug/l #	15
40) Benzene	6.043	78	10054	0.842	ug/l	94
43) Isopropyl Acetate	6.239	43	124453	19.388	ug/l #	56
44) Trichloroethene	7.135	130	2133	Below Cal		96
51) 4-Methyl-2-Pentanone	8.506	43	28924	6.991	ug/l #	52
56) Ethyl methacrylate	8.842	69	24693	5.288	ug/l #	62
59) 2-Hexanone	9.567	43	12895	4.116	ug/l	67
67) Ethyl Benzene	10.195	91	8534	0.614	ug/l	89
68) m/p-Xylenes	10.305	106	7313	1.349	ug/l	91
69) o-Xylene	10.646	106	1902	0.355	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	88687	23.898	ug/l #	38
78) n-propylbenzene	11.311	91	3350	0.233	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	88687	79.504	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	4136	0.386	ug/l	95
95) Naphthalene	13.780	128	4274	0.358	ug/l #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
Data File : VX029585.D
Acq On : 18 Jun 2022 21:15
Operator : JC/MD
Sample : N3290-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-19

Quant Time: Jun 20 01:37:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration




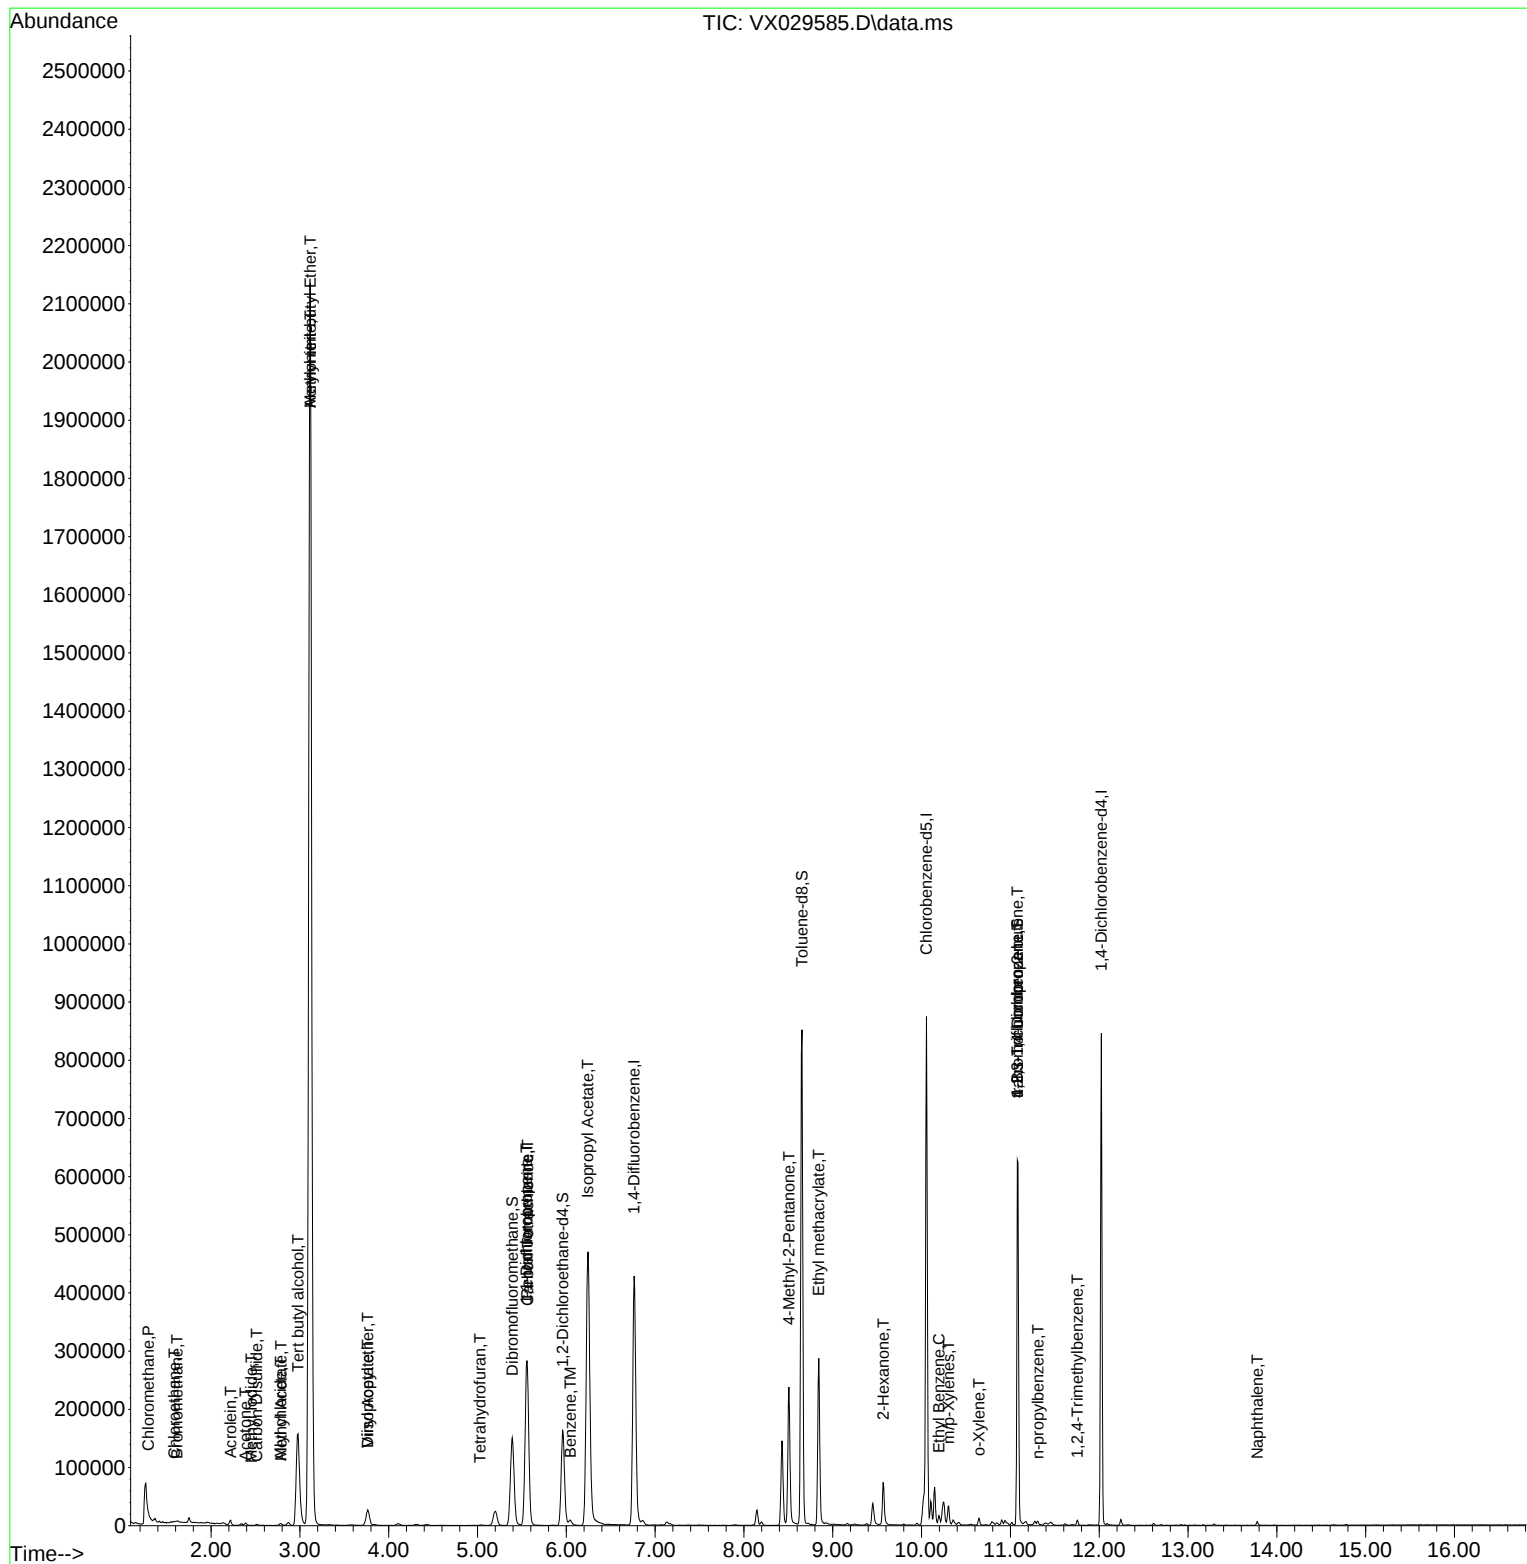




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion:168 Resp: 272600
Ion Ratio Lower Upper
168 100
99 62.0 41.7 62.5

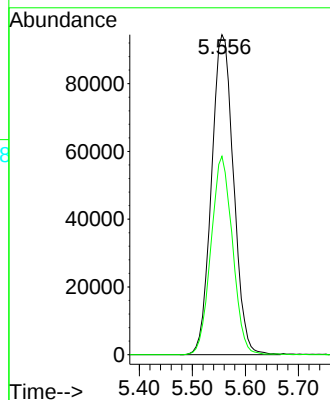

#3
Chloromethane
Concen: 0.291 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 50 Resp: 1035
Ion Ratio Lower Upper
50 100
52 40.0 26.4 39.6#



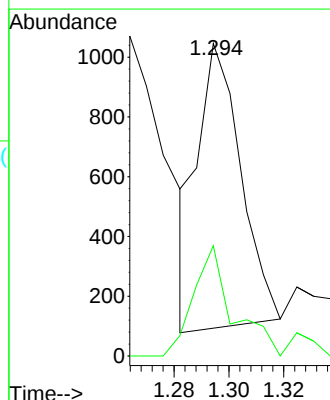



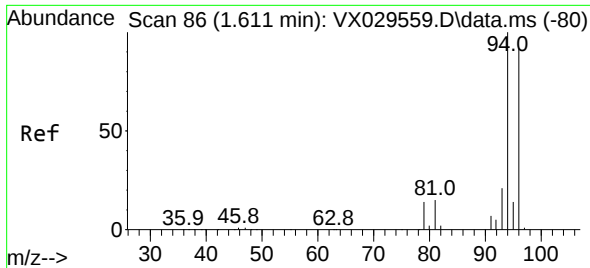

#5
Bromomethane
Concen: 0.481 ug/l
RT: 1.617 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 94 Resp: 803
Ion Ratio Lower Upper
94 100
96 97.4 75.3 112.9

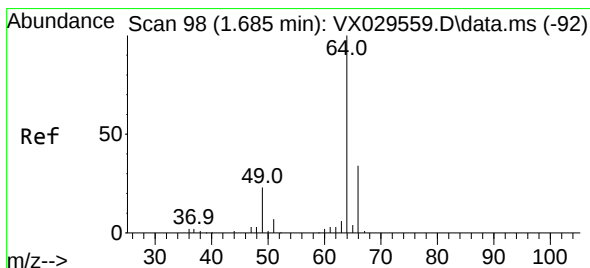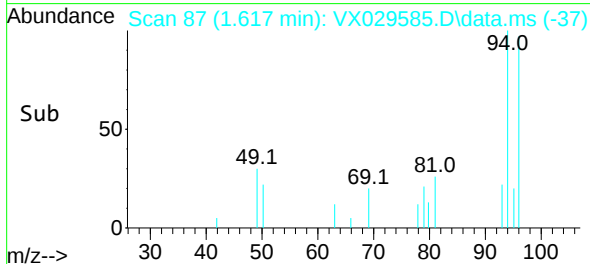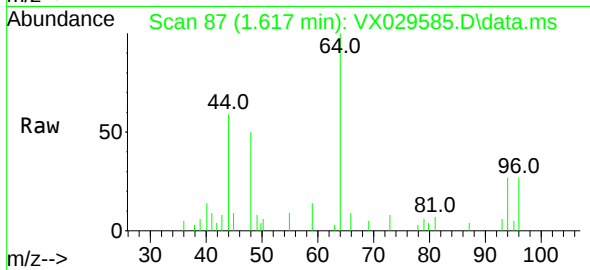

#6
Chloroethane
Concen: 2.774 ug/l
RT: 1.587 min Scan# 82
Delta R.T. -0.098 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15


Tgt Ion: 64 Resp: 3883
Ion Ratio Lower Upper
64 100
66 3.9 25.3 37.9#

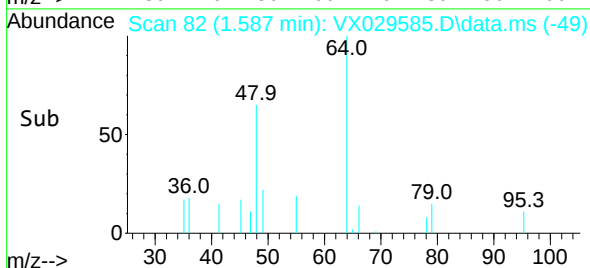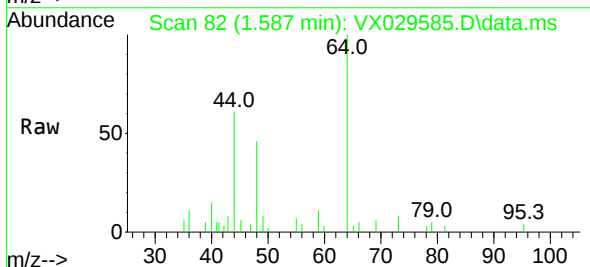



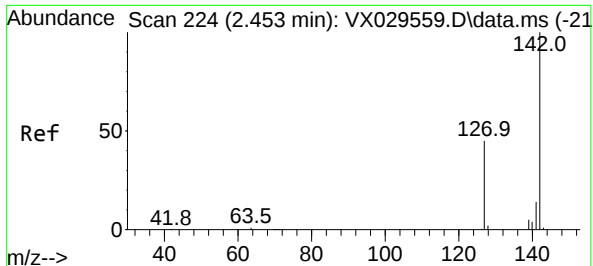


#10
Methyl Iodide
Concen: 3.119 ug/l
RT: 2.453 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15


Instrument :
MSVOA_X
ClientSampleId :
MW-19





Tgt Ion:142 Resp: 351
Ion Ratio Lower Upper
142 100
127 29.3 33.9 50.9#
141 0.0 11.4 17.2#

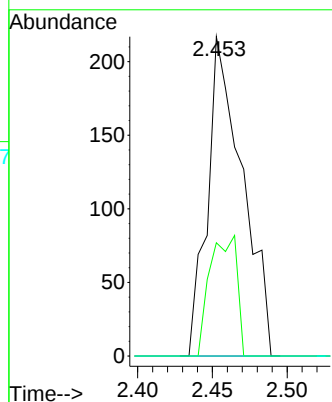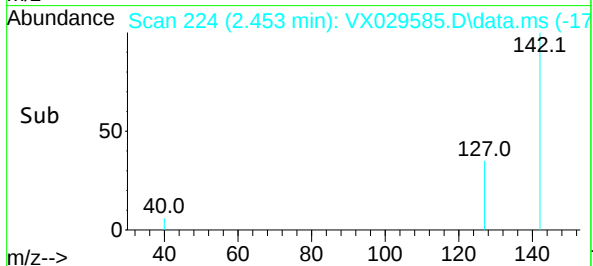


#11
Tert butyl alcohol
Concen: 319.590 ug/l
RT: 2.977 min Scan# 310
Delta R.T. -0.006 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

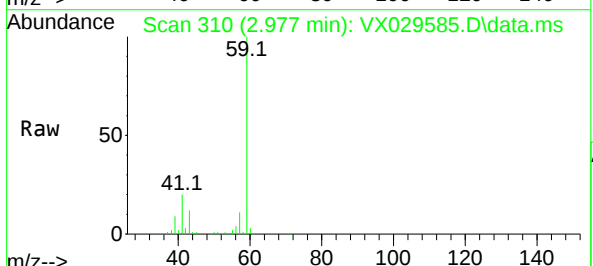

Tgt Ion: 59 Resp: 249288
Ion Ratio Lower Upper
59 100
57 10.6 8.3 12.5

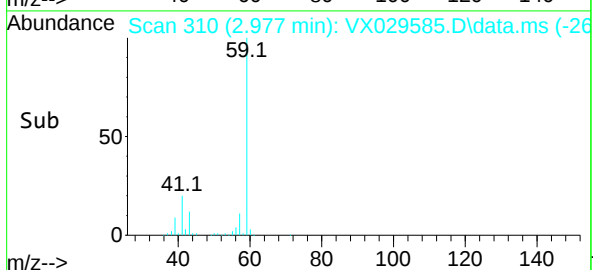

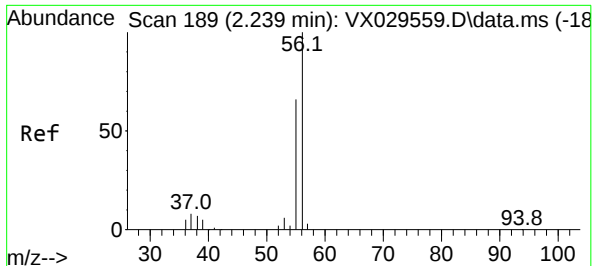

#13

Acrolein

Concen: 1.605 ug/l

RT: 2.221 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :





MW-19

Tgt Ion: 56 Resp: 319

Ion Ratio Lower Upper

56 100

55 1392.5 55.0 82.6#

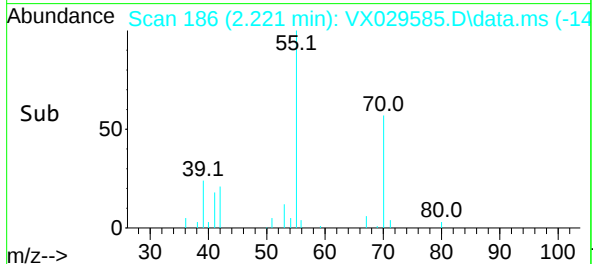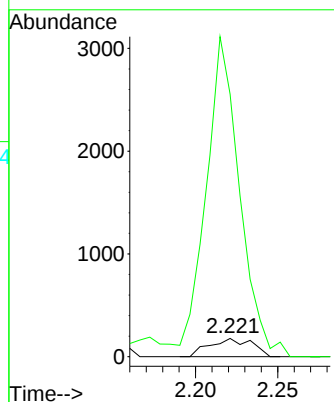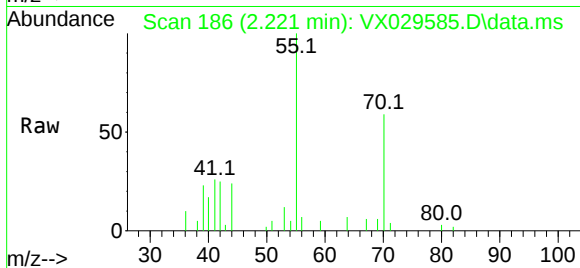

#14

Allyl chloride

Concen: 0.244 ug/l

RT: 2.782 min Scan# 278

Delta R.T. 0.116 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15




Tgt Ion: 41 Resp: 1090


Ion Ratio Lower Upper

41 100

39 43.7 50.4 75.6#

76 0.0 32.7 49.1#

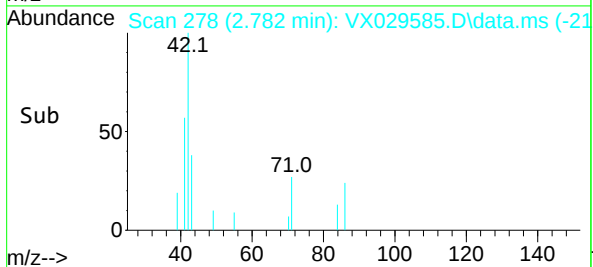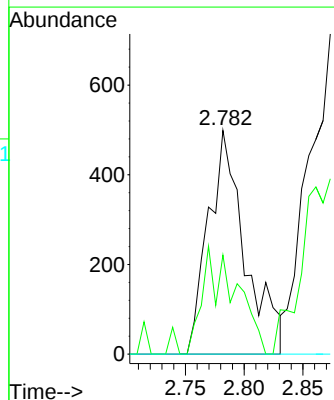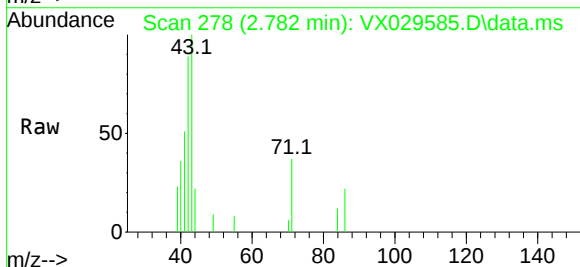



#15

Acrylonitrile

Concen: 13.229 ug/l

RT: 3.117 min Scan# 31

Delta R.T. 0.049 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :

MW-19





Tgt Ion: 53 Resp: 22328

Ion Ratio Lower Upper

53 100

52 19.0 65.7 98.5#

51 75.4 28.4 42.6#

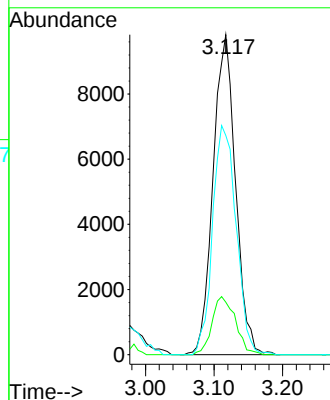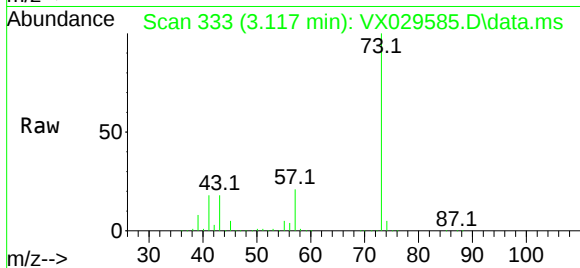

#16

Acetone

Concen: 3.269 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX029585.D




Acq: 18 Jun 2022 21:15


Tgt Ion: 43 Resp: 4702

Ion Ratio Lower Upper

43 100


58 31.1 28.8 43.2

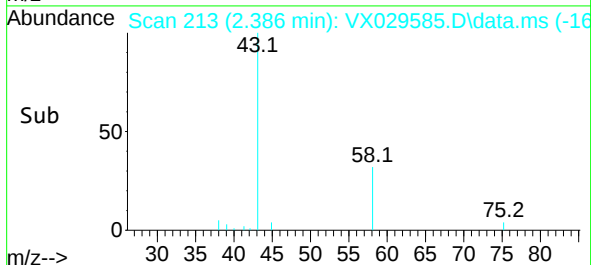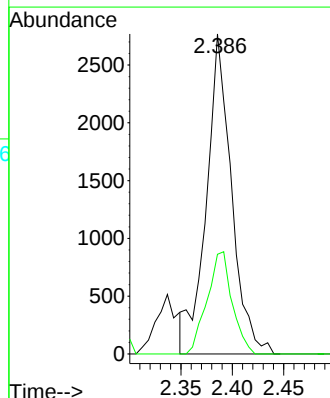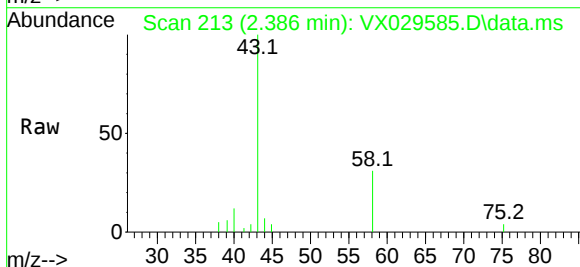



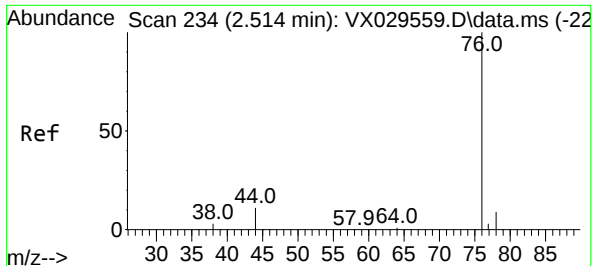


#17
Carbon Disulfide
Concen: 0.358 ug/l
RT: 2.514 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Instrument :
MSVOA_X
ClientSampleId :
MW-19







Tgt Ion: 76 Resp: 2563
Ion Ratio Lower Upper
76 100
78 12.2 7.2 10.8#

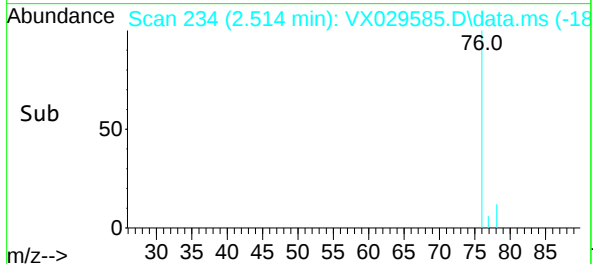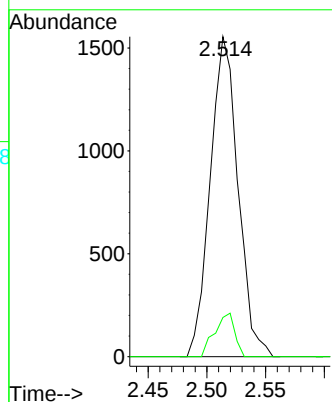

#18
Methyl Acetate
Concen: 0.683 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.079 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 43 Resp: 2596
Ion Ratio Lower Upper
43 100
74 0.0 22.8 34.2#


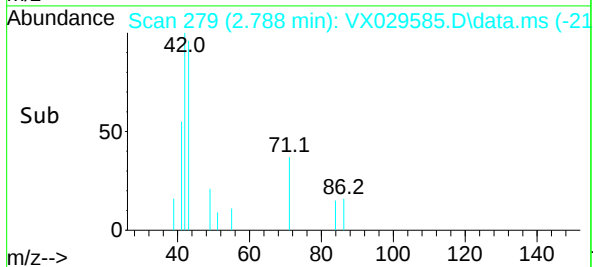
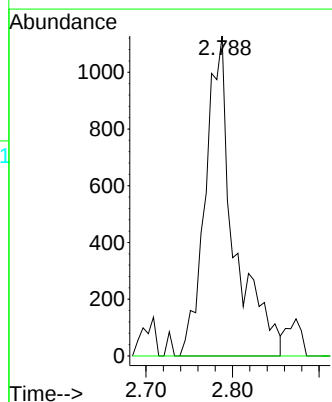
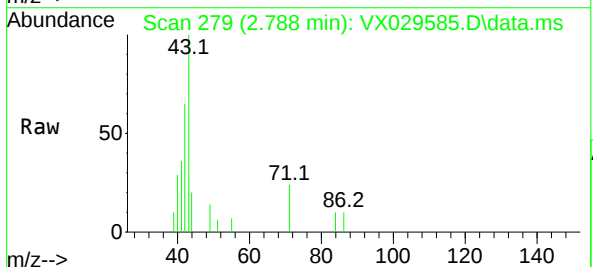




#19
Methyl tert-butyl Ether
Concen: 269.416 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 73 Resp: 2583113
Ion Ratio Lower Upper
73 100
57 21.1 16.8 25.2

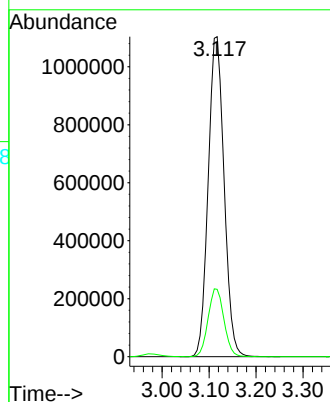

#22
Diisopropyl ether
Concen: 3.224 ug/l
RT: 3.763 min Scan# 439
Delta R.T. 0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 45 Resp: 28437
Ion Ratio Lower Upper
45 100
43 49.2 50.8 76.2#
87 33.6 26.6 39.8
59 13.9 10.5 15.7


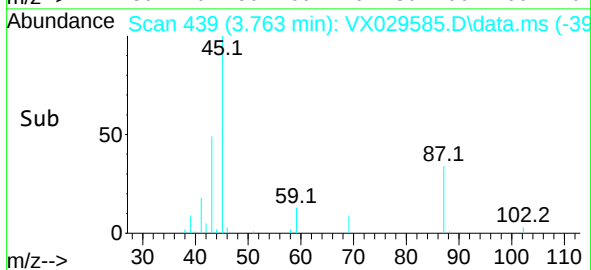
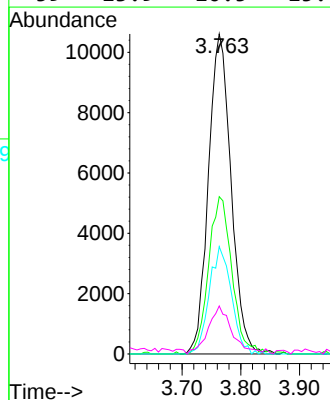



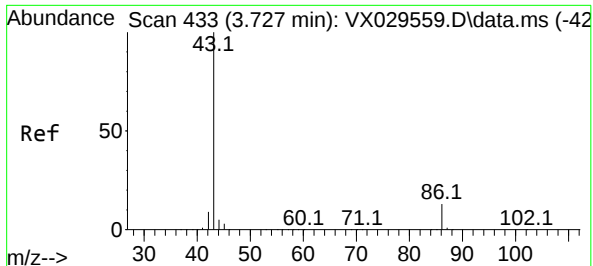

#23
 Vinyl Acetate
 Concen: 1.957 ug/l
 RT: 3.763 min Scan# 41
 Delta R.T. 0.036 min
 Lab File: VX029585.D
 Acq: 18 Jun 2022 21:15




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-19


Tgt Ion: 43 Resp: 14413
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.8 16.2#

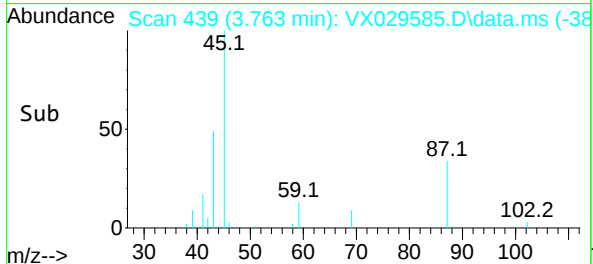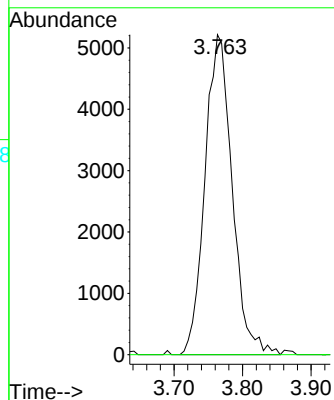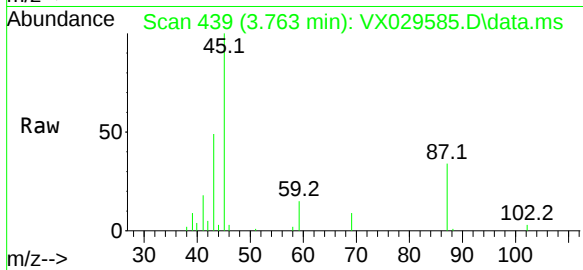

#29
 Tetrahydrofuran
 Concen: 0.263 ug/l
 RT: 5.025 min Scan# 646
 Delta R.T. 0.012 min
 Lab File: VX029585.D
 Acq: 18 Jun 2022 21:15

Tgt Ion: 42 Resp: 399
 Ion Ratio Lower Upper
 42 100
 72 54.4 44.1 66.1
 71 89.2 40.5 60.7#

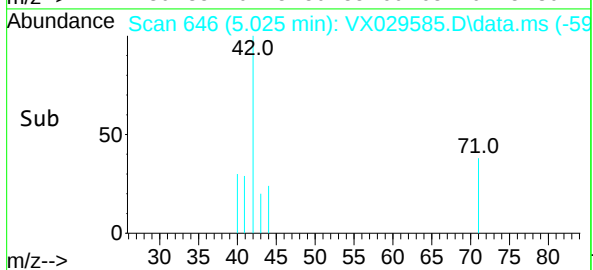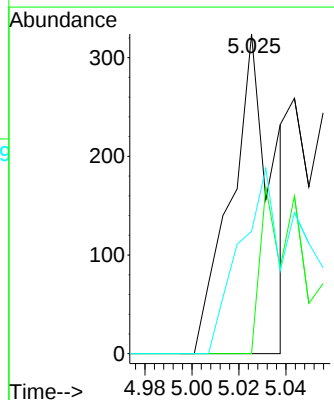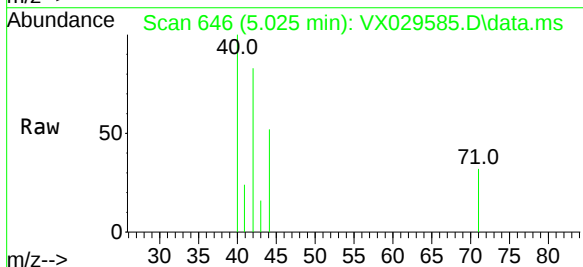



#33

1,2-Dichloroethane-d4

Concen: 43.429 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :





MW-19

Tgt Ion: 65 Resp: 156712

Ion Ratio Lower Upper

65 100

67 52.1 0.0 107.4

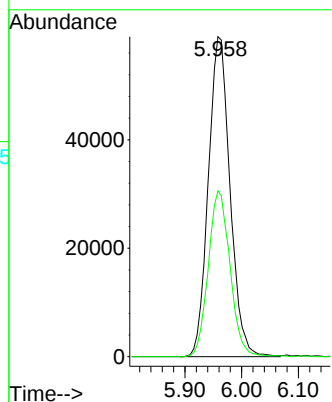

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15




Tgt Ion: 114 Resp: 456598


Ion Ratio Lower Upper

114 100

63 18.9 0.0 36.8

88 16.8 0.0 32.4

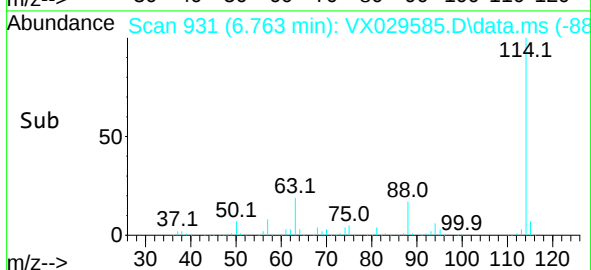

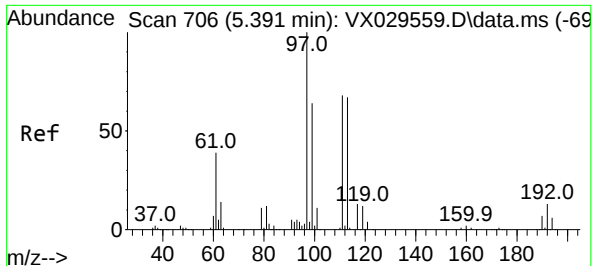

#35

Dibromofluoromethane

Concen: 45.885 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :

MW-19





Tgt Ion:113 Resp: 136536

Ion Ratio Lower Upper

113 100

111 102.2 82.8 124.2

192 18.2 16.9 25.3

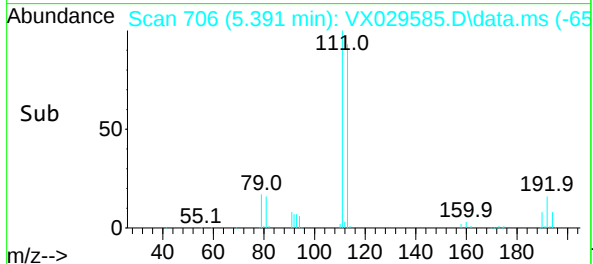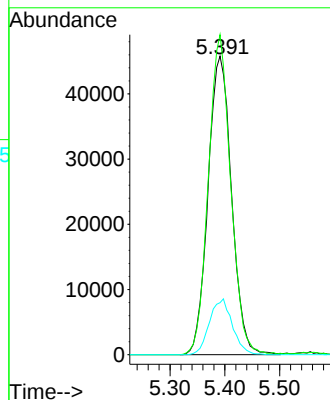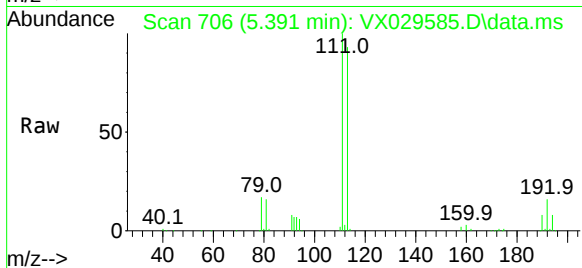

#36

1,1-Dichloropropene

Concen: 5.192 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15




Tgt Ion: 75 Resp: 20909


Ion Ratio Lower Upper

75 100

110 10.0 18.3 54.8#


77 0.0 24.8 37.2#

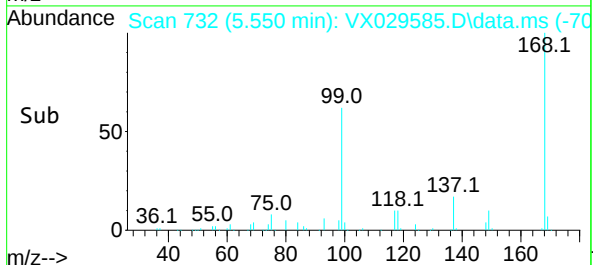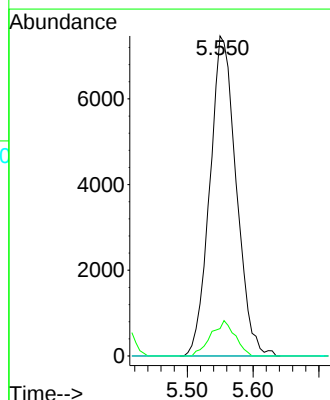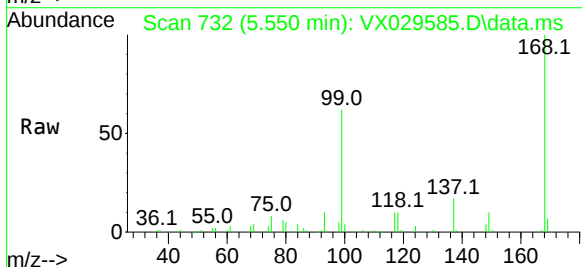



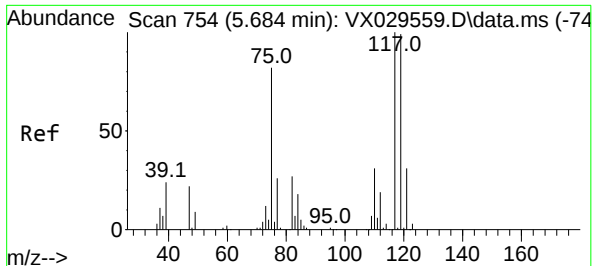


#38
Carbon Tetrachloride
Concen: 7.074 ug/l
RT: 5.562 min Scan# 711
Delta R.T. -0.122 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Instrument :
MSVOA_X
ClientSampleId :
MW-19







Tgt Ion:117 Resp: 28016
Ion Ratio Lower Upper
117 100
119 4.4 77.3 115.9#
121 0.0 24.2 36.2#

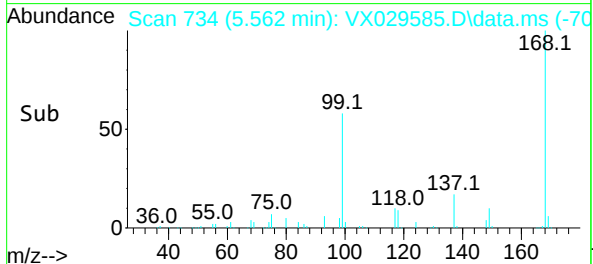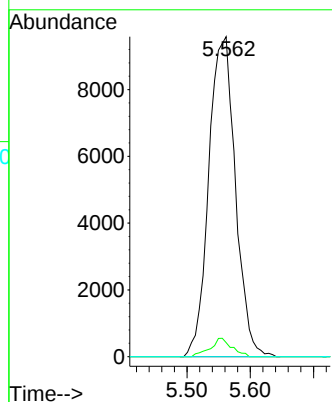

#40
Benzene
Concen: 0.842 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 78 Resp: 10054
Ion Ratio Lower Upper
78 100
77 27.1 19.3 28.9

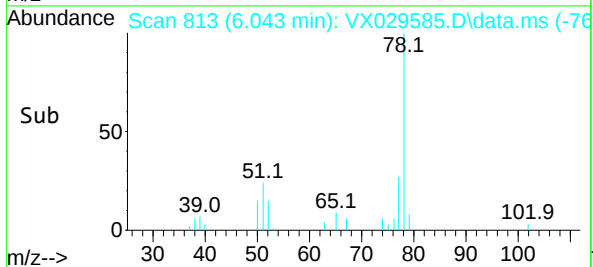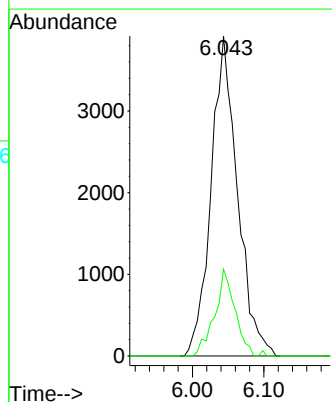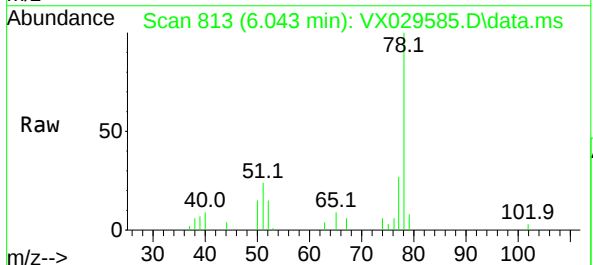



#43

Isopropyl Acetate

Concen: 19.388 ug/l

RT: 6.239 min Scan# 84

Delta R.T. -0.103 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :

MW-19





Tgt Ion: 43 Resp: 124453

Ion Ratio Lower Upper

43 100

61 0.0 18.5 27.7#

87 0.0 13.0 19.6#

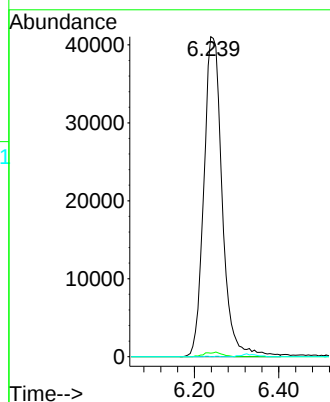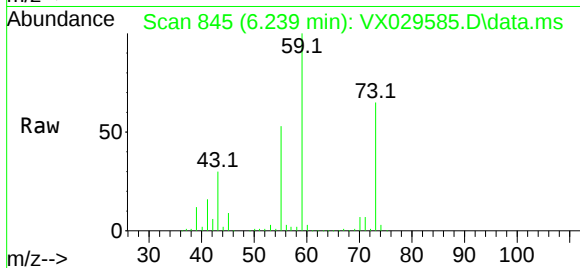

#44

Trichloroethene

Concen: Below Cal

RT: 7.135 min Scan# 992

Delta R.T. 0.006 min

Lab File: VX029585.D




Acq: 18 Jun 2022 21:15


Tgt Ion:130 Resp: 2133

Ion Ratio Lower Upper

130 100

95 90.5 0.0 188.8


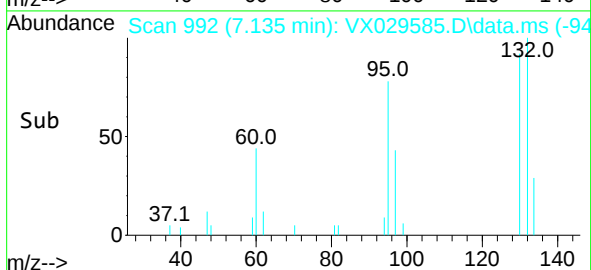
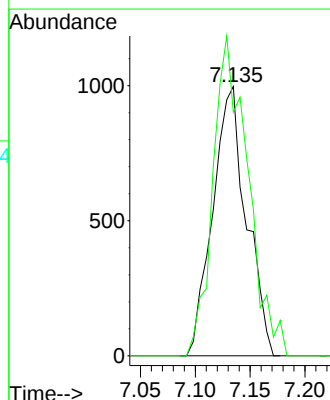
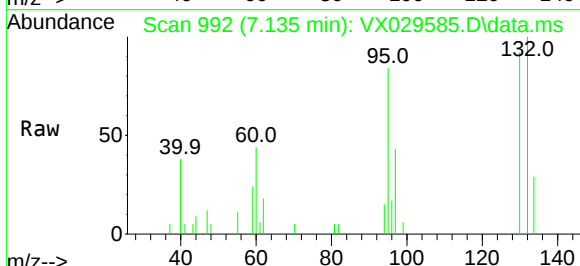


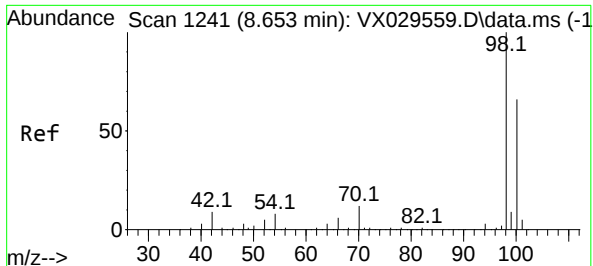

#50
Toluene-d8
Concen: 48.163 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 98 Resp: 523550
Ion Ratio Lower Upper
98 100
100 66.8 52.6 78.8

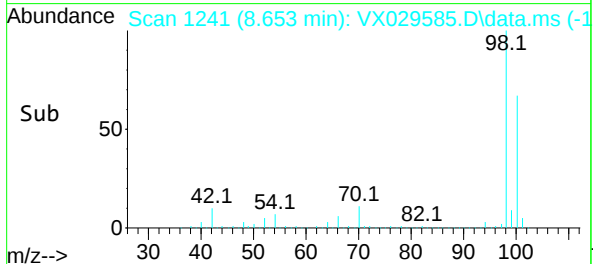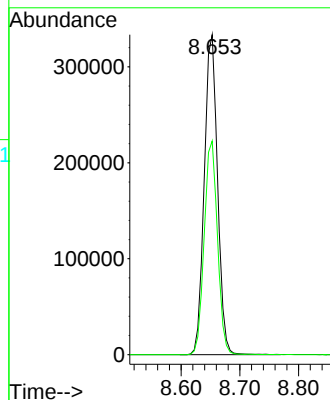

#51
4-Methyl-2-Pentanone
Concen: 6.991 ug/l
RT: 8.506 min Scan# 1217
Delta R.T. -0.068 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 43 Resp: 28924
Ion Ratio Lower Upper
43 100
58 13.9 36.1 54.1#


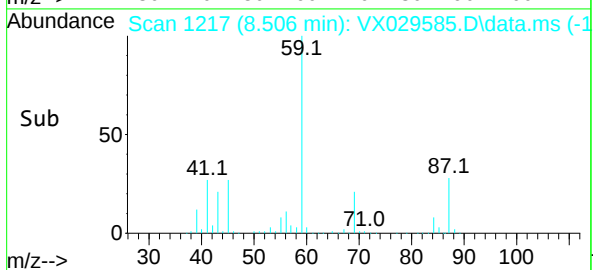
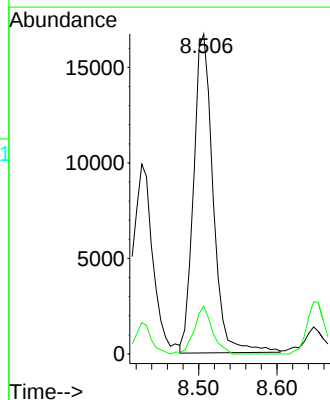
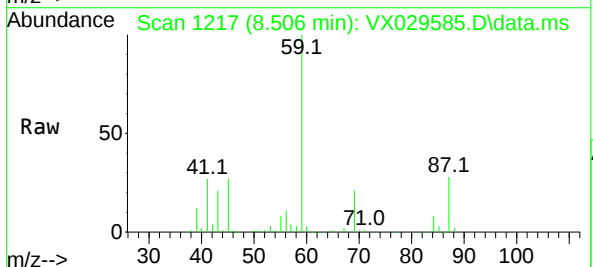




#56
Ethyl methacrylate
Concen: 5.288 ug/l
RT: 8.842 min Scan# 11
Delta R.T. -0.274 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 69 Resp: 24693
Ion Ratio Lower Upper
69 100
41 89.3 43.8 65.6#
39 37.5 22.2 33.2#



#59
2-Hexanone
Concen: 4.116 ug/l
RT: 9.567 min Scan# 1391
Delta R.T. 0.134 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 43 Resp: 12895
Ion Ratio Lower Upper
43 100
58 89.2 31.9 95.7





#62

4-Bromofluorobenzene

Concen: 45.377 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :

MW-19





Tgt Ion: 95 Resp: 186015

Ion Ratio Lower Upper

95 100

174 72.4 0.0 163.0

176 69.6 0.0 155.0

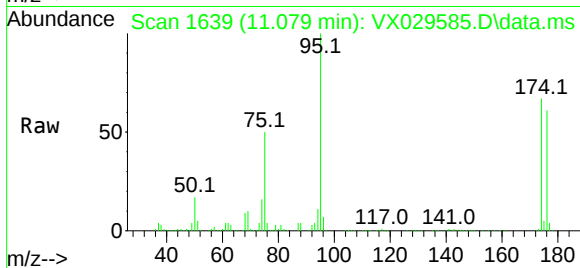

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX029585.D

Acq: 18 Jun 2022 21:15




Tgt Ion: 117 Resp: 393707


Ion Ratio Lower Upper

117 100

82 56.3 41.8 62.8

119 33.4 24.8 37.2




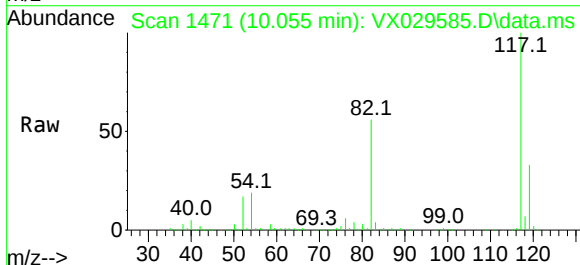




#67
Ethyl Benzene
Concen: 0.614 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 91 Resp: 8534
Ion Ratio Lower Upper
91 100
106 24.9 24.6 36.8

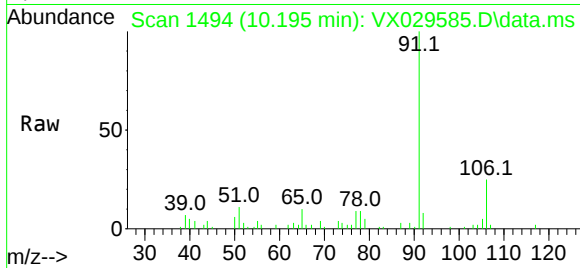

#68
m/p-Xylenes
Concen: 1.349 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 106 Resp: 7313
Ion Ratio Lower Upper
106 100
91 214.3 160.4 240.6









#69
o-Xylene
Concen: 0.355 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion:106 Resp: 1902
Ion Ratio Lower Upper
106 100
91 209.4 106.1 318.1

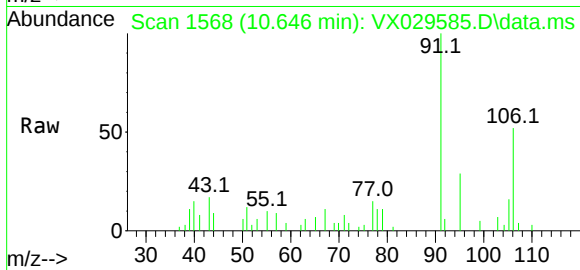

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion:152 Resp: 170347
Ion Ratio Lower Upper
152 100
115 62.9 37.5 112.7
150 156.7 0.0 338.2


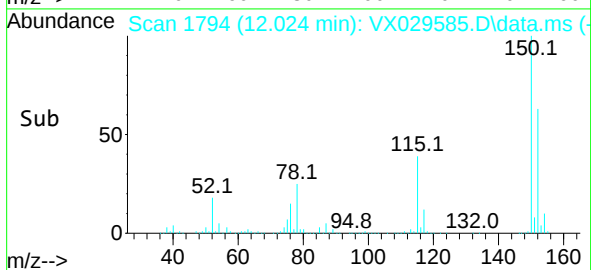






#76
1,2,3-Trichloropropane
Concen: 23.898 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 75 Resp: 88687
Ion Ratio Lower Upper
75 100
77 1.2 19.4 58.2#

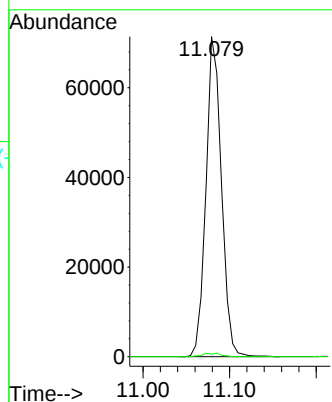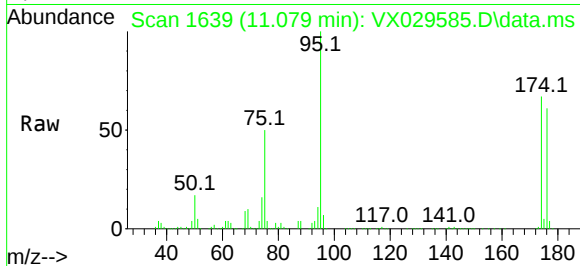

#78
n-propylbenzene
Concen: 0.233 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 91 Resp: 3350
Ion Ratio Lower Upper
91 100
120 22.5 11.6 34.8



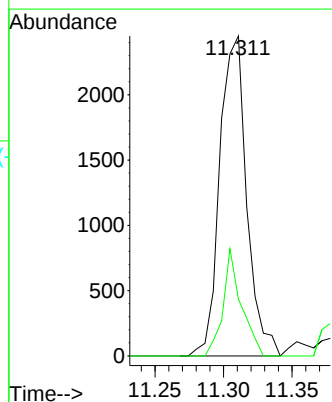





#81
trans-1,4-Dichloro-2-butene
Concen: 79.504 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15




Instrument :
MSVOA_X
ClientSampleId :
MW-19


Tgt Ion: 75 Resp: 88687
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

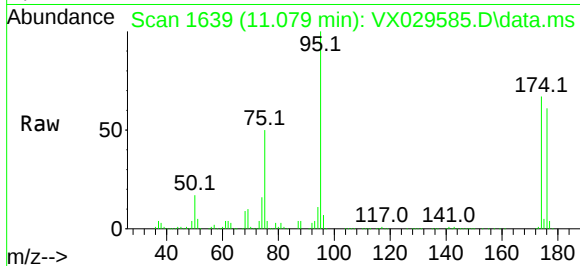

#84
1,2,4-Trimethylbenzene
Concen: 0.386 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX029585.D
Acq: 18 Jun 2022 21:15

Tgt Ion: 105 Resp: 4136
Ion Ratio Lower Upper
105 100
120 42.2 22.6 67.8

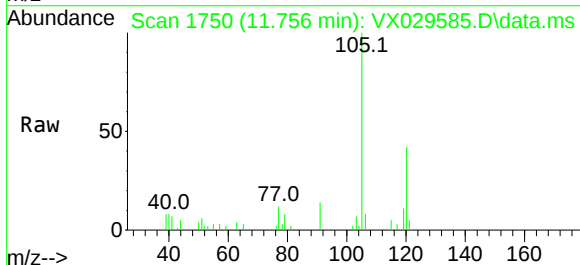



#95

Naphthalene

Concen: 0.358 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX029585.D


Acq: 18 Jun 2022 21:15

Instrument :

MSVOA_X

ClientSampleId :

MW-19

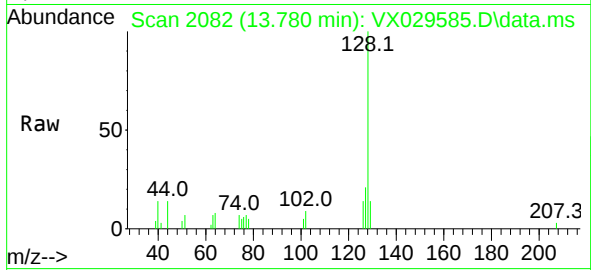

Tgt Ion:128 Resp: 4274

Ion Ratio Lower Upper

128 100

127 16.5 10.2 15.4#

129 12.0 8.7 13.1

