

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX061822\
 Data File : VX029596.D
 Acq On : 19 Jun 2022 02:17
 Operator : JC/MD
 Sample : N3290-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-28D2

Quant Time: Jun 20 01:39:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 20 01:31:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	273804	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	465466	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	402651	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	178750	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	156807	43.264	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.520%
35) Dibromofluoromethane	5.391	113	137973	45.485	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.980%
50) Toluene-d8	8.653	98	526066	47.472	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	94.940%
62) 4-Bromofluorobenzene	11.079	95	190856	45.671	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.340%

Target Compounds						Qvalue
3) Chloromethane	1.294	50	1362	0.381	ug/l	89
5) Bromomethane	1.624	94	640	0.381	ug/l	81
6) Chloroethane	1.691	64	2370	2.190	ug/l #	43
10) Methyl Iodide	2.471	142	602	3.190	ug/l #	86
11) Tert butyl alcohol	2.971	59	579019	751.656	ug/l	99
13) Acrolein	2.221	56	204	1.022	ug/l #	1
15) Acrylonitrile	3.111	53	10193	6.013	ug/l #	30
16) Acetone	2.386	43	7834	5.423	ug/l	94
18) Methyl Acetate	2.971	43	56959	14.912	ug/l #	46
19) Methyl tert-butyl Ether	3.117	73	1159555	120.409	ug/l	99
22) Diisopropyl ether	3.763	45	22391	2.527	ug/l #	83
23) Vinyl Acetate	3.757	43	11214	1.516	ug/l #	66
25) 2-Butanone	4.574	43	1905	0.834	ug/l	94
29) Tetrahydrofuran	5.032	42	752	0.494	ug/l #	76
36) 1,1-Dichloropropene	5.550	75	20396	4.968	ug/l #	49
38) Carbon Tetrachloride	5.556	117	28610	7.086	ug/l #	15
40) Benzene	6.050	78	7949	0.653	ug/l	96
43) Isopropyl Acetate	6.239	43	94128	14.384	ug/l #	58
44) Trichloroethene	7.135	130	2018	Below Cal		81
51) 4-Methyl-2-Pentanone	8.500	43	14886	3.529	ug/l #	56
56) Ethyl methacrylate	8.842	69	16761	3.521	ug/l #	67
59) 2-Hexanone	9.567	43	8651	2.709	ug/l	74
67) Ethyl Benzene	10.195	91	4629	0.326	ug/l #	89
68) m/p-Xylenes	10.305	106	13553	2.445	ug/l	99
69) o-Xylene	10.646	106	1494	0.273	ug/l	89
76) 1,2,3-Trichloropropane	11.079	75	90413	23.218	ug/l #	38
78) n-propylbenzene	11.305	91	7513	0.498	ug/l	93
79) 2-Chlorotoluene	11.305	91	7513	0.804	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	2463	0.218	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	90413	77.241	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	4892	0.435	ug/l	98
95) Naphthalene	13.780	128	14356	1.145	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 20 01:39:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061822W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 20 01:31:01 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion:168 Resp: 273804
Ion Ratio Lower Upper
168 100
99 60.0 41.7 62.5



#3
Chloromethane
Concen: 0.381 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 50 Resp: 1362
Ion Ratio Lower Upper
50 100
52 26.5 26.4 39.6




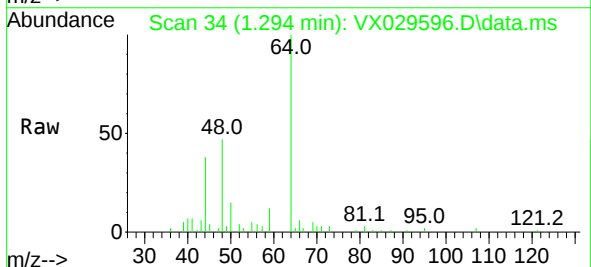


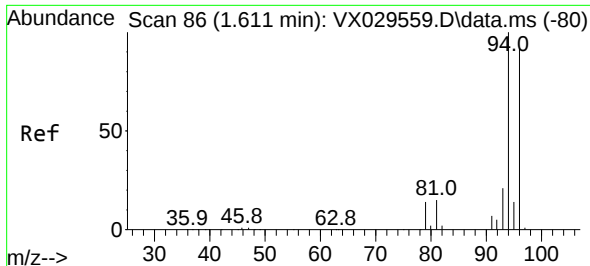

#5
Bromomethane
Concen: 0.381 ug/l
RT: 1.624 min Scan# 81
Delta R.T. 0.013 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 94 Resp: 640
Ion Ratio Lower Upper
94 100
96 76.2 75.3 112.9

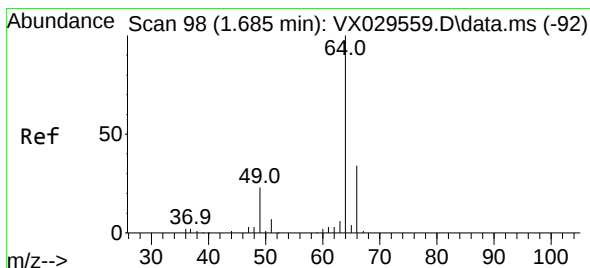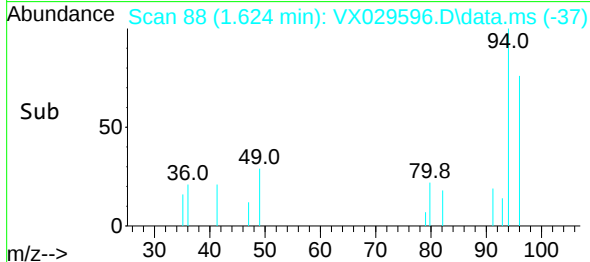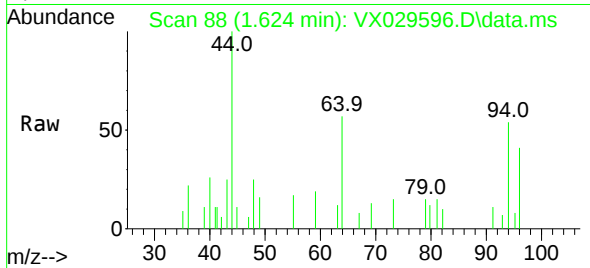

#6
Chloroethane
Concen: 2.190 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17


Tgt Ion: 64 Resp: 2370
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#

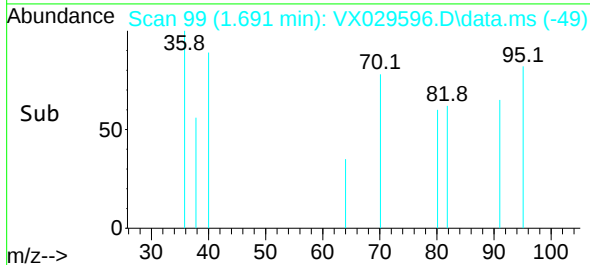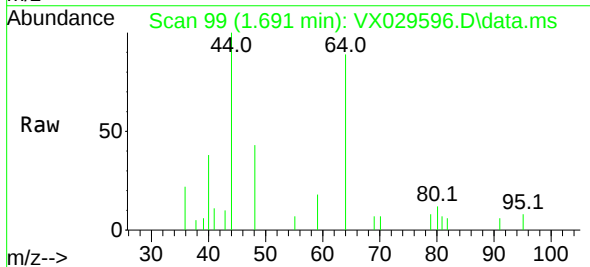


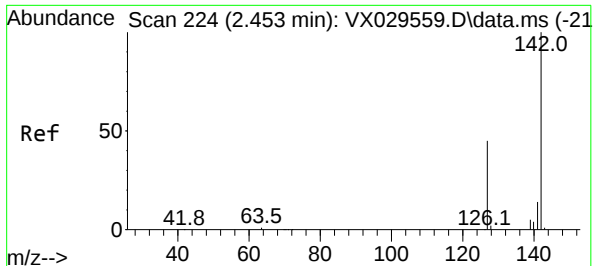


#10
Methyl Iodide
Concen: 3.190 ug/l
RT: 2.471 min Scan# 21
Delta R.T. 0.018 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Instrument :
MSVOA_X
ClientSampleId :
MW-28D2



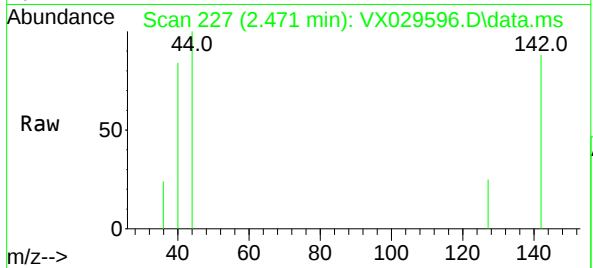



Tgt Ion:142 Resp: 602
Ion Ratio Lower Upper
142 100
127 36.4 33.9 50.9
141 3.8 11.4 17.2#

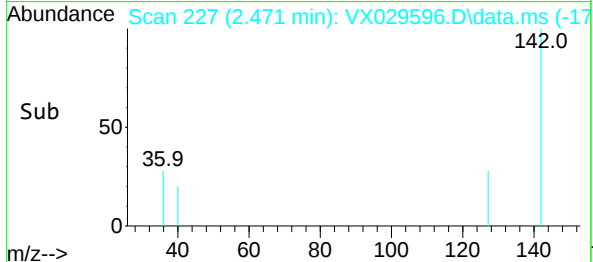

#11
Tert butyl alcohol
Concen: 751.656 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.012 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 59 Resp: 579019
Ion Ratio Lower Upper
59 100
57 10.1 8.3 12.5


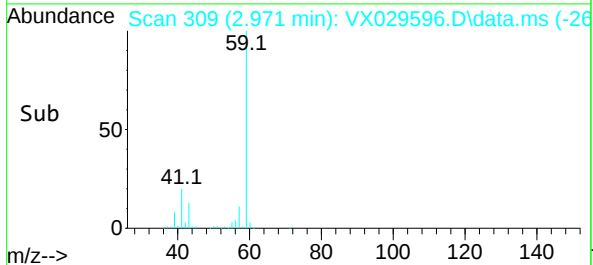

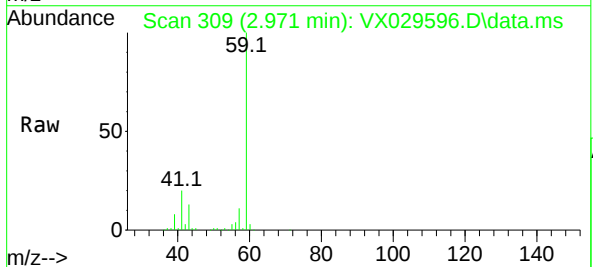




#13
Acrolein
Concen: 1.022 ug/l
RT: 2.221 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 56 Resp: 204
Ion Ratio Lower Upper
56 100
55 1967.2 55.0 82.6#

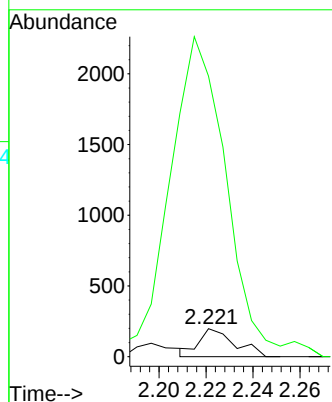

#15
Acrylonitrile
Concen: 6.013 ug/l
RT: 3.111 min Scan# 332
Delta R.T. 0.043 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 53 Resp: 10193
Ion Ratio Lower Upper
53 100
52 18.5 65.7 98.5#
51 75.3 28.4 42.6#


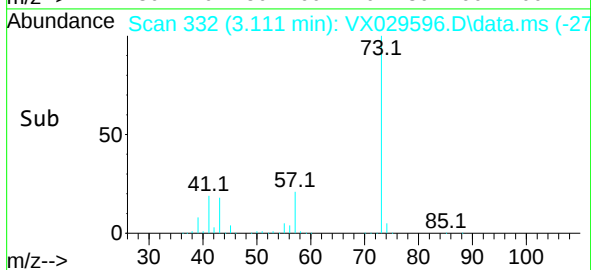






#16
Acetone
Concen: 5.423 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 43 Resp: 7834
Ion Ratio Lower Upper
43 100
58 32.4 28.8 43.2

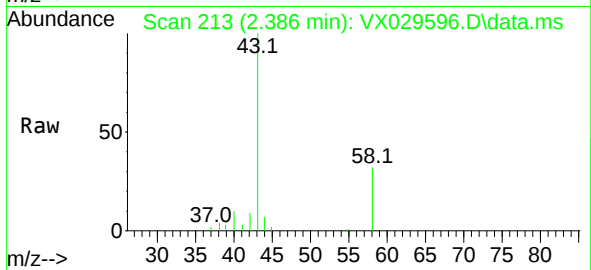

#18
Methyl Acetate
Concen: 14.912 ug/l
RT: 2.971 min Scan# 309
Delta R.T. 0.262 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 43 Resp: 56959
Ion Ratio Lower Upper
43 100
74 0.0 22.8 34.2#




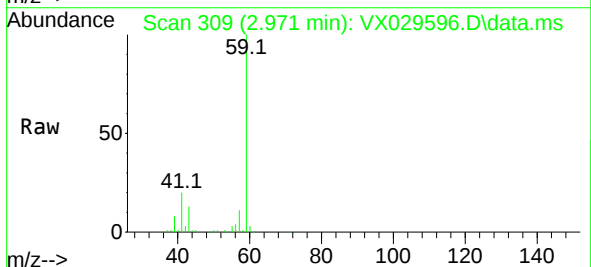




#19
Methyl tert-butyl Ether
Concen: 120.409 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 73 Resp: 1159555
Ion Ratio Lower Upper
73 100
57 20.6 16.8 25.2

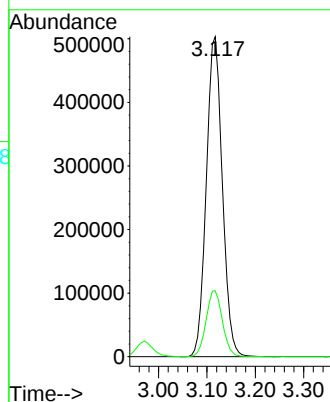

#22
Diisopropyl ether
Concen: 2.527 ug/l
RT: 3.763 min Scan# 439
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 45 Resp: 22391
Ion Ratio Lower Upper
45 100
43 43.6 50.8 76.2#
87 36.1 26.6 39.8
59 14.6 10.5 15.7


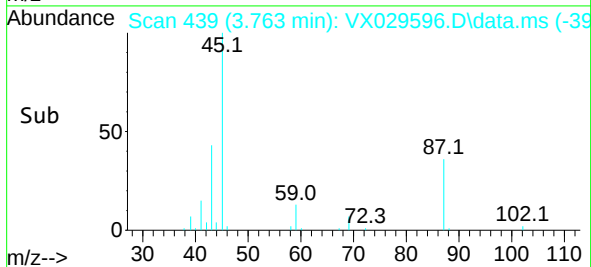

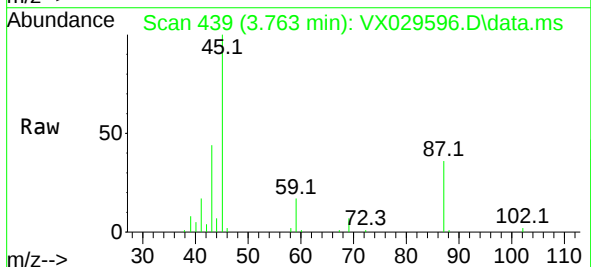


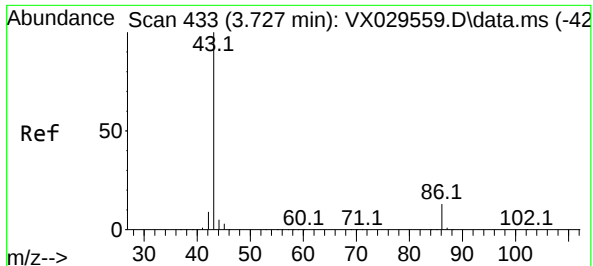

#23
 Vinyl Acetate
 Concen: 1.516 ug/l
 RT: 3.757 min Scan# 41
 Delta R.T. 0.030 min
 Lab File: VX029596.D
 Acq: 19 Jun 2022 02:17




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-28D2


Tgt Ion: 43 Resp: 11214
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.8 16.2#

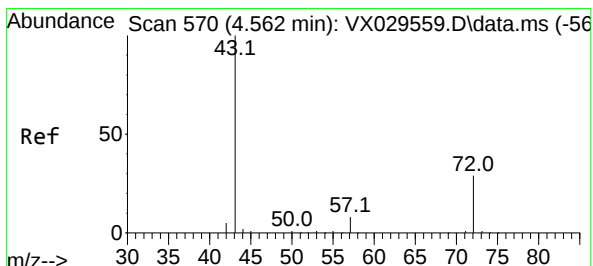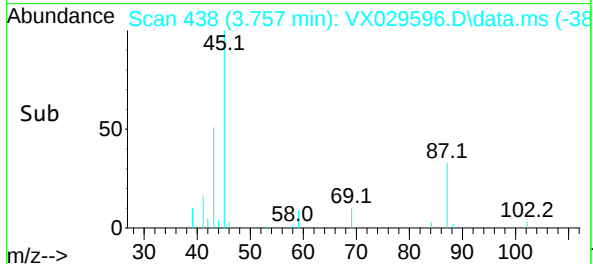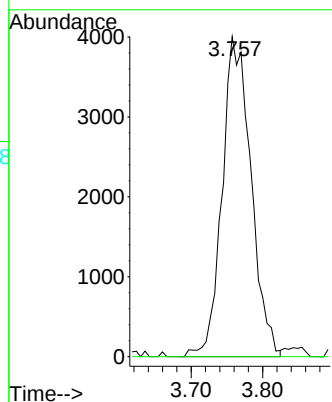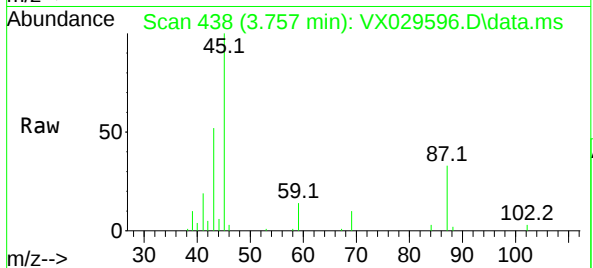

#25
 2-Butanone
 Concen: 0.834 ug/l
 RT: 4.574 min Scan# 572
 Delta R.T. 0.012 min
 Lab File: VX029596.D
 Acq: 19 Jun 2022 02:17

Tgt Ion: 43 Resp: 1905
 Ion Ratio Lower Upper
 43 100
 72 34.0 24.4 36.6

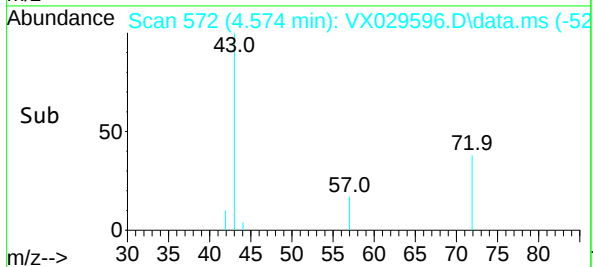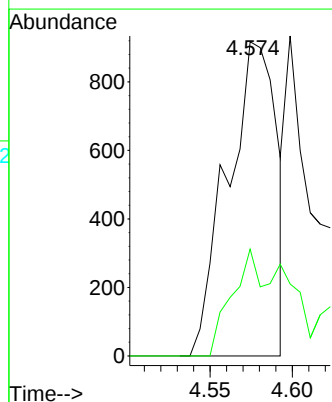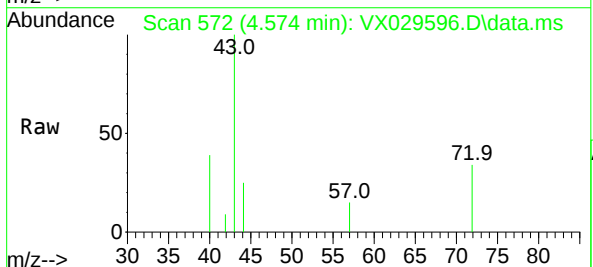

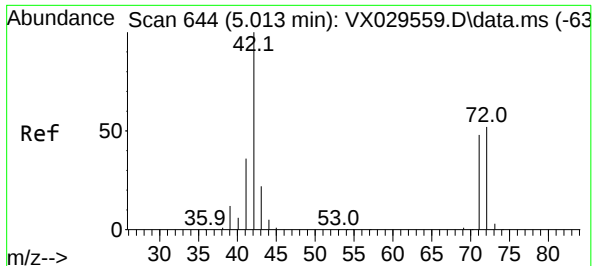

#29

Tetrahydrofuran

Concen: 0.494 ug/l

RT: 5.032 min Scan# 644

Delta R.T. 0.019 min

Lab File: VX029596.D

Acq: 19 Jun 2022 02:17





Instrument :

MSVOA_X

ClientSampleId :

MW-28D2

Tgt Ion:	42	Resp:	752
Ion	Ratio	Lower	Upper
42	100		
72	30.9	44.1	66.1#
71	40.8	40.5	60.7

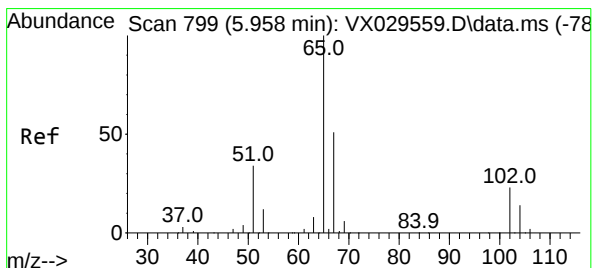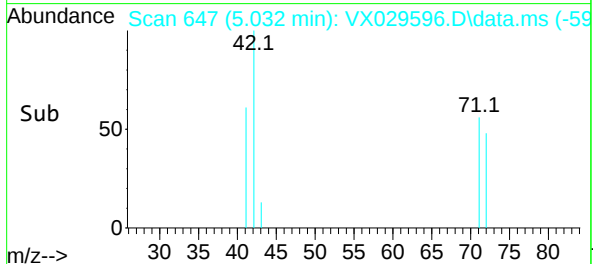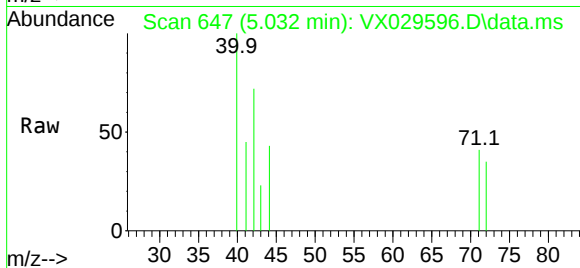

#33

1,2-Dichloroethane-d4

Concen: 43.264 ug/l




RT: 5.958 min Scan# 799


Delta R.T. 0.000 min

Lab File: VX029596.D

Acq: 19 Jun 2022 02:17

Tgt Ion:	65	Resp:	156807
Ion	Ratio	Lower	Upper
65	100		
67	52.4	0.0	107.4


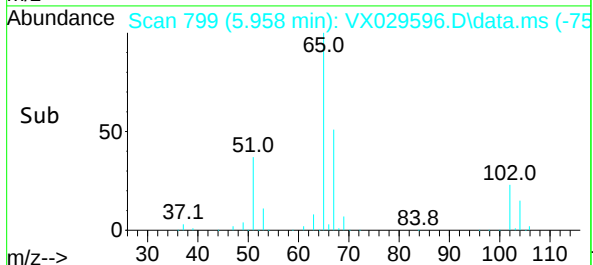

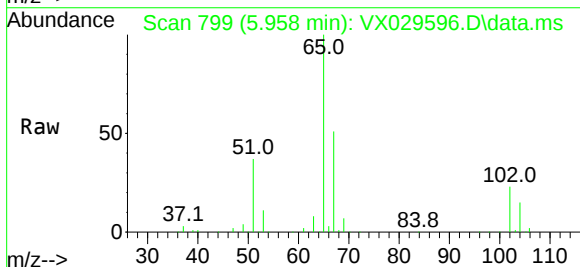




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion:114 Resp: 465466
Ion Ratio Lower Upper
114 100
63 19.3 0.0 36.8
88 16.6 0.0 32.4



#35
Dibromofluoromethane
Concen: 45.485 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion:113 Resp: 137973
Ion Ratio Lower Upper
113 100
111 101.8 82.8 124.2
192 18.7 16.9 25.3

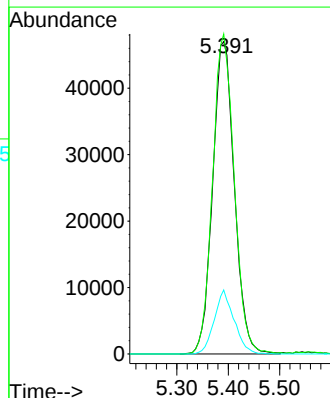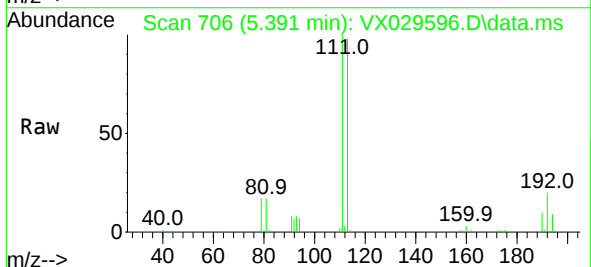



#36

1,1-Dichloropropene

Concen: 4.968 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.146 min

Lab File: VX029596.D

Acq: 19 Jun 2022 02:17

Instrument :

MSVOA_X

ClientSampleId :

MW-28D2





Tgt Ion: 75 Resp: 20396

Ion Ratio Lower Upper

75 100

110 9.3 18.3 54.8#

77 0.0 24.8 37.2#

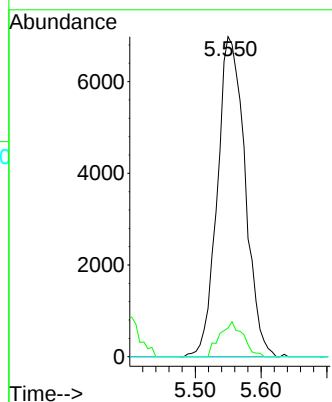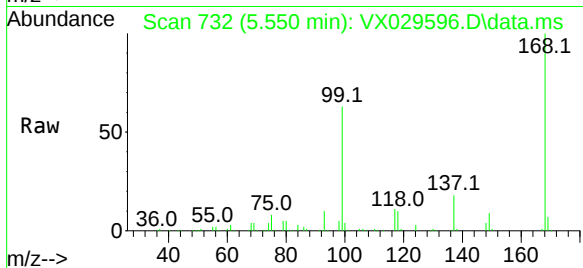

#38

Carbon Tetrachloride

Concen: 7.086 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX029596.D

Acq: 19 Jun 2022 02:17




Tgt Ion:117 Resp: 28610


Ion Ratio Lower Upper

117 100

119 4.6 77.3 115.9#

121 0.0 24.2 36.2#


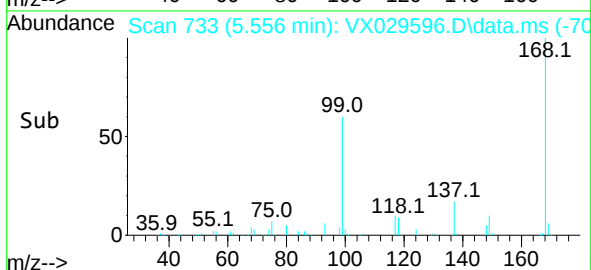

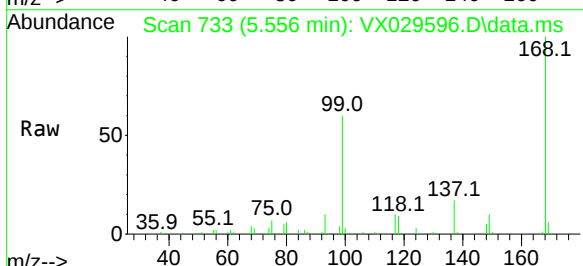


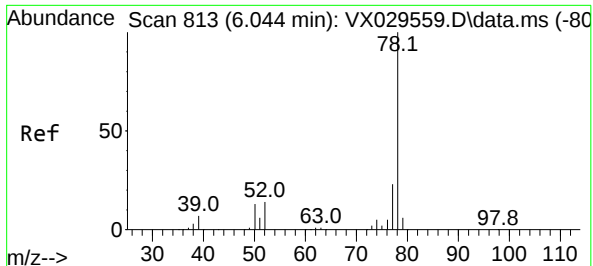

#40
Benzene
Concen: 0.653 ug/l
RT: 6.050 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 78 Resp: 7949
Ion Ratio Lower Upper
78 100
77 26.3 19.3 28.9

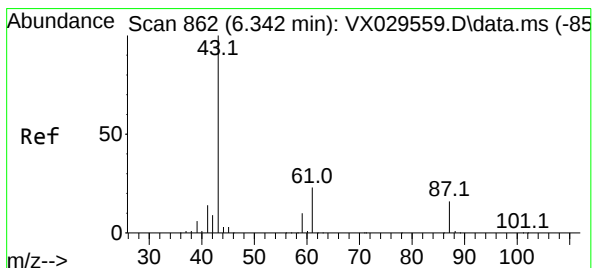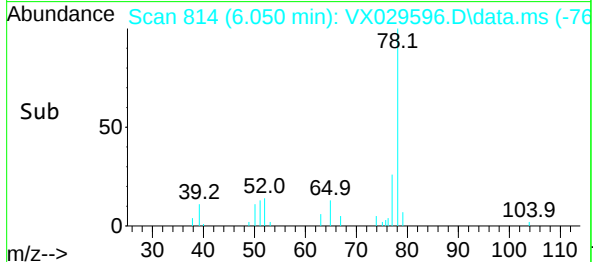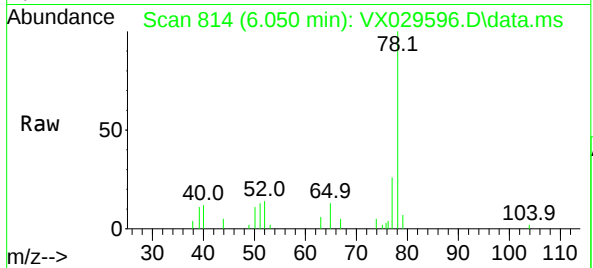

#43
Isopropyl Acetate
Concen: 14.384 ug/l
RT: 6.239 min Scan# 845
Delta R.T. -0.103 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 43 Resp: 94128
Ion Ratio Lower Upper
43 100
61 1.3 18.5 27.7#
87 0.1 13.0 19.6#


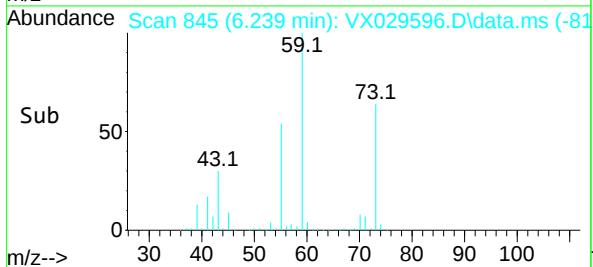

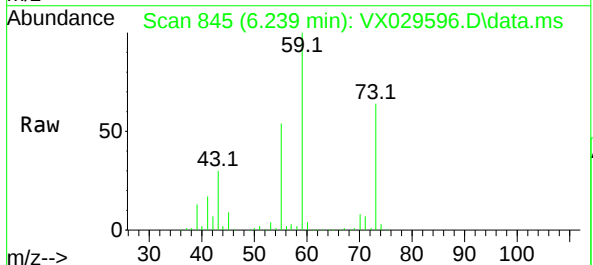




#44
 Trichloroethene
 Concen: Below Cal
 RT: 7.135 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX029596.D
 Acq: 19 Jun 2022 02:17




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-28D2


Tgt Ion:130 Resp: 2018
 Ion Ratio Lower Upper
 130 100
 95 113.0 0.0 188.8



#50
 Toluene-d8
 Concen: 47.472 ug/l
 RT: 8.653 min Scan# 1241
 Delta R.T. -0.000 min
 Lab File: VX029596.D
 Acq: 19 Jun 2022 02:17

Tgt Ion: 98 Resp: 526066
 Ion Ratio Lower Upper
 98 100
 100 67.2 52.6 78.8


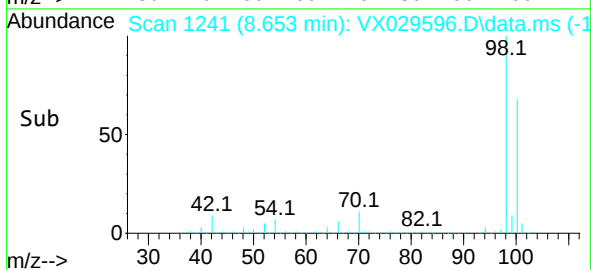

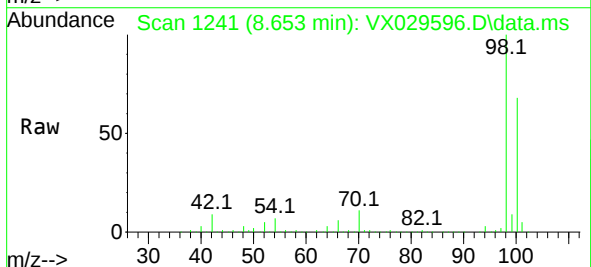




#51
4-Methyl-2-Pentanone
Concen: 3.529 ug/l
RT: 8.500 min Scan# 11
Delta R.T. -0.074 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 43 Resp: 14886
Ion Ratio Lower Upper
43 100
58 16.0 36.1 54.1#



#56
Ethyl methacrylate
Concen: 3.521 ug/l
RT: 8.842 min Scan# 1272
Delta R.T. -0.274 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 69 Resp: 16761
Ion Ratio Lower Upper
69 100
41 85.7 43.8 65.6#
39 35.3 22.2 33.2#

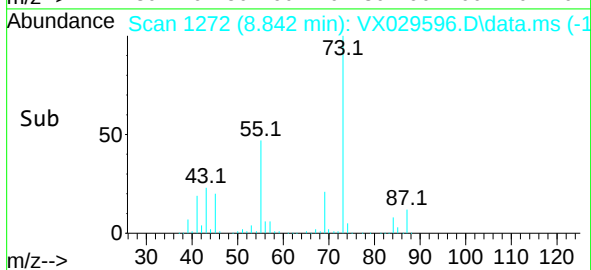

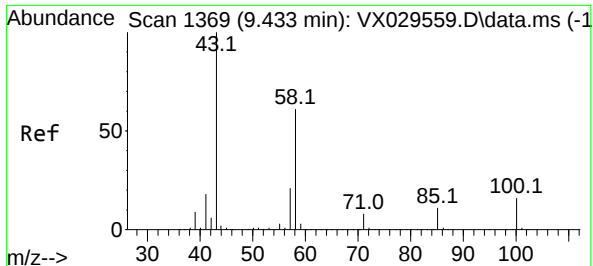

#59

2-Hexanone

Concen: 2.709 ug/l

RT: 9.567 min Scan# 11

Delta R.T. 0.134 min

Lab File: VX029596.D

Acq: 19 Jun 2022 02:17

Instrument :

MSVOA_X

ClientSampleId :





MW-28D2

Tgt Ion: 43 Resp: 8651

Ion Ratio Lower Upper

43 100

58 84.3 31.9 95.7

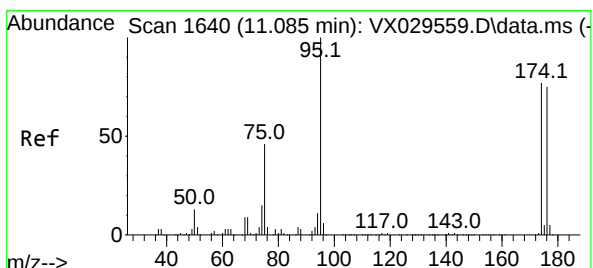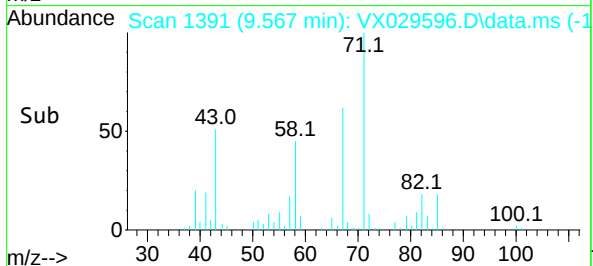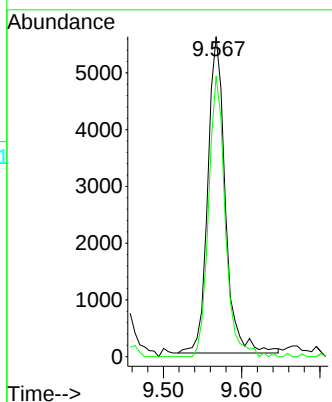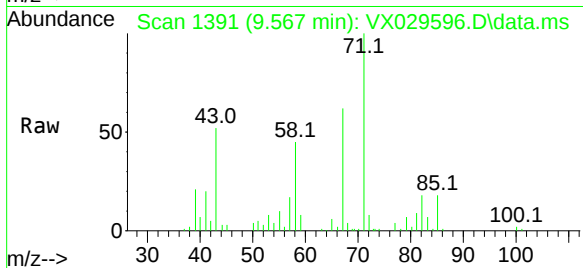

#62

4-Bromofluorobenzene

Concen: 45.671 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX029596.D

Acq: 19 Jun 2022 02:17




Tgt Ion: 95 Resp: 190856


Ion Ratio Lower Upper

95 100

174 71.4 0.0 163.0

176 70.7 0.0 155.0


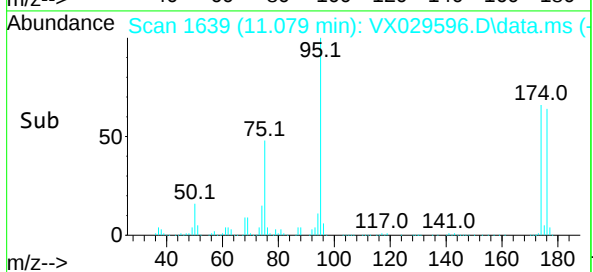
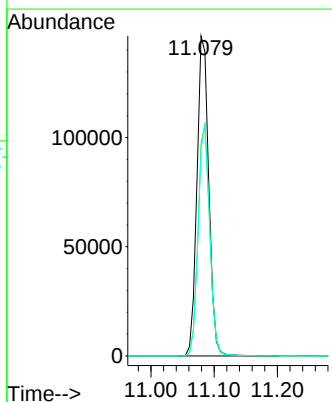
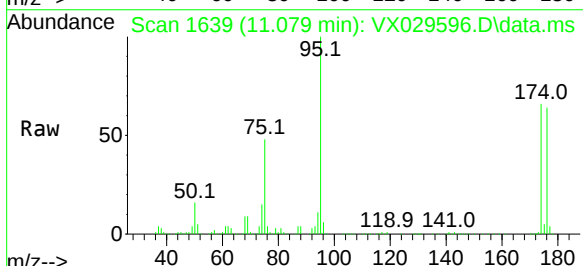




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion:117 Resp: 402651
Ion Ratio Lower Upper
117 100
82 54.4 41.8 62.8
119 31.7 24.8 37.2

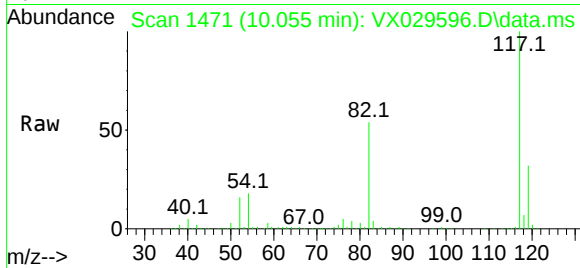

#67
Ethyl Benzene
Concen: 0.326 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 91 Resp: 4629
Ion Ratio Lower Upper
91 100
106 24.4 24.6 36.8#




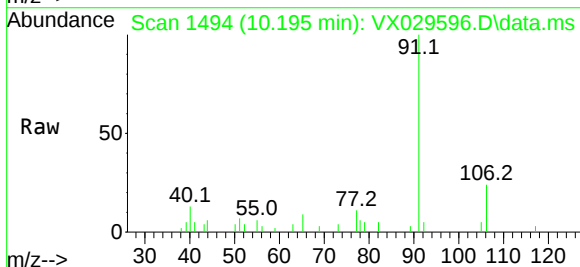


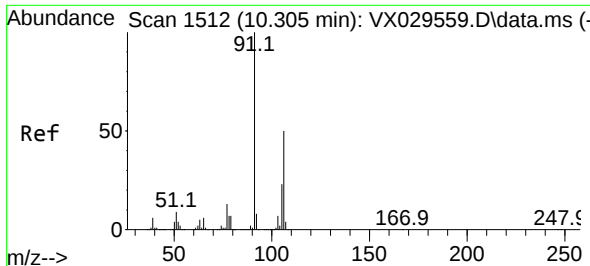

#68
m/p-Xylenes
Concen: 2.445 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion:106 Resp: 13553
Ion Ratio Lower Upper
106 100
91 202.2 160.4 240.6

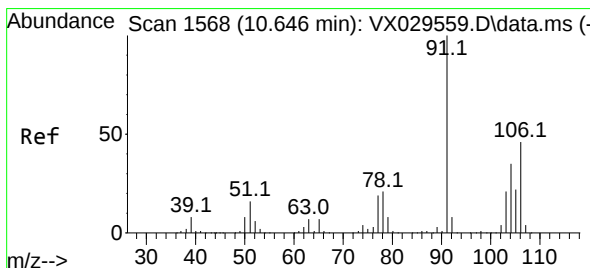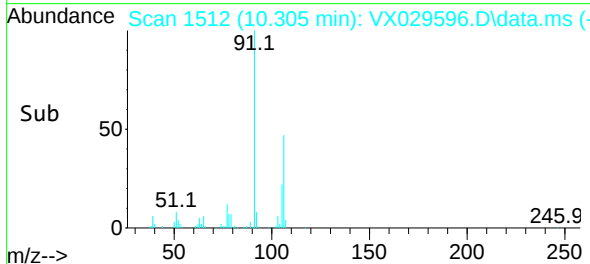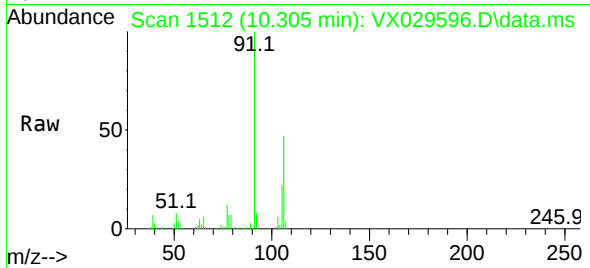

#69
o-Xylene
Concen: 0.273 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion:106 Resp: 1494
Ion Ratio Lower Upper
106 100
91 228.6 106.1 318.1


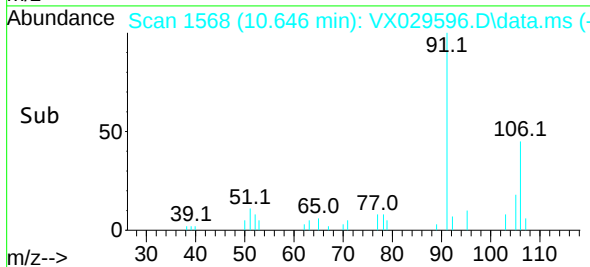

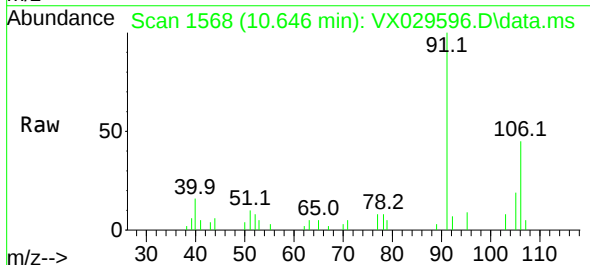




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion:152 Resp: 178750
Ion Ratio Lower Upper
152 100
115 61.8 37.5 112.7
150 156.6 0.0 338.2

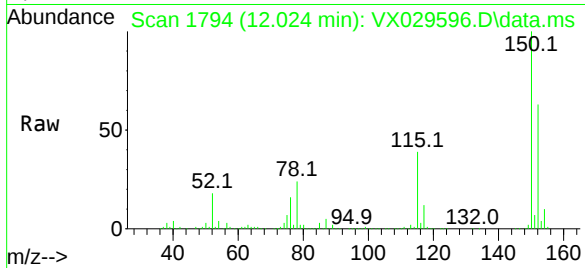

#76
1,2,3-Trichloropropane
Concen: 23.218 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 75 Resp: 90413
Ion Ratio Lower Upper
75 100
77 1.1 19.4 58.2#


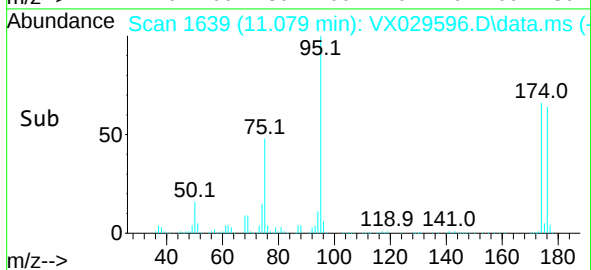

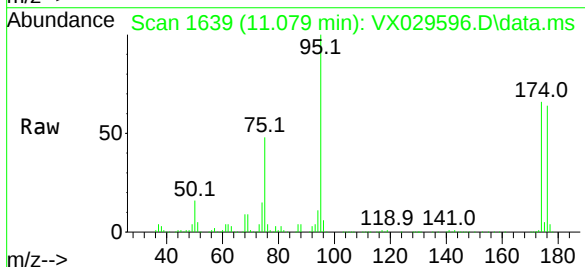


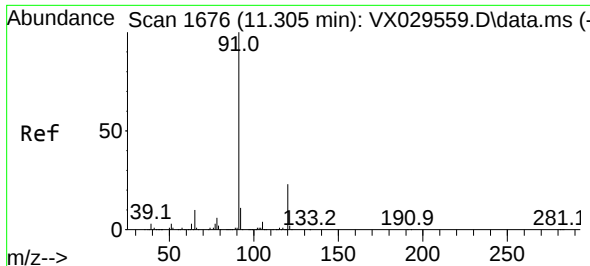

#78
n-propylbenzene
Concen: 0.498 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion: 91 Resp: 7513
Ion Ratio Lower Upper
91 100
120 19.9 11.6 34.8

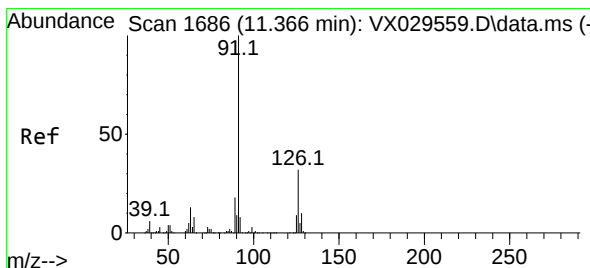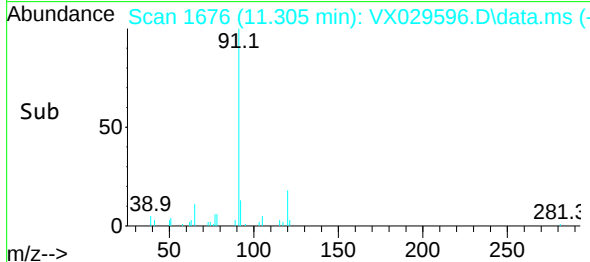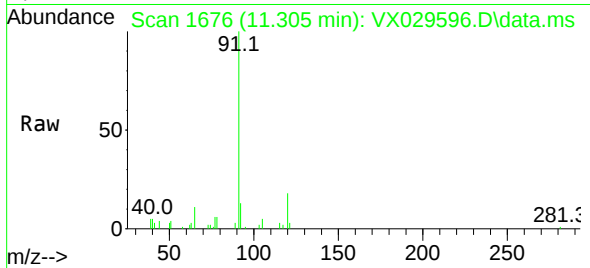

#79
2-Chlorotoluene
Concen: 0.804 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 91 Resp: 7513
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#


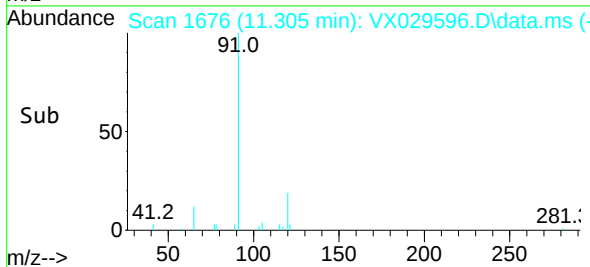

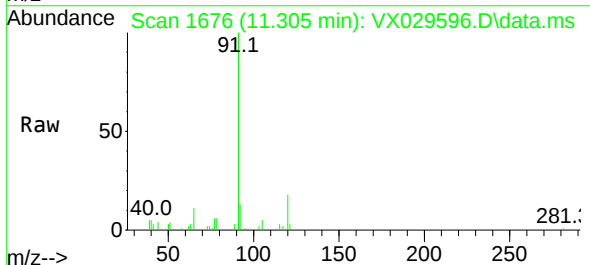




#80
1,3,5-Trimethylbenzene
Concen: 0.218 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17




Instrument :
MSVOA_X
ClientSampleId :
MW-28D2


Tgt Ion:105 Resp: 2463
Ion Ratio Lower Upper
105 100
120 50.5 24.3 72.9

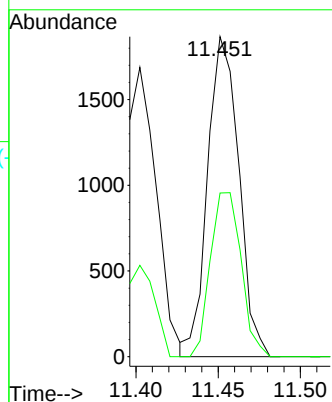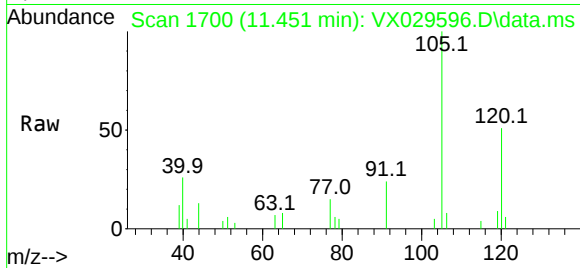

#81
trans-1,4-Dichloro-2-butene
Concen: 77.241 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion: 75 Resp: 90413
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#




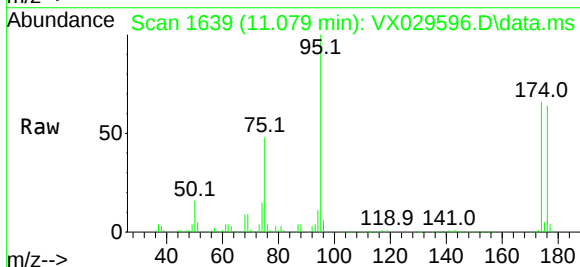




#84
1,2,4-Trimethylbenzene
Concen: 0.435 ug/l
RT: 11.756 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Instrument :
MSVOA_X
ClientSampleId :
MW-28D2

Tgt Ion:105 Resp: 4892
Ion Ratio Lower Upper
105 100
120 43.7 22.6 67.8

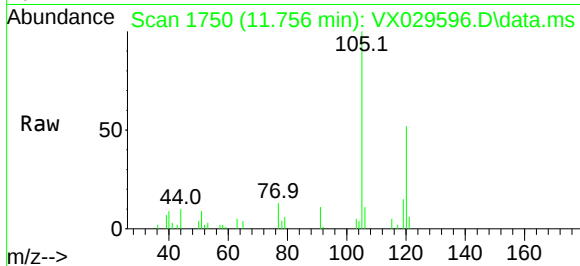

#95
Naphthalene
Concen: 1.145 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX029596.D
Acq: 19 Jun 2022 02:17

Tgt Ion:128 Resp: 14356
Ion Ratio Lower Upper
128 100
127 11.5 10.2 15.4
129 11.5 8.7 13.1

